


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121321\
 Data File : VV023938.D
 Acq On : 13 Dec 2021 09:18
 Operator : SY/MD
 Sample : BFB207
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB207

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM112221.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Dec 14 01:14:27 2021

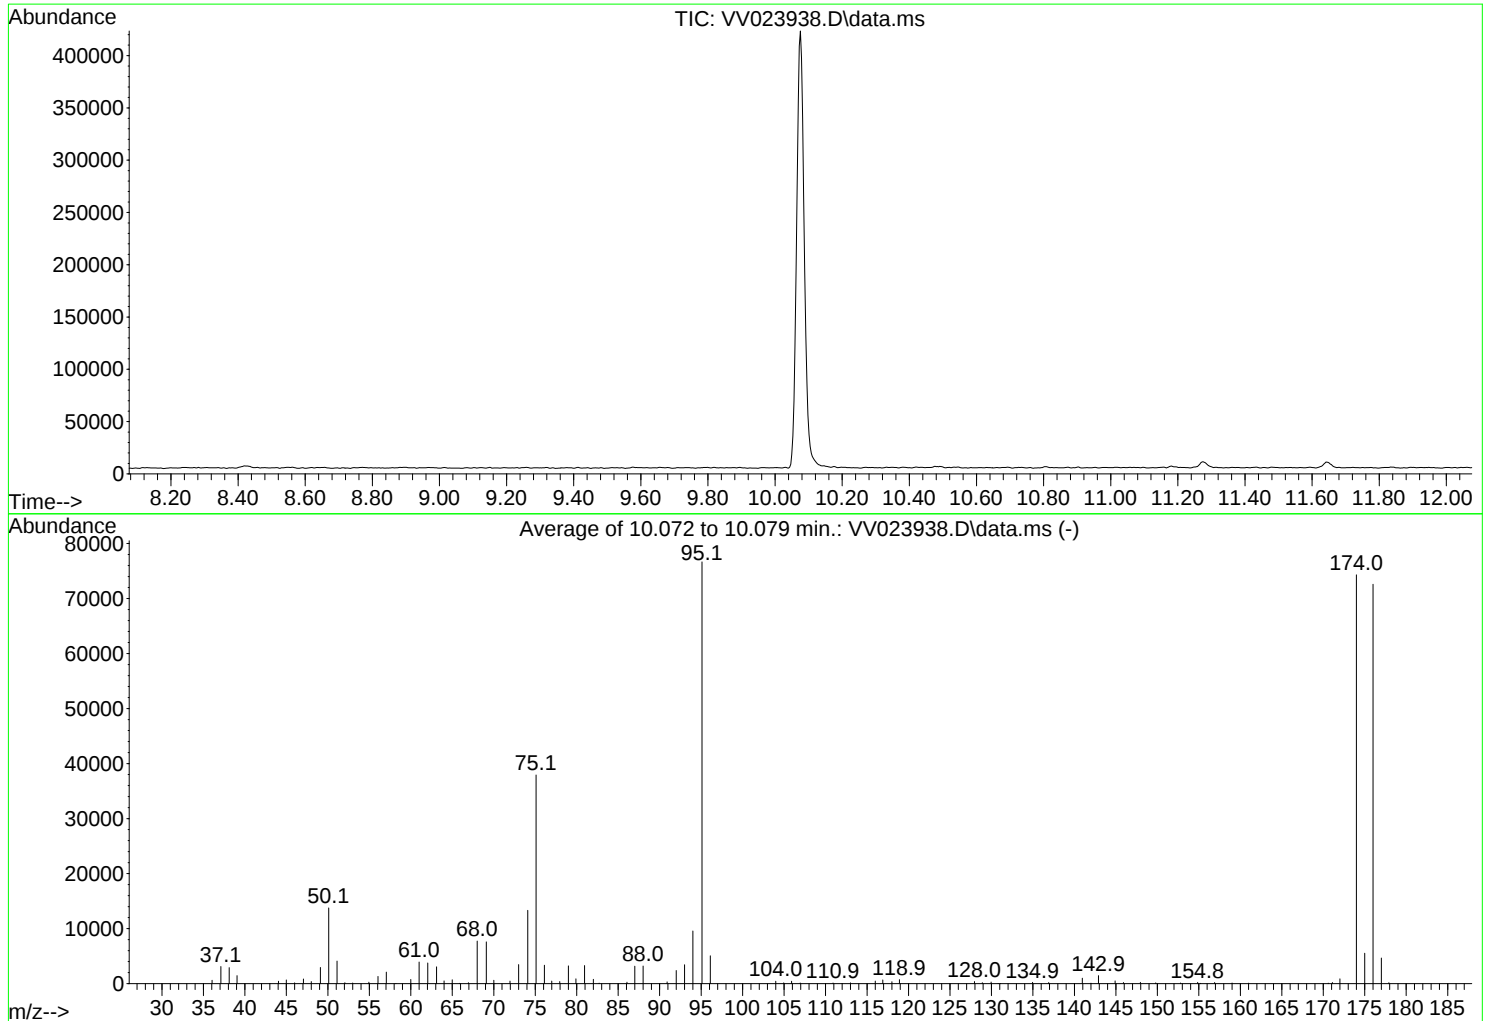

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	13771	PASS
75	95	30	80	49.5	37915	PASS
95	95	100	100	100.0	76672	PASS
96	95	5	9	6.6	5076	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	96.9	74312	PASS
175	174	5	9	7.4	5517	PASS
176	174	95	101	97.7	72603	PASS
177	176	5	9	6.4	4671	PASS

m/z	Abundance
40.00	6023.0
44.10	211.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	561.0
37.10	3202.0
38.10	2895.0
39.10	1496.0
40.00	5822.0
44.00	665.0
45.00	697.0
46.00	163.0
47.00	888.0
48.00	412.0
49.10	3017.0
50.10	14058.0
51.10	4126.0
52.00	183.0
53.00	123.0
54.90	318.0
56.00	1226.0
57.10	2162.0
58.20	116.0
60.00	817.0
61.00	4001.0
62.00	3774.0
63.10	3227.0
64.00	455.0
65.00	734.0
67.10	188.0
68.00	7633.0
69.10	7495.0
70.00	631.0
72.00	448.0
73.00	3475.0
74.10	13316.0
75.10	38752.0
76.10	3330.0
77.00	463.0
78.00	362.0
79.00	3240.0
79.90	885.0
80.90	3245.0
82.00	778.0
86.10	252.0
87.00	3308.0
88.00	3213.0
90.90	319.0
92.00	2307.0
93.00	3515.0
94.00	9722.0
95.10	76664.0
96.10	5367.0
104.00	425.0
105.00	113.0
105.90	424.0
107.00	114.0
110.90	123.0
113.00	156.0
116.00	463.0
116.90	628.0
118.10	362.0
118.90	716.0
128.00	416.0
128.90	205.0
129.90	282.0
130.80	117.0
135.00	236.0
136.90	207.0
140.00	104.0
141.00	972.0
142.90	1357.0
144.90	487.0
145.90	151.0
147.90	278.0
149.80	146.0
152.80	115.0
154.90	178.0
155.20	162.0
156.90	201.0
158.90	102.0
170.60	154.0
171.10	145.0
172.00	780.0
174.00	72952.0
175.00	5505.0
176.00	71456.0
177.00	4663.0
177.90	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	642.0
37.10	3187.0
38.10	3053.0
39.00	1485.0
40.00	5819.0
44.10	654.0
45.00	671.0
46.00	148.0
47.00	858.0
48.00	399.0
49.10	3047.0
50.10	14172.0
51.10	4231.0
52.10	193.0
53.00	127.0
54.90	274.0
56.10	1320.0
57.00	2178.0
60.00	804.0
61.00	4120.0
62.00	3867.0
63.10	3154.0
64.00	528.0
65.00	732.0
65.90	111.0
66.90	146.0
68.00	7940.0
69.10	7817.0
70.00	646.0
71.90	502.0
73.00	3594.0
74.10	13735.0
75.10	39144.0
76.10	3492.0
77.00	470.0
77.90	401.0
79.00	3341.0
79.90	900.0
80.90	3377.0
82.00	804.0
82.70	117.0
86.10	300.0
87.00	3354.0
88.00	3279.0
90.90	344.0
92.00	2451.0
93.00	3506.0
94.00	9880.0
95.10	79208.0
96.10	5202.0
104.00	474.0
105.00	142.0
105.90	475.0
107.00	124.0
110.90	122.0
113.00	154.0
116.00	492.0
116.90	673.0
118.00	337.0
118.90	759.0
127.90	412.0
128.90	174.0
130.00	291.0
131.10	105.0
135.00	243.0
136.90	192.0
140.90	1015.0
142.00	116.0
142.90	1533.0
144.90	514.0
145.90	210.0
148.00	253.0
149.80	149.0
152.80	142.0
154.80	233.0
156.90	223.0
159.00	106.0
161.00	122.0
170.60	138.0
171.10	182.0
172.00	909.0
174.00	76752.0
175.00	5673.0
176.00	75344.0
177.00	4837.0
177.90	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.10	612.0
37.10	2916.0
38.10	2797.0
39.00	1353.0
40.00	5809.0
43.00	103.0
44.10	619.0
45.00	619.0
46.00	124.0
47.10	757.0
48.00	355.0
49.10	2784.0
50.10	13083.0
51.10	3908.0
52.10	196.0
53.00	107.0
55.00	226.0
56.10	1361.0
57.00	1982.0
60.00	671.0
61.00	3707.0
62.10	3626.0
63.10	2793.0
64.00	513.0
65.00	659.0
65.90	102.0
66.90	172.0
68.00	7648.0
69.10	7493.0
70.00	596.0
71.90	452.0
73.00	3326.0
74.10	12955.0
75.10	35848.0
76.10	3205.0
77.00	448.0
77.90	400.0
79.00	3094.0
79.90	823.0
81.00	3242.0
82.00	804.0
82.70	130.0
86.00	252.0
87.00	2838.0
88.00	3129.0
90.90	321.0
92.00	2403.0
93.00	3259.0
94.00	9097.0
95.10	74144.0
96.10	4659.0
104.00	432.0
104.90	151.0
105.90	411.0
106.90	126.0
110.90	105.0
112.00	110.0
113.00	151.0
116.00	441.0
116.90	680.0
117.90	329.0
118.90	688.0
127.90	352.0
128.90	162.0
130.00	272.0
134.90	198.0
136.90	189.0
140.90	960.0
142.00	114.0
142.90	1497.0
144.90	496.0
145.90	225.0
147.90	201.0
149.80	122.0
152.80	135.0
154.90	252.0
156.90	221.0
159.10	153.0
161.00	153.0
171.10	249.0
172.00	951.0
174.00	73232.0
175.00	5372.0
176.00	71008.0
177.00	4514.0
177.90	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207