

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029654.D
 Acq On : 13 Dec 2022 16:24
 Operator : SY/MD
 Sample : N5950-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF52

Quant Time: Dec 13 22:53:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 13 22:49:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	518077	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	479257	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	251659	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	130288	41.068	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.140%
7) Chloroethane-d5	1.565	69	110390	45.632	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.260%
11) 1,1-Dichloroethene-d2	2.105	63	171864	34.732	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.460%
21) 2-Butanone-d5	3.870	46	180359	93.194	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.190%
24) Chloroform-d	4.339	84	246691	41.322	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.640%
26) 1,2-Dichloroethane-d4	5.021	65	143136	41.979	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.960%
32) Benzene-d6	5.043	84	528793	41.757	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.520%
36) 1,2-Dichloropropane-d6	6.063	67	162737	42.071	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.140%
41) Toluene-d8	7.307	98	470909	39.466	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	78.940%#
43) trans-1,3-Dichloroprop...	7.612	79	65994	33.787	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.580%
47) 2-Hexanone-d5	8.082	63	143542	86.901	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	86.900%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	232620	42.084	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	84.160%
66) 1,2-Dichlorobenzene-d4	11.612	152	196836	41.088	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.180%
Target Compounds						
13) Acetone	2.156	43	23943	18.991	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029654.D
Acq On : 13 Dec 2022 16:24
Operator : SY/MD
Sample : N5950-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF52

Quant Time: Dec 13 22:53:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 13 22:49:59 2022
Response via : Initial Calibration

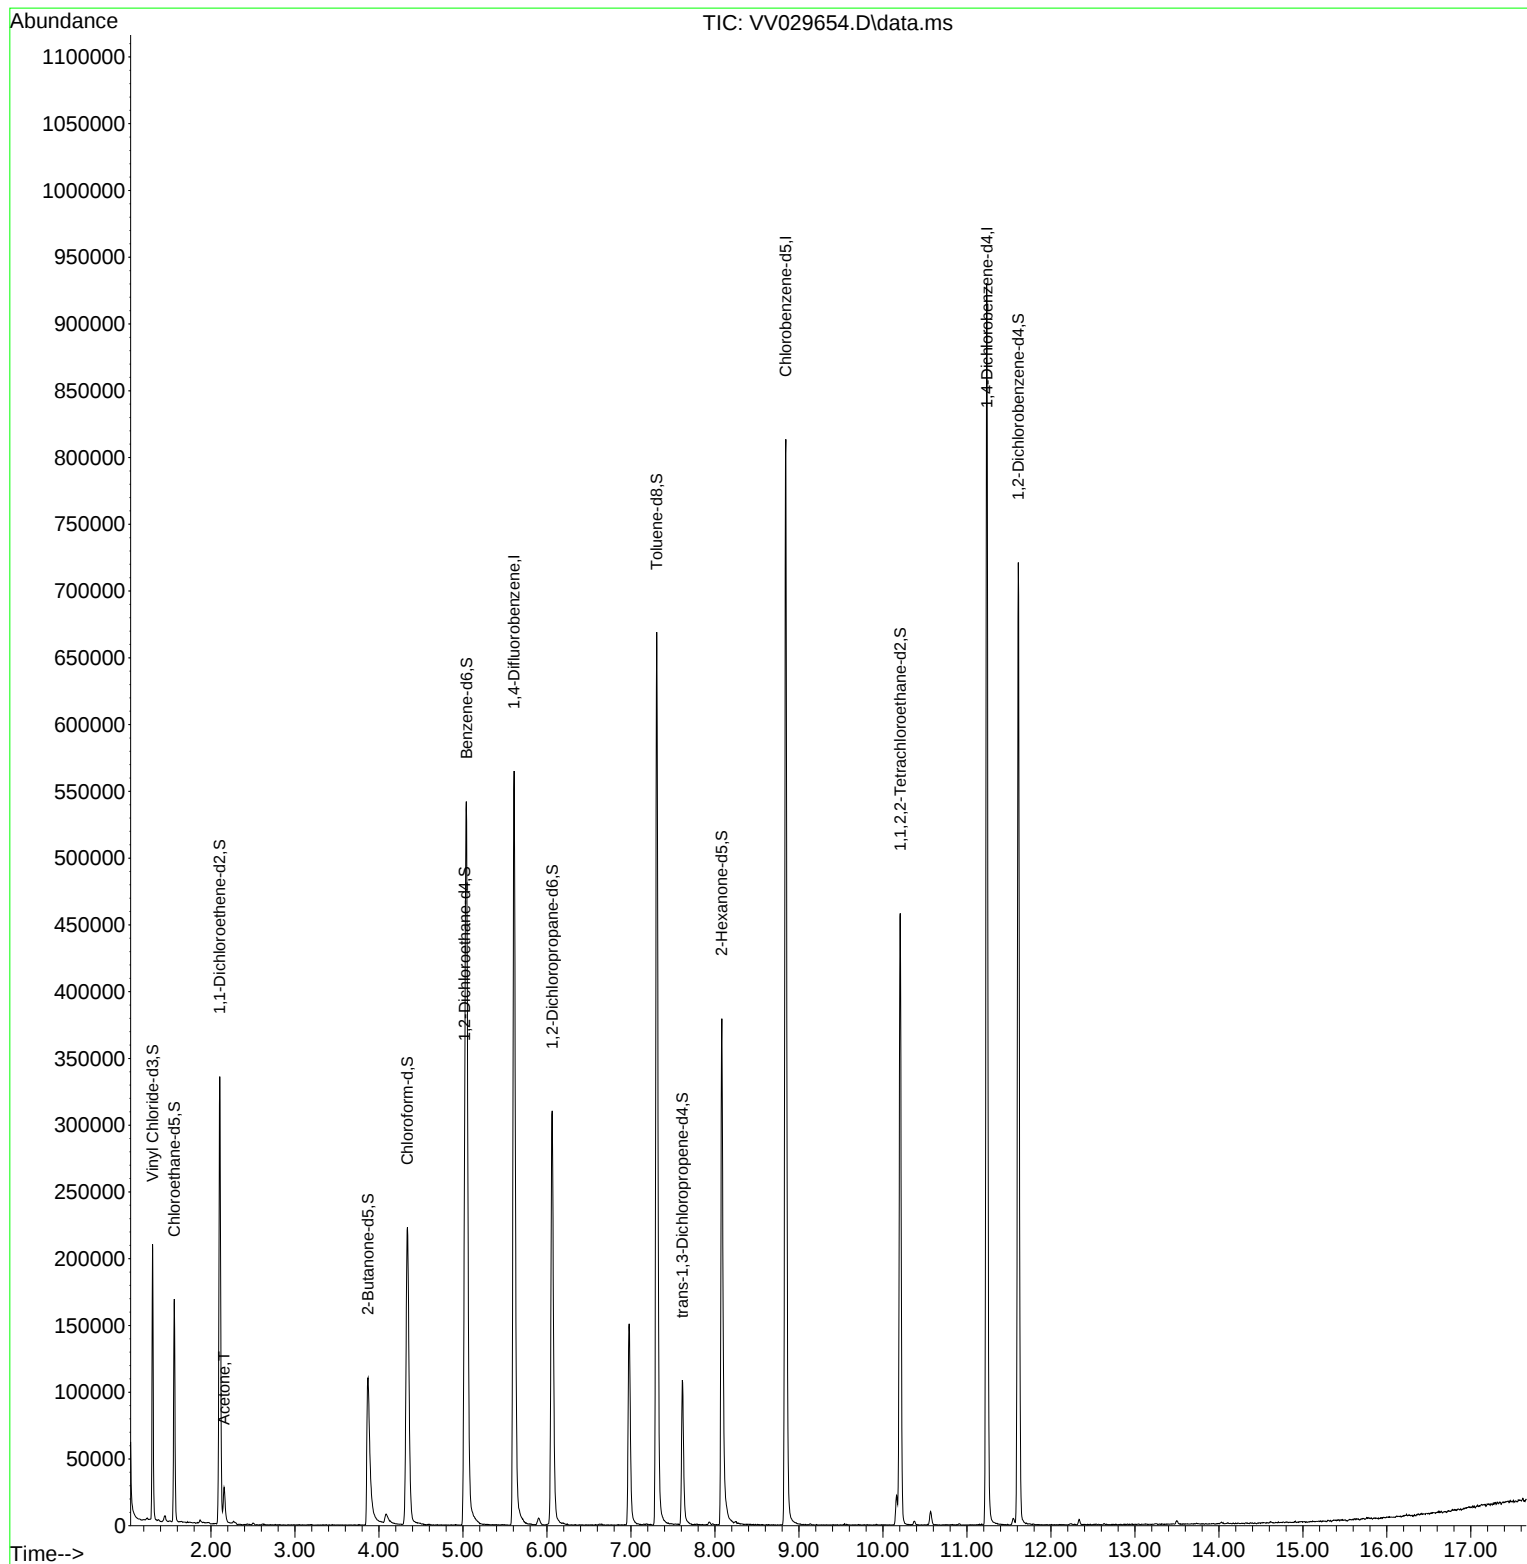

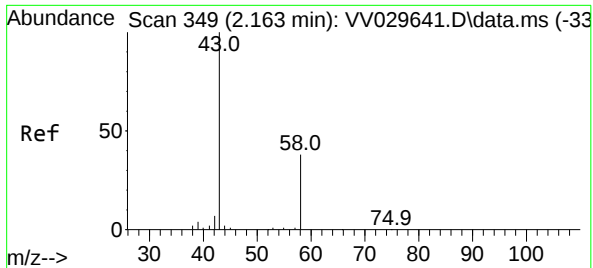

#13
 Acetone
 Concen: 18.991 ug/L
 RT: 2.156 min Scan# 34
 Delta R.T. -0.006 min
 Lab File: VV029654.D
 Acq: 13 Dec 2022 16:24

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF52

Tgt Ion: 43 Resp: 23943
 Ion Ratio Lower Upper
 43 100
 58 39.1 0.0 74.8

