

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029659.D
 Acq On : 13 Dec 2022 18:22
 Operator : SY/MD
 Sample : N5980-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP3

Quant Time: Dec 13 22:54:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 13 22:49:59 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	365479	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	338139	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	177918	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	115453	51.587	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	103.180%	
7) Chloroethane-d5	1.564	69	95550	55.989	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	111.980%	
11) 1,1-Dichloroethene-d2	2.105	63	148957	42.672	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	85.340%	
21) 2-Butanone-d5	3.873	46	151263	110.794	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	110.790%	
24) Chloroform-d	4.339	84	208679	49.549	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	99.100%	
26) 1,2-Dichloroethane-d4	5.024	65	128406	53.383	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	106.760%	
32) Benzene-d6	5.043	84	454394	50.857	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	101.720%	
36) 1,2-Dichloropropane-d6	6.063	67	141289	51.770	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	103.540%	
41) Toluene-d8	7.307	98	401691	47.715	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	95.420%	
43) trans-1,3-Dichloroprop...	7.616	79	58851	42.704	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	85.400%	
47) 2-Hexanone-d5	8.082	63	125061	107.310	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	107.310%	
56) 1,1,2,2-Tetrachloroeth...	10.204	84	197338	50.600	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	101.200%	
66) 1,2-Dichlorobenzene-d4	11.612	152	167704	49.516	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	99.040%	
Target Compounds						Qvalue
13) Acetone	2.166	43	3026	3.402	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029659.D
Acq On : 13 Dec 2022 18:22
Operator : SY/MD
Sample : N5980-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP3

Quant Time: Dec 13 22:54:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 13 22:49:59 2022
Response via : Initial Calibration

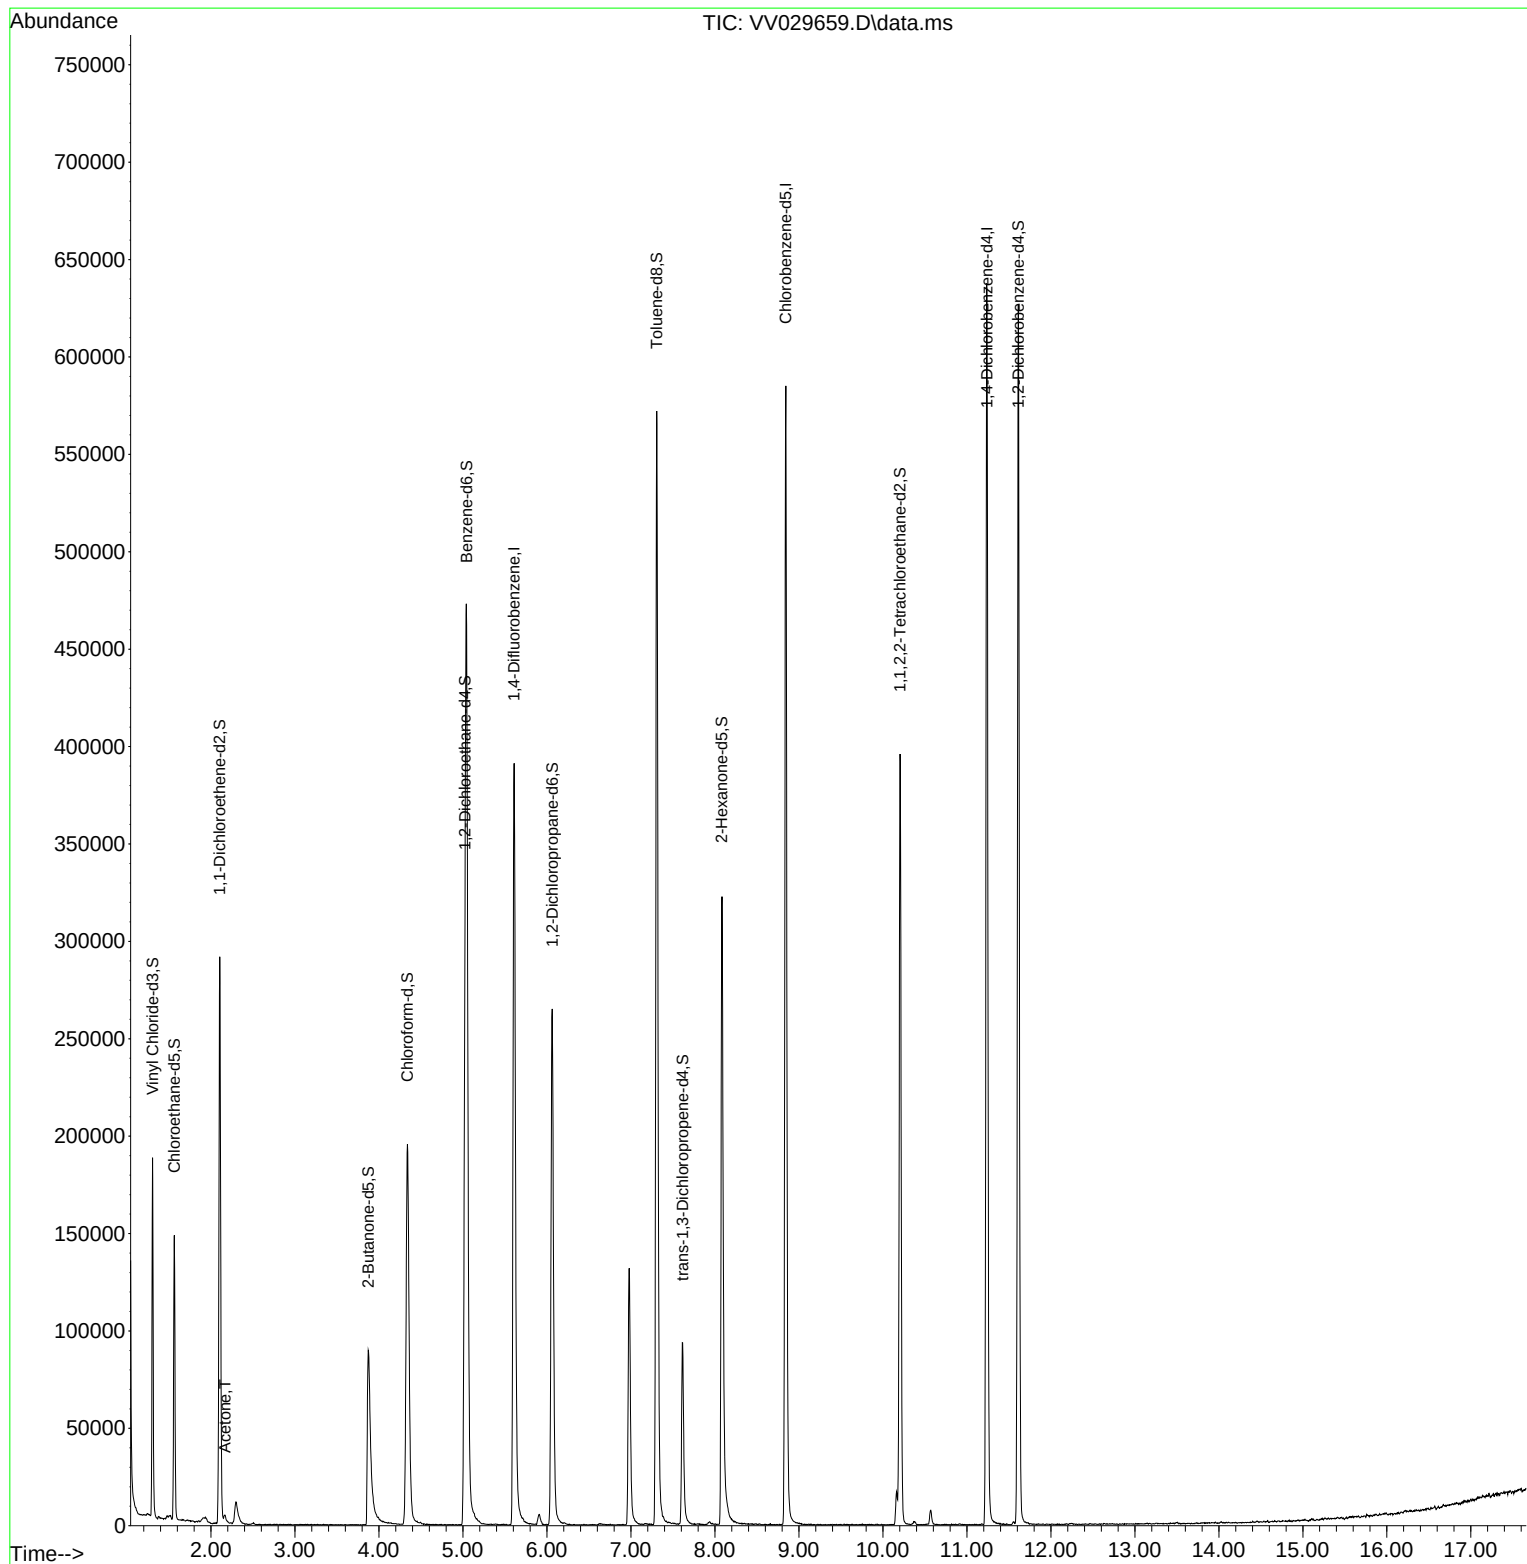

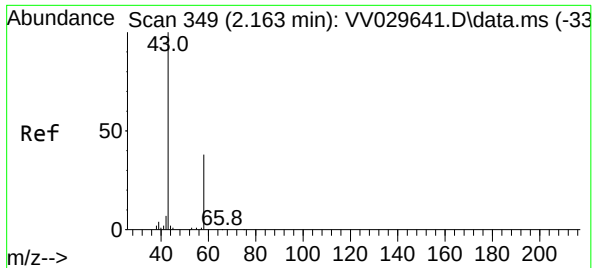

#13
 Acetone
 Concen: 3.402 ug/L
 RT: 2.166 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV029659.D
 Acq: 13 Dec 2022 18:22

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP3

Tgt Ion: 43 Resp: 3026
 Ion Ratio Lower Upper
 43 100
 58 41.7 0.0 74.8

