

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029660.D
 Acq On : 13 Dec 2022 18:46
 Operator : SY/MD
 Sample : N5980-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP4

Quant Time: Dec 13 22:54:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 13 22:49:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	453320	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	417986	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	218855	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	119056	42.889	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	85.780%		
7) Chloroethane-d5	1.564	69	102015	48.194	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	96.380%		
11) 1,1-Dichloroethene-d2	2.105	63	159356	36.805	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.620%		
21) 2-Butanone-d5	3.873	46	164514	97.150	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.150%		
24) Chloroform-d	4.339	84	225913	43.247	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.500%		
26) 1,2-Dichloroethane-d4	5.024	65	134475	45.073	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.140%		
32) Benzene-d6	5.043	84	489635	44.332	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.660%		
36) 1,2-Dichloropropane-d6	6.063	67	154081	45.672	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.340%		
41) Toluene-d8	7.307	98	434635	41.766	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.540%		
43) trans-1,3-Dichloroprop...	7.612	79	63766	37.431	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.860%		
47) 2-Hexanone-d5	8.082	63	134686	93.492	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	93.490%		
56) 1,1,2,2-Tetrachloroeth...	10.204	84	217182	45.050	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	90.100%		
66) 1,2-Dichlorobenzene-d4	11.612	152	180275	43.271	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.540%		
Target Compounds					Qvalue	
13) Acetone	2.162	43	3041	2.757	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029660.D
Acq On : 13 Dec 2022 18:46
Operator : SY/MD
Sample : N5980-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP4

Quant Time: Dec 13 22:54:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 13 22:49:59 2022
Response via : Initial Calibration

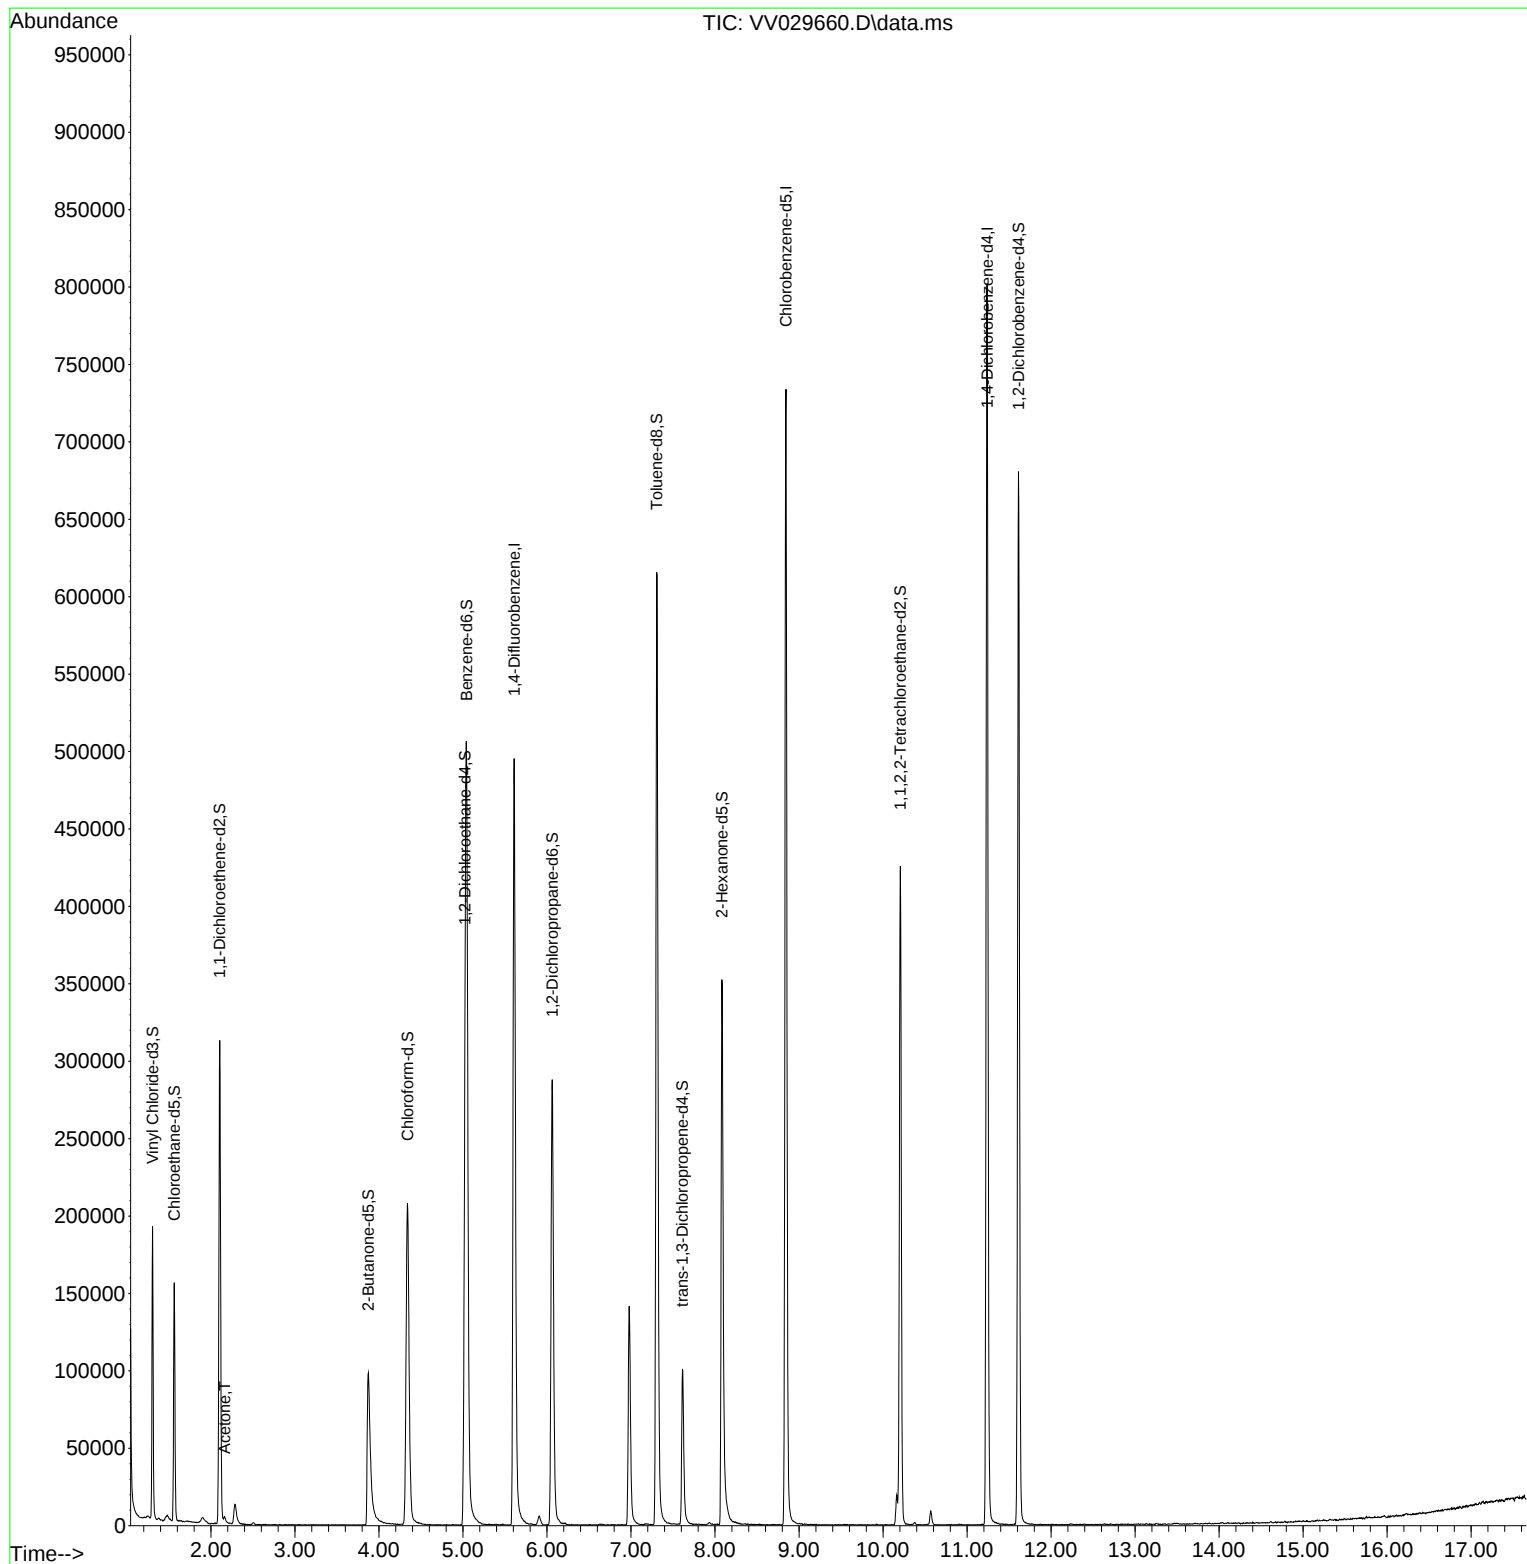

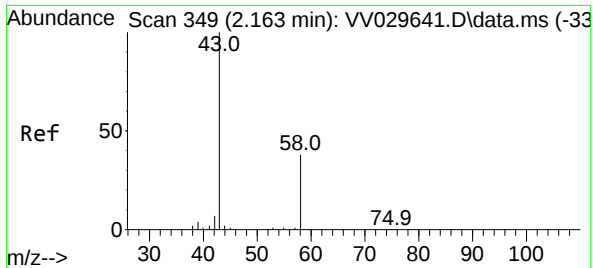

#13
 Acetone
 Concen: 2.757 ug/L
 RT: 2.162 min Scan# 34
 Delta R.T. -0.000 min
 Lab File: VV029660.D
 Acq: 13 Dec 2022 18:46

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP4

Tgt Ion:	43	Resp:	3041
Ion Ratio	Lower	Upper	
43	100		
58	35.5	0.0	74.8

