

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029675.D
 Acq On : 14 Dec 2022 01:02
 Operator : SY/MD
 Sample : N5980-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ8

Quant Time: Dec 14 01:34:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 13 23:56:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	470235	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.844	117	434643	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	226027	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	117653	40.859	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.720%
7) Chloroethane-d5	1.564	69	104082	47.402	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.800%
11) 1,1-Dichloroethene-d2	2.105	63	161728	36.009	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.020%
21) 2-Butanone-d5	3.873	46	178715	101.740	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.740%
24) Chloroform-d	4.339	84	237836	43.892	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.780%
26) 1,2-Dichloroethane-d4	5.024	65	144177	46.587	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.180%
32) Benzene-d6	5.043	84	505193	43.988	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.980%
36) 1,2-Dichloropropane-d6	6.063	67	159017	45.329	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.660%
41) Toluene-d8	7.307	98	446018	41.217	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	82.440%
43) trans-1,3-Dichloroprop...	7.612	79	64399	36.354	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	72.700%
47) 2-Hexanone-d5	8.082	63	142702	95.260	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.260%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	226293	45.141	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.280%
66) 1,2-Dichlorobenzene-d4	11.612	152	188262	43.755	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.500%
Target Compounds						
13) Acetone	2.166	43	3228	2.821	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029675.D
Acq On : 14 Dec 2022 01:02
Operator : SY/MD
Sample : N5980-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ8

Quant Time: Dec 14 01:34:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 13 23:56:43 2022
Response via : Initial Calibration

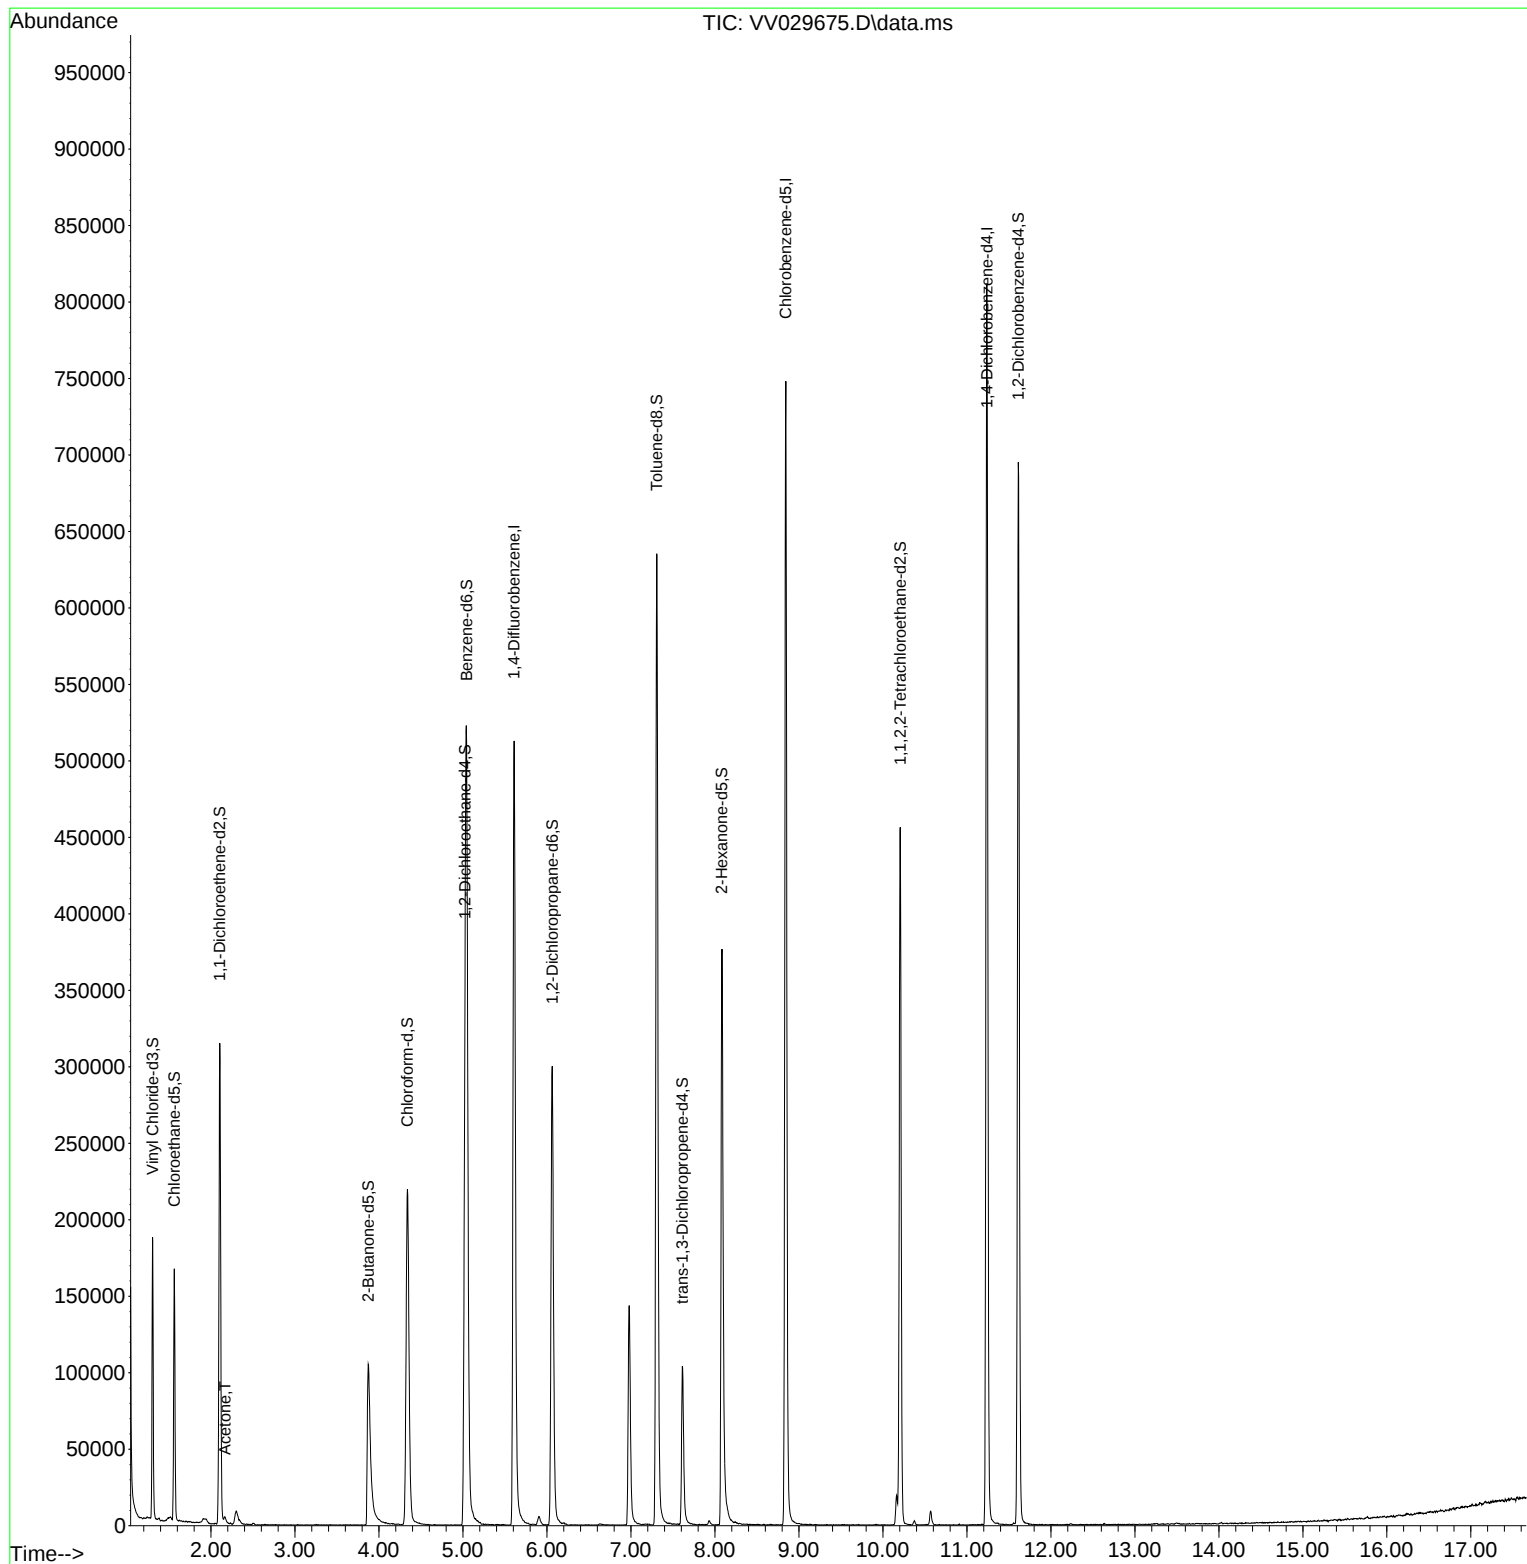

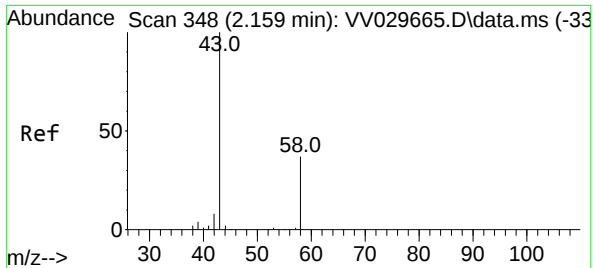

#13
 Acetone
 Concen: 2.821 ug/L
 RT: 2.166 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VV029675.D
 Acq: 14 Dec 2022 01:02

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ8

Tgt Ion: 43 Resp: 3228
 Ion Ratio Lower Upper
 43 100
 58 35.7 0.0 74.8

