

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029643.D
 Acq On : 13 Dec 2022 12:05
 Operator : SY/MD
 Sample : N5915-01DL2 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N00DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	235347	236847	15.66%	1.834%
2	1.564	156	163	179	rVB	193987	212668	14.06%	1.647%
3	2.111	320	333	367	rBV3	646385	1107390	73.20%	8.575%
4	2.503	445	455	470	rVB2	15706	26121	1.73%	0.202%
5	2.616	487	490	495	rVB3	226	162	0.01%	0.001%
6	2.716	513	521	526	rBV2	329	470	0.03%	0.004%
7	2.799	544	547	551	rBV2	247	153	0.01%	0.001%
8	2.841	558	560	562	rBV	230	71	0.00%	0.001%
9	2.857	562	565	567	rBV2	233	133	0.01%	0.001%
10	2.944	589	592	594	rBV	107	61	0.00%	0.000%
11	2.957	594	596	601	rBV	225	176	0.01%	0.001%
12	3.015	612	614	615	rBV	154	66	0.00%	0.001%
13	3.426	738	742	749	rBV2	178	192	0.01%	0.001%
14	3.609	796	799	801	rBV2	145	97	0.01%	0.001%
15	3.770	843	849	852	rBV	197	189	0.01%	0.001%
16	3.828	865	867	868	rBV	244	59	0.00%	0.000%
17	3.841	868	871	872	rBV	172	91	0.01%	0.001%
18	3.876	872	882	921	rBV	100663	297189	19.65%	2.301%
19	4.336	1007	1025	1061	rBV	230524	578549	38.24%	4.480%
20	4.664	1123	1127	1131	rBV3	462	507	0.03%	0.004%
21	4.706	1139	1140	1141	rBV3	119	30	0.00%	0.000%
22	4.735	1147	1149	1151	rBV	125	29	0.00%	0.000%
23	4.841	1178	1182	1184	rBV	119	92	0.01%	0.001%
24	4.879	1192	1194	1197	rBV	137	86	0.01%	0.001%
25	4.924	1205	1208	1211	rBV2	169	109	0.01%	0.001%
26	5.040	1225	1244	1282	rBV2	575676	1512761	100.00%	11.715%
27	5.519	1391	1393	1394	rBV	96	41	0.00%	0.000%
28	5.606	1408	1420	1466	rBV	541360	1100803	72.77%	8.524%
29	6.059	1545	1561	1595	rBV	324376	668902	44.22%	5.180%
30	6.268	1624	1626	1628	rBV	247	146	0.01%	0.001%
31	6.320	1636	1642	1645	rBV	236	271	0.02%	0.002%
32	6.368	1651	1657	1659	rVB	221	171	0.01%	0.001%
33	6.384	1659	1662	1664	rBV2	208	134	0.01%	0.001%
34	6.413	1670	1671	1674	rBV2	190	100	0.01%	0.001%
35	6.477	1690	1691	1692	rBV2	138	41	0.00%	0.000%
36	6.487	1693	1694	1695	rVV2	143	39	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029643.D
 Acq On : 13 Dec 2022 12:05
 Operator : SY/MD
 Sample : N5915-01DL2 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N00DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.513	1699	1702	1706	rBV2	248	178	0.01%	0.001%
38	6.545	1710	1712	1714	rVB	223	93	0.01%	0.001%
39	6.593	1722	1727	1729	rBV2	218	169	0.01%	0.001%
40	6.622	1729	1736	1743	rBV5	808	1212	0.08%	0.009%
41	6.693	1755	1758	1762	rVB3	397	274	0.02%	0.002%
42	6.719	1762	1766	1769	rBV4	354	272	0.02%	0.002%
43	6.751	1774	1776	1779	rBV	104	55	0.00%	0.000%
44	6.789	1785	1788	1789	rBV	91	54	0.00%	0.000%
45	6.844	1803	1805	1811	rVB2	463	266	0.02%	0.002%
46	6.892	1818	1820	1822	rBV2	100	54	0.00%	0.000%
47	6.921	1825	1829	1831	rBV2	209	151	0.01%	0.001%
48	6.976	1835	1846	1878	rVV	159621	299993	19.83%	2.323%
49	7.227	1921	1924	1929	rVB3	348	307	0.02%	0.002%
50	7.262	1932	1935	1936	rBV	536	339	0.02%	0.003%
51	7.307	1937	1949	1981	rBV	720023	1269264	83.90%	9.829%
52	7.612	2033	2044	2079	rBV	115223	205840	13.61%	1.594%
53	7.918	2137	2139	2142	rBV2	404	290	0.02%	0.002%
54	8.082	2180	2190	2222	rBV	368617	672389	44.45%	5.207%
55	8.529	2322	2329	2332	rBV3	448	470	0.03%	0.004%
56	8.571	2338	2342	2345	rBV3	389	404	0.03%	0.003%
57	8.638	2359	2363	2364	rBV	265	158	0.01%	0.001%
58	8.674	2372	2374	2375	rBV	281	76	0.01%	0.001%
59	8.696	2379	2381	2384	rVB	280	78	0.01%	0.001%
60	8.709	2384	2385	2386	rBV	109	41	0.00%	0.000%
61	8.844	2414	2427	2460	rBV	794804	1310572	86.63%	10.149%
62	9.072	2496	2498	2501	rBV	280	183	0.01%	0.001%
63	9.140	2516	2519	2523	rVB2	502	335	0.02%	0.003%
64	9.204	2537	2539	2543	rVB	415	237	0.02%	0.002%
65	9.281	2560	2563	2564	rBV	190	104	0.01%	0.001%
66	9.423	2602	2607	2609	rBV2	256	232	0.02%	0.002%
67	9.474	2622	2623	2624	rBV2	137	40	0.00%	0.000%
68	9.493	2628	2629	2632	rVB	297	69	0.00%	0.001%
69	9.513	2632	2635	2638	rBV2	136	125	0.01%	0.001%
70	9.529	2638	2640	2641	rBV2	184	58	0.00%	0.000%
71	9.567	2647	2652	2661	rVB4	507	636	0.04%	0.005%
72	9.879	2746	2749	2753	rVB	119	101	0.01%	0.001%
73	9.918	2757	2761	2770	rVV4	530	679	0.04%	0.005%
74	9.956	2770	2773	2779	rVB3	258	263	0.02%	0.002%
75	10.162	2827	2837	2841	rBV2	22164	32381	2.14%	0.251%
76	10.204	2842	2850	2871	rVB	458292	724262	47.88%	5.609%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029643.D
 Acq On : 13 Dec 2022 12:05
 Operator : SY/MD
 Sample : N5915-01DL2 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5N00DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.345	2892	2894	2895	rVB	223	63	0.00%	0.000%
78	10.365	2895	2900	2901	rBV2	247	201	0.01%	0.002%
79	10.522	2945	2949	2950	rBV	362	235	0.02%	0.002%
80	10.567	2955	2963	2974	rVB	9982	15754	1.04%	0.122%
81	10.654	2988	2990	2993	rVB	251	100	0.01%	0.001%
82	10.773	3022	3027	3029	rBV2	410	359	0.02%	0.003%
83	10.812	3037	3039	3044	rVB2	414	264	0.02%	0.002%
84	10.844	3044	3049	3050	rBV2	291	220	0.01%	0.002%
85	10.905	3062	3068	3070	rBV3	604	593	0.04%	0.005%
86	10.998	3095	3097	3100	rVB	212	99	0.01%	0.001%
87	11.046	3109	3112	3119	rVB3	358	353	0.02%	0.003%
88	11.088	3124	3125	3128	rVB	210	72	0.00%	0.001%
89	11.127	3135	3137	3144	rBV4	241	257	0.02%	0.002%
90	11.181	3147	3154	3156	rBV3	614	763	0.05%	0.006%
91	11.236	3160	3171	3201	rBV	913485	1409627	93.18%	10.916%
92	11.439	3230	3234	3238	rBV3	535	487	0.03%	0.004%
93	11.513	3254	3257	3261	rVB	354	178	0.01%	0.001%
94	11.535	3262	3264	3265	rBV	268	68	0.00%	0.001%
95	11.612	3275	3288	3310	rBV	770297	1212014	80.12%	9.386%
96	11.857	3361	3364	3365	rBV2	288	142	0.01%	0.001%
97	12.194	3465	3469	3475	rBV3	296	440	0.03%	0.003%
98	12.632	3601	3605	3607	rBV3	971	842	0.06%	0.007%
99	12.998	3717	3719	3720	rBV3	285	110	0.01%	0.001%
100	13.252	3791	3798	3808	rBV5	1417	2583	0.17%	0.020%




Sum of corrected areas: 12913474

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029643.D
Acq On : 13 Dec 2022 12:05
Operator : SY/MD
Sample : N5915-01DL2 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N00DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

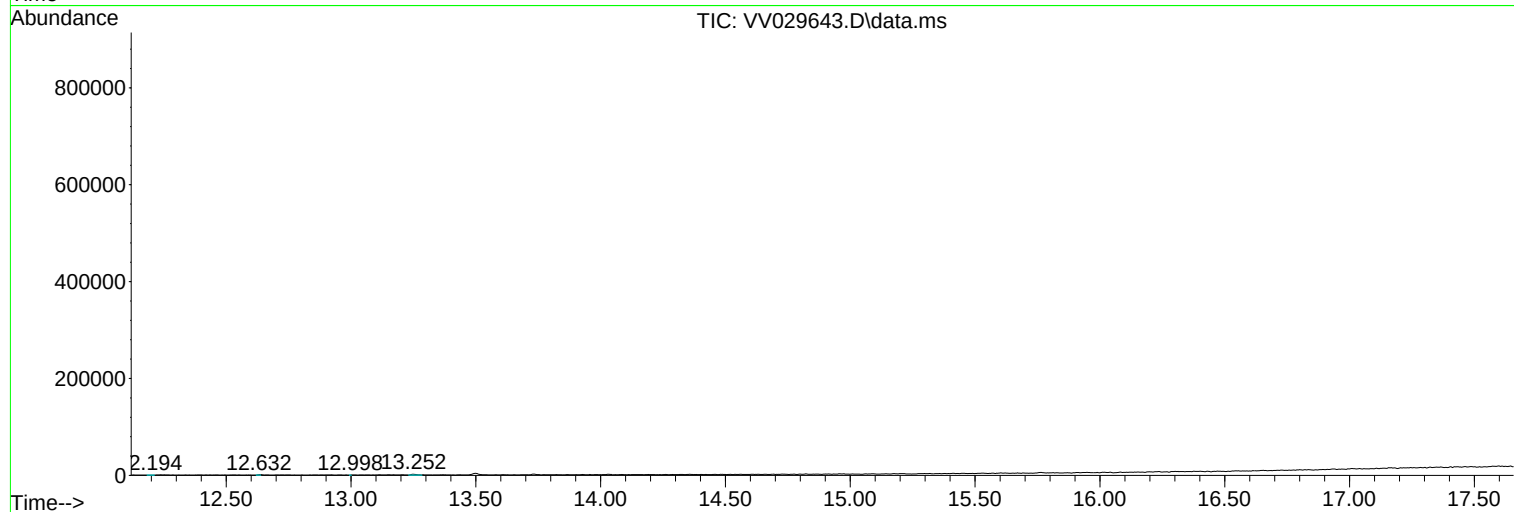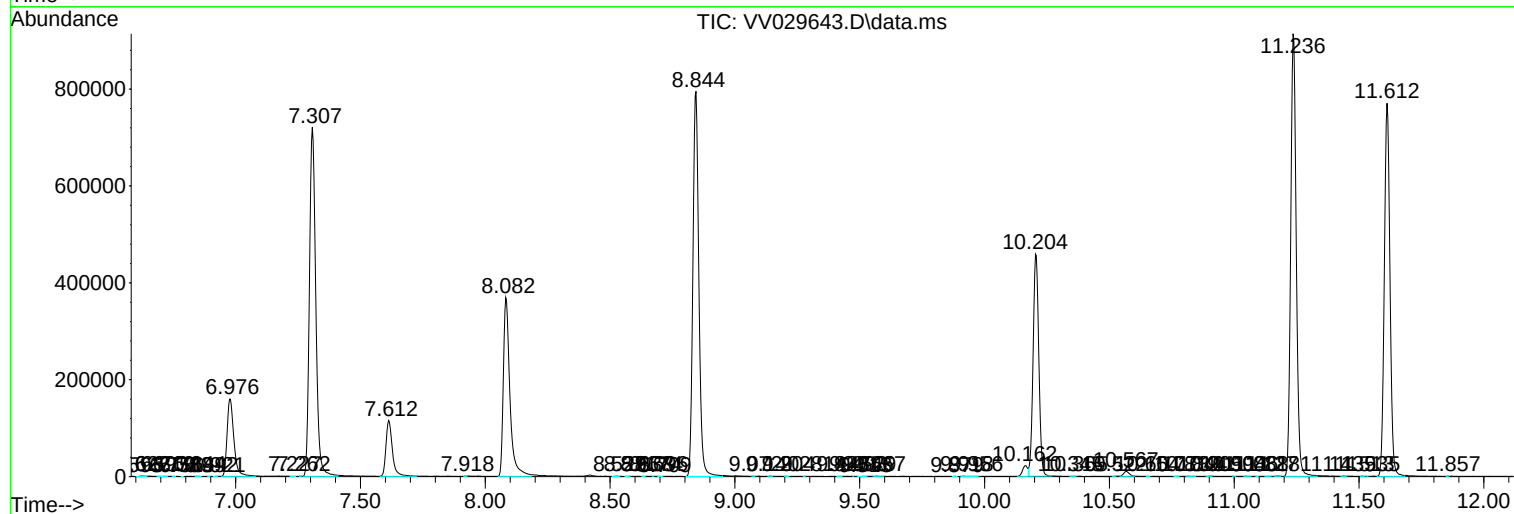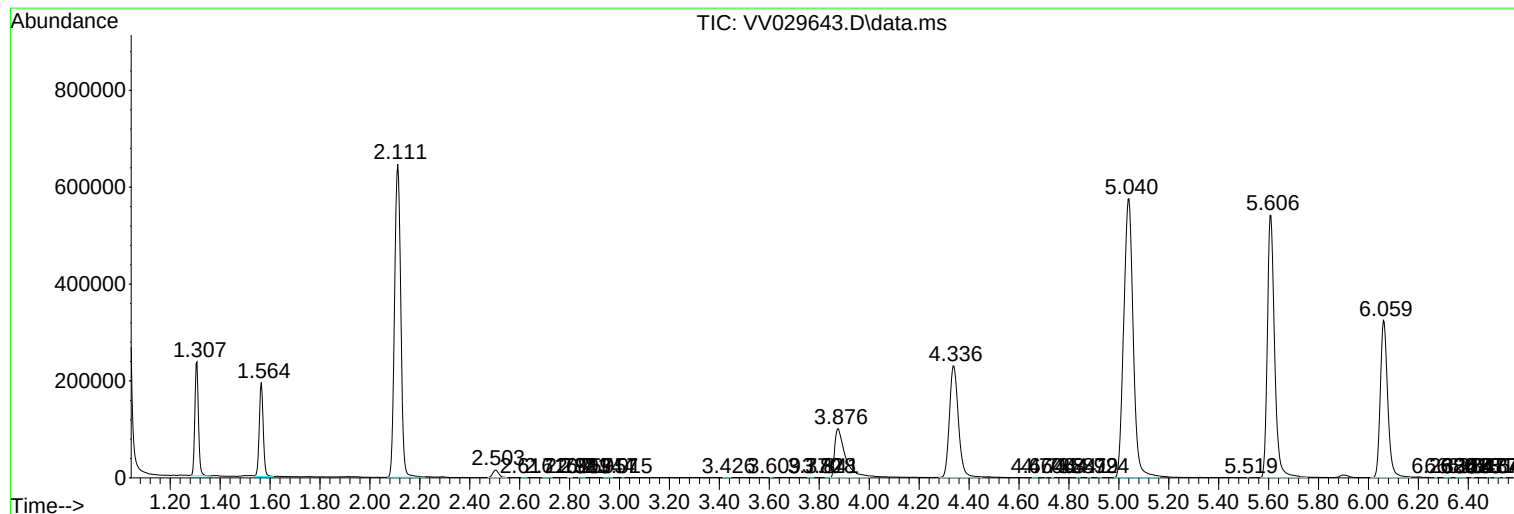

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029643.D
Acq On : 13 Dec 2022 12:05
Operator : SY/MD
Sample : N5915-01DL2 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N00DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029643.D
Acq On : 13 Dec 2022 12:05
Operator : SY/MD
Sample : N5915-01DL2 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5N00DL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------