

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029644.D
 Acq On : 13 Dec 2022 12:29
 Operator : SY/MD
 Sample : N5915-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	210628	215047	14.33%	1.761%
2	1.564	156	163	176	rVB	180086	202101	13.46%	1.655%
3	2.066	316	319	321	rBV2	940	624	0.04%	0.005%
4	2.105	321	331	348	rVV	349471	503779	33.56%	4.126%
5	2.285	385	387	389	rBV2	853	351	0.02%	0.003%
6	2.503	446	455	471	rVB	9039	15093	1.01%	0.124%
7	2.693	512	514	517	rVV	165	88	0.01%	0.001%
8	2.793	541	545	548	rVV2	314	206	0.01%	0.002%
9	2.940	588	591	593	rBV2	241	134	0.01%	0.001%
10	3.085	633	636	640	rBV2	161	139	0.01%	0.001%
11	3.127	647	649	654	rVB2	210	132	0.01%	0.001%
12	3.185	664	667	670	rBV	137	105	0.01%	0.001%
13	3.272	692	694	702	rVB2	280	184	0.01%	0.002%
14	3.313	702	707	708	rBV2	149	121	0.01%	0.001%
15	3.387	727	730	732	rBV	186	91	0.01%	0.001%
16	3.420	737	740	741	rBV	151	82	0.01%	0.001%
17	3.452	746	750	751	rBV	229	136	0.01%	0.001%
18	3.551	778	781	783	rBV2	129	87	0.01%	0.001%
19	3.677	815	820	824	rBV2	126	121	0.01%	0.001%
20	3.709	828	830	832	rVV	244	102	0.01%	0.001%
21	3.725	832	835	839	rVB2	211	150	0.01%	0.001%
22	3.828	864	867	870	rBV	114	77	0.01%	0.001%
23	3.876	872	882	919	rBV	104863	305492	20.35%	2.502%
24	4.339	1009	1026	1057	rBV	230237	574346	38.26%	4.704%
25	4.699	1136	1138	1141	rBV2	215	150	0.01%	0.001%
26	4.751	1152	1154	1158	rBV	209	121	0.01%	0.001%
27	4.786	1161	1165	1168	rBV2	275	168	0.01%	0.001%
28	4.809	1168	1172	1173	rBV	183	124	0.01%	0.001%
29	4.821	1173	1176	1182	rVB3	345	330	0.02%	0.003%
30	4.854	1182	1186	1194	rBV2	193	256	0.02%	0.002%
31	4.886	1194	1196	1200	rVB2	234	118	0.01%	0.001%
32	4.921	1201	1207	1208	rBV	268	192	0.01%	0.002%
33	4.973	1219	1223	1225	rBV	283	252	0.02%	0.002%
34	5.040	1226	1244	1284	rBV2	573223	1500983	100.00%	12.294%
35	5.278	1315	1318	1321	rBV3	346	319	0.02%	0.003%
36	5.410	1356	1359	1364	rBV2	209	202	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029644.D
 Acq On : 13 Dec 2022 12:29
 Operator : SY/MD
 Sample : N5915-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.538	1397	1399	1402	rVB2	209	107	0.01%	0.001%
38	5.609	1405	1421	1471	rBV	528277	1087962	72.48%	8.911%
39	5.902	1502	1512	1526	rVB6	5435	11021	0.73%	0.090%
40	6.063	1548	1562	1595	rBV	325402	668228	44.52%	5.473%
41	6.284	1629	1631	1632	rBV	164	79	0.01%	0.001%
42	6.320	1637	1642	1646	rBV3	327	421	0.03%	0.003%
43	6.436	1670	1678	1682	rBV2	209	240	0.02%	0.002%
44	6.497	1694	1697	1701	rBV2	149	117	0.01%	0.001%
45	6.548	1710	1713	1717	rVB2	302	178	0.01%	0.001%
46	6.616	1729	1734	1735	rBV	469	317	0.02%	0.003%
47	6.696	1756	1759	1764	rBV2	256	254	0.02%	0.002%
48	6.715	1764	1765	1768	rVB2	245	81	0.01%	0.001%
49	6.735	1768	1771	1775	rBV2	184	158	0.01%	0.001%
50	6.841	1798	1804	1807	rBV2	311	291	0.02%	0.002%
51	6.879	1812	1816	1817	rBV	207	120	0.01%	0.001%
52	6.979	1835	1847	1876	rBV	161128	300435	20.02%	2.461%
53	7.146	1897	1899	1901	rBV	271	133	0.01%	0.001%
54	7.259	1932	1934	1936	rBV	361	192	0.01%	0.002%
55	7.307	1936	1949	1987	rBV	699778	1249822	83.27%	10.237%
56	7.612	2035	2044	2068	rBV	112352	199659	13.30%	1.635%
57	7.844	2114	2116	2119	rVB2	319	130	0.01%	0.001%
58	8.085	2180	2191	2233	rBV	389309	718168	47.85%	5.882%
59	8.487	2314	2316	2317	rBV	326	118	0.01%	0.001%
60	8.513	2322	2324	2326	rBV	221	128	0.01%	0.001%
61	8.603	2350	2352	2353	rBV	172	86	0.01%	0.001%
62	8.625	2357	2359	2362	rVV	357	236	0.02%	0.002%
63	8.667	2371	2372	2376	rVB3	308	170	0.01%	0.001%
64	8.747	2393	2397	2398	rBV2	364	201	0.01%	0.002%
65	8.799	2410	2413	2415	rBV2	218	126	0.01%	0.001%
66	8.844	2415	2427	2454	rBV	778600	1282479	85.44%	10.504%
67	9.107	2507	2509	2511	rVB2	363	103	0.01%	0.001%
68	9.172	2527	2529	2532	rBV2	160	111	0.01%	0.001%
69	9.252	2551	2554	2555	rBV2	269	156	0.01%	0.001%
70	9.368	2588	2590	2592	rBV	141	76	0.01%	0.001%
71	9.529	2635	2640	2644	rBV	7591	6077	0.40%	0.050%
72	9.548	2644	2646	2650	rVB	2525	1473	0.10%	0.012%
73	9.731	2701	2703	2706	rBV2	135	86	0.01%	0.001%
74	9.750	2706	2709	2711	rBV2	124	86	0.01%	0.001%
75	9.796	2719	2723	2726	rVB3	283	195	0.01%	0.002%
76	9.918	2757	2761	2769	rBV3	455	607	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029644.D
 Acq On : 13 Dec 2022 12:29
 Operator : SY/MD
 Sample : N5915-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.011	2786	2790	2794	rBV2	207	206	0.01%	0.002%
78	10.043	2798	2800	2803	rVB	320	121	0.01%	0.001%
79	10.104	2817	2819	2822	rVB3	192	110	0.01%	0.001%
80	10.162	2826	2837	2841	rBV	21322	31123	2.07%	0.255%
81	10.204	2842	2850	2872	rVB	481364	748833	49.89%	6.133%
82	10.529	2948	2951	2955	rVV3	488	450	0.03%	0.004%
83	10.567	2955	2963	2977	rVB2	9539	15718	1.05%	0.129%
84	10.654	2987	2990	2992	rBV2	135	84	0.01%	0.001%
85	10.725	3008	3012	3013	rBV2	155	112	0.01%	0.001%
86	10.840	3045	3048	3049	rBV2	242	135	0.01%	0.001%
87	10.873	3056	3058	3060	rBV2	215	79	0.01%	0.001%
88	10.902	3064	3067	3074	rVB4	552	630	0.04%	0.005%
89	11.175	3146	3152	3158	rBV3	846	1189	0.08%	0.010%
90	11.236	3158	3171	3193	rBV	878832	1367353	91.10%	11.199%
91	11.612	3274	3288	3318	rBV	764635	1188375	79.17%	9.733%
92	11.966	3396	3398	3400	rBV	246	86	0.01%	0.001%
93	12.297	3499	3501	3503	rBV	225	125	0.01%	0.001%
94	12.413	3535	3537	3540	rBV2	486	265	0.02%	0.002%
95	12.545	3576	3578	3579	rBV	223	78	0.01%	0.001%
96	12.635	3601	3606	3608	rBV3	1048	829	0.06%	0.007%
97	12.667	3615	3616	3619	rBV2	278	111	0.01%	0.001%
98	12.828	3664	3666	3668	rBV2	333	204	0.01%	0.002%
99	13.049	3732	3735	3736	rBV2	306	165	0.01%	0.001%
100	13.165	3769	3771	3774	rVB2	384	124	0.01%	0.001%


Sum of corrected areas: 12209135

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029644.D
Acq On : 13 Dec 2022 12:29
Operator : SY/MD
Sample : N5915-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

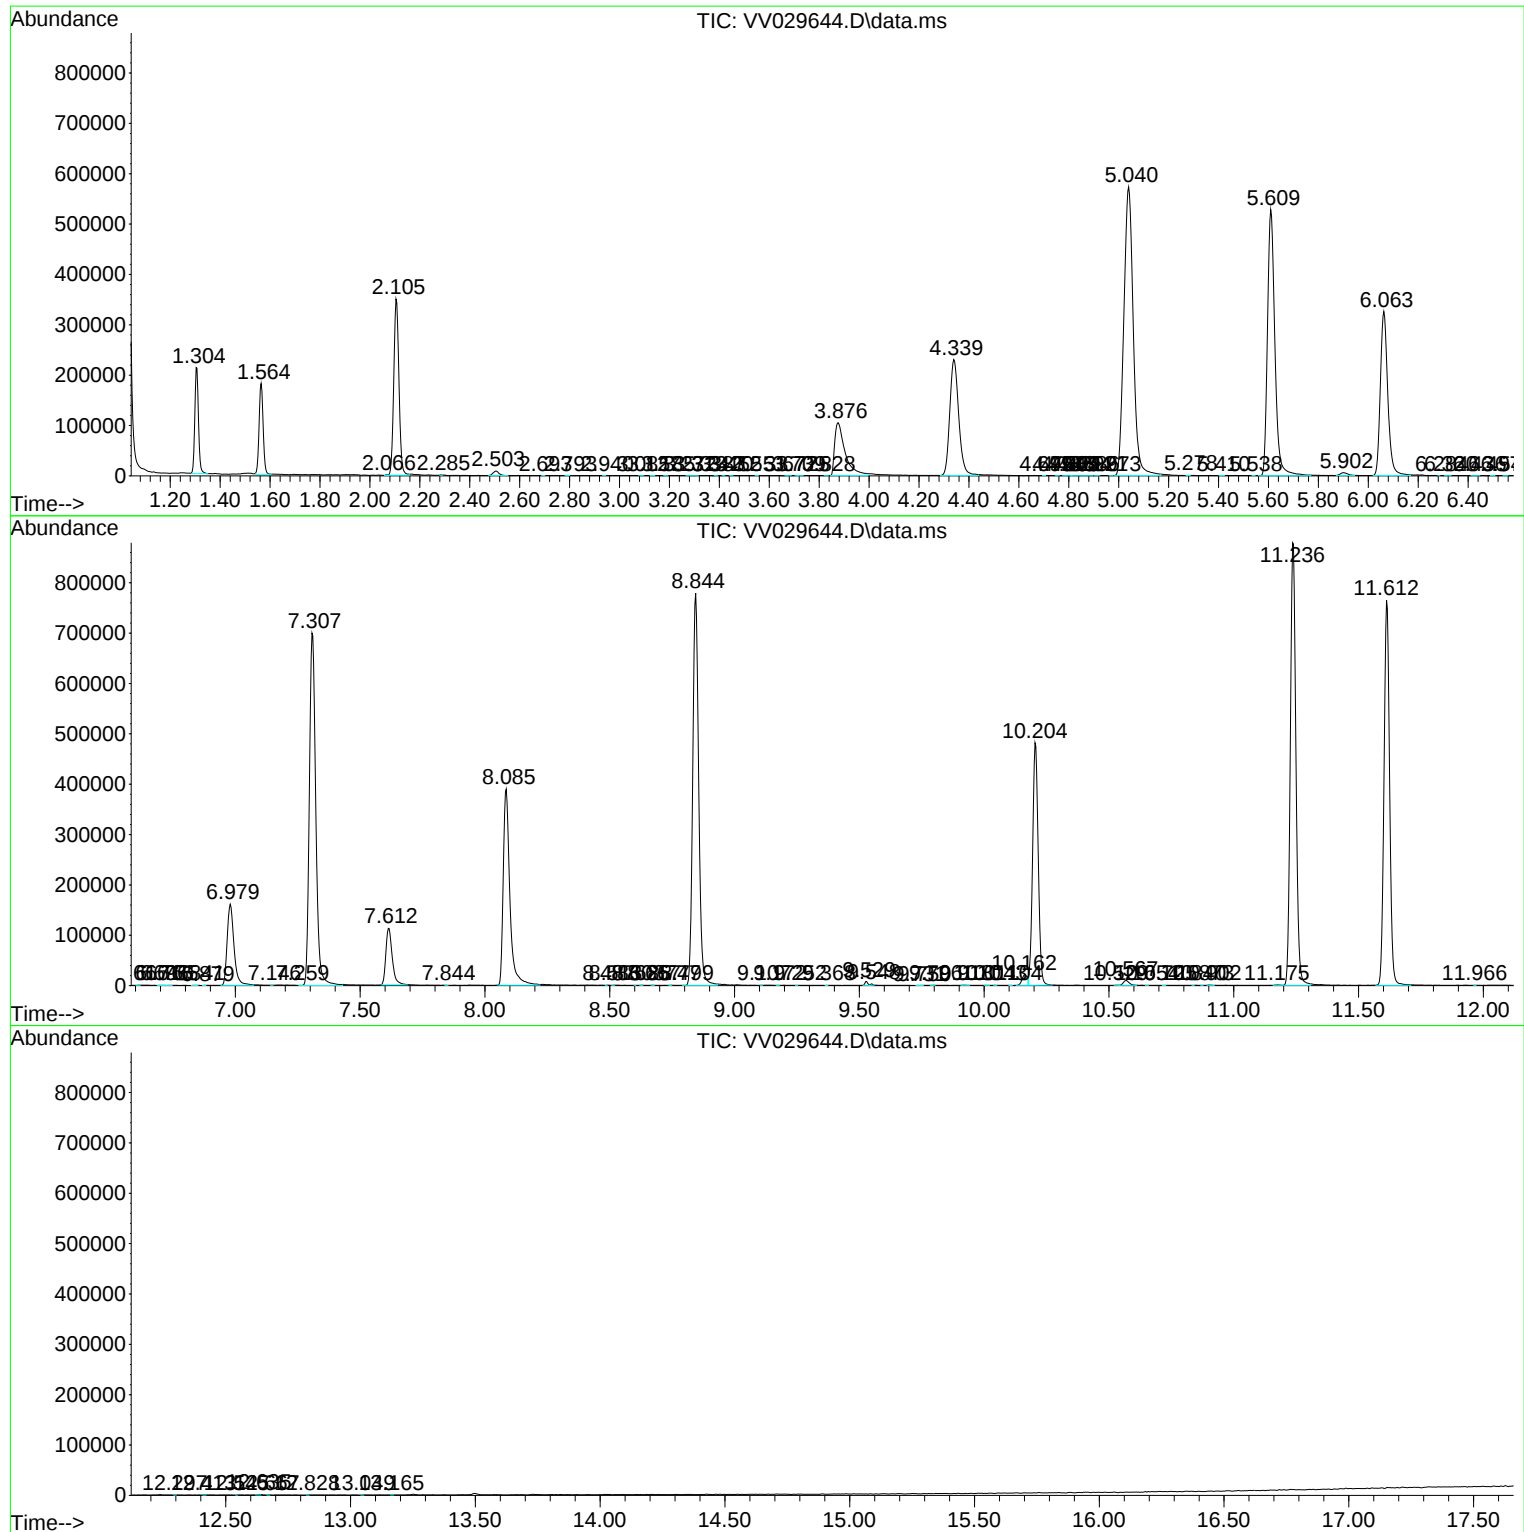

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029644.D
Acq On : 13 Dec 2022 12:29
Operator : SY/MD
Sample : N5915-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029644.D
Acq On : 13 Dec 2022 12:29
Operator : SY/MD
Sample : N5915-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc