

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029645.D
 Acq On : 13 Dec 2022 12:52
 Operator : SY/MD
 Sample : N5928-06DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ69DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029645.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	98	rVB2	253208	262235	18.23%	2.031%
2	1.561	155	162	176	rVB	176995	204227	14.20%	1.581%
3	2.104	321	331	347	rBV	349493	503839	35.03%	3.902%
4	2.506	448	456	464	rVB5	3144	4953	0.34%	0.038%
5	2.571	474	476	480	rBV3	329	193	0.01%	0.001%
6	2.760	528	535	544	rBV3	2236	3529	0.25%	0.027%
7	2.944	589	592	593	rBV	247	128	0.01%	0.001%
8	3.031	617	619	621	rBV	181	94	0.01%	0.001%
9	3.185	652	667	694	rBV	75500	161182	11.21%	1.248%
10	3.423	739	741	743	rBV	167	57	0.00%	0.000%
11	3.455	748	751	754	rBV	172	124	0.01%	0.001%
12	3.664	810	816	819	rBV	178	230	0.02%	0.002%
13	3.728	832	836	840	rBV2	134	136	0.01%	0.001%
14	3.899	871	889	935	rBV3	285707	929669	64.64%	7.199%
15	4.339	1009	1026	1059	rBV	225358	554242	38.53%	4.292%
16	4.600	1092	1107	1133	rVB2	70237	178556	12.41%	1.383%
17	4.799	1168	1169	1174	rVB2	141	68	0.00%	0.001%
18	4.825	1174	1177	1179	rBV2	123	70	0.00%	0.001%
19	4.870	1188	1191	1194	rBV2	233	101	0.01%	0.001%
20	4.892	1194	1198	1201	rVB	242	171	0.01%	0.001%
21	4.911	1201	1204	1207	rBV2	104	68	0.00%	0.001%
22	4.934	1208	1211	1214	rVB2	136	79	0.01%	0.001%
23	4.956	1214	1218	1220	rBV2	248	143	0.01%	0.001%
24	5.040	1226	1244	1282	rBV2	545933	1438284	100.00%	11.138%
25	5.452	1368	1372	1374	rBV3	153	145	0.01%	0.001%
26	5.542	1394	1400	1401	rBV2	220	143	0.01%	0.001%
27	5.609	1408	1421	1463	rBV	541046	1100553	76.52%	8.522%
28	5.908	1502	1514	1532	rVB8	8820	20334	1.41%	0.157%
29	6.063	1548	1562	1597	rBV	307948	633822	44.07%	4.908%
30	6.281	1628	1630	1635	rVB2	257	146	0.01%	0.001%
31	6.317	1636	1641	1643	rVV3	325	228	0.02%	0.002%
32	6.329	1643	1645	1648	rVV	182	67	0.00%	0.001%
33	6.349	1648	1651	1653	rVB2	178	81	0.01%	0.001%
34	6.413	1669	1671	1673	rBV	122	63	0.00%	0.000%
35	6.464	1684	1687	1689	rBV2	115	79	0.01%	0.001%
36	6.477	1689	1691	1694	rVV2	198	112	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029645.D
 Acq On : 13 Dec 2022 12:52
 Operator : SY/MD
 Sample : N5928-06DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ69DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.506	1698	1700	1704	rVB2	264	123	0.01%	0.001%
38	6.545	1709	1712	1716	rVB2	249	132	0.01%	0.001%
39	6.583	1720	1724	1728	rBV2	315	253	0.02%	0.002%
40	6.616	1732	1734	1735	rBV	472	199	0.01%	0.002%
41	6.860	1808	1810	1812	rBV	156	50	0.00%	0.000%
42	6.979	1835	1847	1872	rBV	156337	284716	19.80%	2.205%
43	7.307	1937	1949	1985	rBV	681616	1207625	83.96%	9.352%
44	7.616	2033	2045	2069	rBV	108734	193842	13.48%	1.501%
45	7.969	2146	2155	2170	rVB3	18688	33002	2.29%	0.256%
46	8.024	2170	2172	2175	rBV	218	99	0.01%	0.001%
47	8.082	2180	2190	2229	rBV	360552	655866	45.60%	5.079%
48	8.416	2291	2294	2297	rBV2	280	241	0.02%	0.002%
49	8.484	2313	2315	2316	rBV	332	124	0.01%	0.001%
50	8.574	2342	2343	2344	rBV	210	50	0.00%	0.000%
51	8.606	2350	2353	2356	rVB2	528	325	0.02%	0.003%
52	8.702	2381	2383	2385	rVB	145	57	0.00%	0.000%
53	8.715	2385	2387	2389	rVB	207	75	0.01%	0.001%
54	8.741	2391	2395	2397	rBV2	342	200	0.01%	0.002%
55	8.757	2397	2400	2402	rBV2	165	109	0.01%	0.001%
56	8.844	2414	2427	2463	rBV	791313	1295655	90.08%	10.033%
57	9.133	2511	2517	2520	rBV6	675	700	0.05%	0.005%
58	9.214	2540	2542	2546	rVB	231	101	0.01%	0.001%
59	9.278	2559	2562	2565	rBV2	268	164	0.01%	0.001%
60	9.313	2570	2573	2576	rBV2	118	101	0.01%	0.001%
61	9.345	2581	2583	2584	rBV2	173	78	0.01%	0.001%
62	9.352	2584	2585	2589	rVB2	338	175	0.01%	0.001%
63	9.374	2589	2592	2596	rBV2	169	139	0.01%	0.001%
64	9.410	2600	2603	2607	rBV2	209	151	0.01%	0.001%
65	9.445	2612	2614	2617	rBV2	112	78	0.01%	0.001%
66	9.522	2636	2638	2640	rBV	205	117	0.01%	0.001%
67	9.628	2668	2671	2673	rBV	243	103	0.01%	0.001%
68	9.670	2681	2684	2685	rBV2	108	65	0.00%	0.001%
69	9.683	2685	2688	2690	rVV2	326	164	0.01%	0.001%
70	9.725	2697	2701	2703	rBV	221	159	0.01%	0.001%
71	9.808	2723	2727	2732	rBV3	332	294	0.02%	0.002%
72	9.918	2756	2761	2771	rVB3	461	751	0.05%	0.006%
73	9.969	2773	2777	2780	rBV	185	135	0.01%	0.001%
74	10.011	2786	2790	2792	rBV	187	171	0.01%	0.001%
75	10.059	2802	2805	2808	rBV2	175	139	0.01%	0.001%
76	10.088	2811	2814	2817	rBV2	149	113	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029645.D
 Acq On : 13 Dec 2022 12:52
 Operator : SY/MD
 Sample : N5928-06DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ69DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.162	2827	2837	2841	rVV	20611	30214	2.10%	0.234%
78	10.207	2842	2851	2874	rVB	448218	697741	48.51%	5.403%
79	10.320	2884	2886	2887	rBV	164	74	0.01%	0.001%
80	10.410	2911	2914	2917	rBV2	237	156	0.01%	0.001%
81	10.496	2937	2941	2945	rBV2	244	199	0.01%	0.002%
82	10.525	2945	2950	2952	rVV3	845	717	0.05%	0.006%
83	10.567	2956	2963	2978	rVB	10247	16151	1.12%	0.125%
84	10.731	3006	3014	3018	rBV2	1050	1403	0.10%	0.011%
85	10.863	3053	3055	3059	rBV	175	112	0.01%	0.001%
86	10.911	3062	3070	3083	rBV6	1510	2386	0.17%	0.018%
87	10.963	3084	3086	3088	rBV	148	48	0.00%	0.000%
88	11.011	3098	3101	3103	rVB	231	126	0.01%	0.001%
89	11.024	3103	3105	3107	rBV2	211	85	0.01%	0.001%
90	11.040	3107	3110	3112	rVV2	325	194	0.01%	0.002%
91	11.236	3160	3171	3196	rBV	879364	1362405	94.72%	10.550%
92	11.493	3249	3251	3253	rBV2	297	147	0.01%	0.001%
93	11.612	3276	3288	3310	rBV	726604	1123350	78.10%	8.699%
94	11.828	3351	3355	3360	rBV3	412	406	0.03%	0.003%
95	11.914	3375	3382	3386	rBV6	1333	1927	0.13%	0.015%
96	12.046	3420	3423	3425	rBV3	363	237	0.02%	0.002%
97	12.670	3613	3617	3619	rBV2	330	259	0.02%	0.002%
98	12.914	3690	3693	3696	rBV2	350	205	0.01%	0.002%
99	12.988	3714	3716	3718	rBV	304	130	0.01%	0.001%
100	13.162	3768	3770	3773	rBV3	431	158	0.01%	0.001%




Sum of corrected areas: 12913622

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029645.D
Acq On : 13 Dec 2022 12:52
Operator : SY/MD
Sample : N5928-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

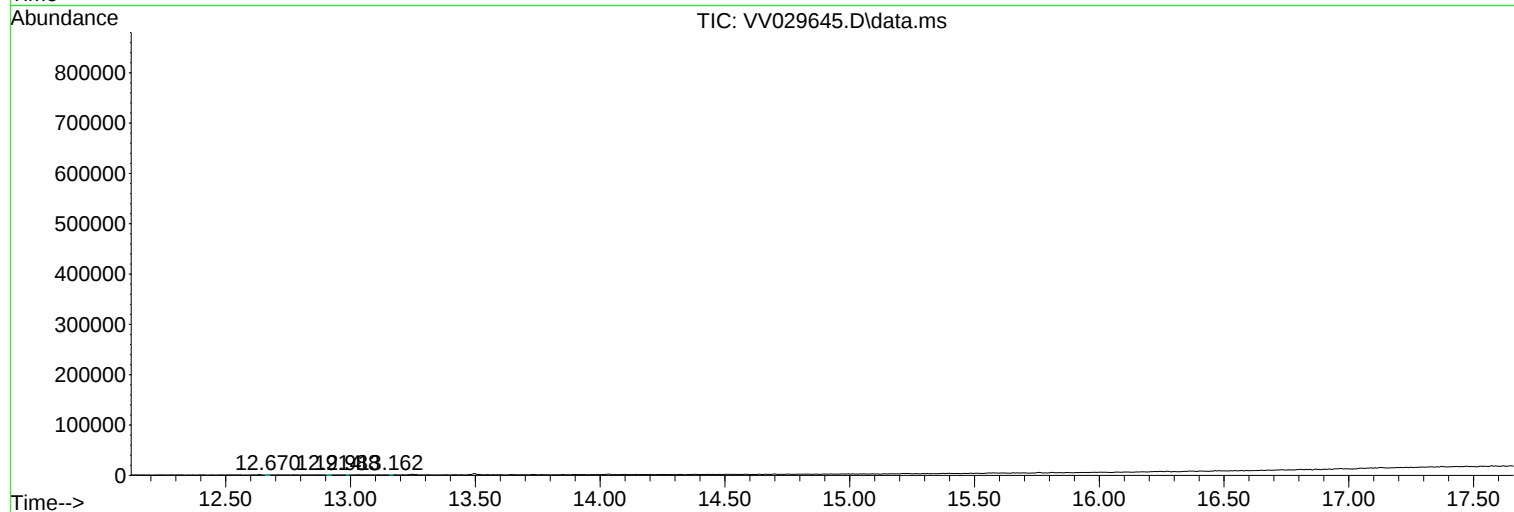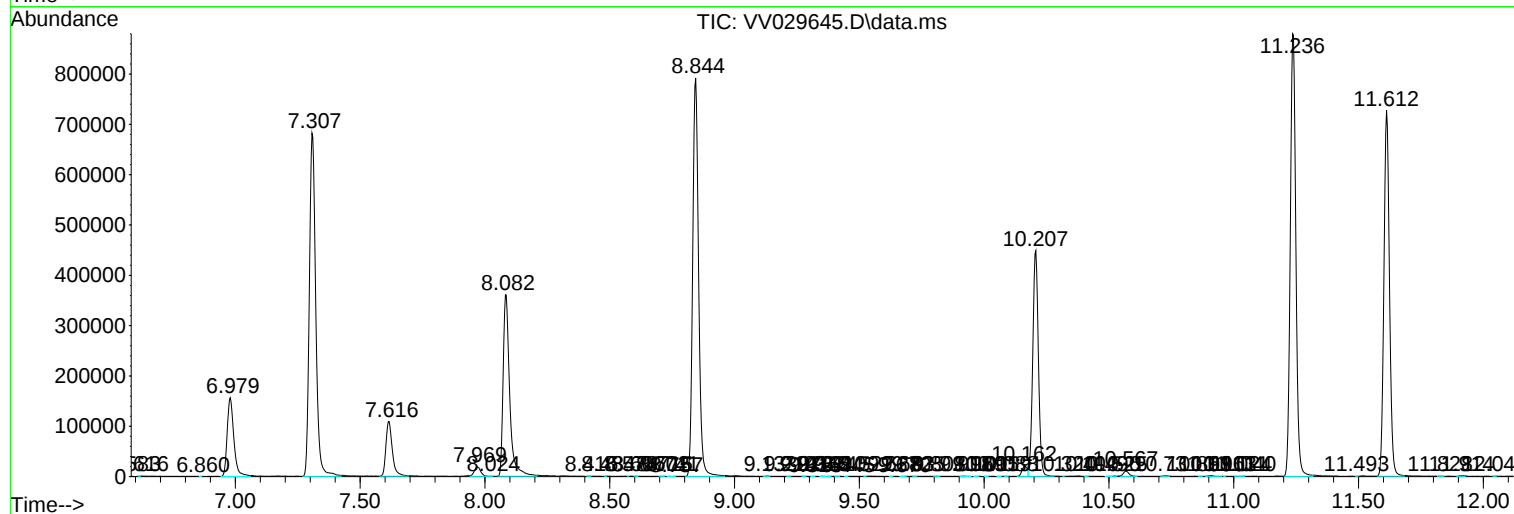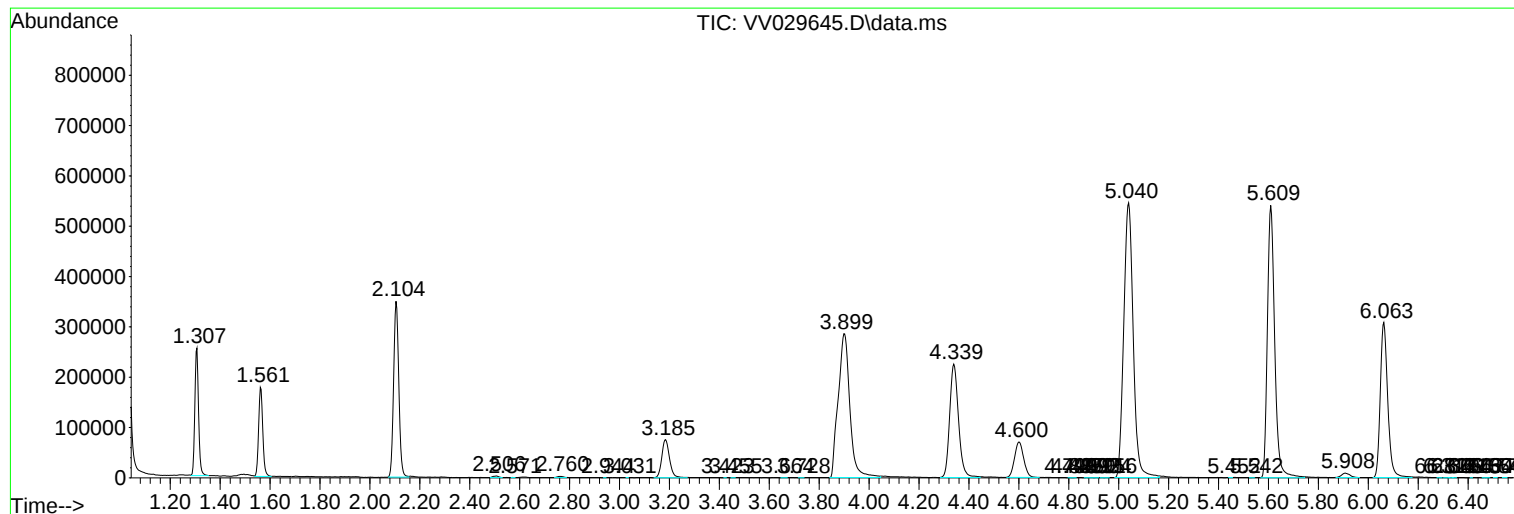

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029645.D
Acq On : 13 Dec 2022 12:52
Operator : SY/MD
Sample : N5928-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029645.D
Acq On : 13 Dec 2022 12:52
Operator : SY/MD
Sample : N5928-06DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ69DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc