

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029647.D
 Acq On : 13 Dec 2022 13:39
 Operator : SY/MD
 Sample : N5928-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	227846	228236	14.69%	1.697%
2	1.564	156	163	177	rVB	190206	211237	13.59%	1.571%
3	2.105	320	331	345	rBV2	377254	553311	35.60%	4.115%
4	2.461	438	442	445	rBV2	380	259	0.02%	0.002%
5	2.484	446	449	450	rBV2	303	176	0.01%	0.001%
6	2.568	471	475	477	rBV2	261	210	0.01%	0.002%
7	2.764	527	536	545	rBV4	3209	5512	0.35%	0.041%
8	2.883	571	573	577	rVB2	203	92	0.01%	0.001%
9	2.934	584	589	593	rBV3	299	383	0.02%	0.003%
10	3.021	613	616	618	rBV	191	117	0.01%	0.001%
11	3.117	643	646	651	rBV	292	248	0.02%	0.002%
12	3.185	651	667	687	rBV	81492	171297	11.02%	1.274%
13	3.362	720	722	726	rVB3	282	138	0.01%	0.001%
14	3.400	731	734	737	rBV2	257	186	0.01%	0.001%
15	3.587	787	792	799	rBV	259	352	0.02%	0.003%
16	3.648	807	811	816	rBV	176	179	0.01%	0.001%
17	3.728	832	836	839	rBV	125	84	0.01%	0.001%
18	3.744	839	841	843	rBV	160	93	0.01%	0.001%
19	3.764	843	847	850	rBV2	155	149	0.01%	0.001%
20	3.818	861	864	866	rBV	192	127	0.01%	0.001%
21	3.873	871	881	884	rBV	123227	197023	12.68%	1.465%
22	4.339	1009	1026	1062	rBV	236604	602342	38.76%	4.479%
23	4.600	1091	1107	1139	rVB	222476	557409	35.87%	4.145%
24	4.821	1172	1176	1180	rBV	363	249	0.02%	0.002%
25	4.844	1180	1183	1185	rBV2	140	85	0.01%	0.001%
26	4.908	1200	1203	1206	rBV	200	135	0.01%	0.001%
27	4.924	1206	1208	1211	rVV	140	85	0.01%	0.001%
28	4.947	1212	1215	1217	rVB	192	107	0.01%	0.001%
29	5.040	1225	1244	1285	rBV2	591855	1554105	100.00%	11.558%
30	5.474	1376	1379	1384	rBV4	472	554	0.04%	0.004%
31	5.555	1401	1404	1407	rBV	184	104	0.01%	0.001%
32	5.609	1407	1421	1460	rBV	549558	1119715	72.05%	8.327%
33	5.911	1502	1515	1532	rBV4	27630	60493	3.89%	0.450%
34	5.989	1537	1539	1543	rVB3	322	209	0.01%	0.002%
35	6.008	1543	1545	1547	rVB	279	114	0.01%	0.001%
36	6.063	1547	1562	1597	rBV	331499	684673	44.06%	5.092%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029647.D
 Acq On : 13 Dec 2022 13:39
 Operator : SY/MD
 Sample : N5928-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.239	1615	1617	1618	rBV	603	228	0.01%	0.002%
38	6.301	1632	1636	1639	rBV	284	230	0.01%	0.002%
39	6.439	1676	1679	1681	rBV2	249	117	0.01%	0.001%
40	6.481	1688	1692	1694	rBV2	232	202	0.01%	0.002%
41	6.500	1696	1698	1702	rVB	268	170	0.01%	0.001%
42	6.526	1702	1706	1708	rBV2	373	251	0.02%	0.002%
43	6.542	1708	1711	1713	rVV3	309	188	0.01%	0.001%
44	6.632	1730	1739	1748	rBV5	911	1798	0.12%	0.013%
45	6.706	1761	1762	1767	rVB3	369	229	0.01%	0.002%
46	6.735	1767	1771	1778	rVB3	321	405	0.03%	0.003%
47	6.773	1778	1783	1786	rBV3	216	213	0.01%	0.002%
48	6.899	1820	1822	1823	rBV3	221	93	0.01%	0.001%
49	6.979	1835	1847	1871	rBV	164582	305794	19.68%	2.274%
50	7.162	1900	1904	1905	rBV2	448	320	0.02%	0.002%
51	7.223	1920	1923	1927	rBV2	337	371	0.02%	0.003%
52	7.307	1936	1949	1980	rBV	735027	1292621	83.17%	9.613%
53	7.612	2034	2044	2072	rBV	116753	206412	13.28%	1.535%
54	7.969	2136	2155	2171	rVB3	80413	145391	9.36%	1.081%
55	8.082	2180	2190	2229	rBV	407433	734391	47.25%	5.462%
56	8.625	2357	2359	2361	rBV	286	109	0.01%	0.001%
57	8.677	2374	2375	2377	rBV	165	81	0.01%	0.001%
58	8.728	2388	2391	2393	rVB	194	117	0.01%	0.001%
59	8.773	2402	2405	2408	rVB2	169	78	0.01%	0.001%
60	8.792	2408	2411	2414	rVB	188	113	0.01%	0.001%
61	8.844	2414	2427	2458	rBV	793879	1322546	85.10%	9.835%
62	9.111	2508	2510	2513	rBV2	395	228	0.01%	0.002%
63	9.133	2513	2517	2521	rBV4	671	562	0.04%	0.004%
64	9.172	2526	2529	2535	rVB3	420	414	0.03%	0.003%
65	9.223	2541	2545	2548	rBV3	284	267	0.02%	0.002%
66	9.288	2560	2565	2568	rBV	185	212	0.01%	0.002%
67	9.313	2570	2573	2577	rBV2	194	182	0.01%	0.001%
68	9.506	2630	2633	2635	rBV2	225	123	0.01%	0.001%
69	9.532	2635	2641	2645	rBV4	426	388	0.02%	0.003%
70	9.574	2649	2654	2657	rVV3	391	382	0.02%	0.003%
71	9.860	2739	2743	2745	rBV2	275	198	0.01%	0.001%
72	9.902	2752	2756	2757	rBV	211	135	0.01%	0.001%
73	9.956	2770	2773	2777	rBV2	238	214	0.01%	0.002%
74	9.992	2781	2784	2786	rBV	236	114	0.01%	0.001%
75	10.027	2792	2795	2797	rBV	321	201	0.01%	0.001%
76	10.059	2802	2805	2811	rVB2	305	293	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029647.D
 Acq On : 13 Dec 2022 13:39
 Operator : SY/MD
 Sample : N5928-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.091	2812	2815	2816	rBV2	169	88	0.01%	0.001%
78	10.114	2820	2822	2824	rVB	220	89	0.01%	0.001%
79	10.162	2826	2837	2841	rBV2	21968	32643	2.10%	0.243%
80	10.204	2842	2850	2878	rVB	487715	766674	49.33%	5.702%
81	10.374	2895	2903	2914	rVB2	6371	10563	0.68%	0.079%
82	10.529	2945	2951	2955	rBV3	1534	1746	0.11%	0.013%
83	10.567	2957	2963	2975	rVB2	10328	16511	1.06%	0.123%
84	10.731	3008	3014	3022	rBV5	1290	1718	0.11%	0.013%
85	10.779	3026	3029	3031	rBV	154	82	0.01%	0.001%
86	10.905	3062	3068	3076	rVB4	3165	4323	0.28%	0.032%
87	11.130	3136	3138	3141	rBV	265	125	0.01%	0.001%
88	11.149	3141	3144	3147	rVB2	224	117	0.01%	0.001%
89	11.178	3147	3153	3157	rBV4	1115	1388	0.09%	0.010%
90	11.236	3159	3171	3193	rBV	900491	1409884	90.72%	10.485%
91	11.471	3242	3244	3247	rBV2	272	124	0.01%	0.001%
92	11.612	3276	3288	3308	rBV	795577	1228110	79.02%	9.133%
93	11.869	3366	3368	3369	rBV	261	86	0.01%	0.001%
94	11.966	3393	3398	3402	rBV2	420	384	0.02%	0.003%
95	12.001	3404	3409	3417	rVB4	1034	1577	0.10%	0.012%
96	12.152	3453	3456	3459	rBV2	433	284	0.02%	0.002%
97	12.355	3516	3519	3526	rBV4	473	582	0.04%	0.004%
98	12.458	3544	3551	3562	rBV5	1327	2041	0.13%	0.015%
99	13.033	3727	3730	3734	rVB3	931	602	0.04%	0.004%
100	13.242	3791	3795	3797	rBV3	888	759	0.05%	0.006%




Sum of corrected areas: 13446669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029647.D
Acq On : 13 Dec 2022 13:39
Operator : SY/MD
Sample : N5928-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

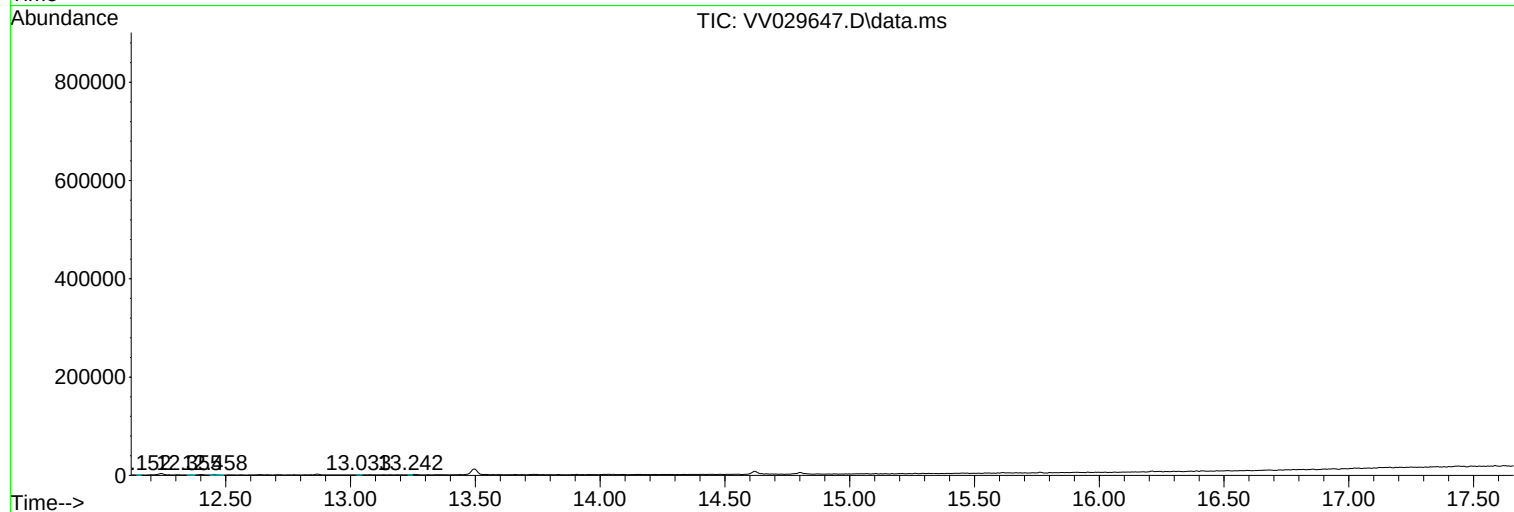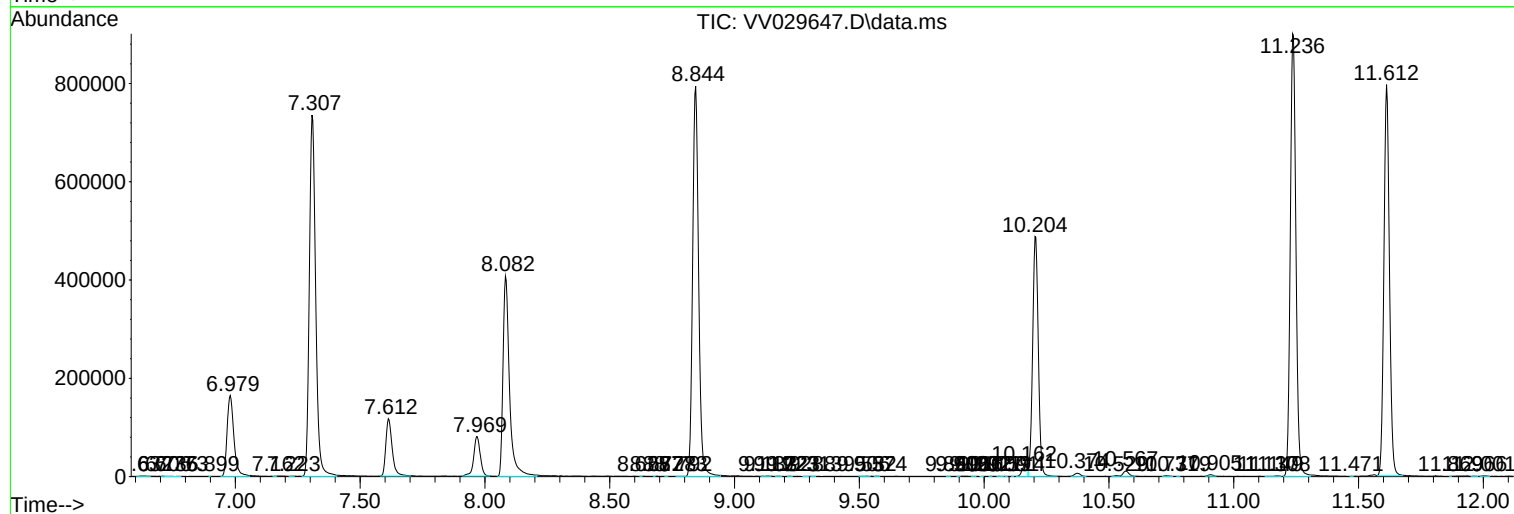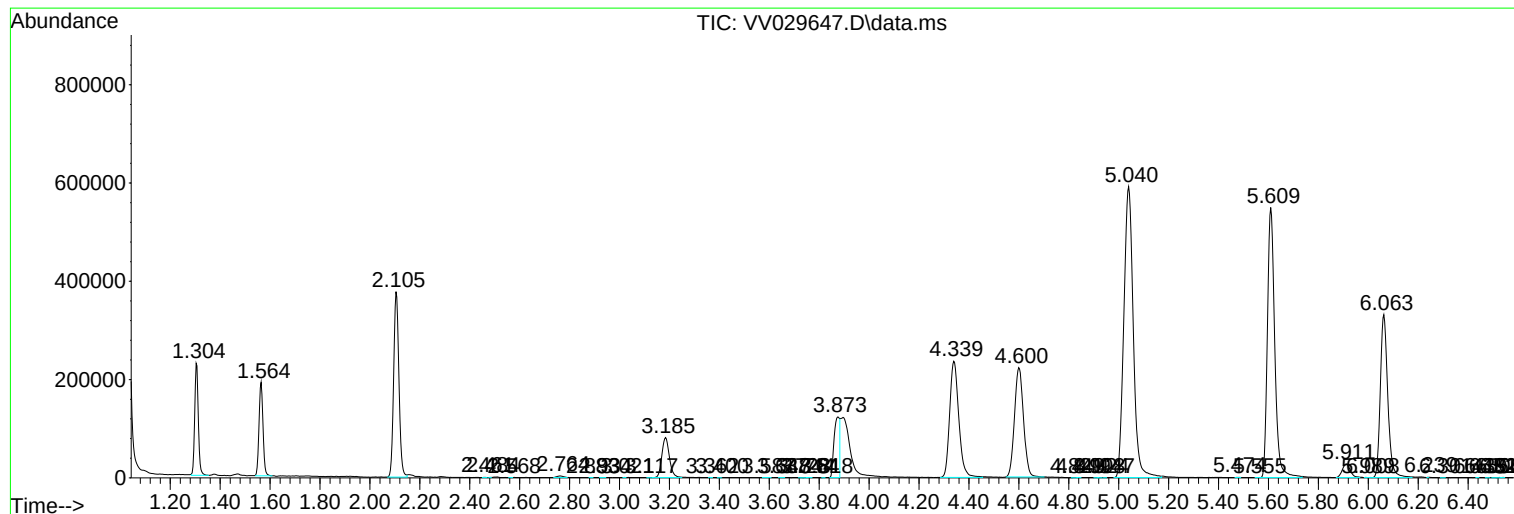

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029647.D
Acq On : 13 Dec 2022 13:39
Operator : SY/MD
Sample : N5928-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029647.D
Acq On : 13 Dec 2022 13:39
Operator : SY/MD
Sample : N5928-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------