

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029648.D
 Acq On : 13 Dec 2022 14:03
 Operator : SY/MD
 Sample : N5928-14DL 25X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ75DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	219591	221312	14.78%	1.768%
2	1.564	156	163	174	rVB	180085	201243	13.44%	1.608%
3	2.105	320	331	349	rBV	359549	513676	34.30%	4.104%
4	2.507	448	456	471	rVB3	5473	8934	0.60%	0.071%
5	2.677	507	509	511	rBV2	230	118	0.01%	0.001%
6	2.793	542	545	549	rBV2	276	237	0.02%	0.002%
7	2.886	572	574	575	rBV	183	64	0.00%	0.001%
8	2.957	593	596	601	rVB2	347	280	0.02%	0.002%
9	3.018	612	615	617	rBV2	125	77	0.01%	0.001%
10	3.060	626	628	632	rBV2	188	165	0.01%	0.001%
11	3.121	644	647	648	rBV2	158	69	0.00%	0.001%
12	3.188	659	668	683	rVB2	4748	9080	0.61%	0.073%
13	3.243	683	685	687	rBV	199	111	0.01%	0.001%
14	3.326	707	711	712	rBV2	189	130	0.01%	0.001%
15	3.545	775	779	782	rBB	181	104	0.01%	0.001%
16	3.574	782	788	789	rBV	177	161	0.01%	0.001%
17	3.609	796	799	800	rBV	230	126	0.01%	0.001%
18	3.661	812	815	818	rBV2	218	158	0.01%	0.001%
19	3.780	849	852	858	rVB4	316	277	0.02%	0.002%
20	3.889	870	886	924	rBV4	110940	444452	29.68%	3.551%
21	4.339	1010	1026	1051	rBV	230626	568356	37.96%	4.541%
22	4.603	1092	1108	1126	rBV3	36449	91666	6.12%	0.732%
23	4.761	1153	1157	1161	rVB2	242	214	0.01%	0.002%
24	4.786	1161	1165	1167	rBV	140	108	0.01%	0.001%
25	4.834	1179	1180	1187	rVB	278	183	0.01%	0.001%
26	4.879	1188	1194	1203	rBV2	206	252	0.02%	0.002%
27	5.040	1225	1244	1275	rBV2	570145	1497423	100.00%	11.963%
28	5.387	1350	1352	1353	rBV2	298	126	0.01%	0.001%
29	5.445	1367	1370	1373	rBV2	212	192	0.01%	0.002%
30	5.609	1407	1421	1462	rBV	562140	1146972	76.60%	9.163%
31	5.902	1503	1512	1528	rVB6	5330	11992	0.80%	0.096%
32	6.063	1548	1562	1593	rBV	322216	668422	44.64%	5.340%
33	6.394	1661	1665	1666	rBV	245	117	0.01%	0.001%
34	6.481	1685	1692	1694	rVB2	307	292	0.02%	0.002%
35	6.500	1694	1698	1700	rBV	172	143	0.01%	0.001%
36	6.526	1704	1706	1711	rVB2	146	82	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029648.D
 Acq On : 13 Dec 2022 14:03
 Operator : SY/MD
 Sample : N5928-14DL 25X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ75DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.548	1711	1713	1714	rBV2	296	127	0.01%	0.001%
38	6.619	1733	1735	1737	rBV2	452	239	0.02%	0.002%
39	6.667	1748	1750	1753	rBV	330	124	0.01%	0.001%
40	6.764	1778	1780	1783	rBV	202	69	0.00%	0.001%
41	6.828	1796	1800	1802	rBV2	220	167	0.01%	0.001%
42	6.860	1807	1810	1814	rVB3	164	133	0.01%	0.001%
43	6.879	1814	1816	1818	rBV	128	67	0.00%	0.001%
44	6.899	1818	1822	1823	rVB	132	81	0.01%	0.001%
45	6.912	1823	1826	1828	rVB	155	92	0.01%	0.001%
46	6.928	1828	1831	1832	rBV2	170	92	0.01%	0.001%
47	6.979	1836	1847	1872	rBV	160284	297905	19.89%	2.380%
48	7.156	1898	1902	1905	rBV2	484	529	0.04%	0.004%
49	7.307	1936	1949	1979	rBV	703550	1258027	84.01%	10.051%
50	7.612	2034	2044	2068	rBV2	111073	202424	13.52%	1.617%
51	7.931	2133	2143	2149	rBV4	1549	2608	0.17%	0.021%
52	8.085	2180	2191	2234	rBV	359847	663328	44.30%	5.299%
53	8.465	2306	2309	2314	rBV3	549	519	0.03%	0.004%
54	8.580	2341	2345	2347	rBV2	334	256	0.02%	0.002%
55	8.606	2351	2353	2358	rBV2	446	332	0.02%	0.003%
56	8.641	2362	2364	2365	rBV	196	62	0.00%	0.000%
57	8.667	2369	2372	2374	rBV2	311	217	0.01%	0.002%
58	8.712	2383	2386	2387	rBV	161	67	0.00%	0.001%
59	8.844	2414	2427	2455	rBV	829418	1348332	90.04%	10.772%
60	9.182	2530	2532	2534	rVB	199	88	0.01%	0.001%
61	9.233	2543	2548	2550	rBV2	316	261	0.02%	0.002%
62	9.246	2550	2552	2555	rVV	166	84	0.01%	0.001%
63	9.275	2559	2561	2563	rVB	361	148	0.01%	0.001%
64	9.474	2621	2623	2625	rBV	201	123	0.01%	0.001%
65	9.535	2637	2642	2651	rBV5	984	1584	0.11%	0.013%
66	9.600	2657	2662	2672	rBV2	281	400	0.03%	0.003%
67	9.645	2674	2676	2683	rVV2	269	282	0.02%	0.002%
68	9.673	2683	2685	2688	rVB2	155	78	0.01%	0.001%
69	9.693	2688	2691	2692	rBV	202	92	0.01%	0.001%
70	9.706	2693	2695	2698	rVV2	258	170	0.01%	0.001%
71	9.738	2701	2705	2708	rBV2	181	118	0.01%	0.001%
72	9.754	2708	2710	2715	rBV	309	227	0.02%	0.002%
73	9.866	2743	2745	2751	rVB2	221	137	0.01%	0.001%
74	9.927	2758	2764	2771	rBV3	298	404	0.03%	0.003%
75	9.960	2772	2774	2777	rVB	194	86	0.01%	0.001%
76	10.053	2799	2803	2805	rBV2	215	162	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029648.D
 Acq On : 13 Dec 2022 14:03
 Operator : SY/MD
 Sample : N5928-14DL 25X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ75DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.095	2812	2816	2818	rBV2	404	234	0.02%	0.002%
78	10.114	2818	2822	2824	rBV2	138	105	0.01%	0.001%
79	10.162	2827	2837	2841	rBV2	20410	30443	2.03%	0.243%
80	10.204	2842	2850	2871	rVB	459874	729420	48.71%	5.828%
81	10.371	2898	2902	2910	rVB3	1312	1777	0.12%	0.014%
82	10.532	2945	2952	2955	rBV2	1839	2120	0.14%	0.017%
83	10.677	2996	2997	2999	rBV	284	61	0.00%	0.000%
84	10.696	2999	3003	3006	rBV	222	145	0.01%	0.001%
85	10.728	3006	3013	3020	rBV5	974	1413	0.09%	0.011%
86	10.866	3053	3056	3060	rBV2	236	221	0.01%	0.002%
87	10.908	3060	3069	3079	rVB5	2724	4234	0.28%	0.034%
88	10.950	3079	3082	3085	rBV2	186	97	0.01%	0.001%
89	11.072	3118	3120	3123	rBV	382	175	0.01%	0.001%
90	11.165	3147	3149	3150	rBV2	652	256	0.02%	0.002%
91	11.236	3159	3171	3194	rBV	907226	1425536	95.20%	11.389%
92	11.480	3244	3247	3251	rBV2	410	306	0.02%	0.002%
93	11.526	3251	3261	3264	rBV7	1022	1311	0.09%	0.010%
94	11.558	3265	3271	3276	rBV4	1084	1542	0.10%	0.012%
95	11.612	3276	3288	3314	rVV	737680	1148652	76.71%	9.177%
96	11.998	3406	3408	3410	rBV2	550	324	0.02%	0.003%
97	12.056	3423	3426	3428	rBV	336	198	0.01%	0.002%
98	12.304	3499	3503	3505	rBV2	326	183	0.01%	0.001%
99	12.509	3564	3567	3569	rBV2	341	248	0.02%	0.002%
100	13.072	3740	3742	3744	rBV2	507	295	0.02%	0.002%




Sum of corrected areas: 12516851

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029648.D
Acq On : 13 Dec 2022 14:03
Operator : SY/MD
Sample : N5928-14DL 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

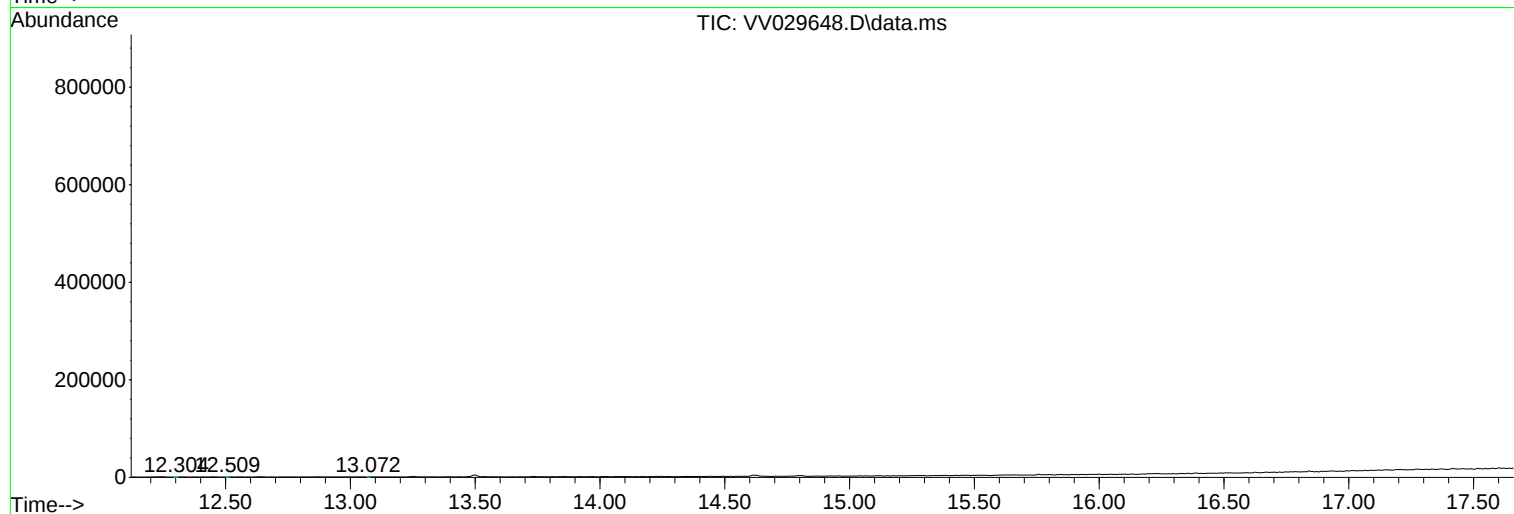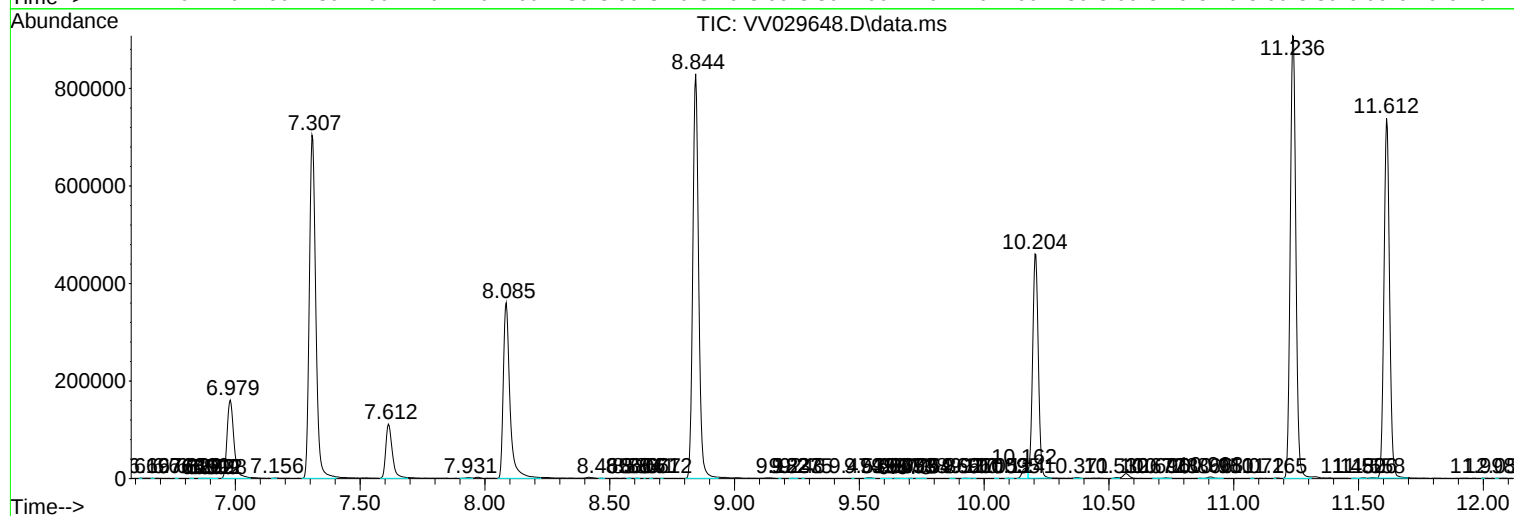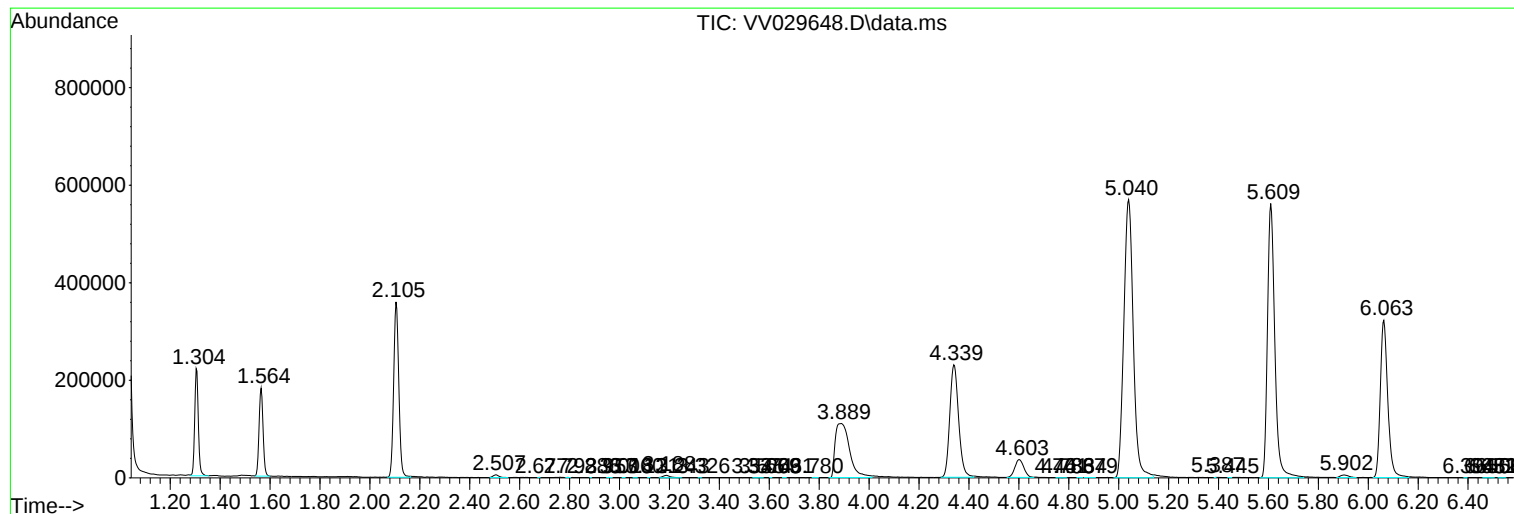

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029648.D
Acq On : 13 Dec 2022 14:03
Operator : SY/MD
Sample : N5928-14DL 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029648.D
Acq On : 13 Dec 2022 14:03
Operator : SY/MD
Sample : N5928-14DL 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------