

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029649.D
 Acq On : 13 Dec 2022 14:27
 Operator : SY/MD
 Sample : N5928-19 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029649.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	229542	233731	12.97%	1.598%
2	1.561	155	162	178	rVB2	166730	227493	12.63%	1.555%
3	2.105	320	331	348	rBV	342791	499001	27.69%	3.411%
4	2.503	446	455	467	rVB2	7149	11839	0.66%	0.081%
5	2.571	475	476	479	rBV	174	98	0.01%	0.001%
6	2.757	525	534	546	rVB3	6142	11007	0.61%	0.075%
7	2.812	546	551	557	rBV3	256	242	0.01%	0.002%
8	2.844	558	561	566	rBV3	249	229	0.01%	0.002%
9	2.908	578	581	583	rBV	147	111	0.01%	0.001%
10	2.941	589	591	595	rVB	228	148	0.01%	0.001%
11	2.979	595	603	609	rBV	390	335	0.02%	0.002%
12	3.040	619	622	624	rBV2	260	176	0.01%	0.001%
13	3.182	652	666	693	rBV2	178443	378126	20.99%	2.585%
14	3.535	773	776	780	rBV2	255	144	0.01%	0.001%
15	3.558	780	783	787	rBV2	148	103	0.01%	0.001%
16	3.741	835	840	843	rBV	205	216	0.01%	0.001%
17	3.902	868	890	930	rBV2	643023	1801818	100.00%	12.316%
18	4.339	1009	1026	1059	rBV	214694	538916	29.91%	3.684%
19	4.600	1091	1107	1136	rVB	252279	628309	34.87%	4.295%
20	4.831	1176	1179	1181	rBV	279	98	0.01%	0.001%
21	4.870	1188	1191	1193	rBV2	155	99	0.01%	0.001%
22	4.941	1209	1213	1216	rBV2	155	131	0.01%	0.001%
23	5.040	1226	1244	1273	rBV2	535290	1403504	77.89%	9.594%
24	5.416	1358	1361	1362	rBV2	234	123	0.01%	0.001%
25	5.609	1407	1421	1470	rBV	537628	1108254	61.51%	7.575%
26	5.908	1502	1514	1533	rBV6	11701	27390	1.52%	0.187%
27	6.063	1548	1562	1590	rBV	300319	622917	34.57%	4.258%
28	6.259	1621	1623	1625	rVB2	266	122	0.01%	0.001%
29	6.272	1625	1627	1629	rBV	173	98	0.01%	0.001%
30	6.310	1635	1639	1641	rBV2	323	248	0.01%	0.002%
31	6.333	1644	1646	1649	rVB2	196	95	0.01%	0.001%
32	6.387	1660	1663	1666	rBV	246	187	0.01%	0.001%
33	6.484	1690	1693	1695	rBV	147	88	0.00%	0.001%
34	6.522	1700	1705	1706	rBV	183	136	0.01%	0.001%
35	6.590	1721	1726	1728	rBV2	184	162	0.01%	0.001%
36	6.699	1758	1760	1763	rBV2	232	160	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029649.D
 Acq On : 13 Dec 2022 14:27
 Operator : SY/MD
 Sample : N5928-19 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.728	1766	1769	1774	rBV	288	282	0.02%	0.002%
38	6.821	1795	1798	1800	rVB	194	109	0.01%	0.001%
39	6.979	1833	1847	1876	rBV	152133	280612	15.57%	1.918%
40	7.156	1900	1902	1903	rBV	283	123	0.01%	0.001%
41	7.236	1924	1927	1929	rBV	575	342	0.02%	0.002%
42	7.307	1936	1949	1966	rBV	661280	1162743	64.53%	7.948%
43	7.612	2034	2044	2072	rBV	107042	189292	10.51%	1.294%
44	7.805	2100	2104	2105	rBV2	322	206	0.01%	0.001%
45	8.082	2180	2190	2231	rBV	338469	615725	34.17%	4.209%
46	8.455	2303	2306	2310	rBV3	349	293	0.02%	0.002%
47	8.481	2310	2314	2316	rBV2	168	146	0.01%	0.001%
48	8.609	2351	2354	2356	rBV2	395	273	0.02%	0.002%
49	8.702	2381	2383	2385	rVB2	266	105	0.01%	0.001%
50	8.751	2393	2398	2403	rBV3	312	327	0.02%	0.002%
51	8.792	2407	2411	2415	rBV2	235	185	0.01%	0.001%
52	8.844	2415	2427	2460	rBV	789749	1303825	72.36%	8.912%
53	9.008	2471	2478	2490	rVB	8681	13161	0.73%	0.090%
54	9.085	2501	2502	2506	rBV	276	159	0.01%	0.001%
55	9.133	2506	2517	2530	rVV2	22193	38347	2.13%	0.262%
56	9.275	2557	2561	2564	rBV2	306	205	0.01%	0.001%
57	9.294	2564	2567	2569	rBV	143	91	0.01%	0.001%
58	9.384	2593	2595	2598	rVB	204	103	0.01%	0.001%
59	9.416	2602	2605	2607	rBV2	259	118	0.01%	0.001%
60	9.487	2625	2627	2631	rVB2	251	157	0.01%	0.001%
61	9.535	2632	2642	2658	rBV	24451	40356	2.24%	0.276%
62	9.628	2666	2671	2672	rBV	215	125	0.01%	0.001%
63	9.696	2684	2692	2699	rBV6	941	1379	0.08%	0.009%
64	9.789	2717	2721	2724	rBV2	440	421	0.02%	0.003%
65	9.924	2755	2763	2772	rVV3	1906	2722	0.15%	0.019%
66	9.995	2782	2785	2788	rBV	386	244	0.01%	0.002%
67	10.037	2795	2798	2801	rBV	243	120	0.01%	0.001%
68	10.053	2801	2803	2806	rVB2	288	149	0.01%	0.001%
69	10.069	2806	2808	2810	rBV2	315	152	0.01%	0.001%
70	10.127	2822	2826	2827	rBV	336	232	0.01%	0.002%
71	10.162	2828	2837	2841	rVV2	21085	30429	1.69%	0.208%
72	10.207	2842	2851	2874	rVB	429729	685053	38.02%	4.683%
73	10.349	2887	2895	2898	rBV4	3679	4999	0.28%	0.034%
74	10.442	2914	2924	2928	rBV	14824	23927	1.33%	0.164%
75	10.529	2943	2951	2958	rBV	18957	27243	1.51%	0.186%
76	10.635	2982	2984	2988	rVB2	267	157	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029649.D
 Acq On : 13 Dec 2022 14:27
 Operator : SY/MD
 Sample : N5928-19 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.728	3004	3013	3024	rVB2	20080	30387	1.69%	0.208%
78	10.805	3035	3037	3039	rBV2	189	92	0.01%	0.001%
79	10.844	3046	3049	3051	rBV	332	206	0.01%	0.001%
80	10.905	3057	3068	3085	rBV	40093	61844	3.43%	0.423%
81	10.963	3085	3086	3092	rVB	325	213	0.01%	0.001%
82	10.992	3092	3095	3099	rBV3	282	217	0.01%	0.001%
83	11.056	3107	3115	3116	rBV2	549	653	0.04%	0.004%
84	11.075	3117	3121	3131	rVB5	1113	1610	0.09%	0.011%
85	11.146	3140	3143	3144	rBV5	298	147	0.01%	0.001%
86	11.181	3144	3154	3160	rVV6	2330	3748	0.21%	0.026%
87	11.236	3160	3171	3191	rVV	889345	1381347	76.66%	9.442%
88	11.326	3191	3199	3213	rVB	28638	45675	2.53%	0.312%
89	11.519	3251	3259	3268	rBV2	10393	17644	0.98%	0.121%
90	11.612	3277	3288	3314	rVB	716485	1117110	62.00%	7.636%
91	11.915	3371	3382	3395	rVB6	9858	21633	1.20%	0.148%
92	11.976	3395	3401	3402	rBV3	385	339	0.02%	0.002%
93	12.008	3404	3411	3419	rVV2	4428	5958	0.33%	0.041%
94	12.297	3496	3501	3502	rBV3	942	719	0.04%	0.005%
95	12.374	3523	3525	3527	rBV	302	181	0.01%	0.001%
96	12.455	3544	3550	3560	rVB2	4181	6182	0.34%	0.042%
97	12.599	3594	3595	3597	rBV	385	189	0.01%	0.001%
98	12.869	3672	3679	3689	rVB3	4874	6871	0.38%	0.047%
99	13.027	3725	3728	3730	rBV3	789	564	0.03%	0.004%
100	13.493	3868	3873	3882	rVB2	4206	5543	0.31%	0.038%




Sum of corrected areas: 14629563

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029649.D
Acq On : 13 Dec 2022 14:27
Operator : SY/MD
Sample : N5928-19 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

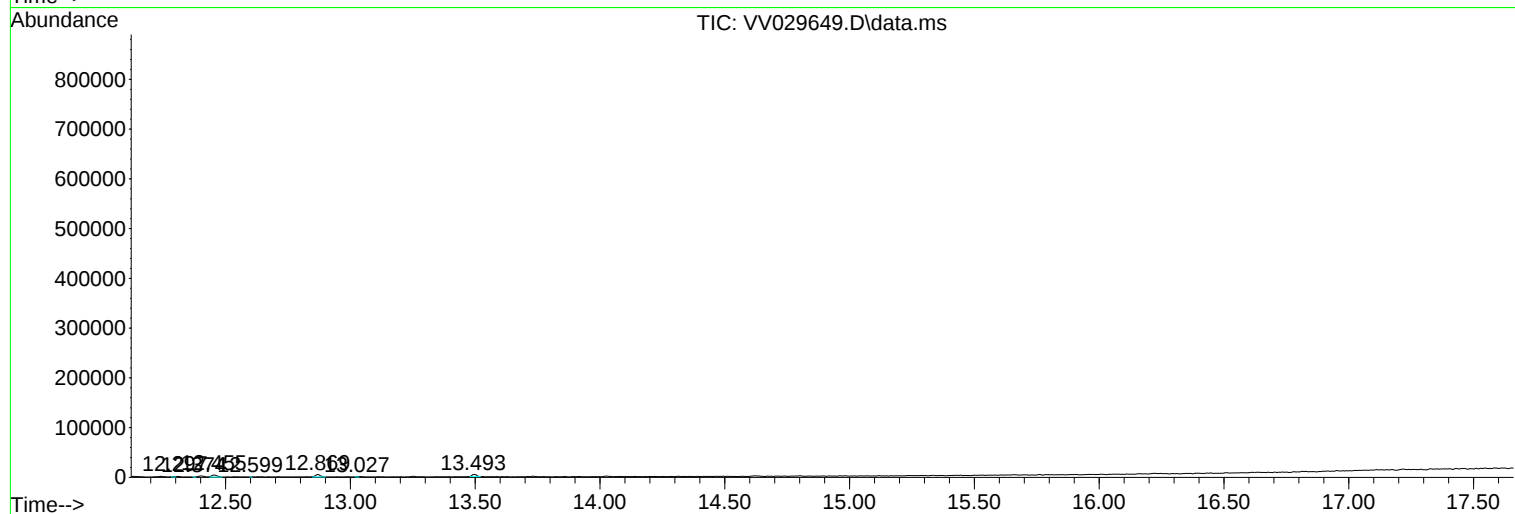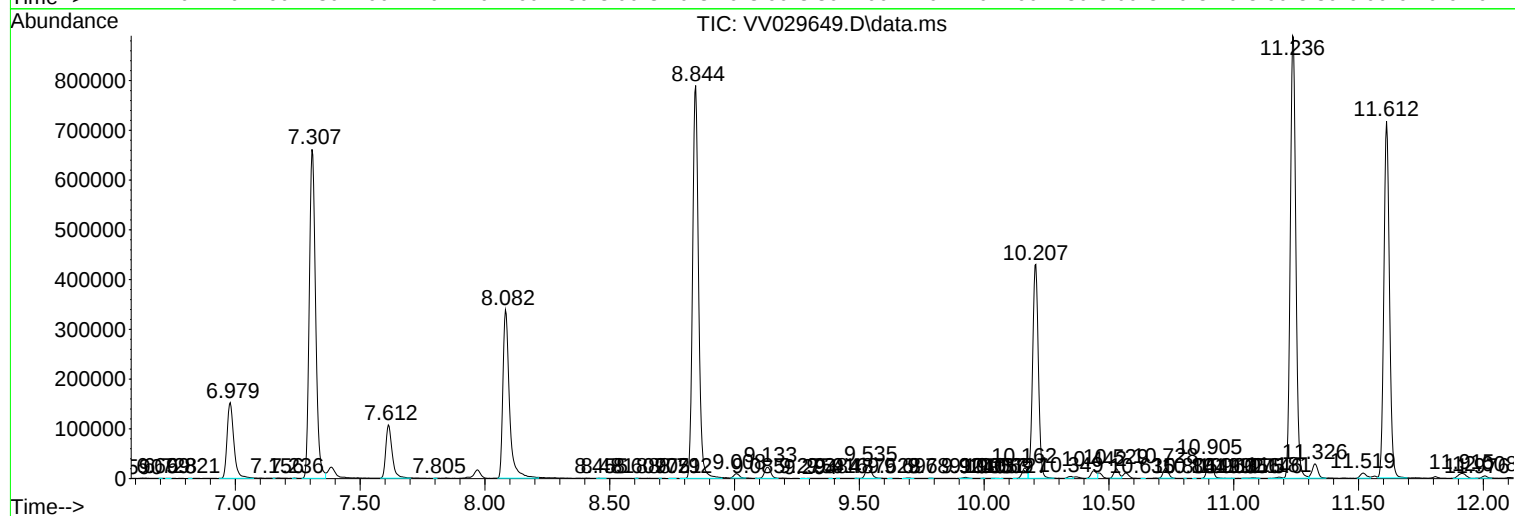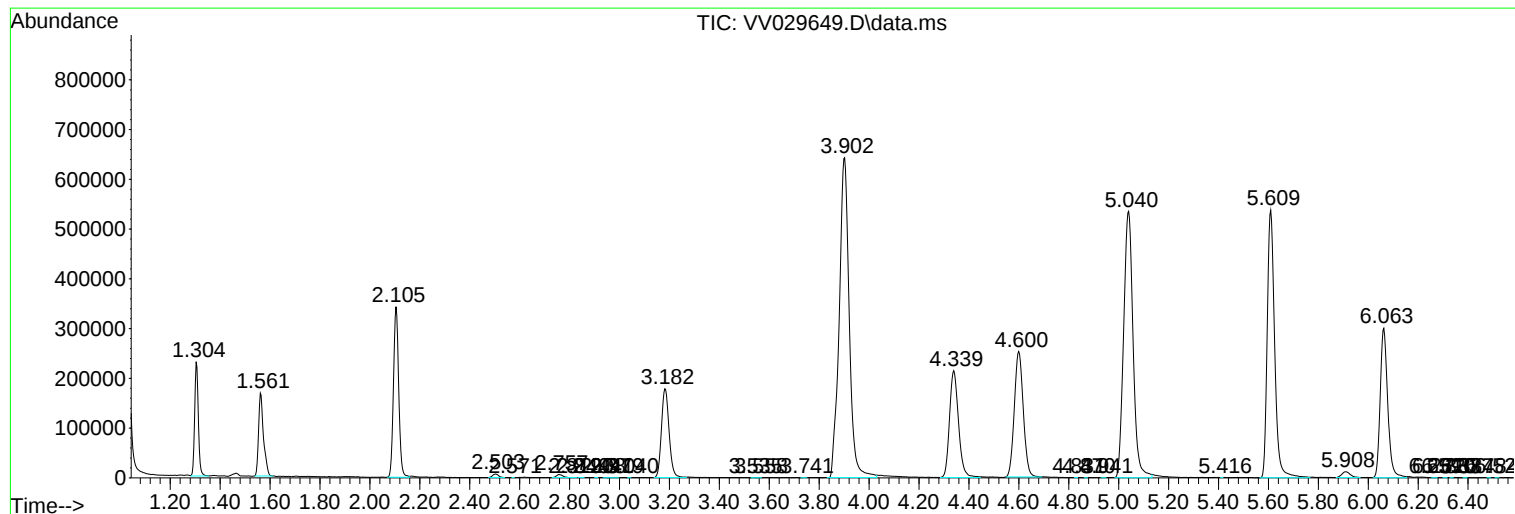

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029649.D
Acq On : 13 Dec 2022 14:27
Operator : SY/MD
Sample : N5928-19 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029649.D
Acq On : 13 Dec 2022 14:27
Operator : SY/MD
Sample : N5928-19 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc