

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029650.D
 Acq On : 13 Dec 2022 14:50
 Operator : SY/MD
 Sample : N5928-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029650.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	221383	215387	3.40%	0.844%
2	1.564	155	163	176	rBV	176109	197099	3.11%	0.773%
3	1.703	201	206	213	rVB	13676	14997	0.24%	0.059%
4	1.751	216	221	226	rBV	16090	18674	0.29%	0.073%
5	2.114	321	334	358	rBV4	1306041	2091726	33.02%	8.199%
6	2.445	435	437	440	rBV	270	152	0.00%	0.001%
7	2.500	449	454	462	rVB4	1659	2484	0.04%	0.010%
8	2.632	492	495	500	rBV3	235	249	0.00%	0.001%
9	2.757	523	534	555	rBV	38056	69103	1.09%	0.271%
10	2.953	592	595	597	rBV	125	101	0.00%	0.000%
11	3.121	644	647	649	rBV2	226	141	0.00%	0.001%
12	3.182	649	666	692	rBV	886804	1855790	29.30%	7.274%
13	3.577	784	789	793	rBV2	243	238	0.00%	0.001%
14	3.603	794	797	801	rVV	193	153	0.00%	0.001%
15	3.722	832	834	837	rVB3	184	108	0.00%	0.000%
16	3.818	861	864	866	rBV	158	97	0.00%	0.000%
17	3.902	871	890	938	rBV2	475963	1392787	21.99%	5.459%
18	4.339	1009	1026	1061	rBV	228021	600798	9.49%	2.355%
19	4.600	1085	1107	1170	rBV	2527714	6334062	100.00%	24.827%
20	5.040	1226	1244	1284	rBV2	558837	1471308	23.23%	5.767%
21	5.384	1349	1351	1353	rBV2	274	125	0.00%	0.000%
22	5.529	1394	1396	1398	rBV	259	102	0.00%	0.000%
23	5.609	1407	1421	1458	rBV	517581	1050799	16.59%	4.119%
24	5.905	1500	1513	1546	rBV	545744	1093585	17.27%	4.286%
25	6.063	1549	1562	1591	rVB	312852	642506	10.14%	2.518%
26	6.320	1637	1642	1645	rBV2	259	267	0.00%	0.001%
27	6.339	1646	1648	1651	rVB2	215	129	0.00%	0.001%
28	6.362	1651	1655	1658	rBV2	282	186	0.00%	0.001%
29	6.407	1663	1669	1673	rBV4	474	489	0.01%	0.002%
30	6.490	1692	1695	1696	rBV	207	124	0.00%	0.000%
31	6.510	1699	1701	1704	rVB2	221	119	0.00%	0.000%
32	6.535	1707	1709	1713	rVB	227	144	0.00%	0.001%
33	6.567	1713	1719	1724	rBV3	356	428	0.01%	0.002%
34	6.632	1731	1739	1744	rBV5	895	1305	0.02%	0.005%
35	6.722	1765	1767	1770	rBV2	352	195	0.00%	0.001%
36	6.770	1779	1782	1784	rBV	328	206	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029650.D
 Acq On : 13 Dec 2022 14:50
 Operator : SY/MD
 Sample : N5928-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.799	1789	1791	1793	rVB	218	92	0.00%	0.000%
38	6.812	1793	1795	1799	rVB2	244	138	0.00%	0.001%
39	6.844	1799	1805	1808	rBV3	432	324	0.01%	0.001%
40	6.979	1835	1847	1872	rBV	157916	293948	4.64%	1.152%
41	7.239	1923	1928	1935	rBV3	324	464	0.01%	0.002%
42	7.307	1937	1949	1976	rBV	681374	1212063	19.14%	4.751%
43	7.612	2034	2044	2066	rBV	110851	194991	3.08%	0.764%
44	7.770	2090	2093	2095	rBV2	425	288	0.00%	0.001%
45	7.834	2103	2113	2129	rVB3	22965	39621	0.63%	0.155%
46	7.966	2142	2154	2180	rVB	986699	1663667	26.27%	6.521%
47	8.082	2181	2190	2221	rBV	375922	653623	10.32%	2.562%
48	8.423	2294	2296	2298	rBV2	239	89	0.00%	0.000%
49	8.468	2305	2310	2312	rBV3	377	287	0.00%	0.001%
50	8.493	2315	2318	2320	rVB2	326	147	0.00%	0.001%
51	8.648	2363	2366	2370	rBV2	184	153	0.00%	0.001%
52	8.792	2408	2411	2414	rBV3	378	284	0.00%	0.001%
53	8.844	2414	2427	2457	rBV	754558	1239397	19.57%	4.858%
54	9.059	2492	2494	2495	rBV	476	126	0.00%	0.000%
55	9.130	2512	2516	2518	rBV3	482	384	0.01%	0.002%
56	9.227	2544	2546	2548	rVB	346	119	0.00%	0.000%
57	9.262	2552	2557	2561	rBV4	353	286	0.00%	0.001%
58	9.317	2571	2574	2579	rVB2	362	249	0.00%	0.001%
59	9.352	2583	2585	2589	rBV2	172	140	0.00%	0.001%
60	9.374	2589	2592	2598	rBV	392	273	0.00%	0.001%
61	9.410	2601	2603	2606	rVB	192	101	0.00%	0.000%
62	9.432	2607	2610	2613	rBV2	224	165	0.00%	0.001%
63	9.545	2638	2645	2650	rBV4	544	656	0.01%	0.003%
64	9.654	2676	2679	2682	rVB2	223	141	0.00%	0.001%
65	9.690	2687	2690	2693	rBV2	313	163	0.00%	0.001%
66	9.725	2698	2701	2704	rVB2	193	136	0.00%	0.001%
67	9.789	2719	2721	2725	rVB2	346	199	0.00%	0.001%
68	9.808	2725	2727	2731	rBV	311	223	0.00%	0.001%
69	9.831	2732	2734	2740	rVB3	262	201	0.00%	0.001%
70	10.050	2798	2802	2803	rBV2	230	139	0.00%	0.001%
71	10.085	2808	2813	2816	rBV2	300	308	0.00%	0.001%
72	10.162	2828	2837	2841	rBV2	20846	29896	0.47%	0.117%
73	10.204	2842	2850	2873	rVB	457200	718769	11.35%	2.817%
74	10.371	2893	2902	2924	rVB3	5995	10286	0.16%	0.040%
75	10.458	2924	2929	2931	rBV2	413	399	0.01%	0.002%
76	10.526	2947	2950	2953	rBV2	313	215	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029650.D
 Acq On : 13 Dec 2022 14:50
 Operator : SY/MD
 Sample : N5928-22
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.571	2953	2964	2972	rBV2	9737	15632	0.25%	0.061%
78	10.763	3019	3024	3028	rBV3	513	384	0.01%	0.002%
79	10.783	3028	3030	3032	rVB	253	112	0.00%	0.000%
80	10.876	3057	3059	3061	rBV	212	124	0.00%	0.000%
81	10.898	3062	3066	3068	rBV2	582	394	0.01%	0.002%
82	10.992	3092	3095	3097	rBV2	213	128	0.00%	0.001%
83	11.043	3109	3111	3117	rVV2	224	180	0.00%	0.001%
84	11.114	3130	3133	3134	rBV2	205	126	0.00%	0.000%
85	11.146	3141	3143	3145	rBV	210	102	0.00%	0.000%
86	11.175	3148	3152	3157	rVB2	691	670	0.01%	0.003%
87	11.239	3157	3172	3196	rBV	811169	1264099	19.96%	4.955%
88	11.551	3266	3269	3273	rBV3	408	317	0.01%	0.001%
89	11.612	3276	3288	3310	rBV	705440	1108152	17.50%	4.343%
90	11.805	3346	3348	3350	rBV2	256	140	0.00%	0.001%
91	11.866	3364	3367	3371	rBV2	494	396	0.01%	0.002%
92	11.908	3377	3380	3385	rBV3	477	411	0.01%	0.002%
93	12.062	3425	3428	3430	rVB	306	165	0.00%	0.001%
94	12.287	3495	3498	3499	rBV	491	287	0.00%	0.001%
95	12.374	3521	3525	3526	rBV	409	283	0.00%	0.001%
96	12.641	3603	3608	3613	rBV5	594	612	0.01%	0.002%
97	13.001	3715	3720	3722	rBV4	540	410	0.01%	0.002%
98	13.159	3767	3769	3771	rBB	339	118	0.00%	0.000%
99	13.352	3826	3829	3831	rBV2	564	476	0.01%	0.002%
100	13.757	3954	3955	3956	rBV	532	136	0.00%	0.001%




Sum of corrected areas: 25513167

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029650.D
Acq On : 13 Dec 2022 14:50
Operator : SY/MD
Sample : N5928-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

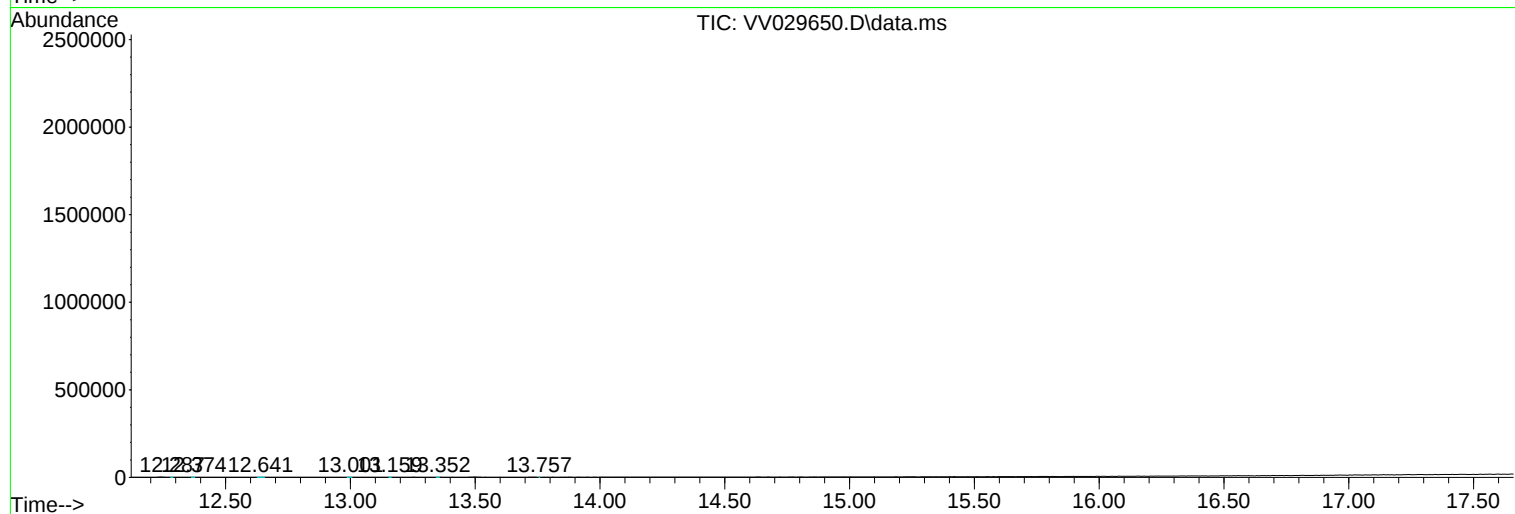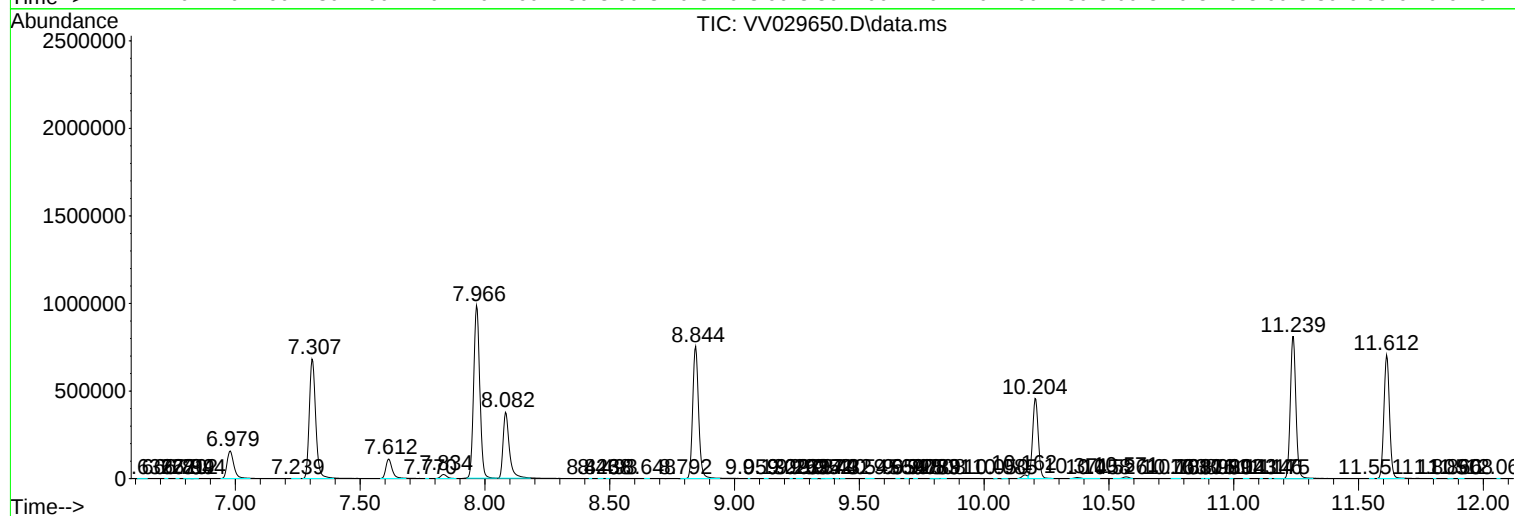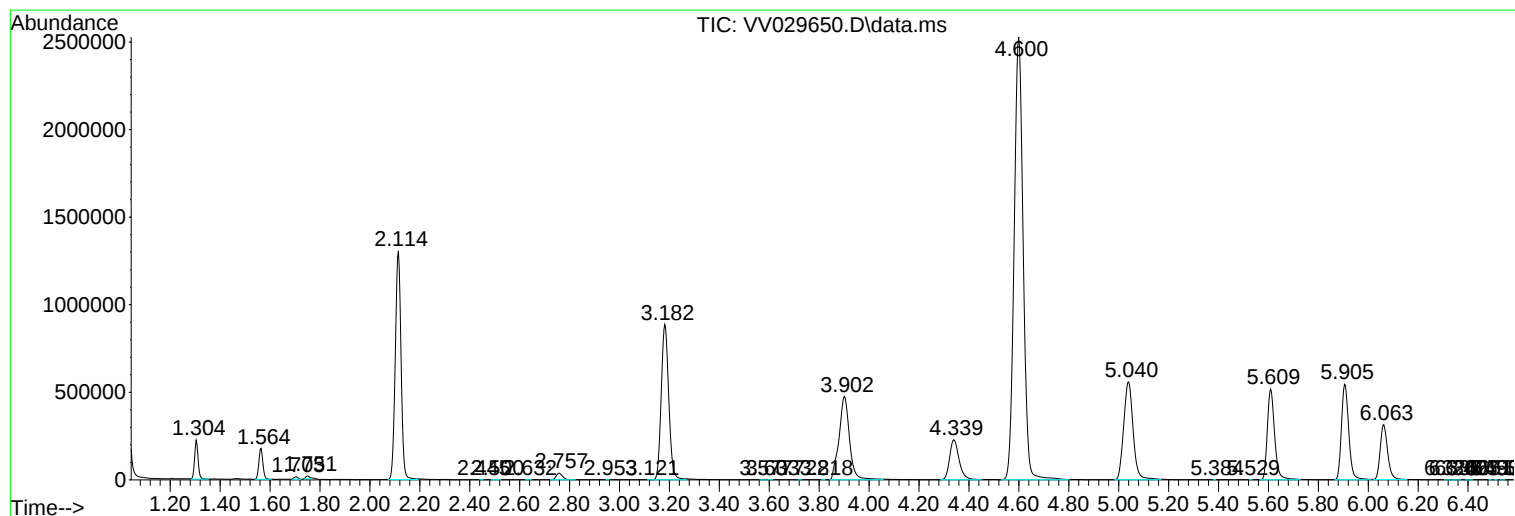

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029650.D
Acq On : 13 Dec 2022 14:50
Operator : SY/MD
Sample : N5928-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029650.D
Acq On : 13 Dec 2022 14:50
Operator : SY/MD
Sample : N5928-22
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------