

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029651.D
 Acq On : 13 Dec 2022 15:14
 Operator : SY/MD
 Sample : VIBLK307
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK307

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	214301	214112	15.12%	1.827%
2	1.564	155	163	179	rVB	171632	193809	13.68%	1.654%
3	2.105	320	331	348	rBV	336214	484850	34.23%	4.137%
4	2.503	445	455	464	rBV4	3464	5624	0.40%	0.048%
5	2.642	496	498	502	rBV2	179	131	0.01%	0.001%
6	2.680	507	510	513	rBV	219	135	0.01%	0.001%
7	2.703	513	517	519	rVB3	354	217	0.02%	0.002%
8	2.725	521	524	528	rBV3	280	248	0.02%	0.002%
9	2.764	532	536	539	rVB	433	244	0.02%	0.002%
10	2.828	553	556	560	rBV2	232	154	0.01%	0.001%
11	2.902	576	579	582	rBV	143	112	0.01%	0.001%
12	2.976	599	602	609	rVB2	266	268	0.02%	0.002%
13	3.034	614	620	623	rBV2	154	131	0.01%	0.001%
14	3.178	662	665	668	rBV3	407	337	0.02%	0.003%
15	3.362	718	722	723	rBV	194	102	0.01%	0.001%
16	3.413	735	738	741	rBV2	133	97	0.01%	0.001%
17	3.490	757	762	764	rBV2	166	146	0.01%	0.001%
18	3.503	764	766	769	rVB	231	96	0.01%	0.001%
19	3.603	792	797	798	rBV	207	131	0.01%	0.001%
20	3.629	804	805	809	rVB	281	125	0.01%	0.001%
21	3.732	832	837	844	rBV2	191	216	0.02%	0.002%
22	3.757	844	845	849	rVB	197	99	0.01%	0.001%
23	3.789	849	855	857	rBV2	152	154	0.01%	0.001%
24	3.834	866	869	870	rBV	171	97	0.01%	0.001%
25	3.870	870	880	919	rBV	100516	285871	20.18%	2.439%
26	4.339	1010	1026	1059	rBV	214868	538133	37.99%	4.592%
27	4.658	1123	1125	1128	rVB3	367	214	0.02%	0.002%
28	4.690	1128	1135	1138	rBV2	370	339	0.02%	0.003%
29	4.841	1178	1182	1184	rBV	223	145	0.01%	0.001%
30	4.960	1214	1219	1223	rBV2	169	184	0.01%	0.002%
31	5.040	1226	1244	1296	rBV2	534804	1416465	100.00%	12.086%
32	5.445	1367	1370	1374	rVB	164	98	0.01%	0.001%
33	5.609	1408	1421	1468	rBV	538446	1098127	77.53%	9.370%
34	5.902	1502	1512	1530	rVB8	5863	13470	0.95%	0.115%
35	6.063	1547	1562	1600	rBV	304514	631676	44.60%	5.390%
36	6.262	1619	1624	1630	rVB4	455	592	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029651.D
 Acq On : 13 Dec 2022 15:14
 Operator : SY/MD
 Sample : VIBLK307
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK307

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.294	1630	1634	1638	rBV2	284	202	0.01%	0.002%
38	6.368	1653	1657	1658	rBV	167	112	0.01%	0.001%
39	6.394	1662	1665	1670	rVB2	162	144	0.01%	0.001%
40	6.513	1697	1702	1704	rBV	217	142	0.01%	0.001%
41	6.542	1709	1711	1713	rBV	203	104	0.01%	0.001%
42	6.571	1716	1720	1723	rBV2	215	167	0.01%	0.001%
43	6.828	1794	1800	1802	rBV2	247	194	0.01%	0.002%
44	6.979	1835	1847	1872	rBV	152094	280616	19.81%	2.394%
45	7.262	1932	1935	1937	rVB2	207	125	0.01%	0.001%
46	7.307	1937	1949	1980	rBV	670806	1177634	83.14%	10.048%
47	7.558	2025	2027	2030	rBV	421	281	0.02%	0.002%
48	7.612	2035	2044	2069	rVV	109325	189885	13.41%	1.620%
49	7.783	2094	2097	2099	rBV2	482	269	0.02%	0.002%
50	7.863	2119	2122	2124	rBV2	143	120	0.01%	0.001%
51	8.082	2179	2190	2228	rBV	349908	637225	44.99%	5.437%
52	8.413	2285	2293	2300	rBV5	1551	2421	0.17%	0.021%
53	8.477	2311	2313	2314	rBV5	304	119	0.01%	0.001%
54	8.593	2345	2349	2350	rBV	222	152	0.01%	0.001%
55	8.696	2376	2381	2383	rVB2	303	219	0.02%	0.002%
56	8.738	2392	2394	2398	rVB2	240	102	0.01%	0.001%
57	8.763	2398	2402	2403	rBV2	188	128	0.01%	0.001%
58	8.844	2413	2427	2457	rBV	789872	1300624	91.82%	11.098%
59	9.133	2515	2517	2520	rBV2	292	209	0.01%	0.002%
60	9.271	2556	2560	2561	rBV2	235	148	0.01%	0.001%
61	9.323	2572	2576	2580	rBV	281	222	0.02%	0.002%
62	9.419	2603	2606	2608	rBV2	158	101	0.01%	0.001%
63	9.471	2619	2622	2625	rBV	244	181	0.01%	0.002%
64	9.535	2639	2642	2646	rBV	574	420	0.03%	0.004%
65	9.564	2649	2651	2654	rVV	301	128	0.01%	0.001%
66	9.580	2654	2656	2660	rVB	275	139	0.01%	0.001%
67	9.654	2673	2679	2680	rBV	234	149	0.01%	0.001%
68	9.783	2716	2719	2721	rBV2	198	117	0.01%	0.001%
69	9.834	2733	2735	2738	rVV2	297	157	0.01%	0.001%
70	9.853	2738	2741	2745	rVV	336	306	0.02%	0.003%
71	9.889	2749	2752	2757	rVB	313	149	0.01%	0.001%
72	9.921	2757	2762	2763	rBV2	200	144	0.01%	0.001%
73	9.953	2770	2772	2775	rVB2	375	170	0.01%	0.001%
74	9.988	2780	2783	2787	rBV	231	161	0.01%	0.001%
75	10.037	2796	2798	2800	rBV2	199	121	0.01%	0.001%
76	10.069	2806	2808	2815	rVB3	219	194	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029651.D
 Acq On : 13 Dec 2022 15:14
 Operator : SY/MD
 Sample : VIBLK307
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK307

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.107	2817	2820	2824	rBV2	205	127	0.01%	0.001%
78	10.165	2827	2838	2841	rBV	19946	28474	2.01%	0.243%
79	10.207	2842	2851	2870	rVB	441109	691058	48.79%	5.896%
80	10.371	2898	2902	2903	rBV2	835	633	0.04%	0.005%
81	10.464	2928	2931	2934	rBV2	162	119	0.01%	0.001%
82	10.497	2938	2941	2946	rVB2	295	180	0.01%	0.002%
83	10.525	2946	2950	2952	rBV2	448	369	0.03%	0.003%
84	10.567	2955	2963	2980	rVB2	10038	16208	1.14%	0.138%
85	10.638	2980	2985	2987	rBV2	285	202	0.01%	0.002%
86	10.683	2995	2999	3002	rBV2	304	229	0.02%	0.002%
87	10.773	3024	3027	3029	rBV	252	171	0.01%	0.001%
88	10.853	3049	3052	3055	rBV2	196	133	0.01%	0.001%
89	10.895	3062	3065	3067	rBV	266	190	0.01%	0.002%
90	10.940	3076	3079	3082	rBV2	171	157	0.01%	0.001%
91	11.239	3160	3172	3194	rBV	887498	1372280	96.88%	11.709%
92	11.545	3264	3267	3268	rBV	337	175	0.01%	0.001%
93	11.612	3275	3288	3317	rBV	716023	1126414	79.52%	9.611%
94	11.828	3353	3355	3357	rBV2	270	130	0.01%	0.001%
95	11.860	3363	3365	3366	rBV2	242	117	0.01%	0.001%
96	11.882	3369	3372	3375	rVV2	244	146	0.01%	0.001%
97	11.918	3381	3383	3384	rBV2	286	107	0.01%	0.001%
98	12.445	3545	3547	3548	rBV	333	101	0.01%	0.001%
99	12.779	3649	3651	3654	rBV	371	182	0.01%	0.002%
100	13.728	3944	3946	3950	rBV4	863	820	0.06%	0.007%




Sum of corrected areas: 11719872

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029651.D
Acq On : 13 Dec 2022 15:14
Operator : SY/MD
Sample : VIBLK307
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK307

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

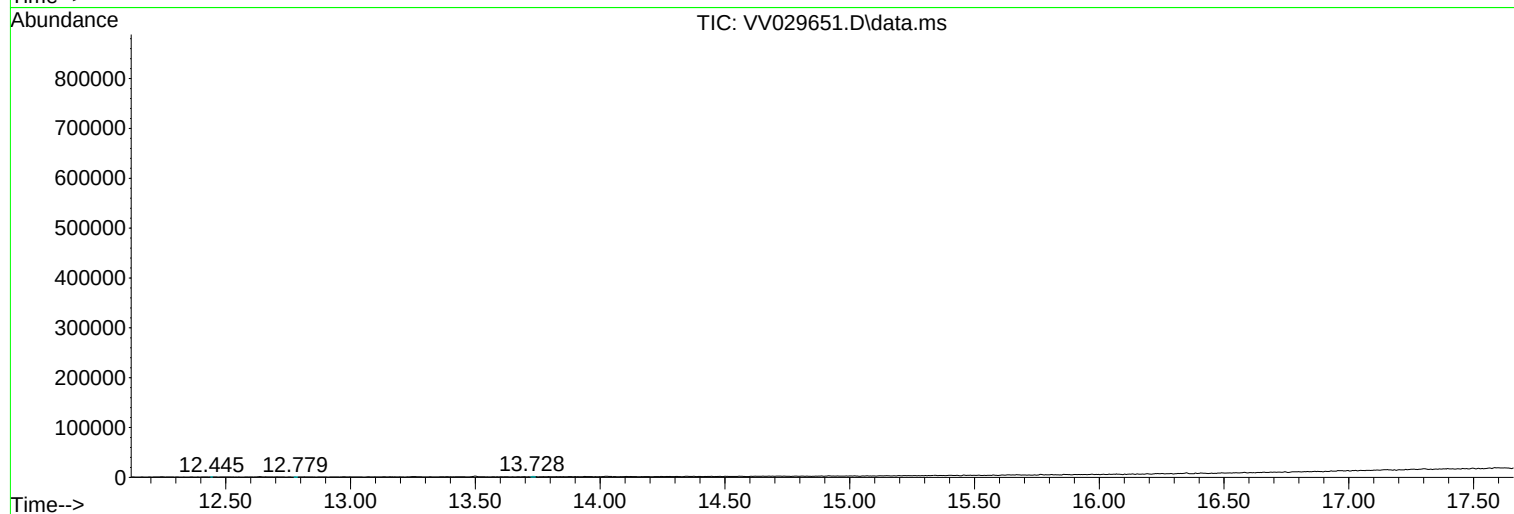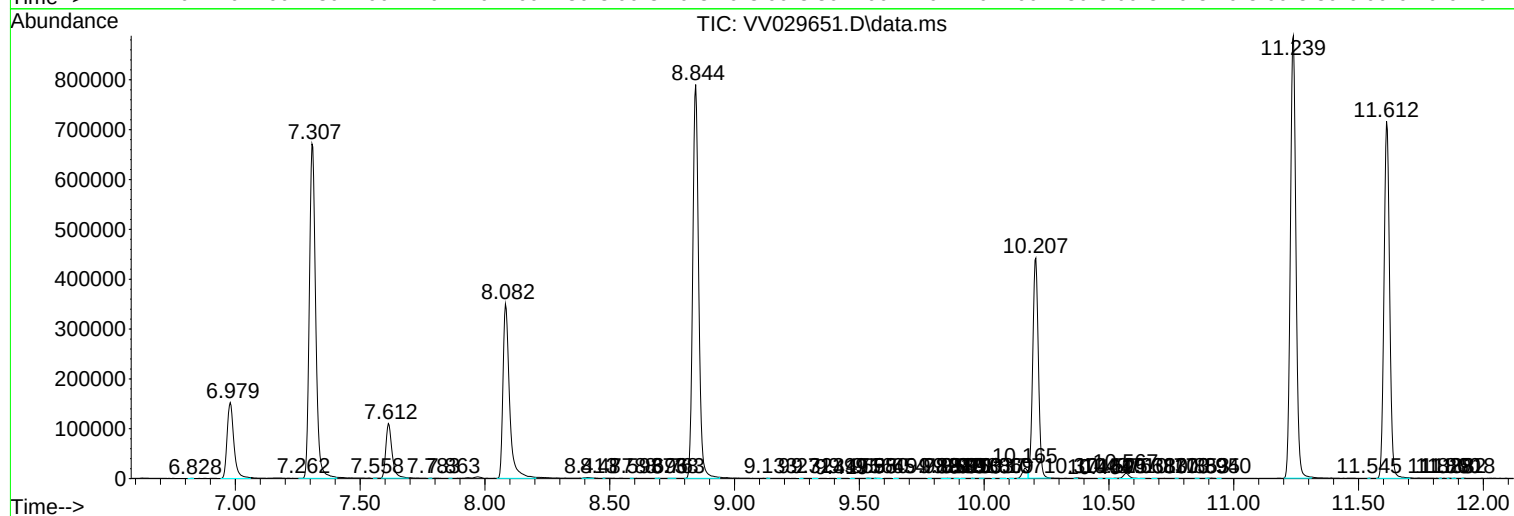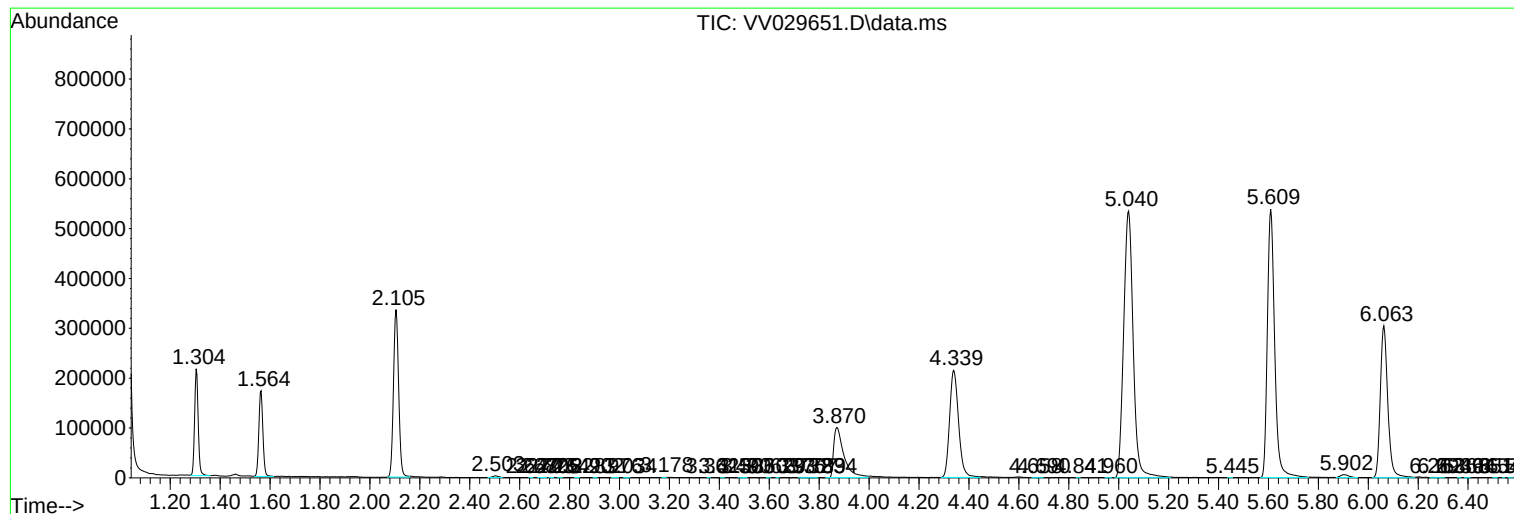

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029651.D
Acq On : 13 Dec 2022 15:14
Operator : SY/MD
Sample : VIBLK307
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK307

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029651.D
Acq On : 13 Dec 2022 15:14
Operator : SY/MD
Sample : VIBLK307
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK307

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc