

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029653.D
 Acq On : 13 Dec 2022 16:01
 Operator : SY/MD
 Sample : N5950-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rVB	210171	202869	14.85%	1.787%
2	1.561	154	162	176	rVB	166984	186206	13.63%	1.640%
3	2.105	320	331	342	rBV	325558	464054	33.98%	4.088%
4	2.159	342	348	361	rVB	23231	36925	2.70%	0.325%
5	2.420	426	429	433	rVB2	325	262	0.02%	0.002%
6	2.465	440	443	447	rVV3	267	208	0.02%	0.002%
7	2.507	447	456	469	rVV6	946	1615	0.12%	0.014%
8	2.635	490	496	503	rVV3	530	823	0.06%	0.007%
9	3.185	657	667	673	rBV2	1214	2070	0.15%	0.018%
10	3.323	706	710	715	rVB2	204	212	0.02%	0.002%
11	3.809	858	861	868	rBV3	214	223	0.02%	0.002%
12	3.873	871	881	918	rBV	96043	274172	20.07%	2.415%
13	4.262	999	1002	1009	rVB2	227	225	0.02%	0.002%
14	4.339	1009	1026	1057	rBV	210084	524615	38.41%	4.622%
15	4.577	1093	1100	1103	rBV4	563	682	0.05%	0.006%
16	4.600	1103	1107	1109	rBV3	372	303	0.02%	0.003%
17	4.764	1154	1158	1164	rBV2	205	239	0.02%	0.002%
18	4.934	1206	1211	1215	rBV2	282	374	0.03%	0.003%
19	5.040	1223	1244	1287	rBV2	518179	1365799	100.00%	12.032%
20	5.294	1320	1323	1328	rBV3	318	319	0.02%	0.003%
21	5.445	1367	1370	1372	rBV3	337	217	0.02%	0.002%
22	5.478	1377	1380	1382	rBV2	398	305	0.02%	0.003%
23	5.609	1407	1421	1469	rBV	510154	1046884	76.65%	9.223%
24	5.863	1495	1500	1502	rBV3	321	232	0.02%	0.002%
25	5.899	1502	1511	1513	rBV4	4161	5540	0.41%	0.049%
26	5.992	1537	1540	1547	rBV4	297	399	0.03%	0.004%
27	6.063	1547	1562	1597	rBV	290637	604162	44.24%	5.323%
28	6.523	1700	1705	1707	rBV2	310	224	0.02%	0.002%
29	6.619	1731	1735	1736	rBV	601	422	0.03%	0.004%
30	6.664	1748	1749	1753	rVB2	507	223	0.02%	0.002%
31	6.683	1753	1755	1758	rBV2	463	238	0.02%	0.002%
32	6.760	1774	1779	1782	rVB	308	262	0.02%	0.002%
33	6.876	1813	1815	1819	rVB2	320	217	0.02%	0.002%
34	6.912	1824	1826	1832	rVB	237	235	0.02%	0.002%
35	6.979	1834	1847	1878	rBV	144571	271822	19.90%	2.395%
36	7.124	1889	1892	1896	rBV3	620	477	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029653.D
 Acq On : 13 Dec 2022 16:01
 Operator : SY/MD
 Sample : N5950-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.166	1902	1905	1910	rVV2	594	581	0.04%	0.005%
38	7.201	1914	1916	1920	rVB4	515	279	0.02%	0.002%
39	7.307	1937	1949	1985	rBV	640998	1135054	83.11%	10.000%
40	7.613	2034	2044	2074	rVV	102635	183852	13.46%	1.620%
41	7.860	2119	2121	2125	rVB2	455	304	0.02%	0.003%
42	7.934	2130	2144	2151	rBV3	2684	5288	0.39%	0.047%
43	7.973	2151	2156	2160	rVV2	1514	1594	0.12%	0.014%
44	8.031	2171	2174	2179	rVB2	350	268	0.02%	0.002%
45	8.082	2179	2190	2225	rBV	349267	630411	46.16%	5.554%
46	8.381	2281	2283	2287	rVB3	479	283	0.02%	0.002%
47	8.426	2294	2297	2300	rBV3	341	218	0.02%	0.002%
48	8.510	2320	2323	2328	rVV3	515	438	0.03%	0.004%
49	8.622	2355	2358	2362	rVB3	285	211	0.02%	0.002%
50	8.680	2373	2376	2380	rVB3	355	267	0.02%	0.002%
51	8.786	2404	2409	2413	rVB3	391	383	0.03%	0.003%
52	8.844	2413	2427	2454	rBV	742459	1228642	89.96%	10.824%
53	9.137	2510	2518	2525	rVB3	1096	1607	0.12%	0.014%
54	9.169	2525	2528	2533	rVB3	267	280	0.02%	0.002%
55	9.201	2533	2538	2543	rBV2	282	257	0.02%	0.002%
56	9.230	2544	2547	2551	rBV4	482	388	0.03%	0.003%
57	9.259	2551	2556	2560	rVB2	293	247	0.02%	0.002%
58	9.342	2578	2582	2585	rVB3	335	232	0.02%	0.002%
59	9.542	2634	2644	2649	rBV4	960	1202	0.09%	0.011%
60	9.603	2659	2663	2665	rBV	283	217	0.02%	0.002%
61	9.754	2709	2710	2715	rVB	332	209	0.02%	0.002%
62	9.780	2715	2718	2723	rBV2	256	215	0.02%	0.002%
63	10.162	2828	2837	2841	rBV2	17841	26800	1.96%	0.236%
64	10.204	2841	2850	2869	rVB	422223	675330	49.45%	5.950%
65	10.371	2891	2902	2912	rVB3	4086	6641	0.49%	0.059%
66	10.439	2919	2923	2924	rBV2	392	279	0.02%	0.002%
67	10.526	2946	2950	2951	rBV	511	262	0.02%	0.002%
68	10.567	2955	2963	2975	rVV2	8268	13794	1.01%	0.122%
69	10.722	3007	3011	3013	rBV3	433	327	0.02%	0.003%
70	10.908	3062	3069	3077	rBV3	1894	2565	0.19%	0.023%
71	11.178	3148	3153	3157	rVB3	600	580	0.04%	0.005%
72	11.236	3159	3171	3195	rBV	840271	1307577	95.74%	11.519%
73	11.516	3254	3258	3260	rBV4	612	455	0.03%	0.004%
74	11.551	3260	3269	3277	rVV5	5415	10824	0.79%	0.095%
75	11.612	3277	3288	3316	rVB	691027	1096454	80.28%	9.660%
76	11.792	3341	3344	3346	rBV2	360	257	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029653.D
 Acq On : 13 Dec 2022 16:01
 Operator : SY/MD
 Sample : N5950-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.841	3356	3359	3362	rVV3	359	210	0.02%	0.002%
78	12.066	3425	3429	3434	rVB3	331	312	0.02%	0.003%
79	12.146	3450	3454	3458	rBV2	231	273	0.02%	0.002%
80	12.223	3474	3478	3479	rBV2	815	393	0.03%	0.003%
81	12.239	3480	3483	3491	rVV4	1228	1568	0.11%	0.014%
82	12.275	3492	3494	3498	rVB3	356	235	0.02%	0.002%
83	12.336	3506	3513	3522	rVB6	3333	4172	0.31%	0.037%
84	12.371	3522	3524	3528	rVB2	366	259	0.02%	0.002%
85	12.394	3528	3531	3535	rBV	435	317	0.02%	0.003%
86	12.474	3554	3556	3559	rVB	407	212	0.02%	0.002%
87	12.490	3559	3561	3565	rBV3	276	221	0.02%	0.002%
88	12.513	3565	3568	3570	rBV2	294	207	0.02%	0.002%
89	12.619	3596	3601	3603	rBV3	294	267	0.02%	0.002%
90	12.635	3603	3606	3609	rVV	508	378	0.03%	0.003%
91	12.712	3628	3630	3634	rVB2	407	264	0.02%	0.002%
92	12.908	3688	3691	3693	rBV	463	261	0.02%	0.002%
93	13.085	3739	3746	3749	rBV4	448	495	0.04%	0.004%
94	13.172	3771	3773	3776	rVB2	423	240	0.02%	0.002%
95	13.249	3792	3797	3801	rVB5	656	637	0.05%	0.006%
96	13.432	3850	3854	3855	rBV2	316	215	0.02%	0.002%
97	13.497	3866	3874	3888	rVB	5952	9564	0.70%	0.084%
98	13.564	3893	3895	3899	rVB	574	390	0.03%	0.003%
99	13.924	4004	4007	4009	rBV3	437	307	0.02%	0.003%
100	14.744	4259	4262	4264	rBV3	668	476	0.03%	0.004%


Sum of corrected areas: 11350999

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029653.D
Acq On : 13 Dec 2022 16:01
Operator : SY/MD
Sample : N5950-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

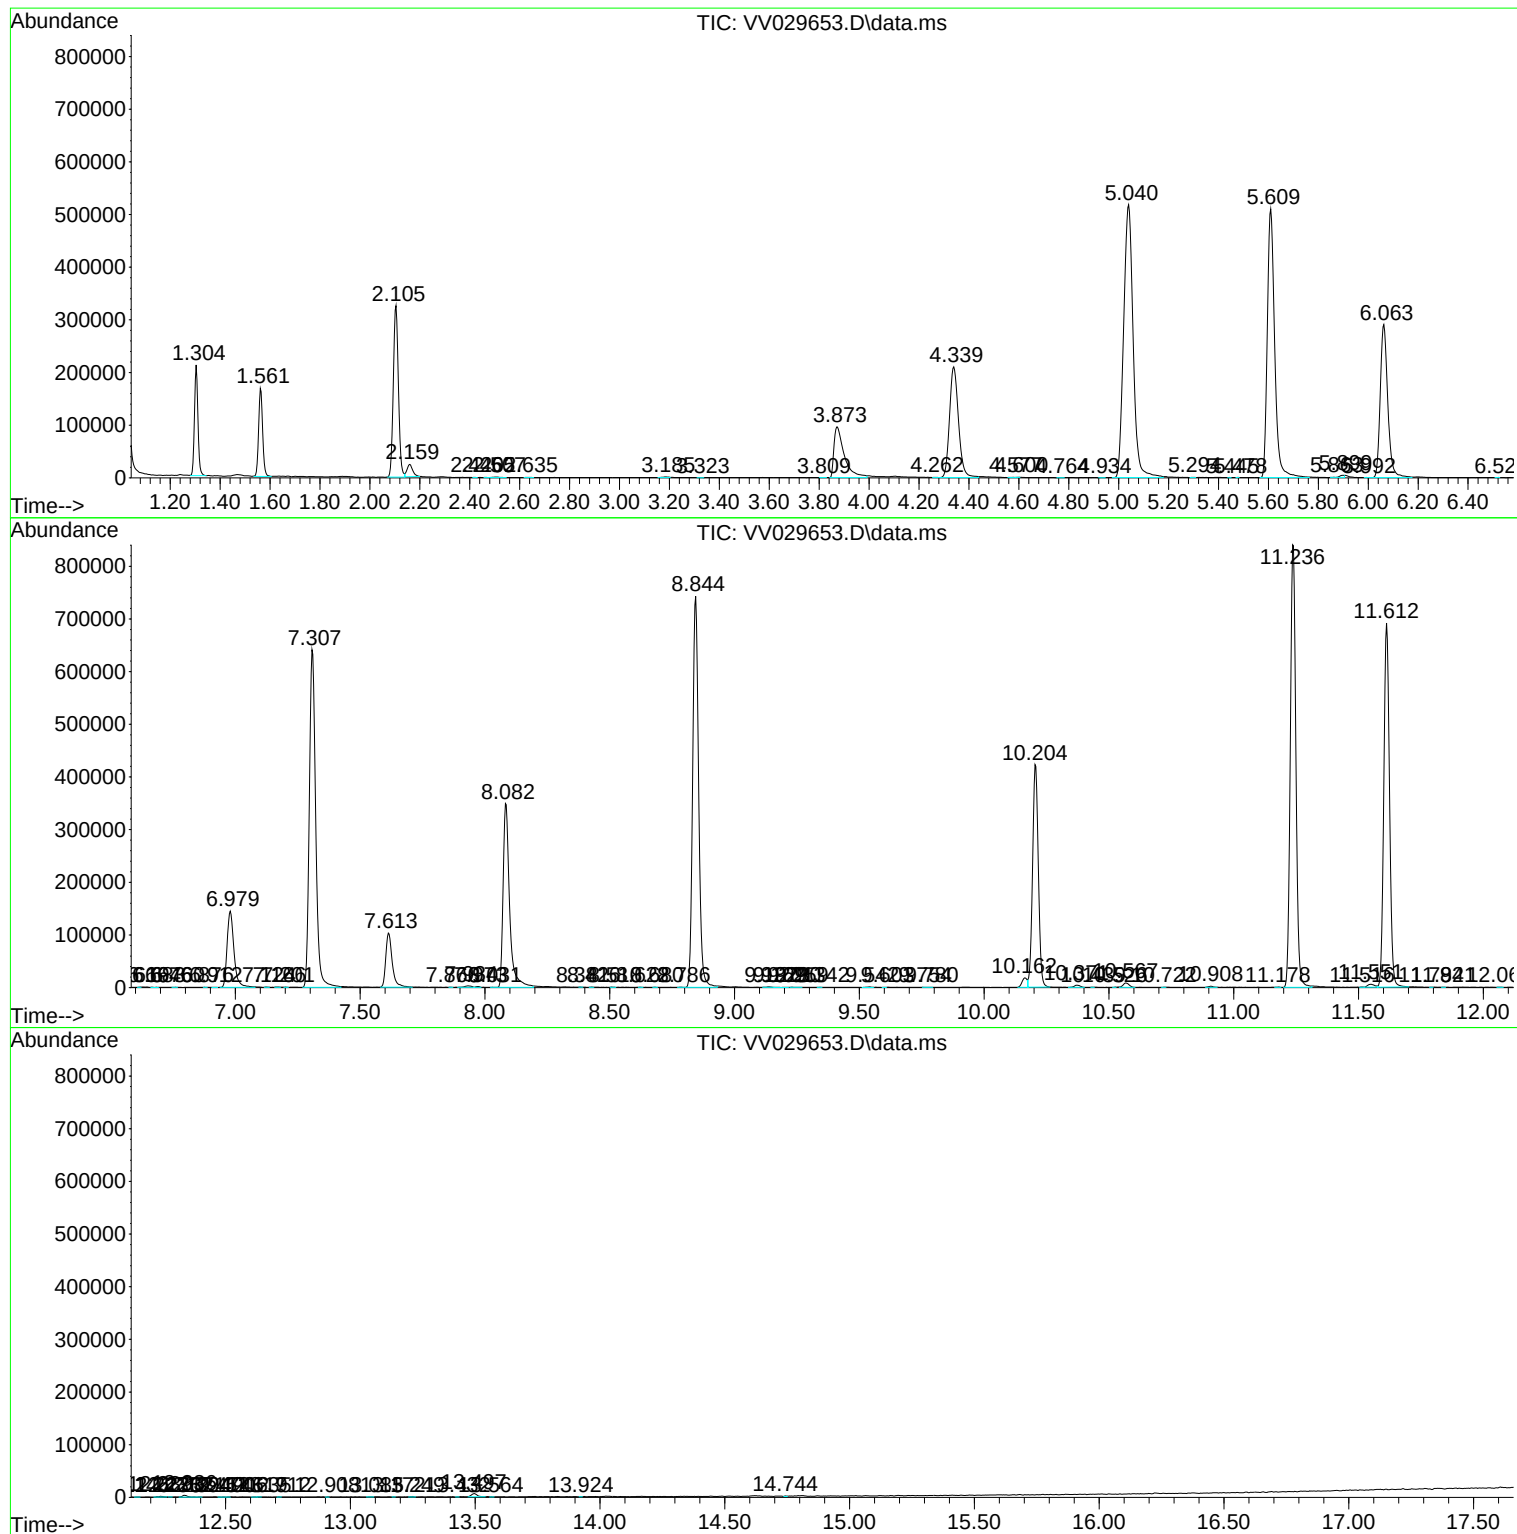

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029653.D
Acq On : 13 Dec 2022 16:01
Operator : SY/MD
Sample : N5950-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029653.D
Acq On : 13 Dec 2022 16:01
Operator : SY/MD
Sample : N5950-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF56

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc