

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029654.D
 Acq On : 13 Dec 2022 16:24
 Operator : SY/MD
 Sample : N5950-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029654.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	206262	203268	14.11%	1.687%
2	1.565	155	163	179	rVB	166969	191494	13.29%	1.589%
3	2.105	320	331	341	rBV	334865	478989	33.24%	3.975%
4	2.368	411	413	417	rVB	295	148	0.01%	0.001%
5	2.500	449	454	464	rVB4	1371	2063	0.14%	0.017%
6	2.587	479	481	484	rBV2	238	160	0.01%	0.001%
7	2.609	486	488	489	rBB2	140	121	0.01%	0.001%
8	2.764	534	536	542	rBV2	355	235	0.02%	0.002%
9	2.818	550	553	557	rVB3	312	240	0.02%	0.002%
10	2.860	562	566	568	rBV2	194	167	0.01%	0.001%
11	2.915	580	583	585	rBV	318	246	0.02%	0.002%
12	3.040	619	622	624	rBV	196	147	0.01%	0.001%
13	3.089	633	637	639	rBV2	240	171	0.01%	0.001%
14	3.146	651	655	656	rBV	290	174	0.01%	0.001%
15	3.191	661	669	672	rVV3	338	442	0.03%	0.004%
16	3.269	690	693	696	rVB2	184	112	0.01%	0.001%
17	3.326	707	711	714	rBV	213	192	0.01%	0.002%
18	3.372	722	725	730	rVB3	367	342	0.02%	0.003%
19	3.407	730	736	739	rBV2	263	200	0.01%	0.002%
20	3.545	776	779	783	rBV2	137	115	0.01%	0.001%
21	3.712	829	831	833	rVB2	229	100	0.01%	0.001%
22	3.770	847	849	855	rVB2	320	211	0.01%	0.002%
23	3.870	870	880	922	rBV	110214	302654	21.00%	2.511%
24	4.339	1009	1026	1051	rBV	222436	554000	38.45%	4.597%
25	4.571	1096	1098	1100	rBV2	268	174	0.01%	0.001%
26	4.651	1119	1123	1127	rVB2	299	246	0.02%	0.002%
27	4.680	1127	1132	1134	rBV	303	249	0.02%	0.002%
28	4.696	1134	1137	1140	rVB2	326	147	0.01%	0.001%
29	4.822	1174	1176	1183	rVB	203	153	0.01%	0.001%
30	4.860	1183	1188	1189	rBV2	253	154	0.01%	0.001%
31	4.896	1195	1199	1201	rBV2	192	166	0.01%	0.001%
32	4.915	1203	1205	1210	rBV3	366	250	0.02%	0.002%
33	5.040	1226	1244	1294	rVV2	541840	1440991	100.00%	11.958%
34	5.471	1373	1378	1381	rBV3	324	391	0.03%	0.003%
35	5.609	1407	1421	1458	rBV	564812	1143469	79.35%	9.489%
36	5.902	1502	1512	1527	rVB6	5040	10738	0.75%	0.089%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029654.D
 Acq On : 13 Dec 2022 16:24
 Operator : SY/MD
 Sample : N5950-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.063	1548	1562	1591	rBV	309251	642085	44.56%	5.328%
38	6.294	1630	1634	1636	rVB2	241	171	0.01%	0.001%
39	6.384	1659	1662	1665	rBV3	226	172	0.01%	0.001%
40	6.458	1682	1685	1688	rBV2	164	108	0.01%	0.001%
41	6.577	1719	1722	1724	rBV2	334	209	0.01%	0.002%
42	6.625	1730	1737	1743	rBV3	737	1262	0.09%	0.010%
43	6.683	1753	1755	1758	rVB3	281	135	0.01%	0.001%
44	6.715	1761	1765	1767	rBV	274	145	0.01%	0.001%
45	6.764	1777	1780	1785	rVB2	199	141	0.01%	0.001%
46	6.847	1804	1806	1808	rVB	311	126	0.01%	0.001%
47	6.928	1829	1831	1835	rBV3	287	189	0.01%	0.002%
48	6.979	1835	1847	1870	rBV	150542	280576	19.47%	2.328%
49	7.182	1907	1910	1911	rBV2	501	251	0.02%	0.002%
50	7.307	1936	1949	1977	rBV	668724	1184087	82.17%	9.826%
51	7.612	2034	2044	2072	rBV	108153	192034	13.33%	1.594%
52	7.934	2137	2144	2151	rBV4	1984	3119	0.22%	0.026%
53	8.082	2179	2190	2227	rBV	378952	685108	47.54%	5.685%
54	8.481	2311	2314	2315	rBV2	510	281	0.02%	0.002%
55	8.510	2320	2323	2326	rVV2	481	317	0.02%	0.003%
56	8.609	2350	2354	2355	rBV	419	220	0.02%	0.002%
57	8.638	2360	2363	2367	rVV3	418	318	0.02%	0.003%
58	8.680	2371	2376	2379	rBV3	197	223	0.02%	0.002%
59	8.747	2394	2397	2399	rVV	228	102	0.01%	0.001%
60	8.789	2406	2410	2412	rBB2	218	148	0.01%	0.001%
61	8.844	2412	2427	2459	rBV	813099	1356070	94.11%	11.253%
62	9.172	2526	2529	2535	rBV2	202	127	0.01%	0.001%
63	9.210	2539	2541	2546	rVB2	398	227	0.02%	0.002%
64	9.326	2573	2577	2581	rVV2	203	227	0.02%	0.002%
65	9.455	2615	2617	2623	rVB2	371	244	0.02%	0.002%
66	9.497	2623	2630	2634	rBV	269	290	0.02%	0.002%
67	9.545	2638	2645	2650	rVB2	977	747	0.05%	0.006%
68	9.571	2650	2653	2658	rBV2	459	372	0.03%	0.003%
69	9.632	2668	2672	2673	rBV	155	111	0.01%	0.001%
70	9.709	2692	2696	2699	rVB2	421	282	0.02%	0.002%
71	9.821	2729	2731	2735	rVB	372	201	0.01%	0.002%
72	9.844	2735	2738	2740	rBV	228	129	0.01%	0.001%
73	9.924	2757	2763	2766	rBV3	534	543	0.04%	0.005%
74	10.008	2785	2789	2792	rVB	232	167	0.01%	0.001%
75	10.027	2792	2795	2799	rBV2	242	224	0.02%	0.002%
76	10.162	2827	2837	2841	rBV2	22147	32334	2.24%	0.268%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029654.D
 Acq On : 13 Dec 2022 16:24
 Operator : SY/MD
 Sample : N5950-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EYF52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.207	2842	2851	2877	rVB	457782	728052	50.52%	6.041%
78	10.339	2890	2892	2893	rBV	291	141	0.01%	0.001%
79	10.371	2896	2902	2912	rVB4	2613	4025	0.28%	0.033%
80	10.532	2947	2952	2954	rBV2	545	415	0.03%	0.003%
81	10.567	2954	2963	2974	rVV	10025	16567	1.15%	0.137%
82	10.651	2987	2989	2993	rBV	184	98	0.01%	0.001%
83	10.712	3003	3008	3009	rBV	259	161	0.01%	0.001%
84	10.751	3019	3020	3026	rBV2	194	106	0.01%	0.001%
85	10.792	3031	3033	3035	rBV	183	97	0.01%	0.001%
86	10.879	3058	3060	3062	rBV	327	159	0.01%	0.001%
87	10.911	3062	3070	3076	rVV4	892	1374	0.10%	0.011%
88	10.953	3079	3083	3089	rBV2	175	207	0.01%	0.002%
89	11.001	3096	3098	3099	rBV2	211	99	0.01%	0.001%
90	11.178	3148	3153	3156	rBV3	671	512	0.04%	0.004%
91	11.236	3159	3171	3204	rBV	929739	1425078	98.90%	11.826%
92	11.551	3262	3269	3276	rBV4	4545	7276	0.50%	0.060%
93	11.612	3277	3288	3316	rVB	719965	1139494	79.08%	9.456%
94	12.101	3437	3440	3444	rBV3	353	311	0.02%	0.003%
95	12.230	3470	3480	3484	rBV4	989	1627	0.11%	0.014%
96	12.336	3507	3513	3521	rVV6	3889	5235	0.36%	0.043%
97	12.378	3524	3526	3528	rBV	341	141	0.01%	0.001%
98	12.442	3544	3546	3550	rBV2	335	193	0.01%	0.002%
99	12.625	3601	3603	3605	rBV	598	359	0.02%	0.003%
100	13.496	3869	3874	3876	rBV4	2194	2182	0.15%	0.018%




Sum of corrected areas: 12050850

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029654.D
Acq On : 13 Dec 2022 16:24
Operator : SY/MD
Sample : N5950-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

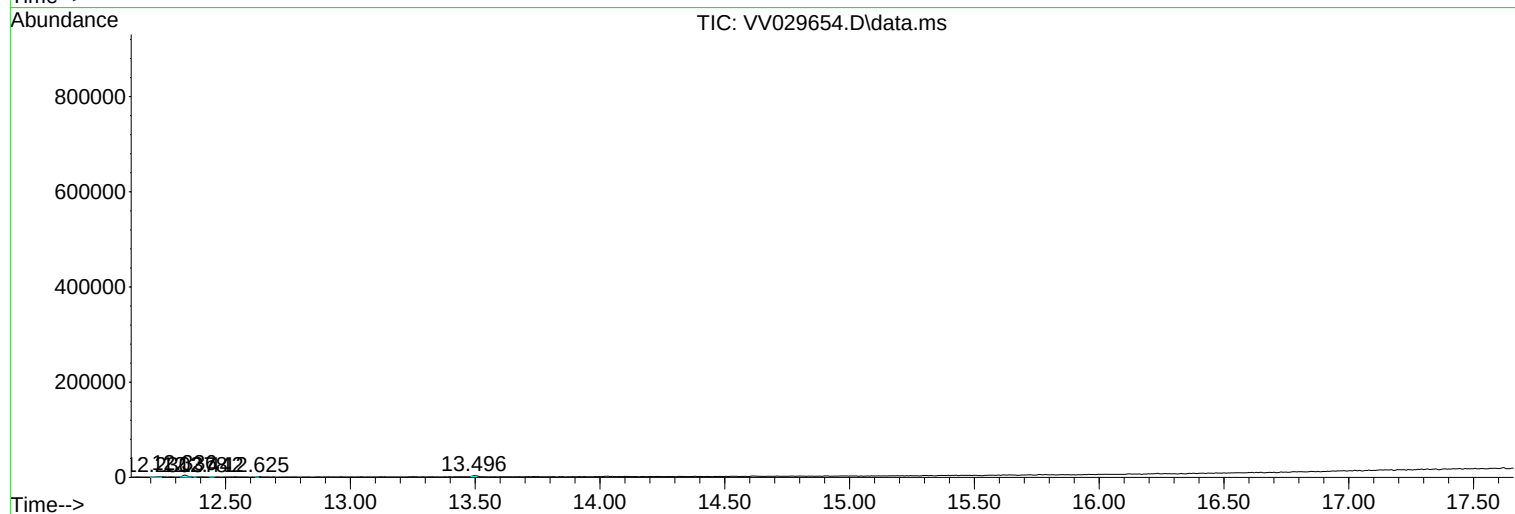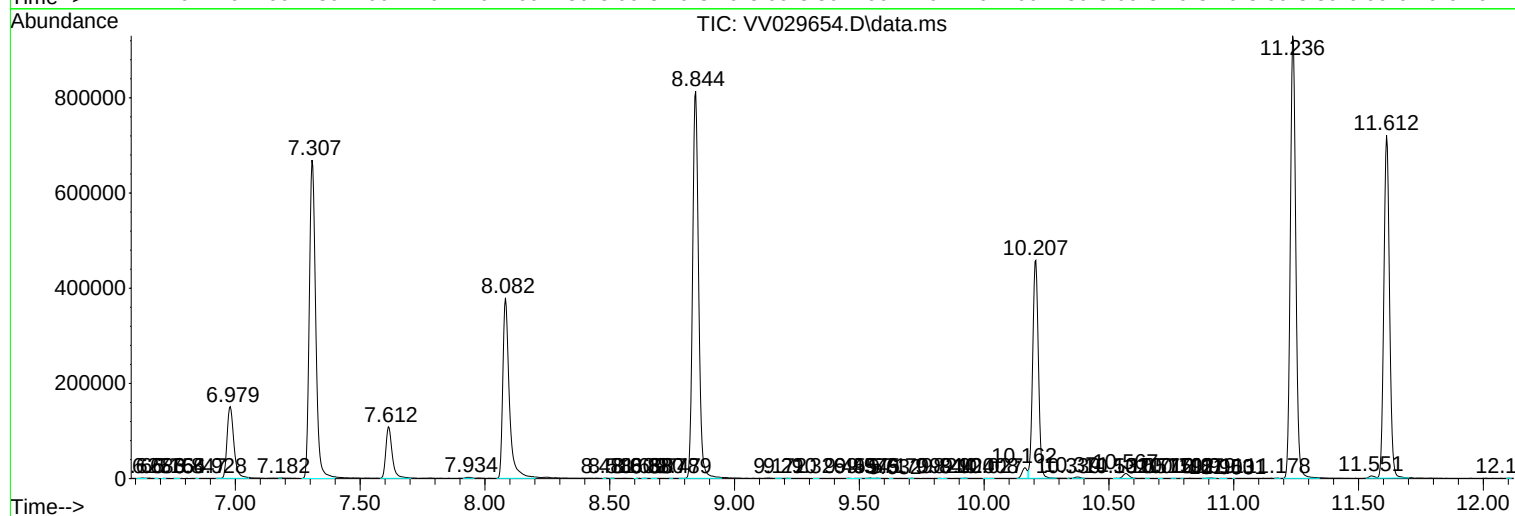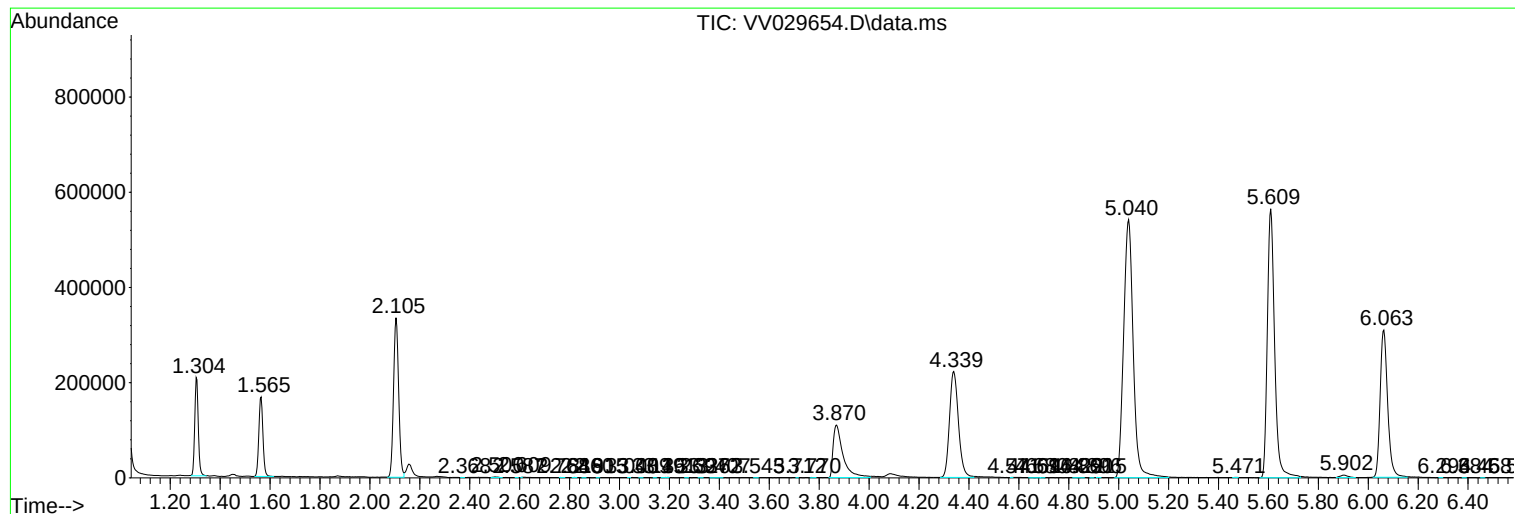

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029654.D
Acq On : 13 Dec 2022 16:24
Operator : SY/MD
Sample : N5950-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029654.D
Acq On : 13 Dec 2022 16:24
Operator : SY/MD
Sample : N5950-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EYF52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------