

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029655.D
 Acq On : 13 Dec 2022 16:48
 Operator : SY/MD
 Sample : N5981-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ES8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rVB	206075	205152	14.21%	1.687%
2	1.564	155	163	174	rVB	170123	189497	13.12%	1.558%
3	1.886	254	263	275	rBV3	5243	9696	0.67%	0.080%
4	1.973	288	290	297	rVB5	766	647	0.04%	0.005%
5	2.044	310	312	313	rBV	481	231	0.02%	0.002%
6	2.105	320	331	343	rBV2	341574	498128	34.50%	4.097%
7	2.233	370	371	374	rVB2	744	377	0.03%	0.003%
8	2.275	374	384	405	rVB	19645	39271	2.72%	0.323%
9	2.503	449	455	461	rVB3	1384	1929	0.13%	0.016%
10	2.619	487	491	493	rBV3	330	286	0.02%	0.002%
11	2.896	573	577	581	rBV2	322	318	0.02%	0.003%
12	3.146	649	655	660	rBV2	149	206	0.01%	0.002%
13	3.185	660	667	668	rBV2	555	601	0.04%	0.005%
14	3.703	824	828	832	rVB3	271	245	0.02%	0.002%
15	3.825	858	866	870	rBV2	324	500	0.03%	0.004%
16	3.870	870	880	923	rBV	109304	314586	21.79%	2.587%
17	4.339	1008	1026	1053	rBV	225075	564524	39.10%	4.643%
18	4.600	1100	1107	1109	rBV4	886	1055	0.07%	0.009%
19	4.645	1118	1121	1124	rVB	381	239	0.02%	0.002%
20	4.770	1155	1160	1163	rBV2	324	319	0.02%	0.003%
21	5.040	1226	1244	1282	rBV2	550153	1443821	100.00%	11.874%
22	5.384	1349	1351	1355	rVV2	373	325	0.02%	0.003%
23	5.471	1372	1378	1382	rBV3	312	330	0.02%	0.003%
24	5.609	1405	1421	1462	rBV	548475	1131506	78.37%	9.306%
25	5.905	1502	1513	1525	rBV8	4339	9229	0.64%	0.076%
26	6.008	1539	1545	1548	rBV2	180	200	0.01%	0.002%
27	6.063	1548	1562	1599	rBV	313449	649362	44.98%	5.341%
28	6.191	1600	1602	1603	rBV	541	247	0.02%	0.002%
29	6.252	1619	1621	1628	rVB3	462	325	0.02%	0.003%
30	6.349	1649	1651	1658	rBV	224	210	0.01%	0.002%
31	6.436	1674	1678	1681	rBV2	369	212	0.01%	0.002%
32	6.577	1718	1722	1726	rVB2	311	256	0.02%	0.002%
33	6.629	1735	1738	1741	rVB3	466	289	0.02%	0.002%
34	6.828	1794	1800	1804	rBV2	246	284	0.02%	0.002%
35	6.908	1822	1825	1829	rVB2	278	234	0.02%	0.002%
36	6.979	1833	1847	1881	rBV	154857	287140	19.89%	2.362%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029655.D
 Acq On : 13 Dec 2022 16:48
 Operator : SY/MD
 Sample : N5981-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ES8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.166	1901	1905	1907	rBV2	378	274	0.02%	0.002%
38	7.188	1907	1912	1914	rVV3	740	598	0.04%	0.005%
39	7.240	1924	1928	1930	rBV4	431	313	0.02%	0.003%
40	7.307	1936	1949	1979	rBV	676611	1192936	82.62%	9.811%
41	7.612	2033	2044	2072	rBV	108408	195165	13.52%	1.605%
42	7.783	2093	2097	2099	rVB3	404	313	0.02%	0.003%
43	7.831	2110	2112	2115	rVV2	496	268	0.02%	0.002%
44	7.873	2122	2125	2132	rVB4	480	486	0.03%	0.004%
45	7.934	2132	2144	2151	rBV3	1908	3500	0.24%	0.029%
46	7.973	2153	2156	2163	rVB4	1017	986	0.07%	0.008%
47	8.008	2163	2167	2174	rVB3	426	548	0.04%	0.005%
48	8.040	2174	2177	2180	rBV2	314	299	0.02%	0.002%
49	8.082	2180	2190	2228	rBV	388514	705015	48.83%	5.798%
50	8.397	2284	2288	2292	rVB3	476	427	0.03%	0.004%
51	8.426	2293	2297	2301	rBV3	340	355	0.02%	0.003%
52	8.490	2315	2317	2323	rVB4	556	520	0.04%	0.004%
53	8.522	2323	2327	2330	rVB3	408	273	0.02%	0.002%
54	8.567	2340	2341	2345	rBV	273	216	0.01%	0.002%
55	8.677	2371	2375	2378	rBV	337	230	0.02%	0.002%
56	8.767	2397	2403	2406	rVB2	336	275	0.02%	0.002%
57	8.844	2414	2427	2456	rBV	805048	1336485	92.57%	10.992%
58	9.050	2487	2491	2492	rBV2	339	224	0.02%	0.002%
59	9.140	2515	2519	2524	rVV3	523	490	0.03%	0.004%
60	9.230	2543	2547	2551	rBV3	277	223	0.02%	0.002%
61	9.326	2573	2577	2580	rVV2	294	295	0.02%	0.002%
62	9.535	2638	2642	2646	rBV4	475	435	0.03%	0.004%
63	9.892	2749	2753	2758	rBV2	350	339	0.02%	0.003%
64	9.931	2758	2765	2770	rVB4	644	921	0.06%	0.008%
65	10.162	2827	2837	2841	rBV2	21185	31532	2.18%	0.259%
66	10.204	2841	2850	2876	rVB	470405	742136	51.40%	6.104%
67	10.326	2885	2888	2892	rVB2	528	232	0.02%	0.002%
68	10.349	2892	2895	2896	rVV	408	219	0.02%	0.002%
69	10.371	2896	2902	2912	rVB3	2682	3989	0.28%	0.033%
70	10.535	2950	2953	2954	rVV2	385	219	0.02%	0.002%
71	10.571	2954	2964	2977	rVV2	9856	16555	1.15%	0.136%
72	10.735	3010	3015	3018	rBV3	406	362	0.03%	0.003%
73	10.908	3065	3069	3074	rVB2	860	881	0.06%	0.007%
74	10.966	3083	3087	3091	rVB3	245	235	0.02%	0.002%
75	11.136	3135	3140	3142	rBV3	249	211	0.01%	0.002%
76	11.169	3147	3150	3153	rBV3	325	262	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029655.D
 Acq On : 13 Dec 2022 16:48
 Operator : SY/MD
 Sample : N5981-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ES8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.236	3159	3171	3197	rBV	914557	1402775	97.16%	11.537%
78	11.435	3230	3233	3235	rVB4	503	270	0.02%	0.002%
79	11.561	3261	3272	3276	rBV7	2005	3159	0.22%	0.026%
80	11.612	3276	3288	3312	rVV	738685	1153317	79.88%	9.485%
81	11.757	3331	3333	3338	rVB2	749	407	0.03%	0.003%
82	11.821	3351	3353	3357	rVB2	366	266	0.02%	0.002%
83	11.873	3367	3369	3373	rBV	297	220	0.02%	0.002%
84	12.236	3477	3482	3489	rVB4	619	748	0.05%	0.006%
85	12.394	3529	3531	3534	rBV	368	224	0.02%	0.002%
86	12.513	3564	3568	3571	rVB2	332	230	0.02%	0.002%
87	12.545	3574	3578	3581	rBV2	319	316	0.02%	0.003%
88	12.638	3602	3607	3612	rVB4	792	796	0.06%	0.007%
89	12.709	3626	3629	3634	rVB2	286	202	0.01%	0.002%
90	12.927	3695	3697	3701	rVB4	327	226	0.02%	0.002%
91	13.098	3748	3750	3754	rBV2	390	240	0.02%	0.002%
92	13.210	3778	3785	3788	rBV3	555	597	0.04%	0.005%
93	13.230	3788	3791	3793	rBV2	412	288	0.02%	0.002%
94	13.429	3850	3853	3855	rBV	581	397	0.03%	0.003%
95	13.500	3872	3875	3884	rVB4	1843	1486	0.10%	0.012%
96	13.664	3924	3926	3929	rBV2	319	214	0.01%	0.002%
97	13.754	3951	3954	3956	rBV2	388	273	0.02%	0.002%
98	13.908	4000	4002	4006	rBV3	410	226	0.02%	0.002%
99	14.175	4080	4085	4087	rBV3	736	570	0.04%	0.005%
100	14.368	4143	4145	4150	rBV3	584	549	0.04%	0.005%




Sum of corrected areas: 12159015

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029655.D
Acq On : 13 Dec 2022 16:48
Operator : SY/MD
Sample : N5981-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ES8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

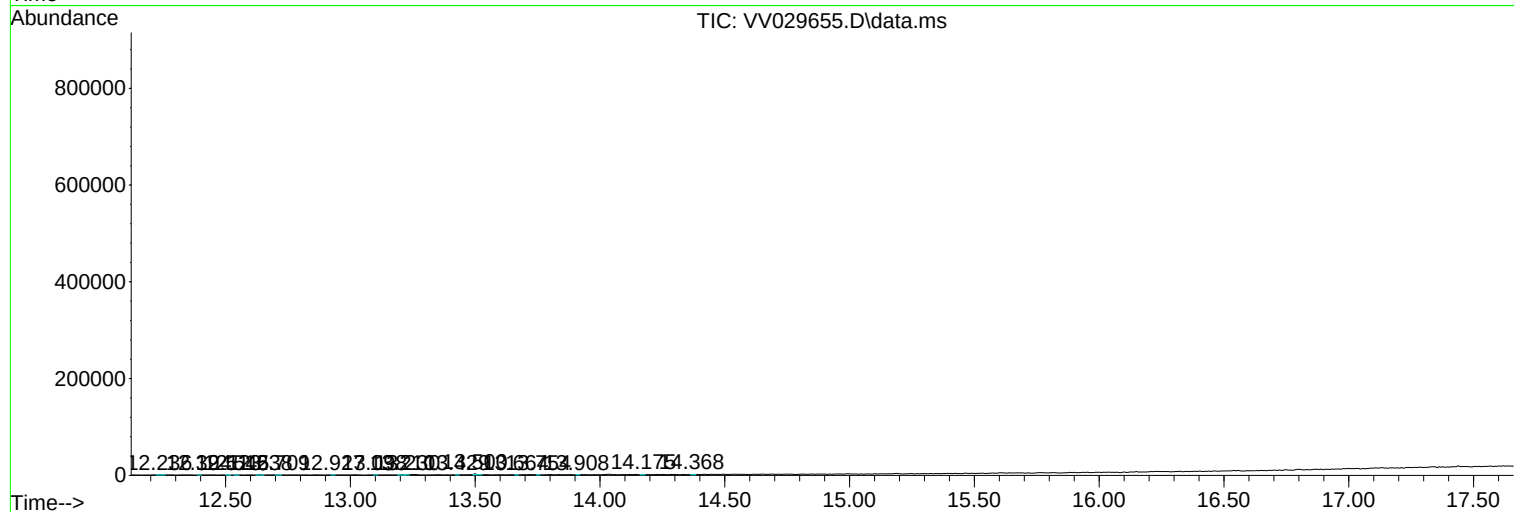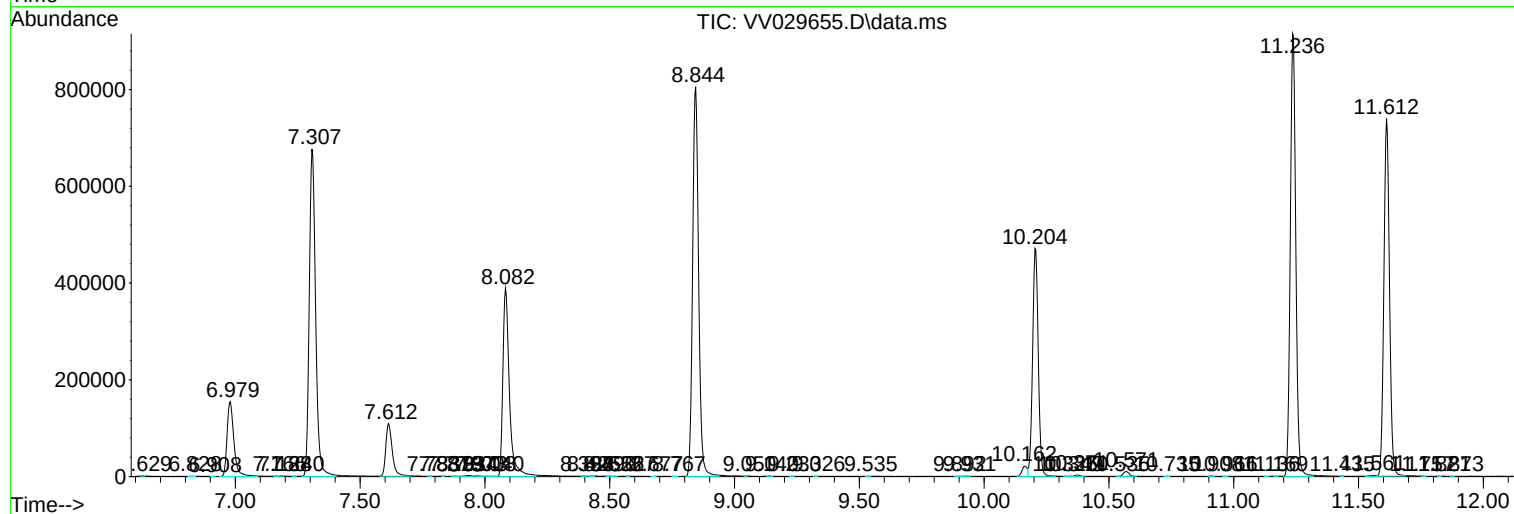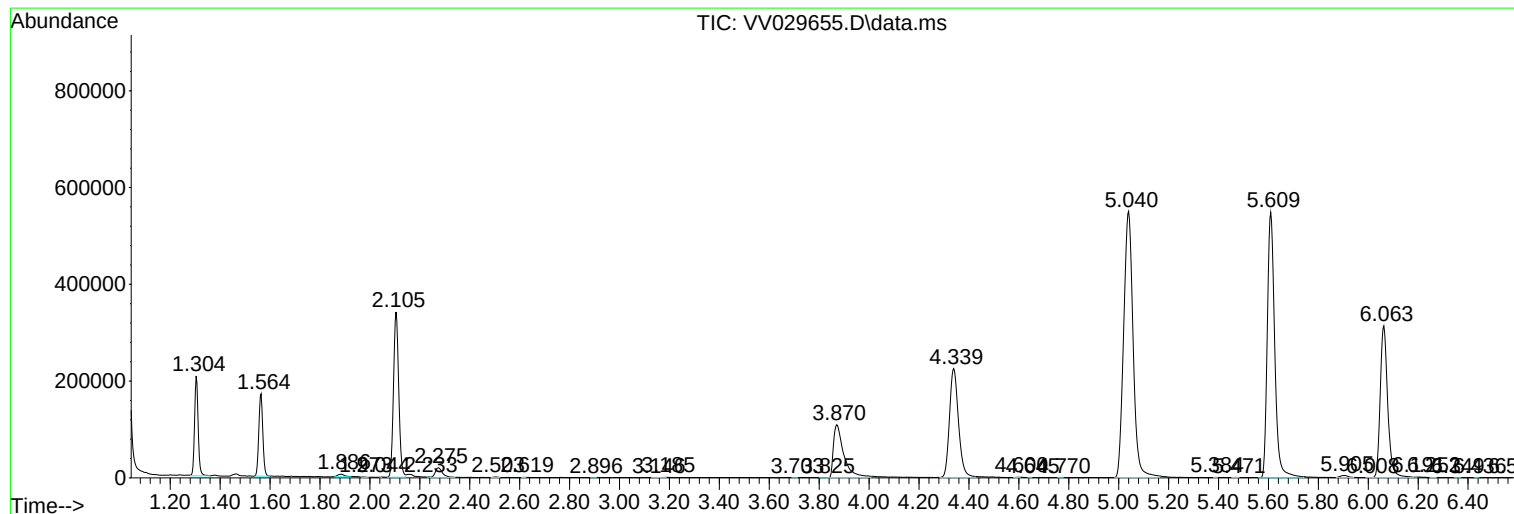

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029655.D
Acq On : 13 Dec 2022 16:48
Operator : SY/MD
Sample : N5981-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ES8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029655.D
Acq On : 13 Dec 2022 16:48
Operator : SY/MD
Sample : N5981-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ES8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------