

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029657.D
 Acq On : 13 Dec 2022 17:35
 Operator : SY/MD
 Sample : N5981-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ET1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	182947	181246	14.53%	1.762%
2	1.564	156	163	176	rVB	153529	170778	13.69%	1.660%
3	2.104	320	331	346	rBV	289506	417307	33.46%	4.056%
4	2.510	449	457	462	rBV5	1267	1707	0.14%	0.017%
5	2.551	469	470	473	rVB2	332	118	0.01%	0.001%
6	2.693	512	514	516	rBV	324	110	0.01%	0.001%
7	2.767	533	537	538	rBV2	253	133	0.01%	0.001%
8	2.821	551	554	556	rBV2	185	126	0.01%	0.001%
9	2.857	561	565	570	rBV2	187	223	0.02%	0.002%
10	2.960	595	597	601	rVB	341	187	0.01%	0.002%
11	2.982	601	604	606	rBV2	176	88	0.01%	0.001%
12	3.034	617	620	625	rBV2	217	209	0.02%	0.002%
13	3.175	655	664	668	rBV3	408	601	0.05%	0.006%
14	3.249	684	687	694	rVB2	222	228	0.02%	0.002%
15	3.349	716	718	722	rBV2	108	83	0.01%	0.001%
16	3.378	723	727	733	rVV2	233	210	0.02%	0.002%
17	3.584	788	791	794	rBV	188	131	0.01%	0.001%
18	3.751	837	843	846	rVB2	231	246	0.02%	0.002%
19	3.776	846	851	854	rBV2	153	126	0.01%	0.001%
20	3.799	854	858	860	rBV	180	120	0.01%	0.001%
21	3.876	872	882	923	rBV	86707	254675	20.42%	2.475%
22	4.339	1011	1026	1053	rBV	192655	478211	38.34%	4.648%
23	4.587	1101	1103	1106	rBV2	165	89	0.01%	0.001%
24	4.603	1106	1108	1113	rVB3	496	315	0.03%	0.003%
25	4.664	1123	1127	1131	rBV2	196	126	0.01%	0.001%
26	4.683	1131	1133	1135	rBV2	124	77	0.01%	0.001%
27	4.757	1154	1156	1162	rVB	283	196	0.02%	0.002%
28	4.796	1165	1168	1170	rBV	113	76	0.01%	0.001%
29	4.854	1181	1186	1187	rBV	245	185	0.01%	0.002%
30	4.892	1196	1198	1200	rBV2	166	70	0.01%	0.001%
31	4.905	1200	1202	1205	rVB	107	57	0.00%	0.001%
32	5.040	1226	1244	1282	rBV2	473326	1247247	100.00%	12.122%
33	5.391	1350	1353	1356	rBV	337	311	0.02%	0.003%
34	5.471	1375	1378	1381	rBV3	223	235	0.02%	0.002%
35	5.558	1402	1405	1408	rBV2	195	141	0.01%	0.001%
36	5.609	1408	1421	1452	rBV	459871	940002	75.37%	9.136%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029657.D
 Acq On : 13 Dec 2022 17:35
 Operator : SY/MD
 Sample : N5981-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ET1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.905	1502	1513	1528	rBV8	4221	9798	0.79%	0.095%
38	5.985	1536	1538	1541	rVB	209	131	0.01%	0.001%
39	6.063	1546	1562	1598	rBV	267643	558758	44.80%	5.431%
40	6.320	1635	1642	1644	rBV2	185	234	0.02%	0.002%
41	6.358	1649	1654	1659	rVB2	374	253	0.02%	0.002%
42	6.394	1659	1665	1668	rBV	171	188	0.02%	0.002%
43	6.468	1685	1688	1689	rBV2	103	61	0.00%	0.001%
44	6.551	1709	1714	1717	rBV2	270	183	0.01%	0.002%
45	6.625	1728	1737	1739	rBV3	604	715	0.06%	0.007%
46	6.718	1764	1766	1769	rBV2	186	67	0.01%	0.001%
47	6.738	1769	1772	1775	rVB	184	108	0.01%	0.001%
48	6.805	1791	1793	1796	rBV	163	139	0.01%	0.001%
49	6.844	1800	1805	1810	rVB3	317	300	0.02%	0.003%
50	6.886	1814	1818	1821	rBV2	300	196	0.02%	0.002%
51	6.979	1835	1847	1872	rBV2	133290	247037	19.81%	2.401%
52	7.156	1900	1902	1906	rBV4	459	305	0.02%	0.003%
53	7.307	1937	1949	1982	rBV	571152	1029875	82.57%	10.009%
54	7.612	2030	2044	2069	rBV	94956	171974	13.79%	1.671%
55	7.763	2090	2091	2094	rBV	353	216	0.02%	0.002%
56	7.879	2123	2127	2128	rBV	214	156	0.01%	0.002%
57	8.021	2167	2171	2173	rBV	309	254	0.02%	0.002%
58	8.085	2180	2191	2219	rBV	325919	594478	47.66%	5.778%
59	8.603	2350	2352	2356	rVB4	414	283	0.02%	0.003%
60	8.622	2356	2358	2359	rBV	151	57	0.00%	0.001%
61	8.644	2362	2365	2366	rBV	255	132	0.01%	0.001%
62	8.728	2385	2391	2393	rBV	244	246	0.02%	0.002%
63	8.744	2394	2396	2400	rVB	417	213	0.02%	0.002%
64	8.770	2400	2404	2408	rBV2	277	201	0.02%	0.002%
65	8.789	2408	2410	2414	rVB2	232	141	0.01%	0.001%
66	8.844	2414	2427	2457	rBV	696631	1127450	90.40%	10.958%
67	9.214	2538	2542	2546	rVB4	382	286	0.02%	0.003%
68	9.236	2547	2549	2552	rVB3	207	109	0.01%	0.001%
69	9.259	2552	2556	2557	rBV	103	68	0.01%	0.001%
70	9.326	2574	2577	2580	rVB2	217	136	0.01%	0.001%
71	9.358	2585	2587	2592	rVB2	202	113	0.01%	0.001%
72	9.394	2592	2598	2604	rBV2	215	302	0.02%	0.003%
73	9.596	2658	2661	2664	rBV	238	198	0.02%	0.002%
74	9.898	2753	2755	2757	rBV	140	71	0.01%	0.001%
75	9.947	2767	2770	2773	rVB2	179	109	0.01%	0.001%
76	10.040	2796	2799	2801	rBV	157	115	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029657.D
 Acq On : 13 Dec 2022 17:35
 Operator : SY/MD
 Sample : N5981-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ET1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.056	2802	2804	2806	rVV	186	64	0.01%	0.001%
78	10.162	2826	2837	2841	rBV	17453	25143	2.02%	0.244%
79	10.207	2842	2851	2869	rVB	396158	627831	50.34%	6.102%
80	10.567	2956	2963	2976	rVB3	7344	12209	0.98%	0.119%
81	10.670	2992	2995	2996	rBV	207	105	0.01%	0.001%
82	10.725	3010	3012	3013	rBV	155	71	0.01%	0.001%
83	10.757	3019	3022	3026	rVB2	243	139	0.01%	0.001%
84	10.779	3026	3029	3032	rVB2	150	72	0.01%	0.001%
85	10.947	3078	3081	3087	rVB2	287	193	0.02%	0.002%
86	11.011	3098	3101	3103	rVB2	249	134	0.01%	0.001%
87	11.027	3103	3106	3107	rBV	126	66	0.01%	0.001%
88	11.175	3146	3152	3155	rBV3	548	547	0.04%	0.005%
89	11.239	3160	3172	3193	rBV	762335	1187061	95.17%	11.537%
90	11.484	3244	3248	3255	rBV2	363	403	0.03%	0.004%
91	11.612	3276	3288	3315	rBV	631085	990691	79.43%	9.629%
92	11.818	3349	3352	3357	rVB2	428	341	0.03%	0.003%
93	11.844	3358	3360	3361	rBV	178	60	0.00%	0.001%
94	11.902	3375	3378	3380	rBV	259	156	0.01%	0.002%
95	12.040	3418	3421	3423	rBV2	293	196	0.02%	0.002%
96	12.127	3444	3448	3452	rBV2	367	378	0.03%	0.004%
97	12.165	3457	3460	3462	rVV2	297	170	0.01%	0.002%
98	12.590	3590	3592	3595	rBV	276	173	0.01%	0.002%
99	12.635	3601	3606	3610	rBV5	638	667	0.05%	0.006%
100	12.709	3626	3629	3636	rBV3	507	494	0.04%	0.005%




Sum of corrected areas: 10289010

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029657.D
Acq On : 13 Dec 2022 17:35
Operator : SY/MD
Sample : N5981-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ET1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

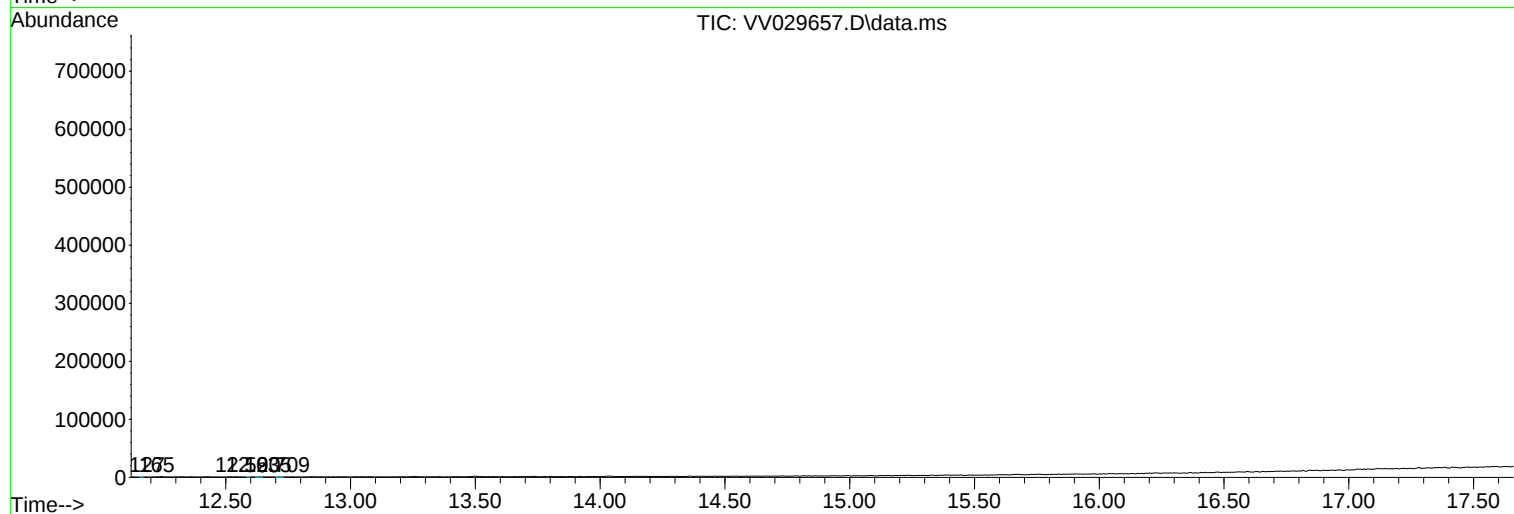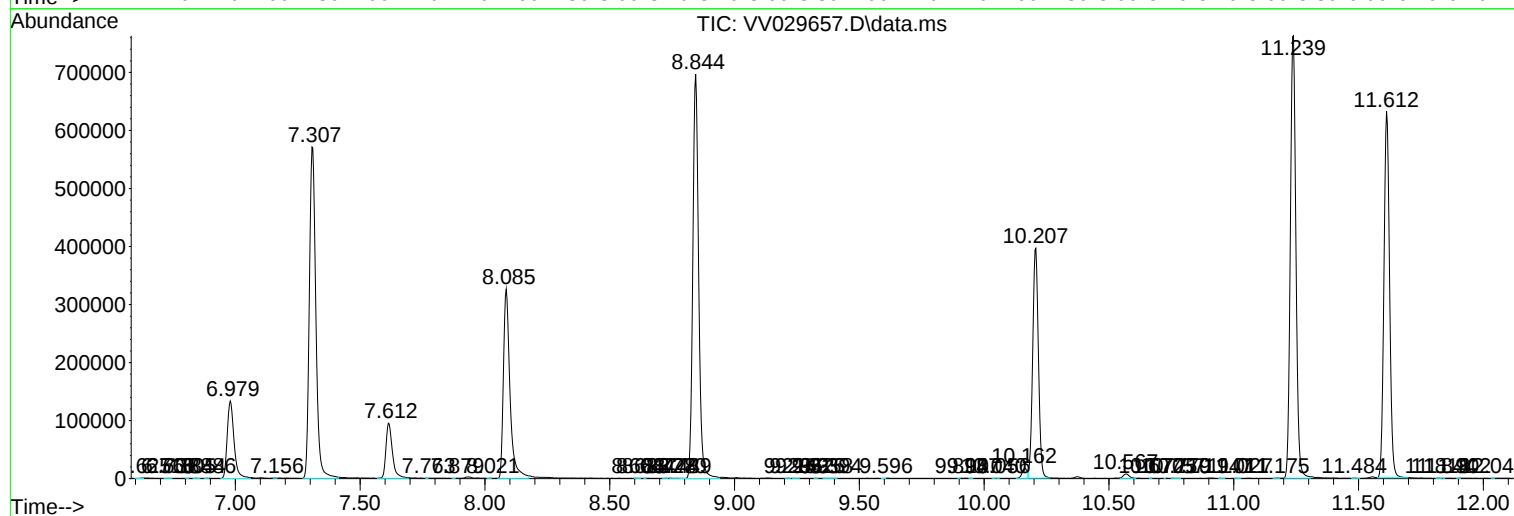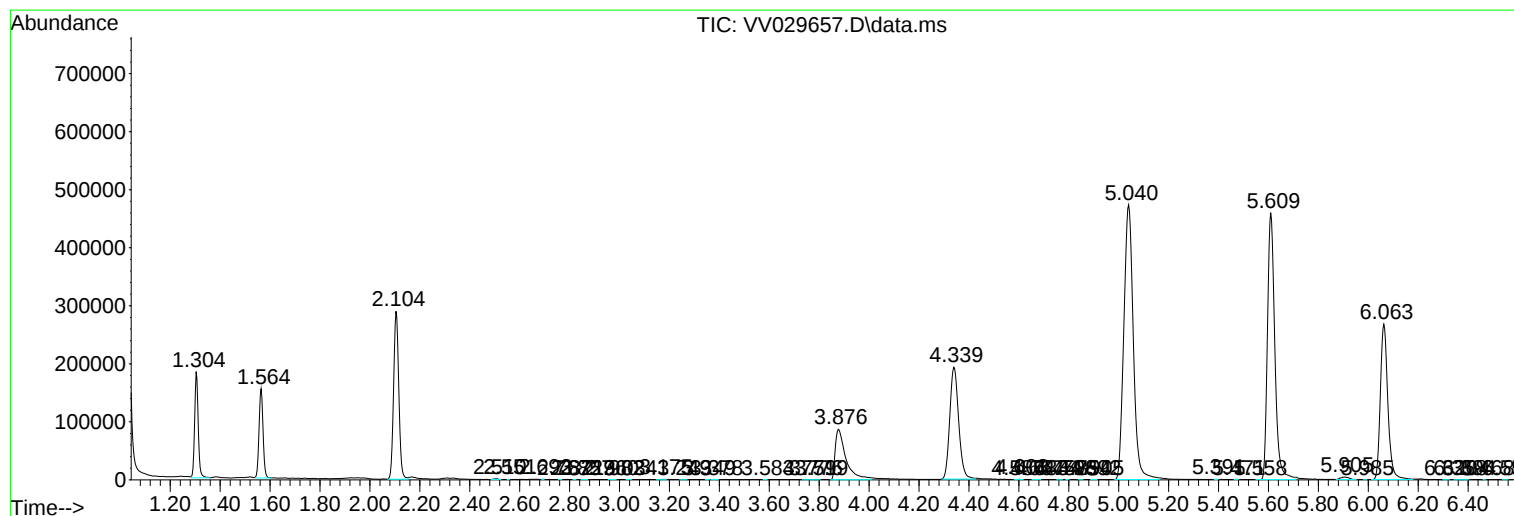

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029657.D
Acq On : 13 Dec 2022 17:35
Operator : SY/MD
Sample : N5981-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ET1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029657.D
Acq On : 13 Dec 2022 17:35
Operator : SY/MD
Sample : N5981-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ET1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------