

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029658.D
 Acq On : 13 Dec 2022 17:59
 Operator : SY/MD
 Sample : N5981-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ET2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	181419	179918	14.00%	1.570%
2	1.564	155	163	177	rVB	152079	168852	13.14%	1.474%
3	2.105	320	331	345	rBV2	313153	482991	37.59%	4.216%
4	2.584	478	480	482	rBV2	209	104	0.01%	0.001%
5	2.764	533	536	538	rBV2	293	179	0.01%	0.002%
6	2.966	594	599	602	rBV	216	223	0.02%	0.002%
7	3.085	631	636	639	rBV3	288	282	0.02%	0.002%
8	3.310	703	706	708	rBV	179	120	0.01%	0.001%
9	3.339	712	715	717	rBV2	165	116	0.01%	0.001%
10	3.532	773	775	778	rVB2	170	67	0.01%	0.001%
11	3.629	802	805	807	rBV2	138	103	0.01%	0.001%
12	3.664	811	816	818	rBV2	216	114	0.01%	0.001%
13	3.735	834	838	842	rBV2	277	259	0.02%	0.002%
14	3.770	847	849	850	rBV	155	69	0.01%	0.001%
15	3.873	871	881	915	rBV2	92236	310467	24.16%	2.710%
16	4.339	1008	1026	1059	rBV	197266	488771	38.04%	4.266%
17	4.596	1094	1106	1107	rBV3	8518	10261	0.80%	0.090%
18	4.706	1136	1140	1142	rBV2	265	186	0.01%	0.002%
19	4.767	1157	1159	1165	rBV2	197	133	0.01%	0.001%
20	4.883	1192	1195	1199	rVB2	254	185	0.01%	0.002%
21	4.963	1217	1220	1223	rBV2	218	115	0.01%	0.001%
22	5.040	1226	1244	1276	rBV2	477162	1255250	97.69%	10.957%
23	5.468	1375	1377	1378	rBV2	146	81	0.01%	0.001%
24	5.526	1393	1395	1399	rBV	117	74	0.01%	0.001%
25	5.609	1408	1421	1461	rBV	436717	894825	69.64%	7.811%
26	5.905	1499	1513	1548	rBV	641788	1284903	100.00%	11.215%
27	6.063	1550	1562	1600	rVB	274121	573029	44.60%	5.002%
28	6.249	1618	1620	1621	rBV	288	116	0.01%	0.001%
29	6.301	1635	1636	1637	rBV	215	67	0.01%	0.001%
30	6.323	1642	1643	1655	rVB	255	253	0.02%	0.002%
31	6.374	1655	1659	1660	rBV2	156	66	0.01%	0.001%
32	6.465	1684	1687	1690	rBV2	103	76	0.01%	0.001%
33	6.516	1701	1703	1707	rVB3	212	138	0.01%	0.001%
34	6.538	1707	1710	1715	rVB	141	118	0.01%	0.001%
35	6.564	1715	1718	1721	rBV	134	105	0.01%	0.001%
36	6.587	1724	1725	1728	rVB	167	78	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029658.D
 Acq On : 13 Dec 2022 17:59
 Operator : SY/MD
 Sample : N5981-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ET2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.612	1728	1733	1734	rBV	285	202	0.02%	0.002%
38	6.635	1735	1740	1742	rBV3	390	345	0.03%	0.003%
39	6.709	1761	1763	1766	rBV	233	137	0.01%	0.001%
40	6.738	1770	1772	1778	rBV	224	210	0.02%	0.002%
41	6.789	1786	1788	1791	rVB	253	115	0.01%	0.001%
42	6.908	1819	1825	1830	rBV3	232	287	0.02%	0.003%
43	6.979	1835	1847	1875	rBV	136065	248836	19.37%	2.172%
44	7.159	1900	1903	1905	rVV3	343	220	0.02%	0.002%
45	7.207	1915	1918	1924	rVB4	467	385	0.03%	0.003%
46	7.239	1925	1928	1934	rBV3	330	230	0.02%	0.002%
47	7.310	1937	1950	1971	rBV	572718	1020758	79.44%	8.910%
48	7.616	2034	2045	2068	rBV	93033	166666	12.97%	1.455%
49	7.783	2095	2097	2102	rBV2	242	261	0.02%	0.002%
50	7.841	2112	2115	2121	rVB4	1037	839	0.07%	0.007%
51	7.866	2121	2123	2128	rBV3	366	246	0.02%	0.002%
52	8.082	2181	2190	2220	rBV	318397	589737	45.90%	5.148%
53	8.567	2337	2341	2344	rBV3	240	186	0.01%	0.002%
54	8.609	2349	2354	2356	rBV4	516	446	0.03%	0.004%
55	8.715	2385	2387	2391	rBV	160	117	0.01%	0.001%
56	8.738	2391	2394	2396	rBV	265	162	0.01%	0.001%
57	8.786	2404	2409	2411	rBV	271	201	0.02%	0.002%
58	8.844	2415	2427	2459	rBV	645659	1060183	82.51%	9.254%
59	9.181	2529	2532	2534	rBV	168	90	0.01%	0.001%
60	9.217	2541	2543	2544	rBV	182	82	0.01%	0.001%
61	9.291	2564	2566	2569	rVB2	323	106	0.01%	0.001%
62	9.342	2580	2582	2585	rBV	242	127	0.01%	0.001%
63	9.500	2628	2631	2632	rBV	209	102	0.01%	0.001%
64	9.760	2710	2712	2715	rBV2	185	90	0.01%	0.001%
65	9.792	2719	2722	2728	rVB2	281	212	0.02%	0.002%
66	9.821	2728	2731	2733	rBV	122	78	0.01%	0.001%
67	10.014	2789	2791	2794	rVV	196	82	0.01%	0.001%
68	10.043	2796	2800	2804	rVB3	292	304	0.02%	0.003%
69	10.127	2822	2826	2827	rBV3	204	126	0.01%	0.001%
70	10.165	2828	2838	2841	rVV2	18298	25527	1.99%	0.223%
71	10.207	2842	2851	2874	rVB	407469	638079	49.66%	5.570%
72	10.329	2886	2889	2894	rBV2	317	257	0.02%	0.002%
73	10.374	2895	2903	2911	rVB4	2634	4169	0.32%	0.036%
74	10.442	2918	2924	2930	rVB2	291	478	0.04%	0.004%
75	10.474	2930	2934	2936	rBV	318	247	0.02%	0.002%
76	10.525	2948	2950	2953	rBV2	309	204	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029658.D
 Acq On : 13 Dec 2022 17:59
 Operator : SY/MD
 Sample : N5981-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ET2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.567	2955	2963	2981	rVB2	8622	14092	1.10%	0.123%
78	10.644	2984	2987	2990	rBV2	252	227	0.02%	0.002%
79	10.683	2996	2999	3001	rBV	257	119	0.01%	0.001%
80	10.706	3004	3006	3011	rBV2	125	133	0.01%	0.001%
81	10.828	3041	3044	3046	rBV2	229	162	0.01%	0.001%
82	10.886	3059	3062	3063	rBV	250	146	0.01%	0.001%
83	10.943	3078	3080	3081	rBV2	252	101	0.01%	0.001%
84	11.053	3113	3114	3119	rVB	214	122	0.01%	0.001%
85	11.162	3145	3148	3149	rBV	224	111	0.01%	0.001%
86	11.236	3159	3171	3195	rBV	688872	1073371	83.54%	9.369%
87	11.558	3266	3271	3276	rBV4	1475	1662	0.13%	0.015%
88	11.612	3277	3288	3309	rVV	609408	950127	73.95%	8.293%
89	11.905	3378	3379	3383	rVB2	233	70	0.01%	0.001%
90	11.927	3383	3386	3387	rBV2	210	124	0.01%	0.001%
91	11.963	3394	3397	3399	rBV2	230	134	0.01%	0.001%
92	11.998	3406	3408	3411	rVB	346	180	0.01%	0.002%
93	12.082	3432	3434	3438	rBV2	188	90	0.01%	0.001%
94	12.101	3438	3440	3443	rVB	306	157	0.01%	0.001%
95	12.120	3443	3446	3448	rBV	341	250	0.02%	0.002%
96	12.207	3469	3473	3474	rBV	286	219	0.02%	0.002%
97	12.291	3497	3499	3501	rBV	302	158	0.01%	0.001%
98	12.509	3561	3567	3570	rBV2	445	493	0.04%	0.004%
99	12.622	3598	3602	3604	rBV2	332	307	0.02%	0.003%
100	12.657	3611	3613	3616	rBV2	400	201	0.02%	0.002%




Sum of corrected areas: 11456579

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029658.D
Acq On : 13 Dec 2022 17:59
Operator : SY/MD
Sample : N5981-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ET2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

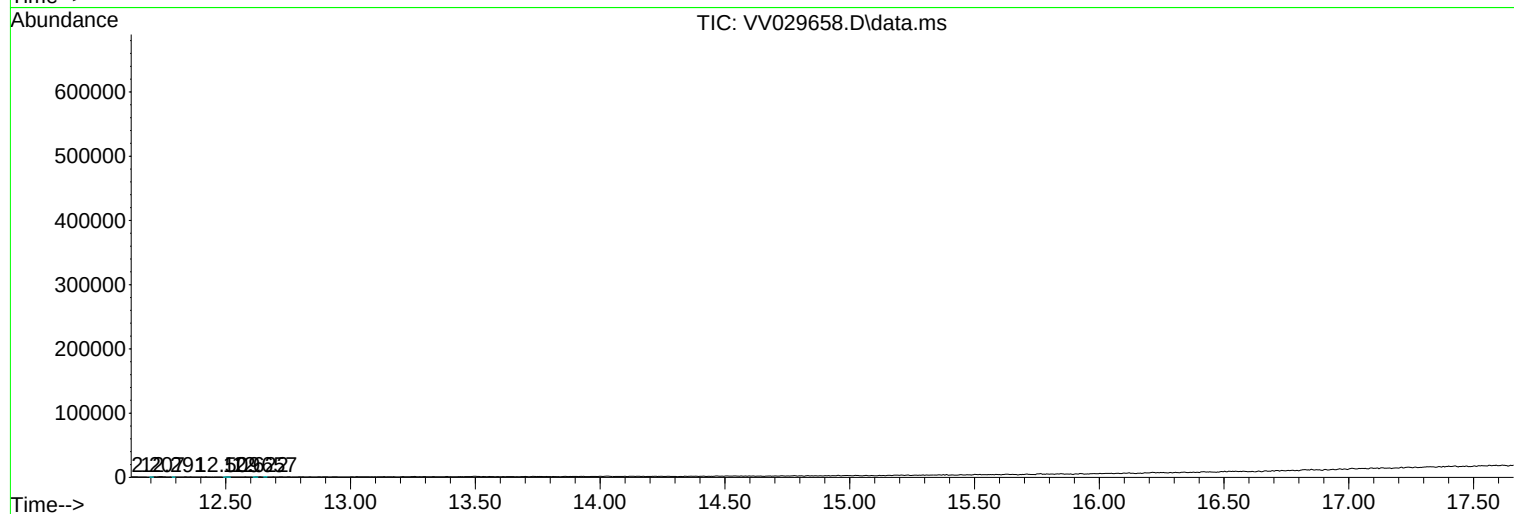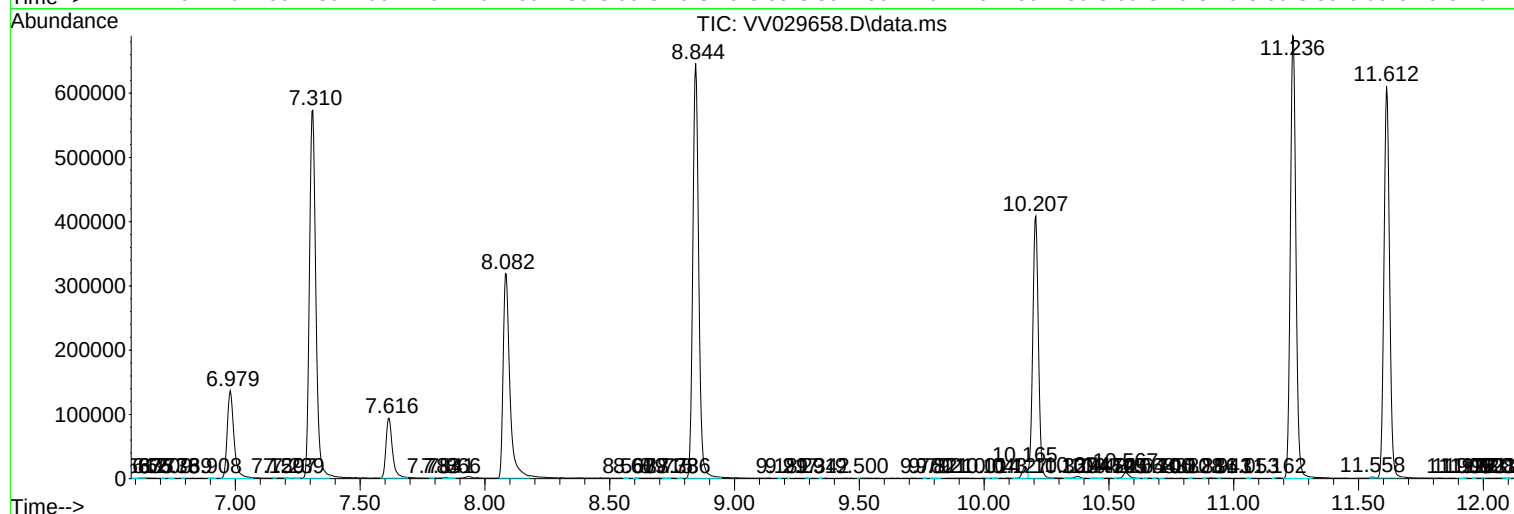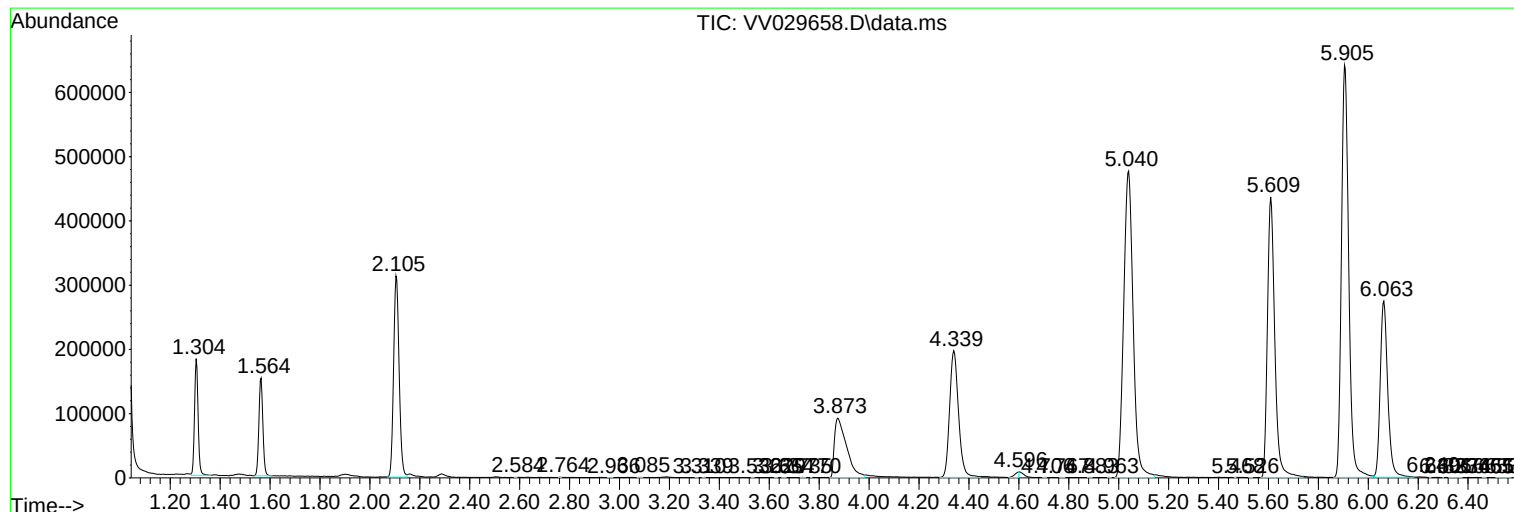

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029658.D
Acq On : 13 Dec 2022 17:59
Operator : SY/MD
Sample : N5981-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ET2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029658.D
Acq On : 13 Dec 2022 17:59
Operator : SY/MD
Sample : N5981-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ET2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc