

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029659.D
 Acq On : 13 Dec 2022 18:22
 Operator : SY/MD
 Sample : N5980-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029659.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	184881	183938	14.82%	1.879%
2	1.564	155	163	182	rVB	146077	167181	13.47%	1.708%
3	2.105	320	331	345	rBV	290813	417391	33.64%	4.264%
4	2.297	382	391	415	rVB2	10985	29456	2.37%	0.301%
5	2.458	436	441	442	rBV2	238	228	0.02%	0.002%
6	2.606	485	487	489	rBV	145	88	0.01%	0.001%
7	2.860	564	566	569	rBV2	183	103	0.01%	0.001%
8	3.150	653	656	661	rVB2	288	218	0.02%	0.002%
9	3.410	734	737	739	rBV	153	93	0.01%	0.001%
10	3.600	790	796	798	rBV2	195	213	0.02%	0.002%
11	3.641	806	809	811	rBV2	100	72	0.01%	0.001%
12	3.780	849	852	855	rBV2	131	90	0.01%	0.001%
13	3.815	859	863	868	rBV2	208	295	0.02%	0.003%
14	3.873	872	881	917	rBV	89451	254573	20.52%	2.601%
15	4.339	1009	1026	1059	rBV	195084	495206	39.91%	5.059%
16	4.567	1094	1097	1101	rBV2	438	348	0.03%	0.004%
17	4.670	1125	1129	1132	rBV2	294	248	0.02%	0.003%
18	4.683	1132	1133	1134	rBV2	134	41	0.00%	0.000%
19	4.722	1142	1145	1146	rBV2	174	97	0.01%	0.001%
20	4.957	1211	1218	1219	rBV2	261	248	0.02%	0.003%
21	4.969	1219	1222	1224	rBV2	202	131	0.01%	0.001%
22	5.040	1226	1244	1281	rBV2	472730	1240840	100.00%	12.676%
23	5.458	1371	1374	1375	rBV	205	118	0.01%	0.001%
24	5.516	1389	1392	1400	rVB3	345	322	0.03%	0.003%
25	5.558	1400	1405	1408	rBV	181	190	0.02%	0.002%
26	5.609	1408	1421	1452	rBV	390944	807572	65.08%	8.250%
27	5.908	1504	1514	1526	rBV6	5228	11507	0.93%	0.118%
28	5.982	1535	1537	1538	rBV	149	60	0.00%	0.001%
29	6.063	1547	1562	1601	rBV	264673	553505	44.61%	5.654%
30	6.272	1623	1627	1632	rVB2	374	286	0.02%	0.003%
31	6.442	1676	1680	1685	rVB2	279	234	0.02%	0.002%
32	6.490	1693	1695	1696	rBV	81	36	0.00%	0.000%
33	6.603	1727	1730	1732	rBV2	168	119	0.01%	0.001%
34	6.619	1733	1735	1736	rBV	326	128	0.01%	0.001%
35	6.725	1766	1768	1770	rBV	117	44	0.00%	0.000%
36	6.754	1774	1777	1781	rVB	391	276	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029659.D
 Acq On : 13 Dec 2022 18:22
 Operator : SY/MD
 Sample : N5980-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.776	1781	1784	1789	rBV2	135	123	0.01%	0.001%
38	6.831	1799	1801	1802	rBV	116	27	0.00%	0.000%
39	6.892	1819	1820	1821	rBV	125	34	0.00%	0.000%
40	6.905	1822	1824	1827	rVB2	229	90	0.01%	0.001%
41	6.979	1834	1847	1879	rBV	131647	245853	19.81%	2.512%
42	7.159	1900	1903	1906	rBV2	473	407	0.03%	0.004%
43	7.307	1937	1949	1972	rBV	571630	1005973	81.07%	10.277%
44	7.612	2035	2044	2070	rBV	92797	164635	13.27%	1.682%
45	7.818	2106	2108	2111	rBV2	327	125	0.01%	0.001%
46	7.879	2125	2127	2129	rBV	219	145	0.01%	0.001%
47	7.937	2138	2145	2152	rVB3	1169	1748	0.14%	0.018%
48	8.085	2180	2191	2220	rBV	322295	591771	47.69%	6.045%
49	8.661	2368	2370	2371	rVB	442	154	0.01%	0.002%
50	8.709	2384	2385	2389	rVB	229	117	0.01%	0.001%
51	8.734	2389	2393	2400	rBV2	190	273	0.02%	0.003%
52	8.844	2415	2427	2465	rBV	584394	960601	77.42%	9.813%
53	9.062	2493	2495	2497	rBV2	245	62	0.00%	0.001%
54	9.095	2502	2505	2507	rBV2	265	160	0.01%	0.002%
55	9.133	2516	2517	2518	rBV	242	71	0.01%	0.001%
56	9.288	2563	2565	2567	rBV	187	76	0.01%	0.001%
57	9.313	2571	2573	2575	rVB	182	60	0.00%	0.001%
58	9.374	2590	2592	2593	rBV	139	35	0.00%	0.000%
59	9.397	2597	2599	2601	rBV	274	118	0.01%	0.001%
60	9.464	2618	2620	2623	rBV	132	86	0.01%	0.001%
61	9.532	2637	2641	2643	rBV2	352	260	0.02%	0.003%
62	9.574	2651	2654	2658	rVB2	237	157	0.01%	0.002%
63	9.628	2668	2671	2672	rBV	204	91	0.01%	0.001%
64	9.734	2702	2704	2707	rVB	177	72	0.01%	0.001%
65	9.754	2708	2710	2711	rVB2	389	112	0.01%	0.001%
66	9.789	2719	2721	2723	rVB	190	75	0.01%	0.001%
67	9.799	2723	2724	2728	rBV2	132	70	0.01%	0.001%
68	9.818	2728	2730	2732	rVV	137	36	0.00%	0.000%
69	9.918	2755	2761	2764	rBV2	359	426	0.03%	0.004%
70	9.982	2778	2781	2786	rVB	274	242	0.02%	0.002%
71	10.008	2786	2789	2791	rBV	132	83	0.01%	0.001%
72	10.162	2828	2837	2841	rBV2	16929	24377	1.96%	0.249%
73	10.204	2842	2850	2873	rVB	395297	624673	50.34%	6.381%
74	10.567	2955	2963	2977	rVB3	7258	11884	0.96%	0.121%
75	10.818	3039	3041	3043	rBV	386	139	0.01%	0.001%
76	10.908	3065	3069	3073	rBV2	501	516	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029659.D
 Acq On : 13 Dec 2022 18:22
 Operator : SY/MD
 Sample : N5980-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.947	3079	3081	3085	rVB	305	173	0.01%	0.002%
78	10.972	3085	3089	3094	rBV	225	255	0.02%	0.003%
79	11.062	3114	3117	3122	rBV2	179	182	0.01%	0.002%
80	11.095	3124	3127	3130	rVV2	241	126	0.01%	0.001%
81	11.159	3144	3147	3148	rBV2	177	79	0.01%	0.001%
82	11.178	3148	3153	3159	rVB4	495	495	0.04%	0.005%
83	11.236	3159	3171	3194	rBV	637230	1002851	80.82%	10.245%
84	11.429	3228	3231	3233	rBV	450	259	0.02%	0.003%
85	11.464	3240	3242	3243	rBV	264	124	0.01%	0.001%
86	11.551	3265	3269	3270	rBV2	1171	802	0.06%	0.008%
87	11.612	3276	3288	3312	rBV	625712	980617	79.03%	10.018%
88	11.950	3387	3393	3394	rBV3	458	415	0.03%	0.004%
89	12.075	3430	3432	3434	rBV	338	160	0.01%	0.002%
90	12.336	3508	3513	3515	rBV3	383	385	0.03%	0.004%
91	12.464	3550	3553	3558	rBV3	493	467	0.04%	0.005%
92	12.628	3602	3604	3605	rBV3	401	144	0.01%	0.001%

Sum of corrected areas: 9788986




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029659.D
Acq On : 13 Dec 2022 18:22
Operator : SY/MD
Sample : N5980-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

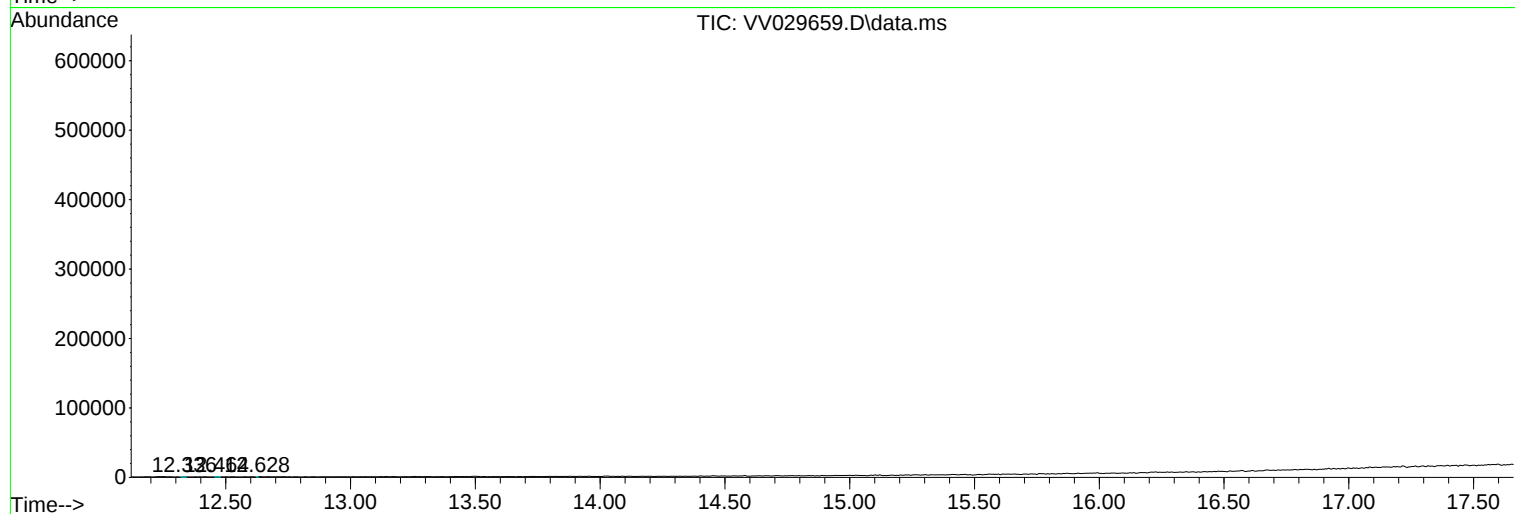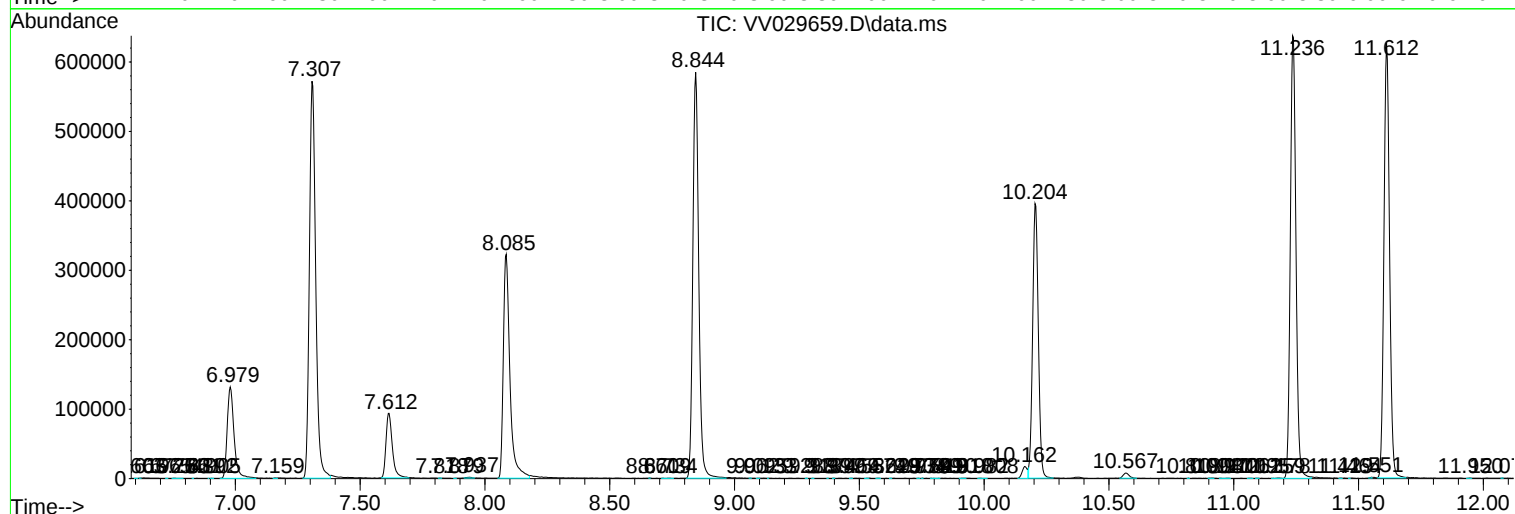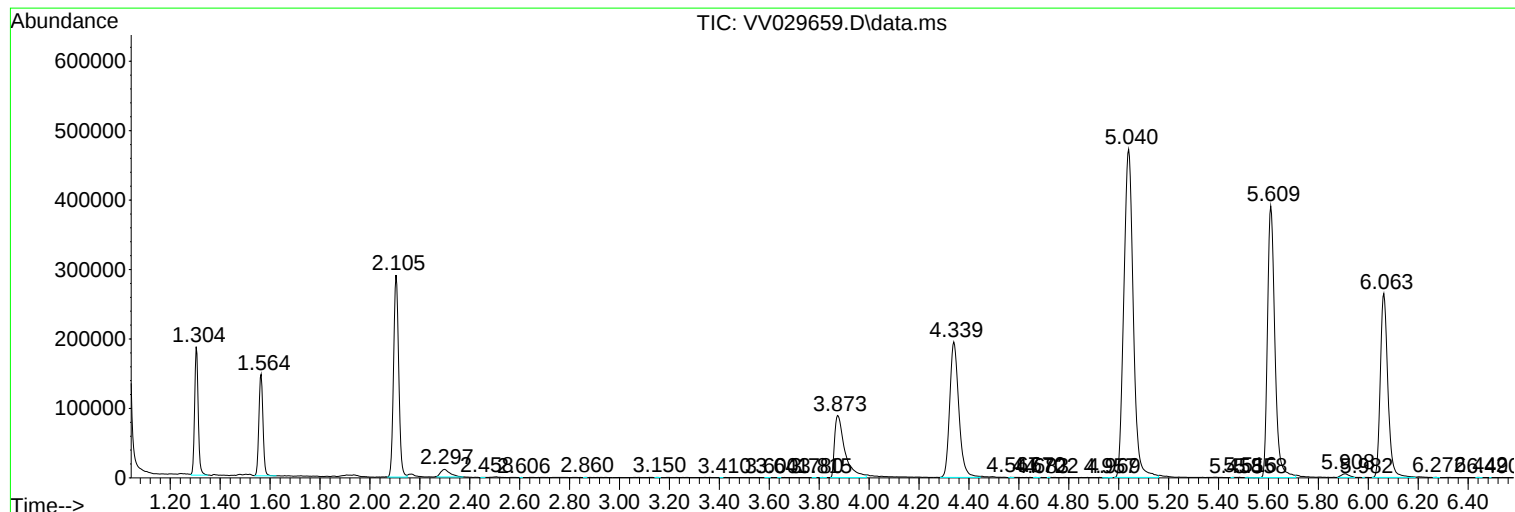

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029659.D
Acq On : 13 Dec 2022 18:22
Operator : SY/MD
Sample : N5980-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029659.D
Acq On : 13 Dec 2022 18:22
Operator : SY/MD
Sample : N5980-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------