

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029660.D
 Acq On : 13 Dec 2022 18:46
 Operator : SY/MD
 Sample : N5980-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029660.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	189320	189399	14.14%	1.721%
2	1.564	155	163	174	rVB	153699	175631	13.11%	1.596%
3	2.105	320	331	345	rBV	312053	447518	33.41%	4.068%
4	2.285	379	387	409	rVB	12683	29023	2.17%	0.264%
5	2.404	422	424	426	rBV2	310	92	0.01%	0.001%
6	2.478	444	447	449	rBV2	309	229	0.02%	0.002%
7	2.503	449	455	462	rVB4	1377	2253	0.17%	0.020%
8	2.535	462	465	467	rBV2	253	140	0.01%	0.001%
9	2.732	524	526	529	rBV2	199	142	0.01%	0.001%
10	2.764	534	536	539	rBV	359	158	0.01%	0.001%
11	2.912	579	582	583	rBV	149	87	0.01%	0.001%
12	2.953	592	595	597	rBV	255	171	0.01%	0.002%
13	3.002	605	610	615	rVB2	155	197	0.01%	0.002%
14	3.117	643	646	649	rBV2	206	155	0.01%	0.001%
15	3.198	668	671	674	rBV2	170	126	0.01%	0.001%
16	3.214	674	676	678	rBV	154	91	0.01%	0.001%
17	3.243	683	685	693	rBV2	163	172	0.01%	0.002%
18	3.314	704	707	712	rBV2	166	140	0.01%	0.001%
19	3.400	732	734	735	rVB2	295	87	0.01%	0.001%
20	3.487	759	761	765	rVB2	213	130	0.01%	0.001%
21	3.561	781	784	786	rBV	154	98	0.01%	0.001%
22	3.773	848	850	854	rVB2	148	86	0.01%	0.001%
23	3.873	871	881	925	rBV	98063	277915	20.75%	2.526%
24	4.339	1009	1026	1055	rBV	207315	523590	39.09%	4.759%
25	4.667	1125	1128	1132	rVB3	284	161	0.01%	0.001%
26	4.690	1132	1135	1137	rBV	217	145	0.01%	0.001%
27	4.709	1138	1141	1143	rVB3	222	127	0.01%	0.001%
28	4.738	1148	1150	1153	rVB2	180	87	0.01%	0.001%
29	4.780	1160	1163	1167	rBV	223	146	0.01%	0.001%
30	4.802	1167	1170	1173	rVV2	249	147	0.01%	0.001%
31	4.818	1173	1175	1178	rVB	207	113	0.01%	0.001%
32	4.879	1191	1194	1196	rBV2	258	137	0.01%	0.001%
33	4.979	1222	1225	1226	rBV	208	134	0.01%	0.001%
34	5.040	1226	1244	1292	rBV2	506099	1339531	100.00%	12.175%
35	5.452	1369	1372	1374	rBV2	207	121	0.01%	0.001%
36	5.477	1376	1380	1384	rBV2	512	510	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029660.D
 Acq On : 13 Dec 2022 18:46
 Operator : SY/MD
 Sample : N5980-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	5.564	1403	1407	1408	rBV2	211	148	0.01%	0.001%
38	5.609	1408	1421	1450	rBV	494962	998912	74.57%	9.079%
39	5.908	1503	1514	1527	rVB8	5585	12489	0.93%	0.114%
40	5.989	1535	1539	1543	rBV3	196	221	0.02%	0.002%
41	6.008	1543	1545	1548	rBV	199	141	0.01%	0.001%
42	6.063	1548	1562	1594	rBV	287535	598193	44.66%	5.437%
43	6.297	1633	1635	1638	rBV2	278	113	0.01%	0.001%
44	6.339	1644	1648	1651	rBV3	222	171	0.01%	0.002%
45	6.358	1652	1654	1659	rVV2	257	158	0.01%	0.001%
46	6.500	1695	1698	1701	rBV2	261	190	0.01%	0.002%
47	6.513	1701	1702	1707	rVB	276	141	0.01%	0.001%
48	6.538	1707	1710	1713	rVB2	147	97	0.01%	0.001%
49	6.567	1713	1719	1724	rBV2	152	231	0.02%	0.002%
50	6.612	1730	1733	1734	rBV3	352	182	0.01%	0.002%
51	6.725	1765	1768	1772	rVB2	294	196	0.01%	0.002%
52	6.760	1777	1779	1782	rBV2	284	118	0.01%	0.001%
53	6.818	1794	1797	1801	rVV2	158	102	0.01%	0.001%
54	6.850	1805	1807	1809	rVB	197	86	0.01%	0.001%
55	6.863	1809	1811	1815	rBV2	197	164	0.01%	0.001%
56	6.892	1818	1820	1823	rBV	323	156	0.01%	0.001%
57	6.979	1836	1847	1877	rBV	141219	262735	19.61%	2.388%
58	7.146	1897	1899	1902	rBV2	207	142	0.01%	0.001%
59	7.246	1928	1930	1933	rVB3	246	113	0.01%	0.001%
60	7.307	1936	1949	1980	rBV	614995	1096906	81.89%	9.970%
61	7.612	2034	2044	2074	rBV	100252	178849	13.35%	1.626%
62	7.911	2131	2137	2138	rBV3	538	495	0.04%	0.004%
63	8.082	2180	2190	2224	rBV	351922	646699	48.28%	5.878%
64	8.481	2312	2314	2316	rBV3	324	209	0.02%	0.002%
65	8.532	2328	2330	2334	rVB2	460	305	0.02%	0.003%
66	8.693	2375	2380	2383	rVB4	406	330	0.02%	0.003%
67	8.709	2383	2385	2386	rBV4	226	102	0.01%	0.001%
68	8.844	2415	2427	2455	rBV	733338	1187720	88.67%	10.795%
69	9.175	2527	2530	2532	rBV2	335	213	0.02%	0.002%
70	9.185	2532	2533	2537	rVB2	250	133	0.01%	0.001%
71	9.281	2561	2563	2565	rBV	239	104	0.01%	0.001%
72	9.371	2589	2591	2593	rBV	156	97	0.01%	0.001%
73	9.435	2603	2611	2618	rBV2	290	428	0.03%	0.004%
74	9.464	2618	2620	2625	rBV3	320	274	0.02%	0.002%
75	9.500	2628	2631	2639	rBV2	207	190	0.01%	0.002%
76	9.535	2639	2642	2645	rBV2	421	352	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029660.D
 Acq On : 13 Dec 2022 18:46
 Operator : SY/MD
 Sample : N5980-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.567	2649	2652	2653	rBV	258	132	0.01%	0.001%
78	9.603	2659	2663	2665	rBV	210	174	0.01%	0.002%
79	9.641	2672	2675	2677	rBV	227	110	0.01%	0.001%
80	9.815	2726	2729	2732	rBV3	251	183	0.01%	0.002%
81	9.918	2758	2761	2764	rBV2	458	337	0.03%	0.003%
82	10.027	2792	2795	2798	rVB2	266	173	0.01%	0.002%
83	10.043	2798	2800	2808	rVB2	280	255	0.02%	0.002%
84	10.101	2816	2818	2822	rBV2	191	92	0.01%	0.001%
85	10.162	2826	2837	2841	rBV	19284	27780	2.07%	0.252%
86	10.207	2842	2851	2870	rVB	425063	677823	50.60%	6.161%
87	10.336	2889	2891	2895	rVB	390	212	0.02%	0.002%
88	10.374	2895	2903	2911	rBV2	1473	2411	0.18%	0.022%
89	10.567	2955	2963	2977	rVB2	8847	14128	1.05%	0.128%
90	10.754	3018	3021	3023	rBV2	265	178	0.01%	0.002%
91	10.808	3036	3038	3041	rVB2	246	127	0.01%	0.001%
92	10.870	3053	3057	3059	rBV3	188	144	0.01%	0.001%
93	10.908	3065	3069	3072	rBV2	479	393	0.03%	0.004%
94	11.178	3147	3153	3154	rBV	349	352	0.03%	0.003%
95	11.239	3160	3172	3195	rBV	801353	1240136	92.58%	11.272%
96	11.612	3275	3288	3317	rBV	679890	1058385	79.01%	9.620%
97	11.972	3398	3400	3403	rBV	258	141	0.01%	0.001%
98	12.165	3456	3460	3464	rBV2	321	320	0.02%	0.003%
99	12.638	3604	3607	3610	rBV3	537	379	0.03%	0.003%
100	12.776	3646	3650	3652	rBV	354	303	0.02%	0.003%




Sum of corrected areas: 11002262

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029660.D
Acq On : 13 Dec 2022 18:46
Operator : SY/MD
Sample : N5980-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

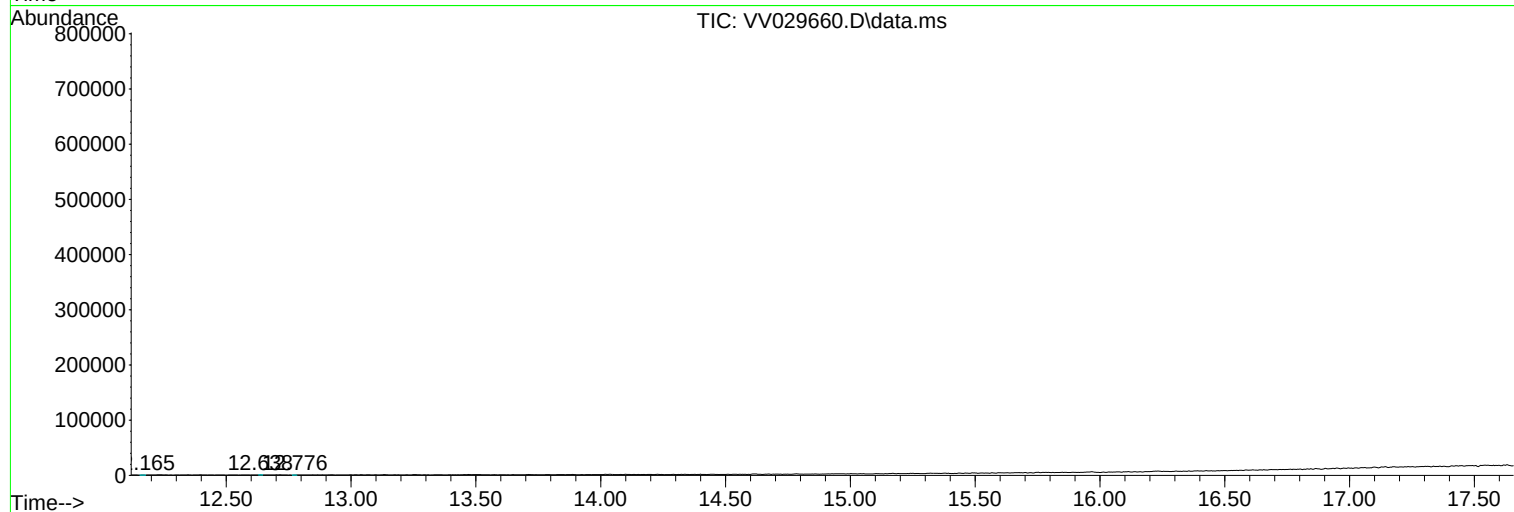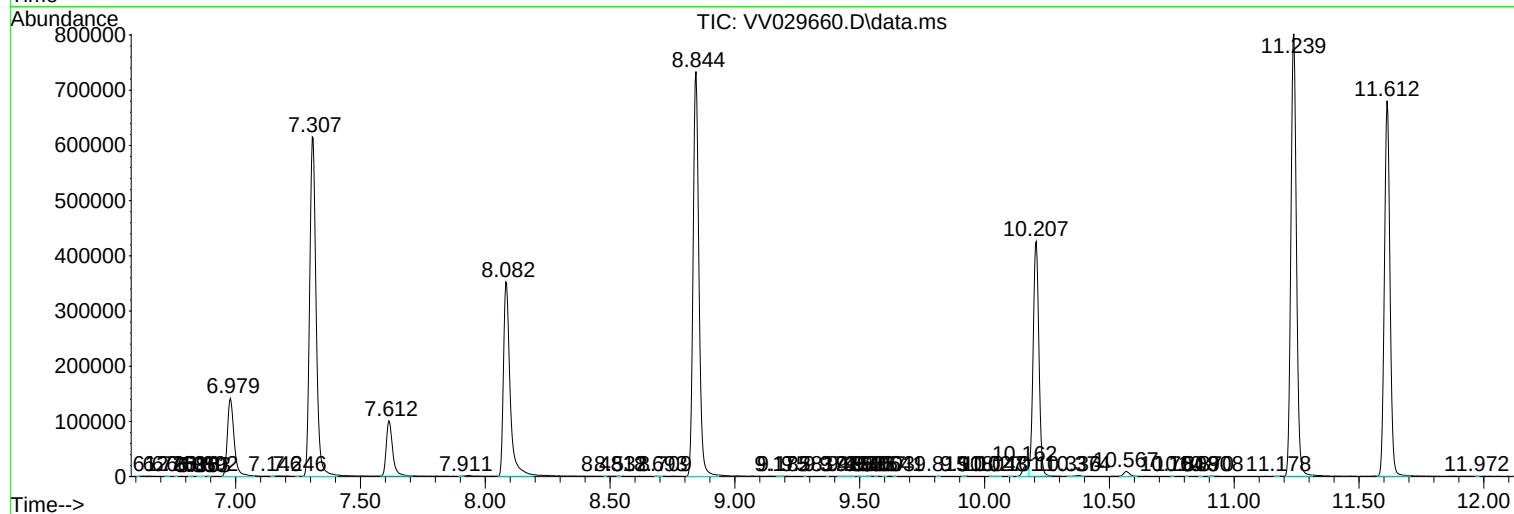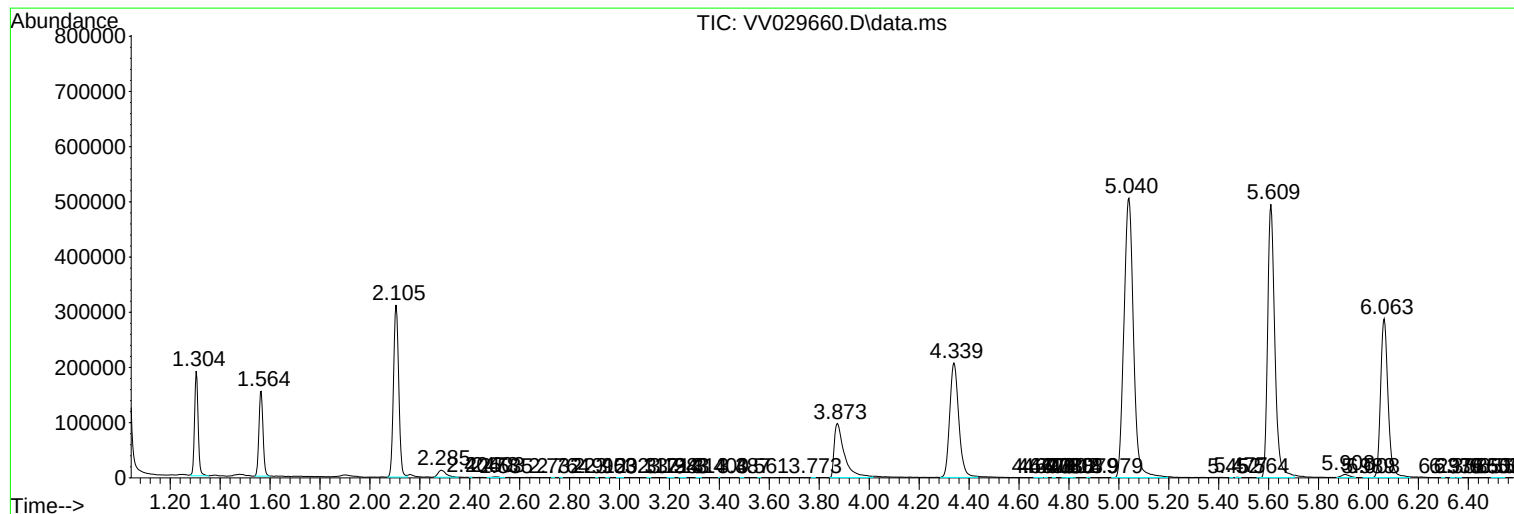

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029660.D
Acq On : 13 Dec 2022 18:46
Operator : SY/MD
Sample : N5980-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029660.D
Acq On : 13 Dec 2022 18:46
Operator : SY/MD
Sample : N5980-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc