

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029661.D
 Acq On : 13 Dec 2022 19:09
 Operator : SY/MD
 Sample : N5980-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	188270	187383	14.62%	1.796%
2	1.564	156	163	177	rVB	150521	171088	13.34%	1.640%
3	2.105	320	331	345	rBV	301882	432569	33.74%	4.147%
4	2.416	426	428	430	rBV	232	139	0.01%	0.001%
5	2.455	437	440	441	rBV2	197	122	0.01%	0.001%
6	2.500	450	454	455	rBV2	978	748	0.06%	0.007%
7	2.625	489	493	495	rBV	391	350	0.03%	0.003%
8	2.870	566	569	571	rBV2	153	90	0.01%	0.001%
9	3.053	623	626	629	rBV2	188	123	0.01%	0.001%
10	3.159	657	659	663	rVB	245	120	0.01%	0.001%
11	3.227	677	680	684	rBV2	190	180	0.01%	0.002%
12	3.297	698	702	705	rBV	169	145	0.01%	0.001%
13	3.326	709	711	715	rVV	145	93	0.01%	0.001%
14	3.381	722	728	733	rVB2	243	222	0.02%	0.002%
15	3.407	733	736	741	rBV2	169	135	0.01%	0.001%
16	3.477	755	758	759	rBV	59	34	0.00%	0.000%
17	3.587	789	792	794	rVB2	210	94	0.01%	0.001%
18	3.822	862	865	868	rBV	162	115	0.01%	0.001%
19	3.873	871	881	918	rBV	93983	261893	20.43%	2.511%
20	4.339	1010	1026	1057	rBV	200758	497182	38.78%	4.766%
21	4.632	1115	1117	1123	rVB2	236	136	0.01%	0.001%
22	4.667	1123	1128	1131	rVB3	271	197	0.02%	0.002%
23	4.696	1133	1137	1138	rBV	252	126	0.01%	0.001%
24	4.735	1144	1149	1155	rBV3	220	281	0.02%	0.003%
25	4.850	1182	1185	1186	rBV	92	50	0.00%	0.000%
26	4.873	1190	1192	1195	rVV	131	44	0.00%	0.000%
27	5.040	1226	1244	1278	rBV2	487608	1282108	100.00%	12.291%
28	5.429	1364	1365	1368	rVB2	290	91	0.01%	0.001%
29	5.477	1373	1380	1388	rVB3	518	727	0.06%	0.007%
30	5.516	1388	1392	1395	rBV	134	123	0.01%	0.001%
31	5.609	1408	1421	1471	rBV	455029	933560	72.81%	8.949%
32	5.973	1530	1534	1537	rVB2	295	230	0.02%	0.002%
33	5.998	1537	1542	1545	rBV	298	334	0.03%	0.003%
34	6.063	1548	1562	1589	rBV	279458	573126	44.70%	5.494%
35	6.259	1621	1623	1627	rVB	396	135	0.01%	0.001%
36	6.307	1634	1638	1639	rBV	302	190	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029661.D
 Acq On : 13 Dec 2022 19:09
 Operator : SY/MD
 Sample : N5980-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.365	1654	1656	1658	rBV2	149	87	0.01%	0.001%
38	6.432	1672	1677	1680	rBV3	264	254	0.02%	0.002%
39	6.471	1686	1689	1692	rBV	267	123	0.01%	0.001%
40	6.490	1692	1695	1699	rVB2	204	151	0.01%	0.001%
41	6.519	1702	1704	1706	rBV2	162	83	0.01%	0.001%
42	6.574	1720	1721	1722	rBV2	140	43	0.00%	0.000%
43	6.622	1729	1736	1739	rBV2	540	628	0.05%	0.006%
44	6.799	1785	1791	1794	rBV2	162	163	0.01%	0.002%
45	6.860	1807	1810	1812	rBV2	215	161	0.01%	0.002%
46	6.895	1819	1821	1824	rVB2	211	97	0.01%	0.001%
47	6.924	1824	1830	1835	rBV2	149	198	0.02%	0.002%
48	6.979	1835	1847	1870	rBV	135234	250163	19.51%	2.398%
49	7.159	1900	1903	1904	rBV	365	205	0.02%	0.002%
50	7.307	1936	1949	1984	rBV	590609	1056783	82.43%	10.131%
51	7.612	2032	2044	2073	rBV	94906	173181	13.51%	1.660%
52	7.854	2116	2119	2120	rBV	272	145	0.01%	0.001%
53	7.931	2136	2143	2144	rBV3	1511	1432	0.11%	0.014%
54	8.085	2180	2191	2232	rBV	330506	617690	48.18%	5.921%
55	8.397	2286	2288	2290	rBV	245	161	0.01%	0.002%
56	8.590	2344	2348	2351	rBV3	467	358	0.03%	0.003%
57	8.667	2368	2372	2374	rBV	245	206	0.02%	0.002%
58	8.709	2383	2385	2387	rVB	167	64	0.00%	0.001%
59	8.844	2410	2427	2455	rBV	662218	1101071	85.88%	10.555%
60	9.140	2514	2519	2521	rBV2	545	427	0.03%	0.004%
61	9.259	2553	2556	2559	rBV2	175	141	0.01%	0.001%
62	9.407	2599	2602	2605	rBV	155	101	0.01%	0.001%
63	9.435	2609	2611	2612	rBV	83	31	0.00%	0.000%
64	9.493	2625	2629	2631	rBV3	252	174	0.01%	0.002%
65	9.513	2631	2635	2637	rVB	117	83	0.01%	0.001%
66	9.532	2640	2641	2642	rBV	381	131	0.01%	0.001%
67	9.725	2694	2701	2705	rBV2	247	370	0.03%	0.004%
68	9.747	2705	2708	2712	rBV	143	141	0.01%	0.001%
69	9.815	2727	2729	2731	rBV2	132	77	0.01%	0.001%
70	9.831	2731	2734	2737	rBV2	158	111	0.01%	0.001%
71	9.863	2742	2744	2745	rVB	143	40	0.00%	0.000%
72	9.921	2759	2762	2763	rBV2	284	189	0.01%	0.002%
73	9.947	2768	2770	2775	rBV2	251	193	0.02%	0.002%
74	10.001	2785	2787	2790	rBV2	190	88	0.01%	0.001%
75	10.091	2810	2815	2817	rBV2	237	224	0.02%	0.002%
76	10.162	2826	2837	2841	rBV	18290	26766	2.09%	0.257%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029661.D
 Acq On : 13 Dec 2022 19:09
 Operator : SY/MD
 Sample : N5980-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.207	2842	2851	2872	rVB	414679	652100	50.86%	6.251%
78	10.374	2895	2903	2916	rVB7	2001	3369	0.26%	0.032%
79	10.439	2916	2923	2924	rBV2	222	206	0.02%	0.002%
80	10.532	2948	2952	2954	rBV2	498	312	0.02%	0.003%
81	10.570	2955	2964	2973	rVB2	8562	13459	1.05%	0.129%
82	10.712	3005	3008	3011	rBV	332	188	0.01%	0.002%
83	10.802	3034	3036	3040	rVB2	290	181	0.01%	0.002%
84	10.831	3040	3045	3048	rBV3	311	326	0.03%	0.003%
85	11.027	3105	3106	3110	rVB	326	136	0.01%	0.001%
86	11.172	3148	3151	3152	rBV	448	203	0.02%	0.002%
87	11.239	3159	3172	3201	rBV	740095	1160203	90.49%	11.122%
88	11.538	3262	3265	3266	rBV	348	180	0.01%	0.002%
89	11.554	3266	3270	3276	rBV5	1662	2105	0.16%	0.020%
90	11.612	3276	3288	3306	rBV	639965	1018926	79.47%	9.768%
91	11.873	3366	3369	3372	rBV2	398	234	0.02%	0.002%
92	12.075	3431	3432	3434	rBV2	133	54	0.00%	0.001%
93	12.172	3460	3462	3463	rBV2	217	68	0.01%	0.001%
94	12.326	3508	3510	3513	rBV	274	79	0.01%	0.001%
95	12.429	3538	3542	3543	rBV	278	179	0.01%	0.002%
96	12.484	3552	3559	3560	rBV2	393	368	0.03%	0.004%
97	12.567	3581	3585	3586	rBV	528	319	0.02%	0.003%
98	12.667	3612	3616	3618	rBV2	318	235	0.02%	0.002%
99	12.831	3664	3667	3669	rBV2	603	417	0.03%	0.004%
100	12.882	3674	3683	3688	rBV3	479	755	0.06%	0.007%




Sum of corrected areas: 10431619

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029661.D
Acq On : 13 Dec 2022 19:09
Operator : SY/MD
Sample : N5980-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

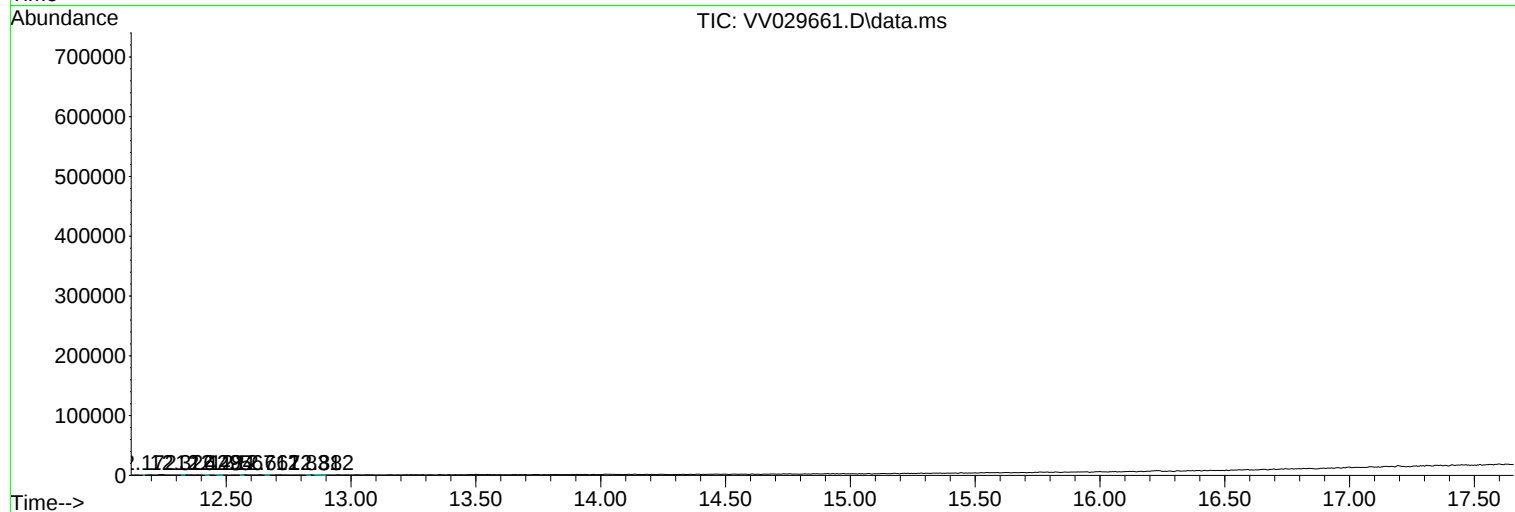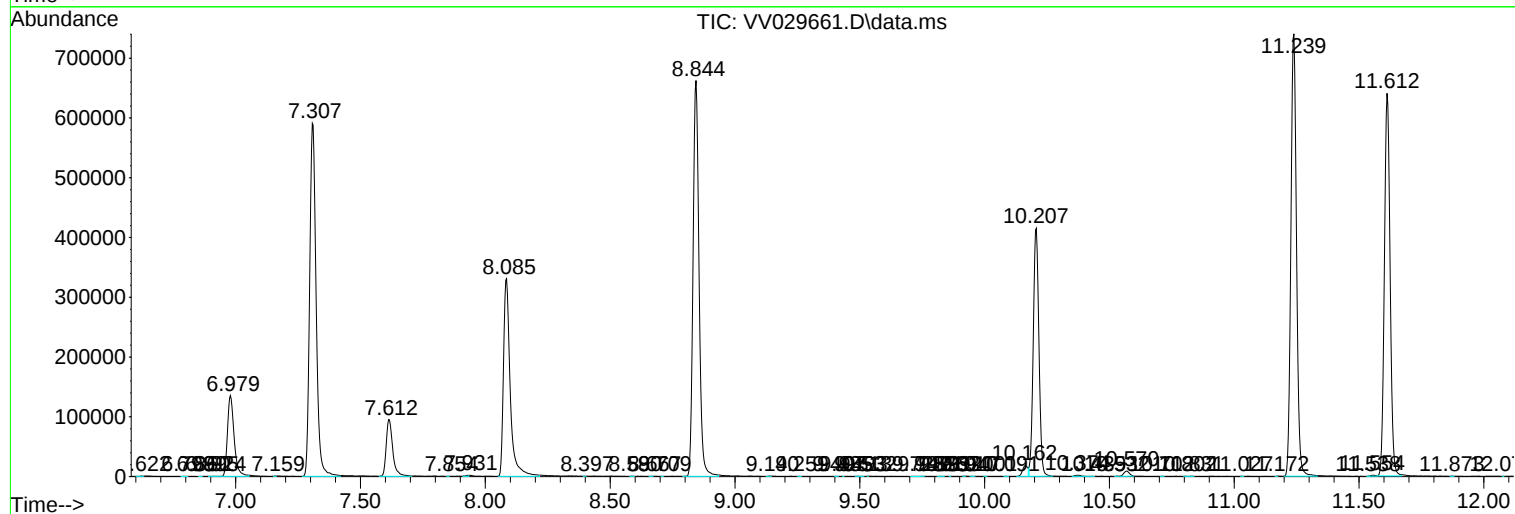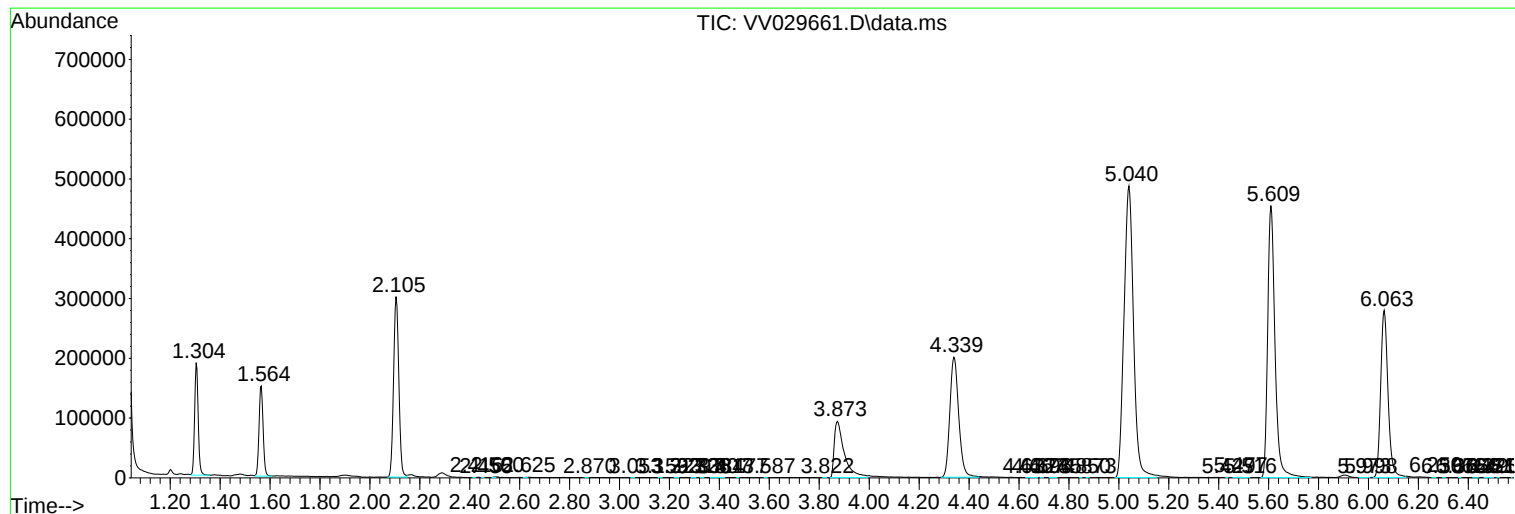

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029661.D
Acq On : 13 Dec 2022 19:09
Operator : SY/MD
Sample : N5980-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029661.D
Acq On : 13 Dec 2022 19:09
Operator : SY/MD
Sample : N5980-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc