

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029662.D
 Acq On : 13 Dec 2022 19:32
 Operator : SY/MD
 Sample : N5980-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029662.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	191265	193043	14.32%	1.705%
2	1.564	156	163	181	rVB	159119	182087	13.51%	1.608%
3	2.105	320	331	345	rBV	312089	448423	33.27%	3.960%
4	2.442	434	436	438	rBV2	312	110	0.01%	0.001%
5	2.500	449	454	455	rBV3	1079	822	0.06%	0.007%
6	2.642	487	498	506	rBV4	810	1568	0.12%	0.014%
7	2.761	533	535	536	rBV4	326	139	0.01%	0.001%
8	2.934	586	589	591	rBV2	207	140	0.01%	0.001%
9	3.031	614	619	621	rBV2	134	118	0.01%	0.001%
10	3.108	640	643	648	rVV2	140	152	0.01%	0.001%
11	3.346	714	717	723	rVB2	178	130	0.01%	0.001%
12	3.407	732	736	738	rVB3	191	161	0.01%	0.001%
13	3.468	750	755	757	rBV	135	102	0.01%	0.001%
14	3.484	757	760	763	rBV	197	138	0.01%	0.001%
15	3.568	783	786	791	rVB	191	123	0.01%	0.001%
16	3.600	791	796	801	rBV2	277	280	0.02%	0.002%
17	3.815	858	863	865	rVB2	156	127	0.01%	0.001%
18	3.834	865	869	872	rBV2	165	135	0.01%	0.001%
19	3.873	872	881	923	rBV	100638	290266	21.53%	2.563%
20	4.339	1010	1026	1056	rBV	210694	525302	38.97%	4.639%
21	4.683	1128	1133	1136	rBV3	378	311	0.02%	0.003%
22	4.748	1151	1153	1159	rVB2	280	190	0.01%	0.002%
23	4.777	1159	1162	1166	rBV2	182	162	0.01%	0.001%
24	4.860	1187	1188	1192	rVB	307	151	0.01%	0.001%
25	4.886	1192	1196	1199	rBV2	275	200	0.01%	0.002%
26	5.040	1226	1244	1272	rBV2	513699	1347890	100.00%	11.903%
27	5.410	1358	1359	1362	rBV	277	120	0.01%	0.001%
28	5.478	1375	1380	1383	rBV	524	397	0.03%	0.004%
29	5.526	1392	1395	1402	rVB2	294	291	0.02%	0.003%
30	5.609	1402	1421	1460	rBV	517989	1061649	78.76%	9.375%
31	5.828	1487	1489	1492	rBV2	284	137	0.01%	0.001%
32	5.912	1502	1515	1537	rVB4	25441	54416	4.04%	0.481%
33	6.063	1548	1562	1597	rBV	297601	610732	45.31%	5.393%
34	6.252	1615	1621	1624	rVB4	453	496	0.04%	0.004%
35	6.288	1627	1632	1635	rBV3	185	184	0.01%	0.002%
36	6.301	1635	1636	1643	rVB2	229	153	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029662.D
 Acq On : 13 Dec 2022 19:32
 Operator : SY/MD
 Sample : N5980-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.519	1701	1704	1708	rVB	329	182	0.01%	0.002%
38	6.551	1708	1714	1717	rBV	184	193	0.01%	0.002%
39	6.629	1731	1738	1741	rBV3	937	1120	0.08%	0.010%
40	6.699	1755	1760	1763	rBV3	268	251	0.02%	0.002%
41	6.719	1763	1766	1771	rVV3	327	256	0.02%	0.002%
42	6.760	1776	1779	1780	rVV	256	113	0.01%	0.001%
43	6.773	1780	1783	1787	rVB2	214	111	0.01%	0.001%
44	6.863	1809	1811	1814	rBV2	175	110	0.01%	0.001%
45	6.905	1821	1824	1827	rVB	215	156	0.01%	0.001%
46	6.924	1827	1830	1832	rBV	278	134	0.01%	0.001%
47	6.979	1835	1847	1881	rBV	142158	265967	19.73%	2.349%
48	7.156	1899	1902	1904	rBV2	377	248	0.02%	0.002%
49	7.223	1920	1923	1925	rBV3	364	246	0.02%	0.002%
50	7.307	1937	1949	1993	rBV	618011	1108494	82.24%	9.789%
51	7.612	2034	2044	2076	rBV	99781	179922	13.35%	1.589%
52	7.866	2121	2123	2125	rBV2	343	169	0.01%	0.001%
53	7.979	2156	2158	2161	rBV2	352	190	0.01%	0.002%
54	8.085	2180	2191	2221	rBV	363954	666816	49.47%	5.888%
55	8.391	2284	2286	2288	rBV2	343	184	0.01%	0.002%
56	8.490	2314	2317	2318	rBV2	323	211	0.02%	0.002%
57	8.587	2344	2347	2350	rBV2	298	166	0.01%	0.001%
58	8.612	2352	2355	2358	rBV2	344	293	0.02%	0.003%
59	8.648	2363	2366	2369	rVB2	344	189	0.01%	0.002%
60	8.677	2370	2375	2377	rBV2	362	258	0.02%	0.002%
61	8.712	2382	2386	2388	rBV	315	201	0.01%	0.002%
62	8.770	2398	2404	2408	rBV2	424	431	0.03%	0.004%
63	8.844	2413	2427	2462	rBV	764597	1256858	93.25%	11.099%
64	9.040	2486	2488	2492	rBV2	369	177	0.01%	0.002%
65	9.091	2501	2504	2506	rBV	316	196	0.01%	0.002%
66	9.127	2513	2515	2516	rBV	338	120	0.01%	0.001%
67	9.230	2541	2547	2548	rBV2	257	191	0.01%	0.002%
68	9.243	2548	2551	2554	rVB2	258	159	0.01%	0.001%
69	9.262	2554	2557	2559	rBV	266	135	0.01%	0.001%
70	9.317	2572	2574	2577	rBV2	202	143	0.01%	0.001%
71	9.349	2582	2584	2588	rBV	261	135	0.01%	0.001%
72	9.439	2609	2612	2616	rVB2	256	175	0.01%	0.002%
73	9.464	2616	2620	2621	rBV	230	150	0.01%	0.001%
74	9.545	2640	2645	2650	rBV3	349	439	0.03%	0.004%
75	9.567	2650	2652	2654	rVB	348	175	0.01%	0.002%
76	9.747	2704	2708	2709	rBV	220	116	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029662.D
 Acq On : 13 Dec 2022 19:32
 Operator : SY/MD
 Sample : N5980-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.876	2745	2748	2754	rVB2	249	181	0.01%	0.002%
78	9.905	2754	2757	2759	rBV	180	125	0.01%	0.001%
79	9.921	2759	2762	2763	rBV	237	140	0.01%	0.001%
80	9.992	2781	2784	2789	rVB2	211	125	0.01%	0.001%
81	10.162	2827	2837	2841	rBV2	19095	27631	2.05%	0.244%
82	10.207	2842	2851	2868	rVB	438999	689231	51.13%	6.086%
83	10.458	2925	2929	2933	rVB2	321	251	0.02%	0.002%
84	10.519	2946	2948	2950	rBV	374	179	0.01%	0.002%
85	10.567	2956	2963	2975	rVB3	8668	13688	1.02%	0.121%
86	10.680	2995	2998	3004	rVB2	248	145	0.01%	0.001%
87	10.712	3004	3008	3009	rBV	187	155	0.01%	0.001%
88	10.899	3063	3066	3067	rBV2	276	141	0.01%	0.001%
89	10.908	3067	3069	3071	rVV	322	125	0.01%	0.001%
90	10.944	3078	3080	3081	rBV	202	113	0.01%	0.001%
91	11.001	3093	3098	3103	rBV3	368	332	0.02%	0.003%
92	11.043	3107	3111	3116	rBV2	269	221	0.02%	0.002%
93	11.130	3135	3138	3143	rBV	364	345	0.03%	0.003%
94	11.236	3159	3171	3191	rBV	846445	1313294	97.43%	11.597%
95	11.545	3264	3267	3270	rBV3	696	589	0.04%	0.005%
96	11.612	3276	3288	3315	rBV	692376	1069691	79.36%	9.446%
97	11.918	3380	3383	3384	rBV2	294	167	0.01%	0.001%
98	11.992	3402	3406	3410	rBV2	362	427	0.03%	0.004%
99	12.243	3479	3484	3485	rBV3	284	260	0.02%	0.002%
100	12.474	3554	3556	3559	rBV2	277	224	0.02%	0.002%




Sum of corrected areas: 11324405

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029662.D
Acq On : 13 Dec 2022 19:32
Operator : SY/MD
Sample : N5980-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

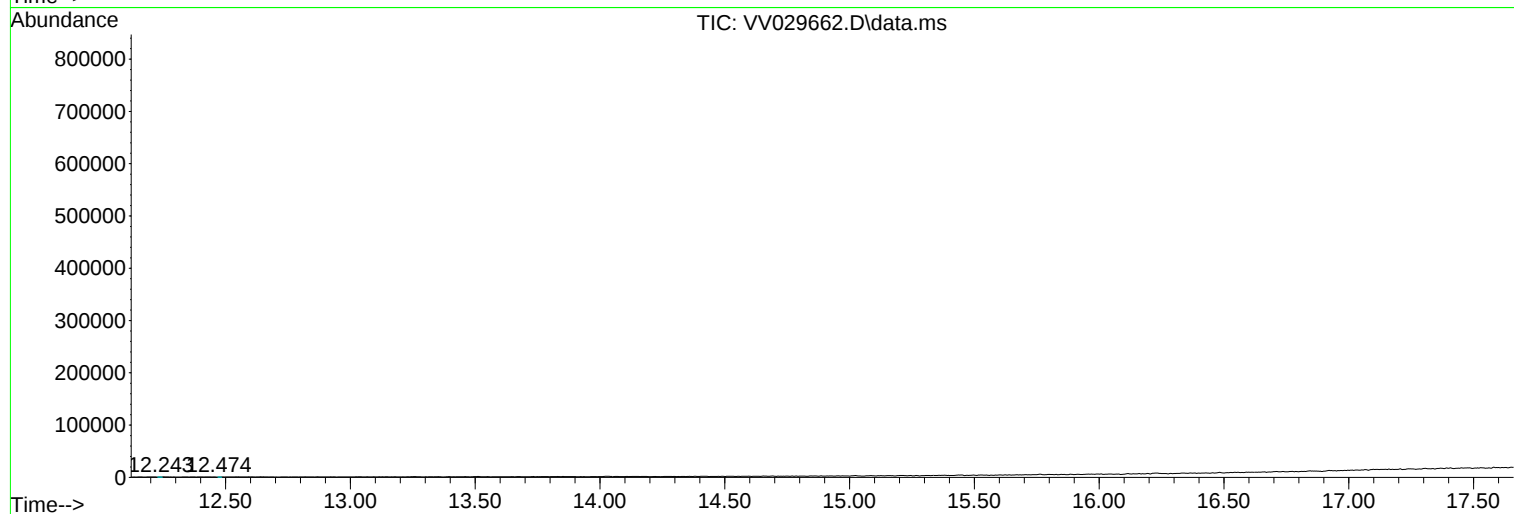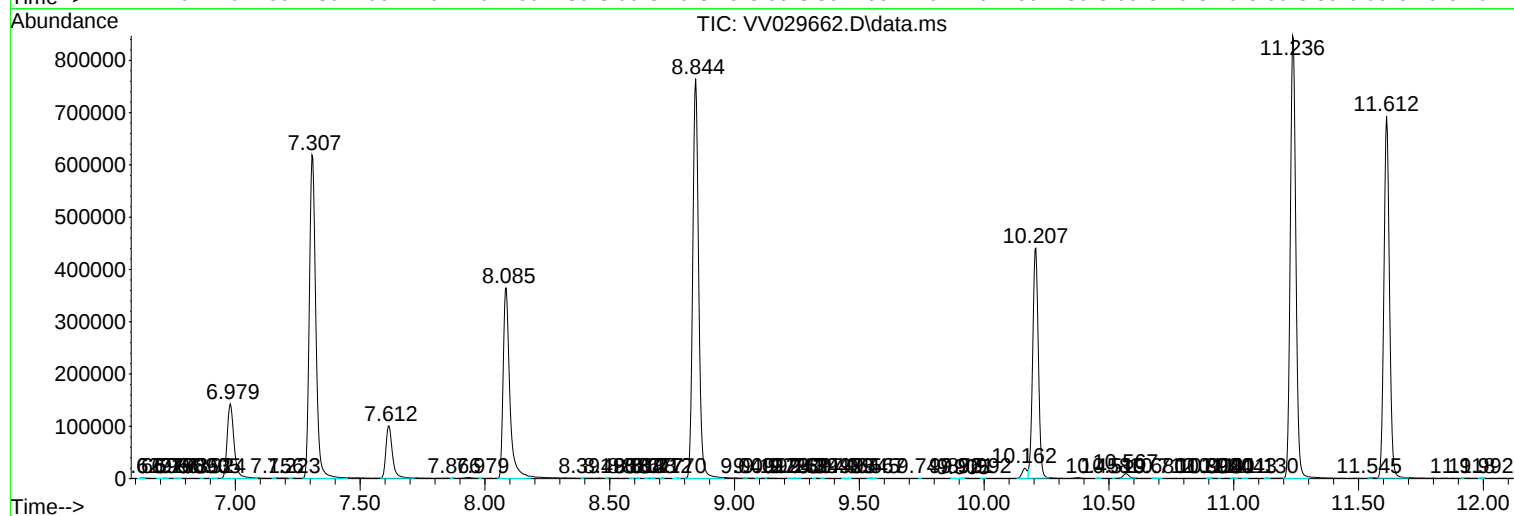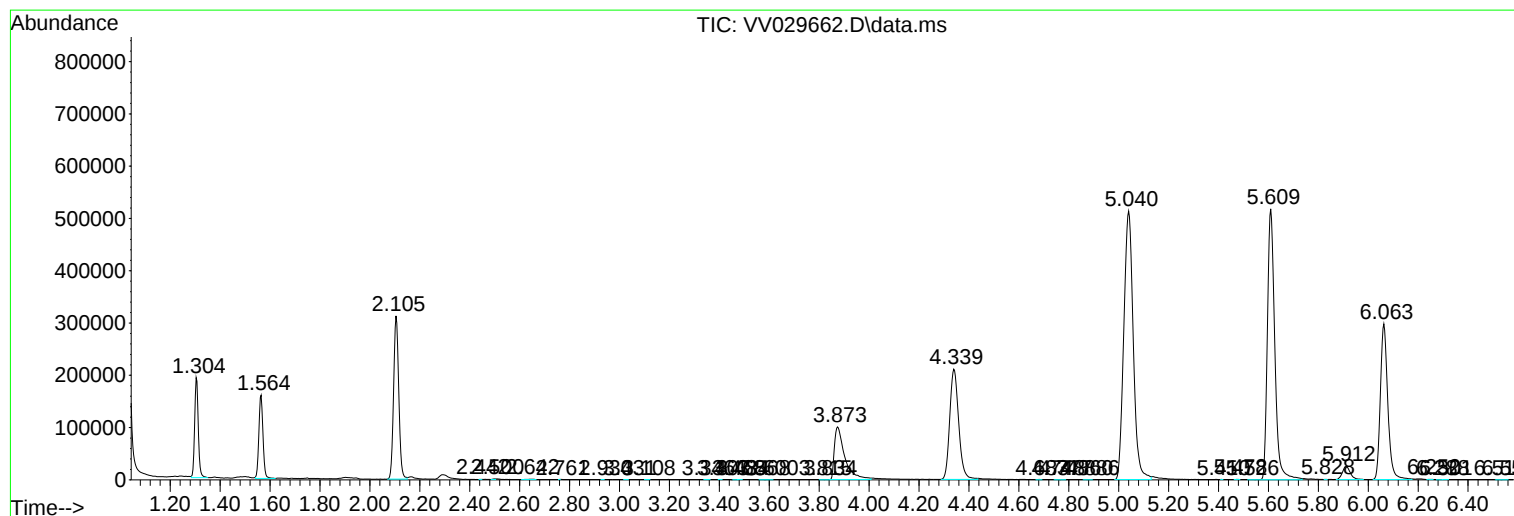

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029662.D
Acq On : 13 Dec 2022 19:32
Operator : SY/MD
Sample : N5980-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029662.D
Acq On : 13 Dec 2022 19:32
Operator : SY/MD
Sample : N5980-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------