

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029663.D
 Acq On : 13 Dec 2022 19:56
 Operator : SY/MD
 Sample : N5980-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029663.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	204974	197370	14.21%	1.686%
2	1.561	154	162	175	rVB	165091	186648	13.44%	1.595%
3	1.970	287	289	293	rBV3	335	199	0.01%	0.002%
4	2.031	304	308	312	rBV3	897	731	0.05%	0.006%
5	2.105	320	331	344	rBV2	328691	477493	34.38%	4.079%
6	2.282	377	386	411	rVB2	18861	41624	3.00%	0.356%
7	2.503	447	455	463	rVB3	2340	3345	0.24%	0.029%
8	2.552	468	470	473	rBV2	393	253	0.02%	0.002%
9	2.693	507	514	515	rBV2	208	210	0.02%	0.002%
10	2.761	526	535	547	rBV5	2686	4644	0.33%	0.040%
11	2.934	584	589	592	rBV2	233	228	0.02%	0.002%
12	3.079	629	634	638	rBV	329	280	0.02%	0.002%
13	3.105	639	642	647	rVV3	353	273	0.02%	0.002%
14	3.191	659	669	674	rVV2	942	1601	0.12%	0.014%
15	3.237	678	683	687	rBV2	323	257	0.02%	0.002%
16	3.870	870	880	918	rBV	102802	296405	21.34%	2.532%
17	4.085	943	947	951	rVB4	683	584	0.04%	0.005%
18	4.256	993	1000	1005	rVB5	509	800	0.06%	0.007%
19	4.339	1009	1026	1053	rBV	216583	540296	38.90%	4.616%
20	4.600	1096	1107	1119	rVB	1654	3320	0.24%	0.028%
21	4.671	1119	1129	1130	rBV3	1109	1615	0.12%	0.014%
22	4.815	1169	1174	1175	rBV	597	397	0.03%	0.003%
23	4.931	1205	1210	1214	rVB2	313	231	0.02%	0.002%
24	4.960	1214	1219	1225	rBV2	183	236	0.02%	0.002%
25	5.040	1225	1244	1292	rBV2	520703	1388834	100.00%	11.865%
26	5.529	1390	1396	1398	rBV3	210	210	0.02%	0.002%
27	5.548	1398	1402	1407	rVB3	306	226	0.02%	0.002%
28	5.609	1407	1421	1452	rBV	527359	1080794	77.82%	9.233%
29	5.902	1501	1512	1527	rVB8	5193	11756	0.85%	0.100%
30	6.063	1547	1562	1592	rBV	301802	626277	45.09%	5.350%
31	6.381	1656	1661	1664	rBV2	250	186	0.01%	0.002%
32	6.503	1692	1699	1700	rBV2	685	614	0.04%	0.005%
33	6.622	1731	1736	1737	rBV2	772	515	0.04%	0.004%
34	6.902	1820	1823	1829	rVB2	250	197	0.01%	0.002%
35	6.979	1836	1847	1873	rBV	147561	274389	19.76%	2.344%
36	7.175	1905	1908	1916	rVB5	508	529	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029663.D
 Acq On : 13 Dec 2022 19:56
 Operator : SY/MD
 Sample : N5980-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	7.204	1916	1917	1920	rVB2	435	191	0.01%	0.002%
38	7.236	1920	1927	1936	rVB9	1755	3155	0.23%	0.027%
39	7.307	1936	1949	1970	rBV	647323	1130660	81.41%	9.659%
40	7.465	1996	1998	2001	rVB	798	290	0.02%	0.002%
41	7.526	2014	2017	2022	rBV3	505	471	0.03%	0.004%
42	7.613	2033	2044	2068	rBV	104115	186000	13.39%	1.589%
43	7.754	2084	2088	2091	rBV3	205	197	0.01%	0.002%
44	7.838	2109	2114	2122	rVB7	1576	2119	0.15%	0.018%
45	7.973	2150	2156	2163	rVB5	2044	2898	0.21%	0.025%
46	8.082	2180	2190	2224	rBV	369990	682078	49.11%	5.827%
47	8.349	2267	2273	2277	rBV5	761	927	0.07%	0.008%
48	8.410	2289	2292	2297	rBV2	358	304	0.02%	0.003%
49	8.449	2303	2304	2308	rVB2	461	206	0.01%	0.002%
50	8.584	2341	2346	2350	rBV2	457	439	0.03%	0.004%
51	8.703	2378	2383	2388	rBV4	271	360	0.03%	0.003%
52	8.844	2415	2427	2454	rBV	792419	1296224	93.33%	11.074%
53	9.008	2472	2478	2488	rVB2	3300	4428	0.32%	0.038%
54	9.137	2510	2518	2527	rBV3	2619	3883	0.28%	0.033%
55	9.539	2636	2643	2648	rBV3	2837	4400	0.32%	0.038%
56	9.651	2676	2678	2684	rVB2	292	197	0.01%	0.002%
57	9.728	2694	2702	2705	rBV2	559	565	0.04%	0.005%
58	9.860	2737	2743	2746	rBV2	190	218	0.02%	0.002%
59	9.924	2755	2763	2771	rBV3	2907	4326	0.31%	0.037%
60	10.162	2827	2837	2841	rBV	20090	29313	2.11%	0.250%
61	10.204	2841	2850	2866	rVB	453561	708836	51.04%	6.056%
62	10.301	2877	2880	2885	rVB4	313	327	0.02%	0.003%
63	10.374	2897	2903	2913	rVB5	1790	2617	0.19%	0.022%
64	10.471	2928	2933	2939	rBV3	248	307	0.02%	0.003%
65	10.532	2944	2952	2956	rBV4	2548	3783	0.27%	0.032%
66	10.567	2956	2963	2981	rVB2	9103	14758	1.06%	0.126%
67	10.905	3060	3068	3078	rBV3	3035	4344	0.31%	0.037%
68	11.069	3115	3119	3124	rBV3	320	339	0.02%	0.003%
69	11.137	3135	3140	3145	rBV	268	315	0.02%	0.003%
70	11.175	3145	3152	3160	rBV3	2300	3376	0.24%	0.029%
71	11.236	3160	3171	3192	rBV	851026	1342294	96.65%	11.467%
72	11.464	3241	3242	3247	rVB2	412	189	0.01%	0.002%
73	11.484	3247	3248	3254	rVB2	345	217	0.02%	0.002%
74	11.558	3263	3271	3276	rBV4	1623	2136	0.15%	0.018%
75	11.612	3276	3288	3312	rBV	697502	1104640	79.54%	9.437%
76	11.809	3343	3349	3350	rBV3	540	422	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029663.D
 Acq On : 13 Dec 2022 19:56
 Operator : SY/MD
 Sample : N5980-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	11.956	3391	3395	3397	rVV2	327	261	0.02%	0.002%
78	11.985	3401	3404	3405	rBV	373	201	0.01%	0.002%
79	11.995	3405	3407	3412	rVB3	452	310	0.02%	0.003%
80	12.108	3439	3442	3447	rVB2	288	190	0.01%	0.002%
81	12.136	3447	3451	3453	rBV3	200	190	0.01%	0.002%
82	12.175	3457	3463	3465	rBV3	238	270	0.02%	0.002%
83	12.275	3492	3494	3498	rVB	387	220	0.02%	0.002%
84	12.400	3529	3533	3534	rBV	349	293	0.02%	0.003%
85	12.413	3534	3537	3545	rVV2	681	924	0.07%	0.008%
86	12.448	3546	3548	3551	rVB3	395	218	0.02%	0.002%
87	12.635	3600	3606	3614	rVB7	2853	3635	0.26%	0.031%
88	12.825	3662	3665	3672	rBV3	490	526	0.04%	0.004%
89	12.915	3689	3693	3697	rBV3	267	291	0.02%	0.002%
90	12.989	3711	3716	3722	rBV2	250	281	0.02%	0.002%
91	13.024	3723	3727	3729	rBV2	313	257	0.02%	0.002%
92	13.091	3744	3748	3750	rVV2	403	367	0.03%	0.003%
93	13.153	3763	3767	3769	rBV3	334	261	0.02%	0.002%
94	13.252	3791	3798	3806	rVV5	2318	3341	0.24%	0.029%
95	13.284	3806	3808	3815	rVB3	361	238	0.02%	0.002%
96	13.497	3866	3874	3887	rBV2	2238	3733	0.27%	0.032%
97	13.728	3941	3946	3949	rBV4	2019	2202	0.16%	0.019%
98	13.783	3961	3963	3967	rBV2	370	303	0.02%	0.003%
99	13.841	3979	3981	3984	rBV2	310	198	0.01%	0.002%
100	14.361	4140	4143	4148	rBV4	474	568	0.04%	0.005%




Sum of corrected areas: 11705594

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029663.D
Acq On : 13 Dec 2022 19:56
Operator : SY/MD
Sample : N5980-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

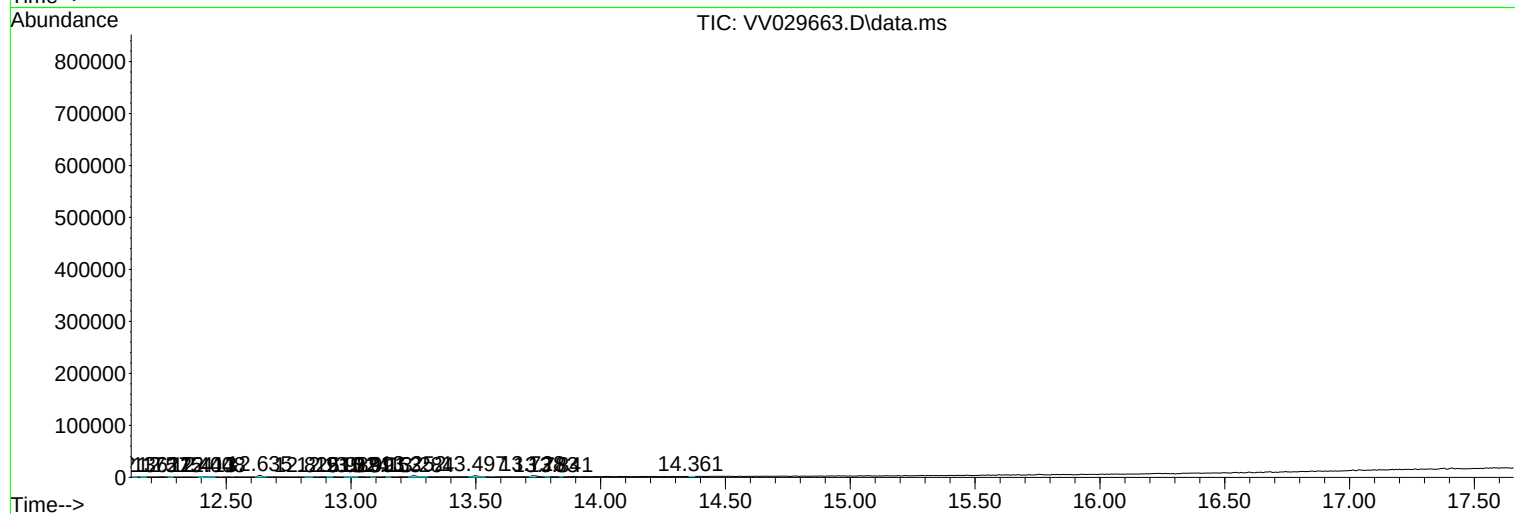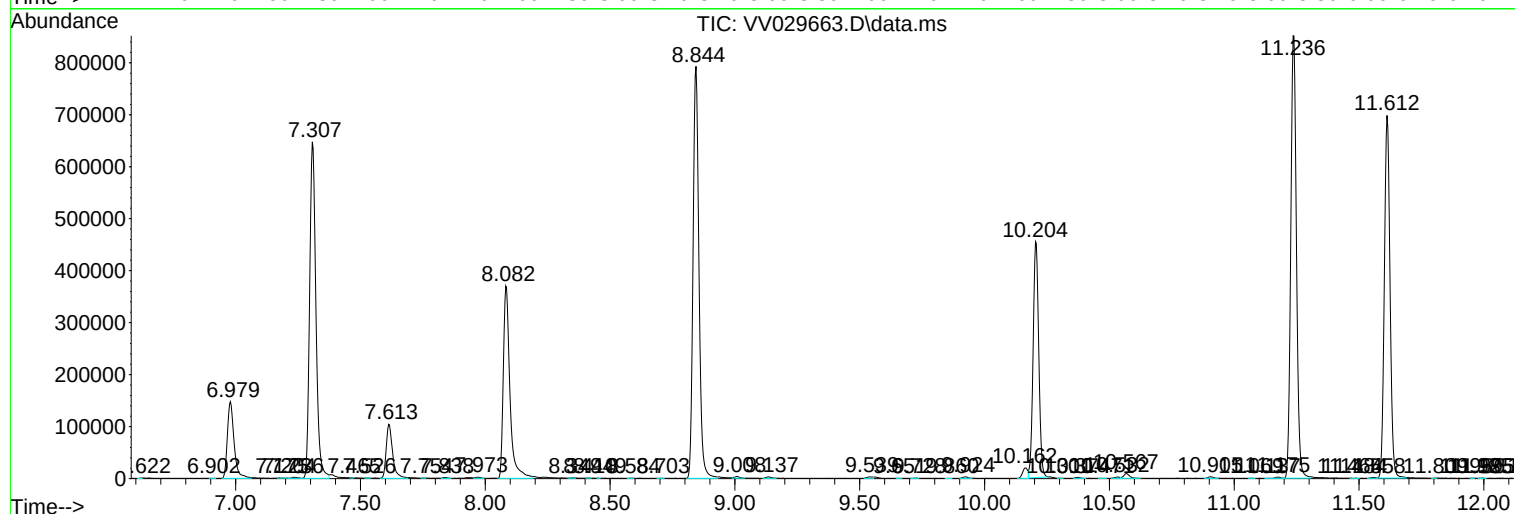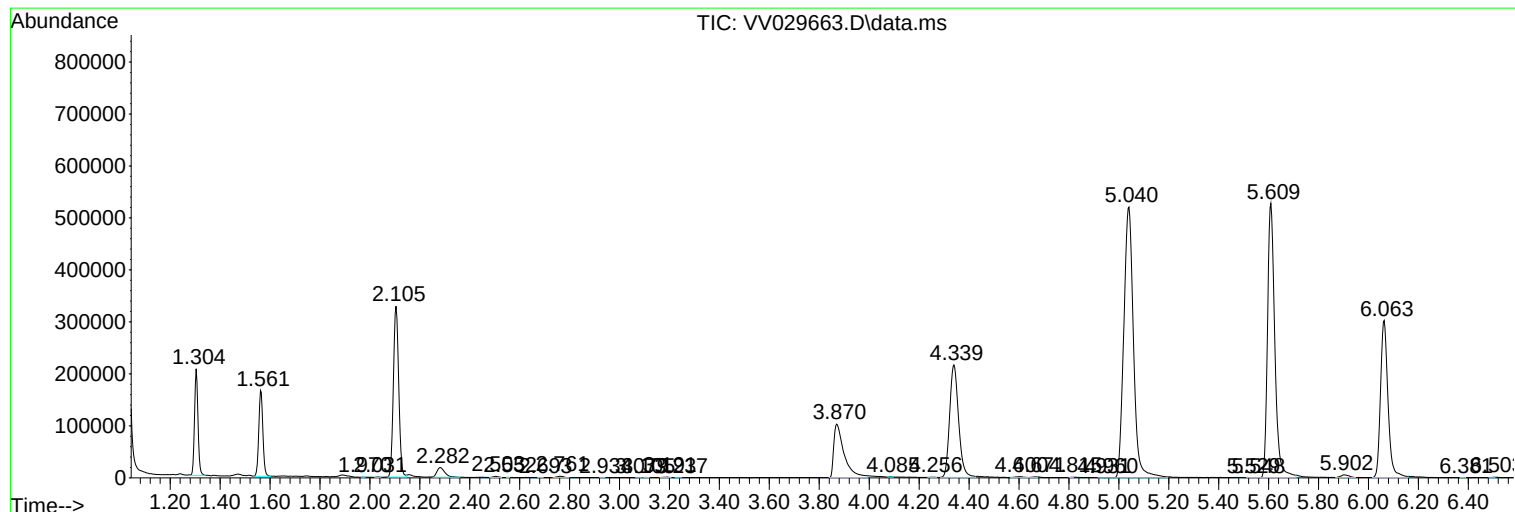

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029663.D
Acq On : 13 Dec 2022 19:56
Operator : SY/MD
Sample : N5980-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029663.D
Acq On : 13 Dec 2022 19:56
Operator : SY/MD
Sample : N5980-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------