

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029667.D
 Acq On : 13 Dec 2022 21:54
 Operator : SY/MD
 Sample : N5928-14DL 25X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ75DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M

Title : VOC Analysis

Signal : TIC: VW029667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	193694	196624	10.99%	1.352%
2	1.564	155	163	178	rVB	170397	189876	10.61%	1.305%
3	2.105	320	331	345	rBV	334319	483747	27.03%	3.326%
4	2.503	447	455	464	rVB2	3761	6240	0.35%	0.043%
5	2.542	464	467	468	rBV	227	97	0.01%	0.001%
6	2.555	469	471	473	rVB2	270	114	0.01%	0.001%
7	2.719	519	522	526	rBV2	177	144	0.01%	0.001%
8	2.760	526	535	546	rBV4	5140	9393	0.52%	0.065%
9	2.918	581	584	586	rBV2	204	138	0.01%	0.001%
10	2.966	592	599	601	rBV2	191	216	0.01%	0.001%
11	2.995	605	608	611	rVV	165	95	0.01%	0.001%
12	3.072	629	632	634	rVV	245	183	0.01%	0.001%
13	3.185	653	667	687	rBV	44000	93226	5.21%	0.641%
14	3.320	708	709	710	rBV	333	88	0.00%	0.001%
15	3.362	720	722	727	rVB	362	234	0.01%	0.002%
16	3.387	727	730	734	rBV	250	169	0.01%	0.001%
17	3.452	747	750	752	rBV	174	93	0.01%	0.001%
18	3.523	770	772	774	rVB	218	87	0.00%	0.001%
19	3.539	774	777	781	rVB2	254	196	0.01%	0.001%
20	3.902	870	890	927	rBV2	630169	1789339	100.00%	12.301%
21	4.339	1011	1026	1049	rBV	222239	548598	30.66%	3.771%
22	4.600	1088	1107	1136	rBV	379890	954583	53.35%	6.562%
23	4.892	1195	1198	1200	rBV	280	131	0.01%	0.001%
24	5.040	1226	1244	1281	rBV2	539317	1423578	79.56%	9.787%
25	5.310	1326	1328	1331	rBV2	316	194	0.01%	0.001%
26	5.436	1365	1367	1372	rVB2	234	119	0.01%	0.001%
27	5.468	1372	1377	1378	rBV2	557	399	0.02%	0.003%
28	5.519	1390	1393	1398	rBV2	235	197	0.01%	0.001%
29	5.609	1408	1421	1453	rBV	553931	1123186	62.77%	7.722%
30	5.902	1501	1512	1530	rVB4	6467	15182	0.85%	0.104%
31	6.063	1548	1562	1592	rVV	305548	636285	35.56%	4.374%
32	6.288	1629	1632	1633	rBV	175	107	0.01%	0.001%
33	6.323	1641	1643	1646	rVB	253	142	0.01%	0.001%
34	6.342	1646	1649	1654	rBV2	184	142	0.01%	0.001%
35	6.436	1672	1678	1687	rBV2	272	407	0.02%	0.003%
36	6.474	1688	1690	1693	rBV2	185	102	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029667.D
 Acq On : 13 Dec 2022 21:54
 Operator : SY/MD
 Sample : N5928-14DL 25X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ75DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.516	1698	1703	1706	rBV3	288	260	0.01%	0.002%
38	6.571	1718	1720	1723	rVB2	187	87	0.00%	0.001%
39	6.593	1723	1727	1729	rBV	158	118	0.01%	0.001%
40	6.625	1729	1737	1739	rBV2	727	804	0.04%	0.006%
41	6.709	1760	1763	1764	rBV	171	101	0.01%	0.001%
42	6.979	1836	1847	1874	rBV	153211	278841	15.58%	1.917%
43	7.307	1936	1949	1967	rBV	660880	1162535	64.97%	7.992%
44	7.612	2034	2044	2077	rVB	109314	192892	10.78%	1.326%
45	7.834	2108	2113	2126	rVB6	1151	1711	0.10%	0.012%
46	7.886	2127	2129	2131	rBV	333	119	0.01%	0.001%
47	8.040	2176	2177	2180	rBV2	304	128	0.01%	0.001%
48	8.082	2180	2190	2224	rBV	381475	692834	38.72%	4.763%
49	8.436	2298	2300	2301	rBV	280	103	0.01%	0.001%
50	8.590	2344	2348	2349	rBV	336	250	0.01%	0.002%
51	8.628	2356	2360	2363	rBV2	484	364	0.02%	0.003%
52	8.657	2367	2369	2375	rBV2	293	193	0.01%	0.001%
53	8.696	2379	2381	2383	rBV2	153	83	0.00%	0.001%
54	8.722	2385	2389	2391	rBV3	372	304	0.02%	0.002%
55	8.796	2410	2412	2414	rBV	461	273	0.02%	0.002%
56	8.844	2415	2427	2464	rVV	801383	1325370	74.07%	9.111%
57	9.098	2503	2506	2507	rBV2	444	206	0.01%	0.001%
58	9.133	2509	2517	2527	rVB2	10183	15416	0.86%	0.106%
59	9.191	2532	2535	2540	rVB4	916	743	0.04%	0.005%
60	9.220	2542	2544	2548	rVB	306	197	0.01%	0.001%
61	9.246	2549	2552	2554	rBV2	233	124	0.01%	0.001%
62	9.281	2561	2563	2566	rBV2	180	82	0.00%	0.001%
63	9.300	2566	2569	2572	rVB2	215	144	0.01%	0.001%
64	9.345	2581	2583	2586	rVV	233	133	0.01%	0.001%
65	9.378	2588	2593	2596	rBV4	281	254	0.01%	0.002%
66	9.426	2606	2608	2613	rVB	252	167	0.01%	0.001%
67	9.452	2613	2616	2617	rBV	312	196	0.01%	0.001%
68	9.535	2633	2642	2658	rBV2	10474	18217	1.02%	0.125%
69	9.661	2679	2681	2683	rBV2	173	99	0.01%	0.001%
70	9.741	2704	2706	2710	rVB	197	106	0.01%	0.001%
71	9.783	2714	2719	2722	rBV3	900	1027	0.06%	0.007%
72	9.818	2727	2730	2733	rVB3	231	138	0.01%	0.001%
73	9.831	2733	2734	2736	rBV3	248	122	0.01%	0.001%
74	10.162	2828	2837	2841	rBV2	20051	29103	1.63%	0.200%
75	10.207	2842	2851	2870	rVB	457832	719075	40.19%	4.943%
76	10.345	2889	2894	2902	rBV4	2124	2008	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029667.D
 Acq On : 13 Dec 2022 21:54
 Operator : SY/MD
 Sample : N5928-14DL 25X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ75DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.439	2914	2923	2929	rBV2	9717	15789	0.88%	0.109%
78	10.529	2943	2951	2957	rBV	9878	13639	0.76%	0.094%
79	10.728	3005	3013	3025	rVB2	8811	13033	0.73%	0.090%
80	10.831	3042	3045	3046	rBV	180	100	0.01%	0.001%
81	10.847	3047	3050	3054	rVB4	292	242	0.01%	0.002%
82	10.905	3059	3068	3078	rBV	20098	30329	1.69%	0.209%
83	10.972	3086	3089	3091	rBV	278	132	0.01%	0.001%
84	10.988	3091	3094	3096	rBV	141	93	0.01%	0.001%
85	11.030	3105	3107	3109	rBV	335	158	0.01%	0.001%
86	11.111	3129	3132	3137	rVB	557	323	0.02%	0.002%
87	11.143	3137	3142	3145	rBV	586	473	0.03%	0.003%
88	11.236	3160	3171	3191	rBV	892669	1385735	77.44%	9.526%
89	11.522	3251	3260	3265	rBV5	4280	7208	0.40%	0.050%
90	11.612	3277	3288	3308	rVB	705789	1122671	62.74%	7.718%
91	11.808	3345	3349	3359	rVB3	1631	1980	0.11%	0.014%
92	11.914	3371	3382	3395	rBV5	5281	11167	0.62%	0.077%
93	12.008	3406	3411	3418	rVB3	2229	2401	0.13%	0.017%
94	12.075	3426	3432	3434	rBV	457	416	0.02%	0.003%
95	12.403	3525	3534	3541	rBV4	1315	2093	0.12%	0.014%
96	12.599	3593	3595	3598	rBV3	714	469	0.03%	0.003%
97	12.635	3601	3606	3613	rVB3	2096	2845	0.16%	0.020%
98	12.824	3663	3665	3666	rBV2	279	99	0.01%	0.001%
99	13.413	3847	3848	3853	rVB3	745	304	0.02%	0.002%
100	13.496	3865	3874	3884	rBV2	9551	15878	0.89%	0.109%




Sum of corrected areas: 14546155

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029667.D
Acq On : 13 Dec 2022 21:54
Operator : SY/MD
Sample : N5928-14DL 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

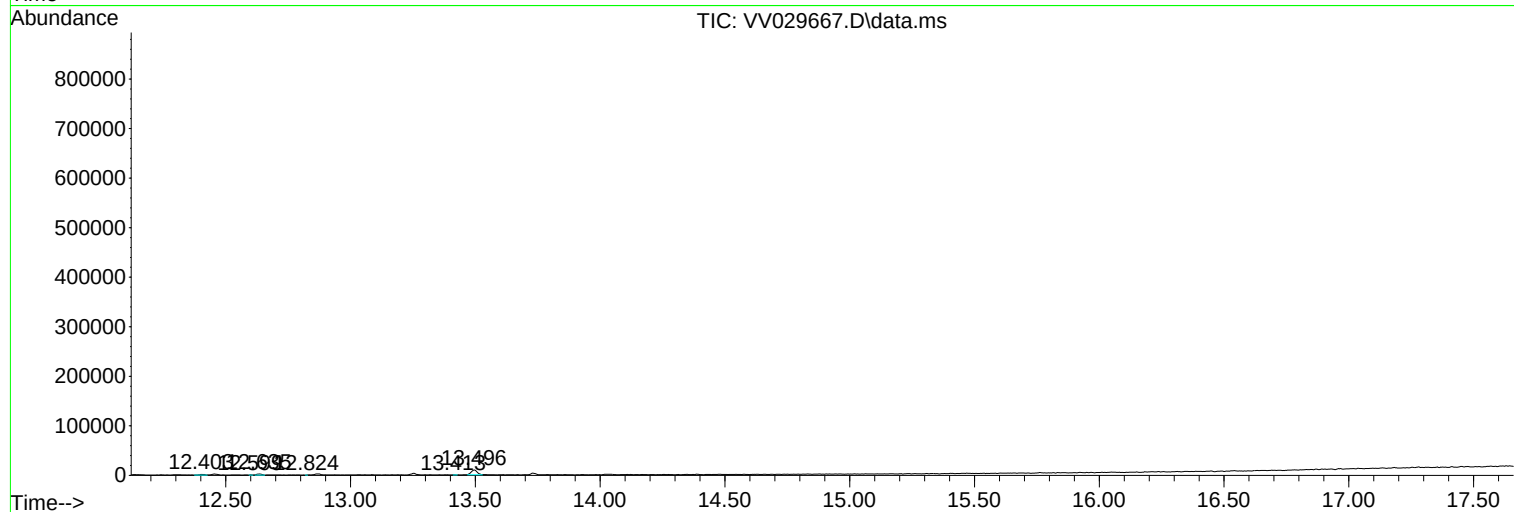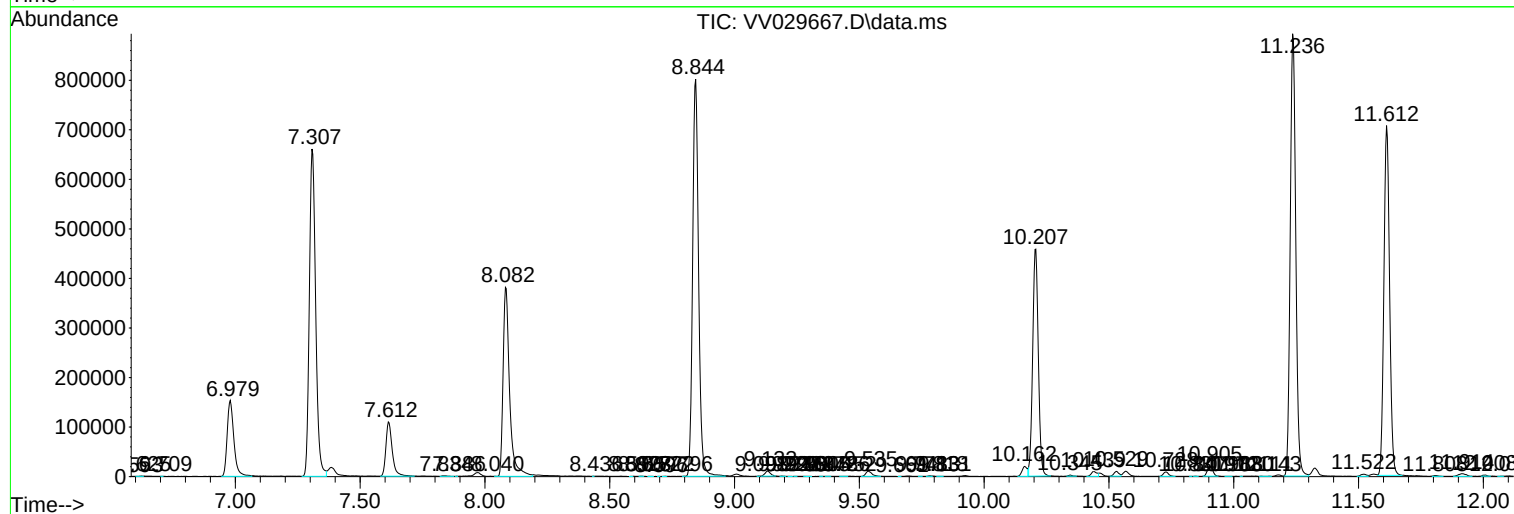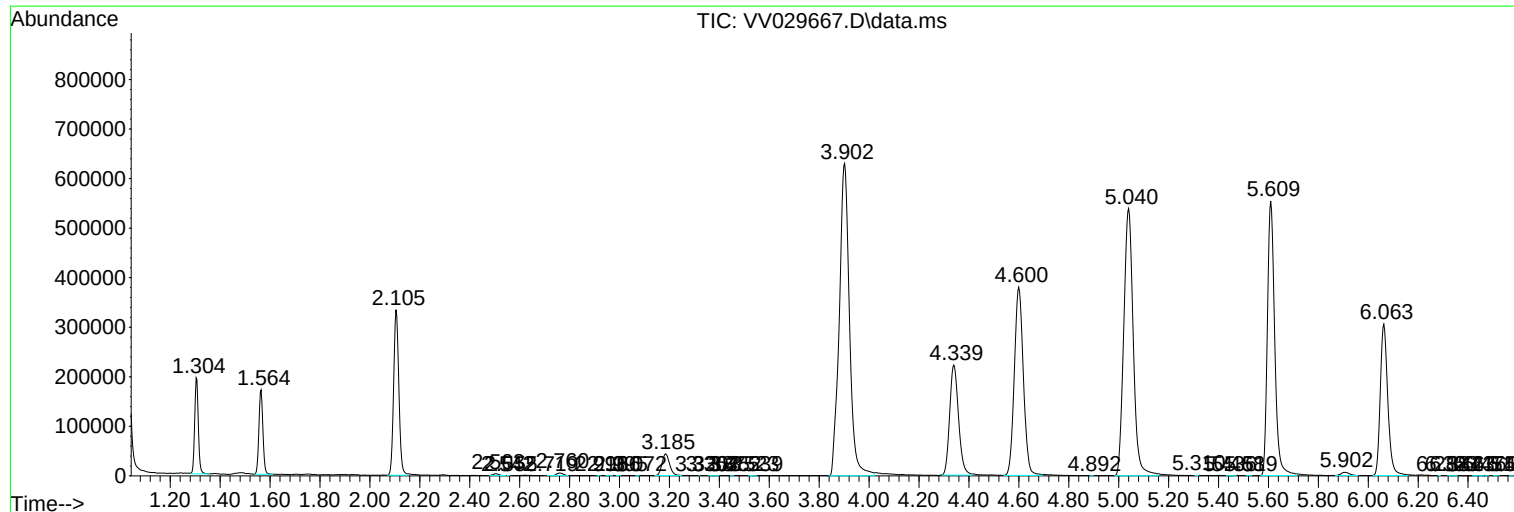

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029667.D
Acq On : 13 Dec 2022 21:54
Operator : SY/MD
Sample : N5928-14DL 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029667.D
Acq On : 13 Dec 2022 21:54
Operator : SY/MD
Sample : N5928-14DL 25X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc