

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029668.D
 Acq On : 13 Dec 2022 22:17
 Operator : SY/MD
 Sample : N5928-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029668.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	227753	227519	14.86%	1.850%
2	1.565	155	163	178	rVB	192587	214268	14.00%	1.742%
3	2.105	320	331	347	rBV	367093	526778	34.41%	4.283%
4	2.503	446	455	470	rVB	9239	15136	0.99%	0.123%
5	2.671	506	507	511	rBV2	161	100	0.01%	0.001%
6	2.905	574	580	582	rBV2	161	179	0.01%	0.001%
7	3.040	620	622	627	rVB2	189	105	0.01%	0.001%
8	3.166	658	661	667	rBV2	136	127	0.01%	0.001%
9	3.211	672	675	678	rVB	189	106	0.01%	0.001%
10	3.298	699	702	703	rBV2	307	162	0.01%	0.001%
11	3.420	737	740	742	rBV	171	111	0.01%	0.001%
12	3.494	759	763	766	rBV	228	220	0.01%	0.002%
13	3.600	790	796	802	rBV2	139	167	0.01%	0.001%
14	3.674	818	819	829	rVB	230	152	0.01%	0.001%
15	3.722	829	834	837	rBV2	144	183	0.01%	0.001%
16	3.790	851	855	859	rBV	216	224	0.01%	0.002%
17	3.873	872	881	929	rBV	111806	330083	21.56%	2.684%
18	4.339	1010	1026	1057	rBV	234348	580126	37.90%	4.716%
19	4.671	1127	1129	1131	rBV	248	153	0.01%	0.001%
20	4.799	1164	1169	1173	rBV2	255	212	0.01%	0.002%
21	4.854	1182	1186	1187	rBV2	181	133	0.01%	0.001%
22	4.899	1196	1200	1203	rBV2	161	139	0.01%	0.001%
23	4.934	1210	1211	1216	rVB	212	108	0.01%	0.001%
24	4.973	1220	1223	1226	rBV2	166	133	0.01%	0.001%
25	5.040	1226	1244	1296	rBV2	575579	1530667	100.00%	12.444%
26	5.532	1395	1397	1401	rVV2	170	96	0.01%	0.001%
27	5.609	1408	1421	1459	rBV	527614	1072482	70.07%	8.719%
28	5.899	1504	1511	1523	rVB8	5113	9925	0.65%	0.081%
29	6.063	1548	1562	1593	rBV	330928	675777	44.15%	5.494%
30	6.326	1641	1644	1647	rBV	144	94	0.01%	0.001%
31	6.423	1671	1674	1676	rBV	291	143	0.01%	0.001%
32	6.468	1683	1688	1691	rBV2	164	177	0.01%	0.001%
33	6.484	1691	1693	1698	rVB2	266	158	0.01%	0.001%
34	6.529	1703	1707	1710	rBV2	144	132	0.01%	0.001%
35	6.568	1716	1719	1722	rBV2	313	231	0.02%	0.002%
36	6.706	1761	1762	1765	rVB	264	122	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029668.D
 Acq On : 13 Dec 2022 22:17
 Operator : SY/MD
 Sample : N5928-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.828	1798	1800	1804	rVB3	188	134	0.01%	0.001%
38	6.867	1810	1812	1815	rBV2	277	131	0.01%	0.001%
39	6.979	1835	1847	1872	rBV	162124	296777	19.39%	2.413%
40	7.153	1899	1901	1902	rBV	343	171	0.01%	0.001%
41	7.227	1922	1924	1926	rBV2	241	95	0.01%	0.001%
42	7.307	1937	1949	1981	rBV	715269	1264819	82.63%	10.283%
43	7.613	2034	2044	2069	rBV	114805	203441	13.29%	1.654%
44	7.786	2096	2098	2100	rBV2	501	206	0.01%	0.002%
45	7.850	2115	2118	2120	rBV3	269	204	0.01%	0.002%
46	8.014	2167	2169	2170	rBV	244	103	0.01%	0.001%
47	8.085	2180	2191	2231	rBV	401347	740522	48.38%	6.020%
48	8.362	2274	2277	2280	rBV3	453	393	0.03%	0.003%
49	8.442	2299	2302	2304	rBV2	316	218	0.01%	0.002%
50	8.484	2313	2315	2317	rVB2	363	115	0.01%	0.001%
51	8.497	2317	2319	2320	rBV2	284	119	0.01%	0.001%
52	8.542	2330	2333	2334	rBV	311	190	0.01%	0.002%
53	8.574	2341	2343	2346	rVB2	473	267	0.02%	0.002%
54	8.596	2346	2350	2352	rBV	154	110	0.01%	0.001%
55	8.619	2355	2357	2362	rVV2	337	236	0.02%	0.002%
56	8.645	2362	2365	2367	rVB3	335	165	0.01%	0.001%
57	8.674	2372	2374	2376	rVB	366	118	0.01%	0.001%
58	8.709	2382	2385	2386	rBV	247	144	0.01%	0.001%
59	8.764	2400	2402	2403	rBV	277	138	0.01%	0.001%
60	8.844	2414	2427	2460	rBV	767396	1271822	83.09%	10.340%
61	9.124	2511	2514	2517	rBV3	311	251	0.02%	0.002%
62	9.291	2563	2566	2569	rBV2	183	119	0.01%	0.001%
63	9.384	2593	2595	2604	rVB2	278	296	0.02%	0.002%
64	9.432	2604	2610	2612	rBV	174	179	0.01%	0.001%
65	9.632	2669	2672	2675	rBV	185	125	0.01%	0.001%
66	9.661	2679	2681	2684	rVB	262	139	0.01%	0.001%
67	9.706	2692	2695	2699	rVB	244	150	0.01%	0.001%
68	9.805	2723	2726	2733	rBV	213	219	0.01%	0.002%
69	9.834	2733	2735	2739	rBV	177	105	0.01%	0.001%
70	9.854	2739	2741	2745	rVB2	306	243	0.02%	0.002%
71	9.883	2745	2750	2752	rBV	220	186	0.01%	0.002%
72	9.918	2757	2761	2768	rBV2	338	486	0.03%	0.004%
73	9.953	2770	2772	2776	rVB	231	111	0.01%	0.001%
74	10.092	2813	2815	2817	rBV	293	116	0.01%	0.001%
75	10.162	2827	2837	2841	rBV2	19876	29149	1.90%	0.237%
76	10.207	2841	2851	2871	rVB	483336	760375	49.68%	6.182%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029668.D
 Acq On : 13 Dec 2022 22:17
 Operator : SY/MD
 Sample : N5928-23
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.365	2896	2900	2907	rBV2	550	698	0.05%	0.006%
78	10.432	2917	2921	2925	rBV2	330	246	0.02%	0.002%
79	10.448	2925	2926	2929	rVV2	164	90	0.01%	0.001%
80	10.461	2929	2930	2933	rVB	222	93	0.01%	0.001%
81	10.529	2946	2951	2954	rBV5	453	492	0.03%	0.004%
82	10.571	2955	2964	2977	rVB2	9711	15903	1.04%	0.129%
83	10.754	3019	3021	3024	rVB	274	143	0.01%	0.001%
84	10.799	3032	3035	3037	rBV	133	120	0.01%	0.001%
85	10.857	3050	3053	3057	rVB	400	222	0.01%	0.002%
86	10.886	3060	3062	3063	rBV	298	110	0.01%	0.001%
87	11.063	3114	3117	3122	rBV3	225	199	0.01%	0.002%
88	11.178	3144	3153	3160	rBV6	1255	1951	0.13%	0.016%
89	11.236	3160	3171	3199	rBV	861438	1331937	87.02%	10.829%
90	11.474	3241	3245	3248	rBV2	256	196	0.01%	0.002%
91	11.493	3248	3251	3257	rBV2	431	372	0.02%	0.003%
92	11.542	3264	3266	3268	rBV2	379	235	0.02%	0.002%
93	11.612	3276	3288	3314	rBV	745694	1184917	77.41%	9.633%
94	11.837	3354	3358	3362	rBV2	407	314	0.02%	0.003%
95	11.892	3370	3375	3380	rBV3	277	237	0.02%	0.002%
96	12.062	3425	3428	3432	rBV2	359	180	0.01%	0.001%
97	12.226	3475	3479	3480	rBV	334	241	0.02%	0.002%
98	12.281	3494	3496	3498	rBV2	370	180	0.01%	0.001%
99	12.580	3586	3589	3591	rBV3	225	146	0.01%	0.001%
100	12.635	3600	3606	3612	rVB4	1242	1455	0.10%	0.012%




Sum of corrected areas: 12300192

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029668.D
Acq On : 13 Dec 2022 22:17
Operator : SY/MD
Sample : N5928-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

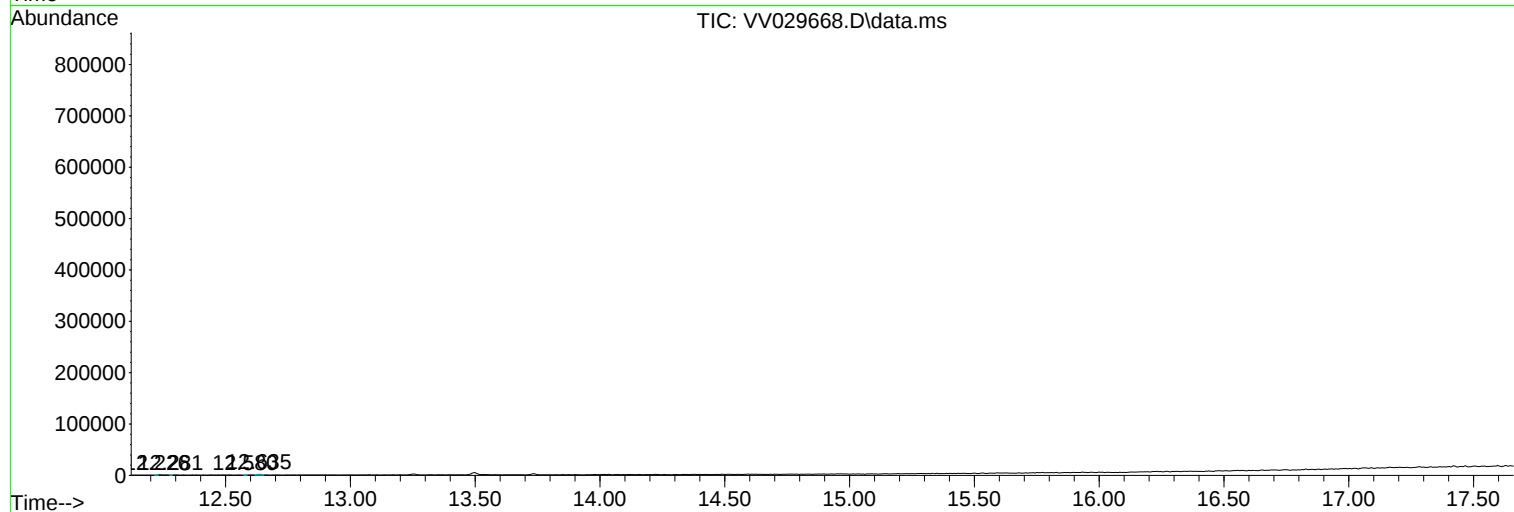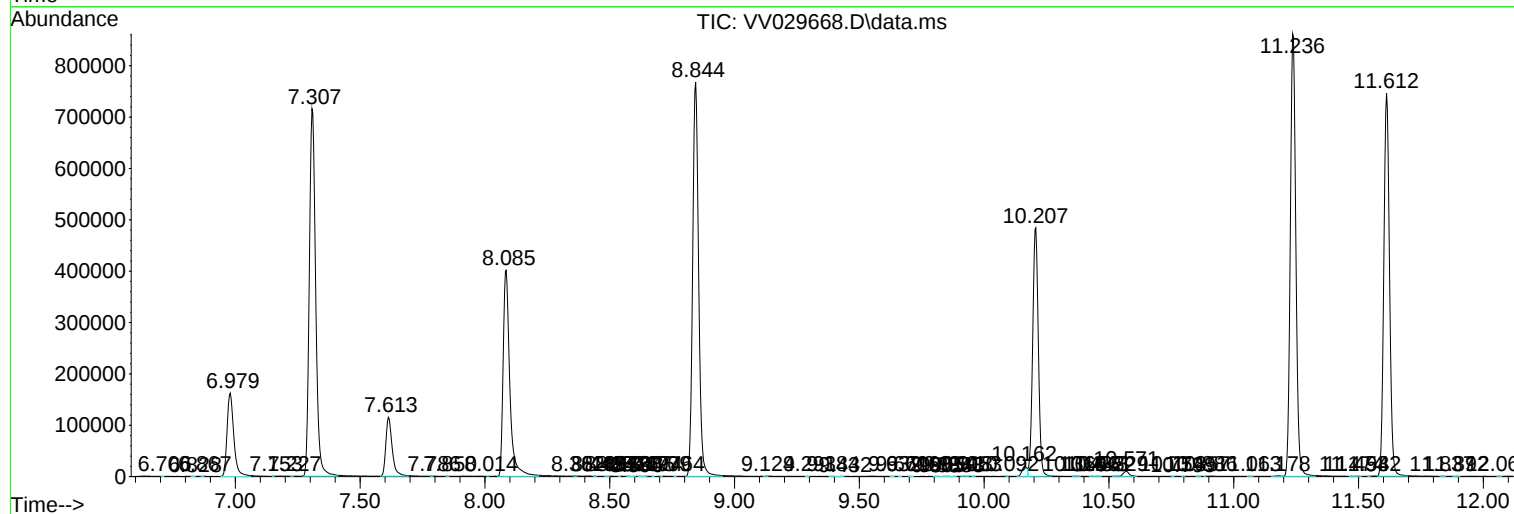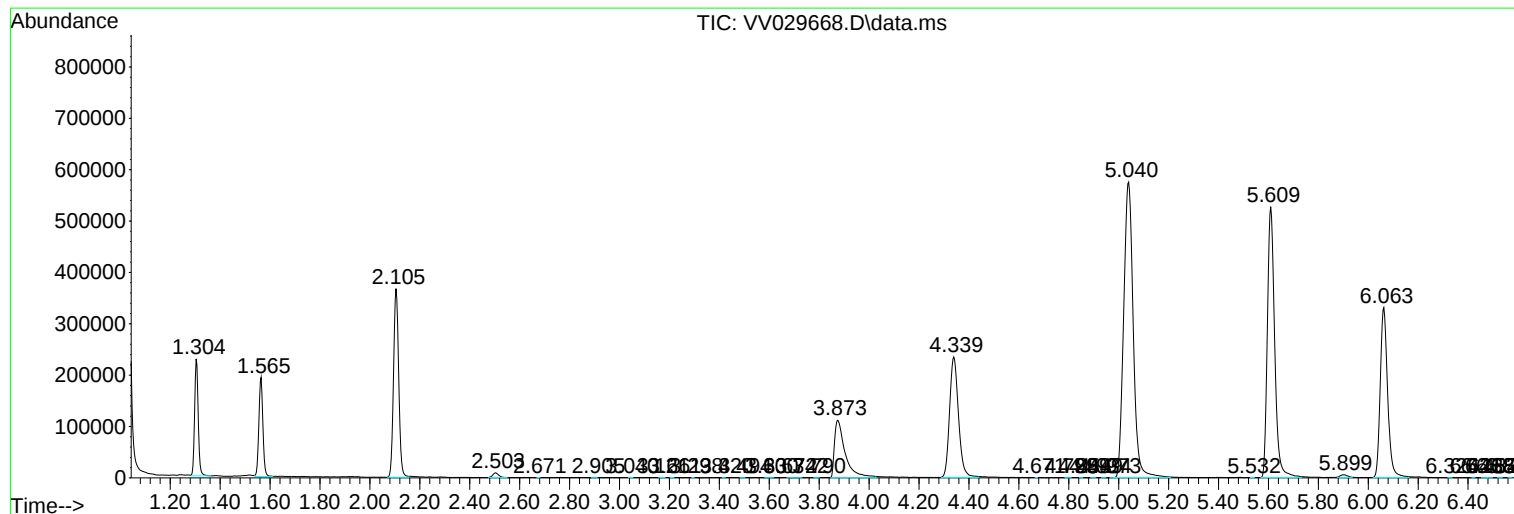

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029668.D
Acq On : 13 Dec 2022 22:17
Operator : SY/MD
Sample : N5928-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029668.D
Acq On : 13 Dec 2022 22:17
Operator : SY/MD
Sample : N5928-23
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc