

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029669.D
 Acq On : 13 Dec 2022 22:41
 Operator : SY/MD
 Sample : N5950-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	221360	223511	14.61%	1.809%
2	1.564	155	163	178	rVB	187213	212068	13.86%	1.717%
3	2.104	320	331	348	rBV	360157	519412	33.95%	4.204%
4	2.281	382	386	387	rBV	800	461	0.03%	0.004%
5	2.445	434	437	442	rBV3	300	213	0.01%	0.002%
6	2.503	446	455	467	rVB3	10027	16049	1.05%	0.130%
7	2.555	467	471	473	rBV2	247	217	0.01%	0.002%
8	2.577	476	478	480	rBV	267	121	0.01%	0.001%
9	2.645	495	499	500	rBV2	222	153	0.01%	0.001%
10	2.703	515	517	520	rBV2	229	117	0.01%	0.001%
11	2.796	543	546	549	rBV	281	163	0.01%	0.001%
12	2.928	583	587	589	rBV2	258	215	0.01%	0.002%
13	3.137	649	652	655	rVB	294	161	0.01%	0.001%
14	3.233	680	682	686	rBV	183	139	0.01%	0.001%
15	3.432	740	744	747	rBV2	161	143	0.01%	0.001%
16	3.471	753	756	760	rBV2	177	158	0.01%	0.001%
17	3.526	768	773	776	rBV2	208	191	0.01%	0.002%
18	3.741	838	840	844	rVB	187	106	0.01%	0.001%
19	3.796	853	857	860	rBV	154	144	0.01%	0.001%
20	3.873	871	881	915	rBV	119606	343532	22.45%	2.781%
21	4.339	1010	1026	1048	rBV	236122	577268	37.73%	4.673%
22	4.657	1118	1125	1129	rBV3	240	231	0.02%	0.002%
23	4.677	1129	1131	1132	rBV3	278	106	0.01%	0.001%
24	4.725	1142	1146	1148	rBV2	162	123	0.01%	0.001%
25	4.802	1168	1170	1175	rVB2	199	117	0.01%	0.001%
26	4.876	1190	1193	1197	rBV2	260	222	0.01%	0.002%
27	4.937	1207	1212	1213	rBV2	305	211	0.01%	0.002%
28	5.040	1225	1244	1286	rBV2	582191	1529895	100.00%	12.384%
29	5.436	1363	1367	1369	rVB2	317	216	0.01%	0.002%
30	5.461	1369	1375	1377	rBV2	421	356	0.02%	0.003%
31	5.516	1386	1392	1394	rBV3	205	213	0.01%	0.002%
32	5.548	1400	1402	1405	rVB2	158	107	0.01%	0.001%
33	5.609	1408	1421	1451	rBV	522335	1061018	69.35%	8.589%
34	5.902	1503	1512	1528	rVB4	5967	12443	0.81%	0.101%
35	6.008	1543	1545	1548	rBV2	220	161	0.01%	0.001%
36	6.063	1548	1562	1598	rBV	329021	688822	45.02%	5.576%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029669.D
 Acq On : 13 Dec 2022 22:41
 Operator : SY/MD
 Sample : N5950-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.432	1671	1677	1680	rBV2	233	181	0.01%	0.001%
38	6.551	1710	1714	1716	rBV	163	132	0.01%	0.001%
39	6.625	1733	1737	1740	rBV4	751	646	0.04%	0.005%
40	6.725	1765	1768	1770	rBV	162	111	0.01%	0.001%
41	6.789	1784	1788	1792	rBV2	147	136	0.01%	0.001%
42	6.812	1792	1795	1801	rVV3	247	217	0.01%	0.002%
43	6.915	1822	1827	1829	rVB2	178	120	0.01%	0.001%
44	6.937	1831	1834	1836	rBV	303	165	0.01%	0.001%
45	6.979	1836	1847	1880	rBV	162519	298314	19.50%	2.415%
46	7.159	1900	1903	1906	rBV4	808	662	0.04%	0.005%
47	7.233	1924	1926	1928	rBV2	325	124	0.01%	0.001%
48	7.307	1937	1949	1980	rBV	714573	1265917	82.75%	10.247%
49	7.612	2032	2044	2073	rBV	116374	203609	13.31%	1.648%
50	7.789	2096	2099	2100	rBV2	372	178	0.01%	0.001%
51	8.082	2180	2190	2221	rBV	425120	774535	50.63%	6.270%
52	8.567	2337	2341	2346	rBV3	561	461	0.03%	0.004%
53	8.609	2346	2354	2360	rBV5	527	798	0.05%	0.006%
54	8.648	2364	2366	2369	rVB2	366	186	0.01%	0.002%
55	8.689	2374	2379	2381	rBV2	315	175	0.01%	0.001%
56	8.702	2381	2383	2387	rVB	193	135	0.01%	0.001%
57	8.734	2389	2393	2396	rBV2	288	256	0.02%	0.002%
58	8.754	2396	2399	2401	rBV	176	109	0.01%	0.001%
59	8.786	2406	2409	2411	rVB3	248	136	0.01%	0.001%
60	8.799	2411	2413	2415	rBV	158	104	0.01%	0.001%
61	8.844	2415	2427	2459	rBV	764253	1268254	82.90%	10.266%
62	9.101	2504	2507	2510	rVB	281	144	0.01%	0.001%
63	9.123	2510	2514	2516	rBV	399	355	0.02%	0.003%
64	9.168	2525	2528	2531	rVB2	493	295	0.02%	0.002%
65	9.381	2591	2594	2596	rBV2	203	118	0.01%	0.001%
66	9.535	2639	2642	2645	rBV2	317	211	0.01%	0.002%
67	9.577	2651	2655	2659	rVB3	544	469	0.03%	0.004%
68	9.728	2698	2702	2709	rBV2	294	372	0.02%	0.003%
69	9.773	2714	2716	2719	rVV3	189	112	0.01%	0.001%
70	9.812	2726	2728	2731	rVB	274	150	0.01%	0.001%
71	9.828	2731	2733	2737	rVB2	312	172	0.01%	0.001%
72	9.850	2737	2740	2741	rBV	251	155	0.01%	0.001%
73	9.914	2757	2760	2762	rBV	269	197	0.01%	0.002%
74	10.040	2792	2799	2802	rBV2	341	370	0.02%	0.003%
75	10.059	2803	2805	2809	rVV2	251	159	0.01%	0.001%
76	10.082	2809	2812	2815	rVB2	285	203	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029669.D
 Acq On : 13 Dec 2022 22:41
 Operator : SY/MD
 Sample : N5950-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.162	2827	2837	2841	rBV	19674	29263	1.91%	0.237%
78	10.207	2842	2851	2869	rVB	501762	782160	51.13%	6.331%
79	10.320	2885	2886	2891	rBV2	319	173	0.01%	0.001%
80	10.361	2896	2899	2901	rBV2	395	269	0.02%	0.002%
81	10.464	2928	2931	2937	rVB2	321	208	0.01%	0.002%
82	10.493	2937	2940	2942	rBV	328	205	0.01%	0.002%
83	10.567	2956	2963	2973	rBV2	9606	14312	0.94%	0.116%
84	10.898	3064	3066	3068	rBV2	310	174	0.01%	0.001%
85	10.947	3078	3081	3086	rBB	223	139	0.01%	0.001%
86	10.972	3086	3089	3091	rBV	183	130	0.01%	0.001%
87	11.066	3114	3118	3119	rBV2	227	177	0.01%	0.001%
88	11.130	3135	3138	3140	rBV2	153	107	0.01%	0.001%
89	11.236	3159	3171	3195	rBV	851003	1328074	86.81%	10.750%
90	11.458	3238	3240	3246	rVB2	480	275	0.02%	0.002%
91	11.612	3275	3288	3309	rBV	743198	1188466	77.68%	9.620%
92	11.873	3367	3369	3371	rVV	301	121	0.01%	0.001%
93	11.921	3382	3384	3386	rBV2	256	114	0.01%	0.001%
94	12.033	3417	3419	3423	rBV	275	171	0.01%	0.001%
95	12.226	3477	3479	3481	rBV2	350	180	0.01%	0.001%
96	12.307	3500	3504	3505	rBV2	326	207	0.01%	0.002%
97	12.361	3518	3521	3524	rBV	390	342	0.02%	0.003%
98	12.483	3556	3559	3563	rBV2	290	226	0.01%	0.002%
99	12.750	3639	3642	3645	rBV2	324	252	0.02%	0.002%
100	12.789	3652	3654	3658	rVB2	448	143	0.01%	0.001%


Sum of corrected areas: 12353814

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029669.D
Acq On : 13 Dec 2022 22:41
Operator : SY/MD
Sample : N5950-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

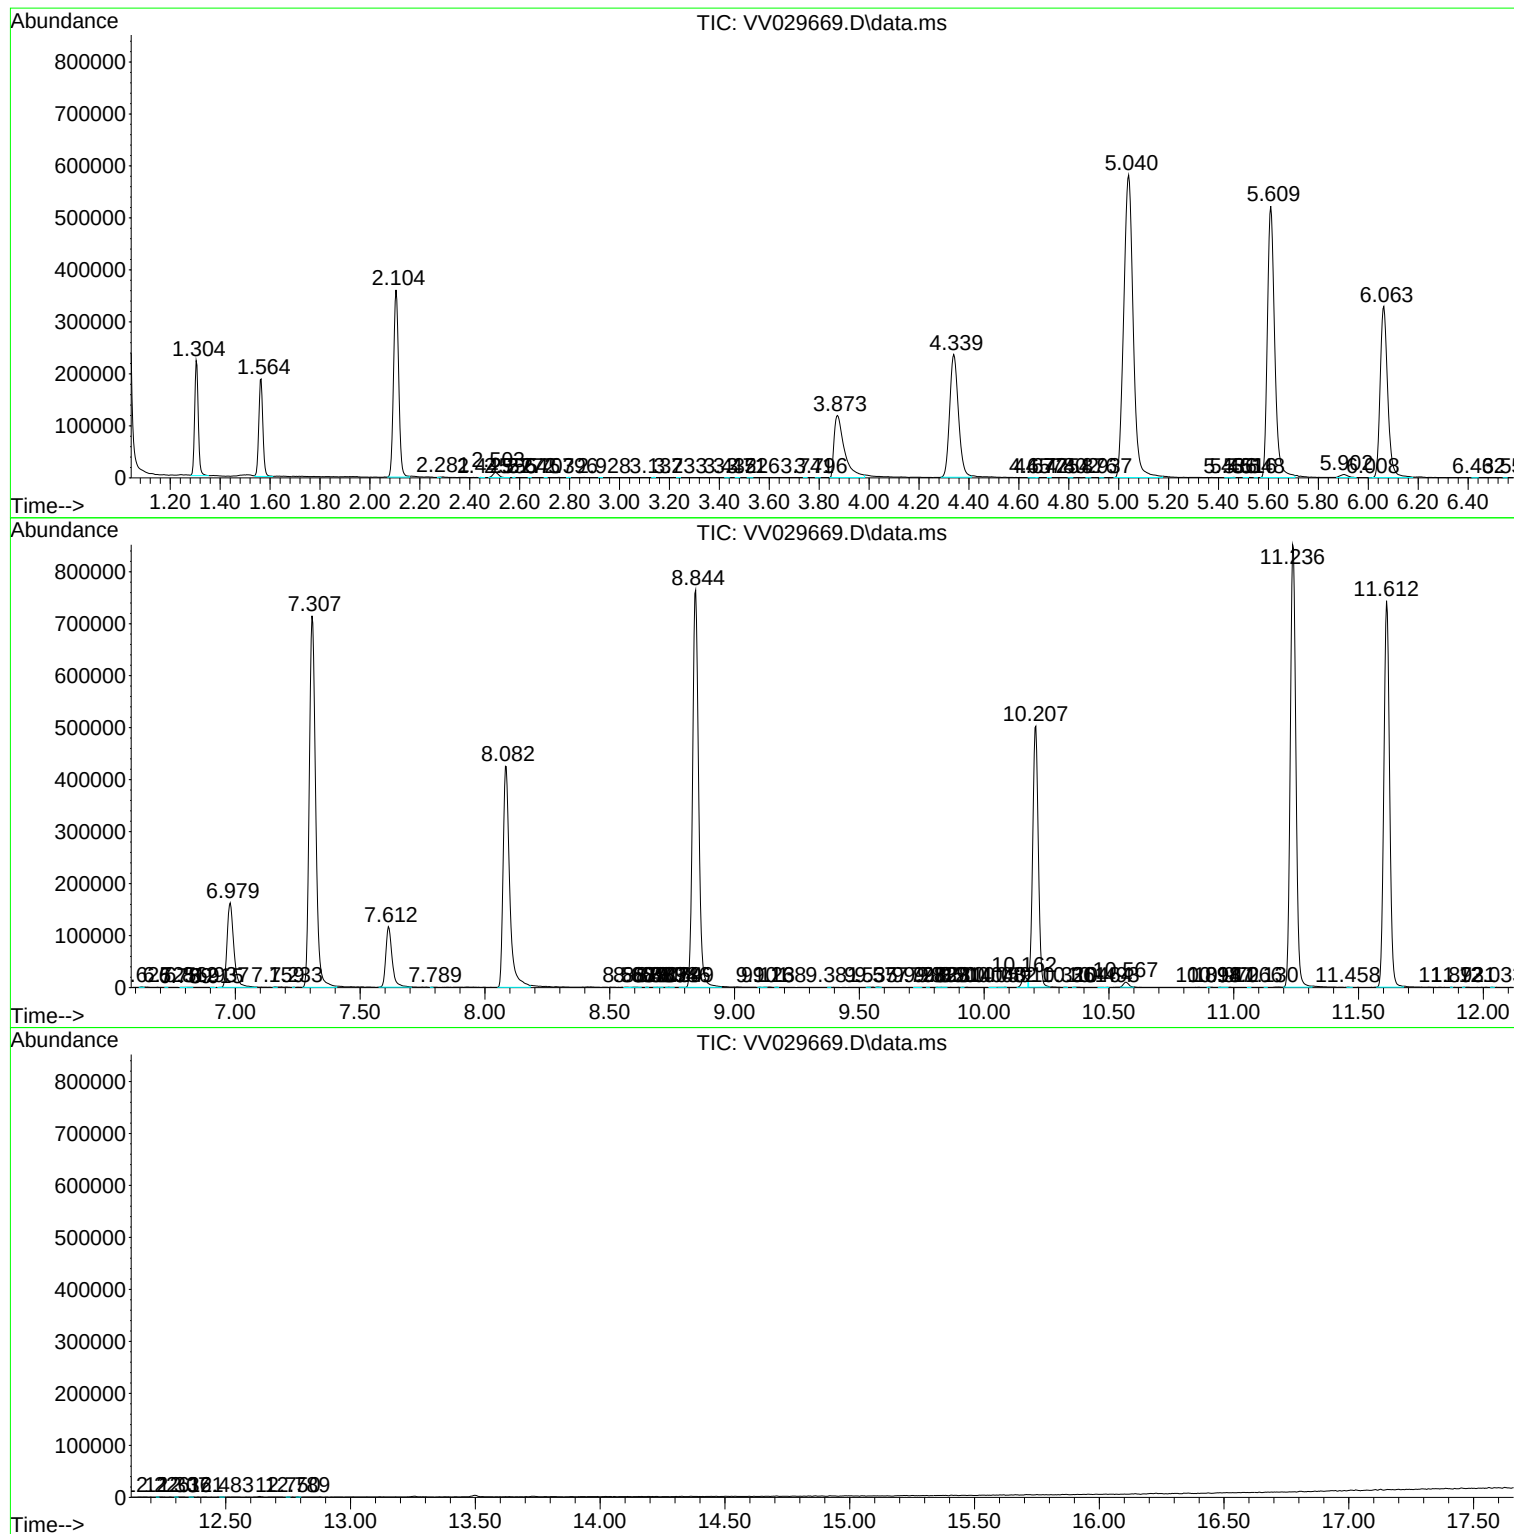

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029669.D
Acq On : 13 Dec 2022 22:41
Operator : SY/MD
Sample : N5950-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029669.D
Acq On : 13 Dec 2022 22:41
Operator : SY/MD
Sample : N5950-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc