

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029670.D
 Acq On : 13 Dec 2022 23:04
 Operator : SY/MD
 Sample : N5980-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	189335	184188	13.64%	1.452%
2	1.565	155	163	177	rVB	164419	185699	13.75%	1.463%
3	2.105	320	331	345	rBV2	331103	507667	37.60%	4.001%
4	2.304	382	393	429	rVB	13408	45814	3.39%	0.361%
5	2.497	449	453	454	rBV2	1030	676	0.05%	0.005%
6	2.568	472	475	479	rBV2	288	147	0.01%	0.001%
7	2.642	491	498	504	rBV3	872	1175	0.09%	0.009%
8	2.764	531	536	538	rBV2	549	445	0.03%	0.004%
9	2.796	544	546	549	rBV	206	70	0.01%	0.001%
10	2.851	561	563	568	rVB2	275	134	0.01%	0.001%
11	3.027	615	618	624	rBV2	242	251	0.02%	0.002%
12	3.153	653	657	658	rBV	185	104	0.01%	0.001%
13	3.185	658	667	668	rBV2	822	947	0.07%	0.007%
14	3.400	731	734	738	rBV2	256	135	0.01%	0.001%
15	3.481	756	759	765	rVB2	156	124	0.01%	0.001%
16	3.609	797	799	804	rVB	268	161	0.01%	0.001%
17	3.642	804	809	812	rVB	128	103	0.01%	0.001%
18	3.761	842	846	850	rBV2	116	134	0.01%	0.001%
19	3.876	872	882	924	rBV	106169	352625	26.12%	2.779%
20	4.339	1010	1026	1060	rBV	209731	524349	38.83%	4.132%
21	4.600	1099	1107	1127	rVB3	6605	16695	1.24%	0.132%
22	4.728	1145	1147	1154	rVB2	285	212	0.02%	0.002%
23	4.761	1154	1157	1160	rBV2	127	85	0.01%	0.001%
24	4.892	1196	1198	1202	rVB	183	66	0.00%	0.001%
25	5.040	1222	1244	1290	rBV2	509227	1350269	100.00%	10.641%
26	5.391	1351	1353	1354	rBV2	230	107	0.01%	0.001%
27	5.458	1369	1374	1376	rBV2	418	302	0.02%	0.002%
28	5.548	1398	1402	1405	rVB2	314	227	0.02%	0.002%
29	5.609	1407	1421	1466	rBV	527177	1079165	79.92%	8.505%
30	5.905	1499	1513	1549	rBV	573948	1150911	85.24%	9.070%
31	6.063	1549	1562	1584	rVV	293395	598155	44.30%	4.714%
32	6.304	1633	1637	1640	rBV2	276	193	0.01%	0.002%
33	6.333	1644	1646	1650	rVB2	172	87	0.01%	0.001%
34	6.352	1650	1652	1655	rVB	132	63	0.00%	0.000%
35	6.410	1667	1670	1672	rBV2	133	79	0.01%	0.001%
36	6.458	1681	1685	1687	rBV2	220	113	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029670.D
 Acq On : 13 Dec 2022 23:04
 Operator : SY/MD
 Sample : N5980-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.516	1699	1703	1705	rBV	179	79	0.01%	0.001%
38	6.613	1730	1733	1734	rBV2	449	244	0.02%	0.002%
39	6.625	1734	1737	1746	rVB2	551	691	0.05%	0.005%
40	6.732	1766	1770	1771	rBV	84	69	0.01%	0.001%
41	6.741	1771	1773	1777	rVB2	295	172	0.01%	0.001%
42	6.889	1816	1819	1823	rVB2	217	147	0.01%	0.001%
43	6.918	1823	1828	1835	rVB2	157	170	0.01%	0.001%
44	6.979	1835	1847	1875	rBV	144088	268995	19.92%	2.120%
45	7.307	1937	1949	1985	rBV	627876	1112140	82.36%	8.764%
46	7.613	2031	2044	2066	rBV	102003	180300	13.35%	1.421%
47	7.834	2110	2113	2121	rVB4	867	788	0.06%	0.006%
48	7.934	2137	2144	2152	rVB4	1705	2237	0.17%	0.018%
49	8.085	2180	2191	2226	rBV	376164	683981	50.66%	5.390%
50	8.490	2316	2317	2320	rBV2	218	109	0.01%	0.001%
51	8.606	2352	2353	2356	rVB2	334	121	0.01%	0.001%
52	8.667	2369	2372	2377	rBV2	234	238	0.02%	0.002%
53	8.686	2377	2378	2381	rVB	377	103	0.01%	0.001%
54	8.725	2387	2390	2393	rVV2	353	273	0.02%	0.002%
55	8.744	2393	2396	2401	rVB2	357	322	0.02%	0.003%
56	8.844	2414	2427	2461	rBV	776232	1274507	94.39%	10.044%
57	9.069	2495	2497	2499	rBV	250	155	0.01%	0.001%
58	9.095	2504	2505	2506	rBV	237	83	0.01%	0.001%
59	9.204	2537	2539	2542	rVB2	270	167	0.01%	0.001%
60	9.384	2593	2595	2598	rBV3	365	207	0.02%	0.002%
61	9.452	2613	2616	2620	rBV2	173	137	0.01%	0.001%
62	9.493	2626	2629	2632	rBV	178	138	0.01%	0.001%
63	9.690	2687	2690	2691	rBV	149	65	0.00%	0.001%
64	9.715	2695	2698	2700	rVB	169	76	0.01%	0.001%
65	9.764	2710	2713	2716	rVB	236	156	0.01%	0.001%
66	9.805	2724	2726	2728	rBV	179	78	0.01%	0.001%
67	9.918	2758	2761	2767	rBV3	672	609	0.05%	0.005%
68	9.992	2782	2784	2786	rVB	187	75	0.01%	0.001%
69	10.030	2790	2796	2797	rBV	177	187	0.01%	0.001%
70	10.127	2822	2826	2828	rBV2	315	240	0.02%	0.002%
71	10.162	2828	2837	2841	rVV2	17945	26624	1.97%	0.210%
72	10.207	2842	2851	2871	rVB	446707	694869	51.46%	5.476%
73	10.349	2894	2895	2896	rBV	385	140	0.01%	0.001%
74	10.368	2897	2901	2902	rBV3	1354	788	0.06%	0.006%
75	10.497	2939	2941	2943	rBV	173	67	0.00%	0.001%
76	10.519	2946	2948	2954	rVV4	451	535	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029670.D
 Acq On : 13 Dec 2022 23:04
 Operator : SY/MD
 Sample : N5980-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.567	2954	2963	2975	rVB	8563	13666	1.01%	0.108%
78	10.683	2994	2999	3003	rBV2	177	180	0.01%	0.001%
79	10.757	3020	3022	3025	rVB	210	108	0.01%	0.001%
80	10.776	3026	3028	3032	rBV	224	140	0.01%	0.001%
81	10.828	3042	3044	3046	rVB	207	87	0.01%	0.001%
82	10.844	3046	3049	3050	rBV	169	79	0.01%	0.001%
83	10.911	3063	3070	3075	rBV3	749	943	0.07%	0.007%
84	10.963	3084	3086	3089	rBV	140	96	0.01%	0.001%
85	11.181	3146	3154	3159	rBV6	901	1142	0.08%	0.009%
86	11.239	3159	3172	3198	rBV	859465	1335069	98.87%	10.521%
87	11.612	3276	3288	3318	rBV	686909	1080089	79.99%	8.512%
88	11.902	3375	3378	3382	rBV2	371	210	0.02%	0.002%
89	11.924	3382	3385	3387	rBV	292	124	0.01%	0.001%
90	12.133	3448	3450	3453	rBV	184	95	0.01%	0.001%
91	12.159	3453	3458	3461	rBV2	456	361	0.03%	0.003%
92	12.191	3466	3468	3472	rBV2	278	161	0.01%	0.001%
93	12.230	3476	3480	3482	rBV2	613	490	0.04%	0.004%
94	12.278	3493	3495	3498	rBV2	212	149	0.01%	0.001%
95	12.381	3524	3527	3532	rBV3	275	221	0.02%	0.002%
96	12.448	3546	3548	3551	rBV2	305	182	0.01%	0.001%
97	12.519	3568	3570	3571	rBV	344	156	0.01%	0.001%
98	12.979	3711	3713	3716	rVB3	442	276	0.02%	0.002%
99	13.252	3793	3798	3805	rVB5	1395	1722	0.13%	0.014%
100	13.963	4015	4019	4023	rBV2	677	705	0.05%	0.006%

Sum of corrected areas: 12689210




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029670.D
Acq On : 13 Dec 2022 23:04
Operator : SY/MD
Sample : N5980-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L

TIC Integration Parameters: LSCINT.P

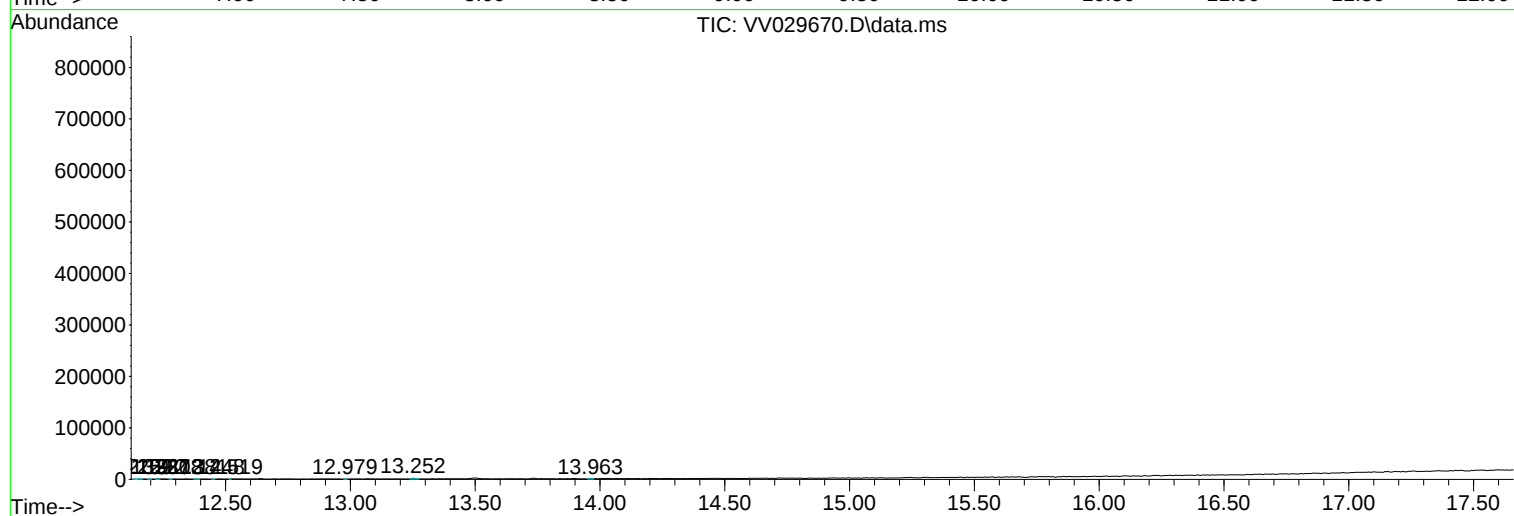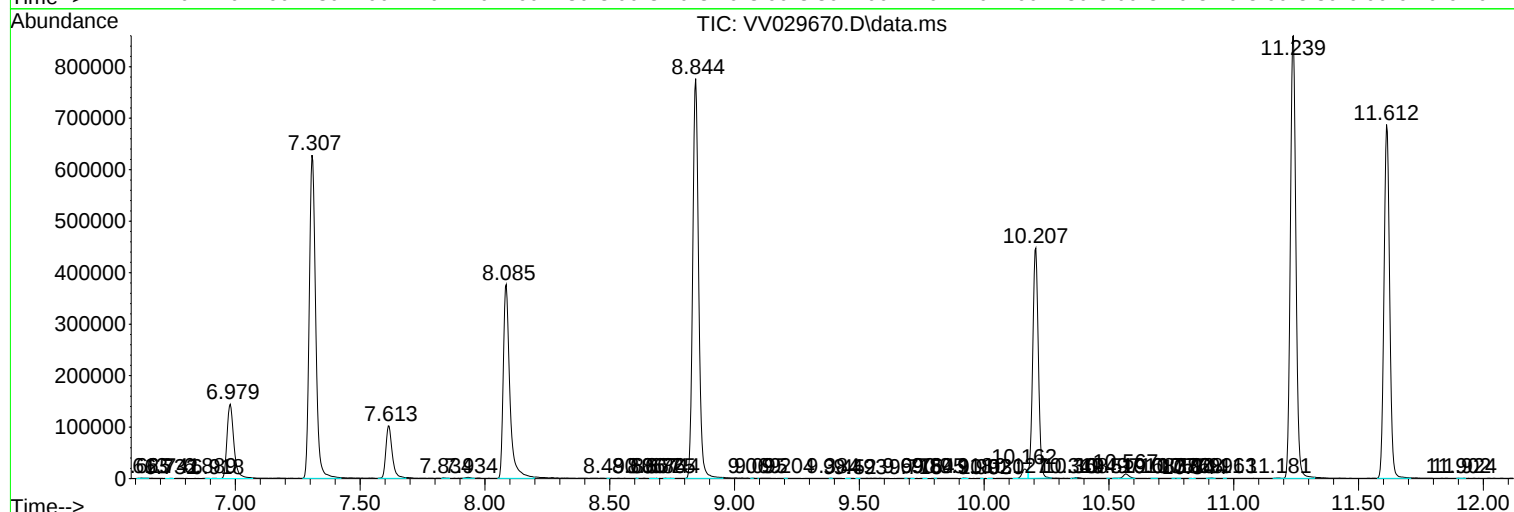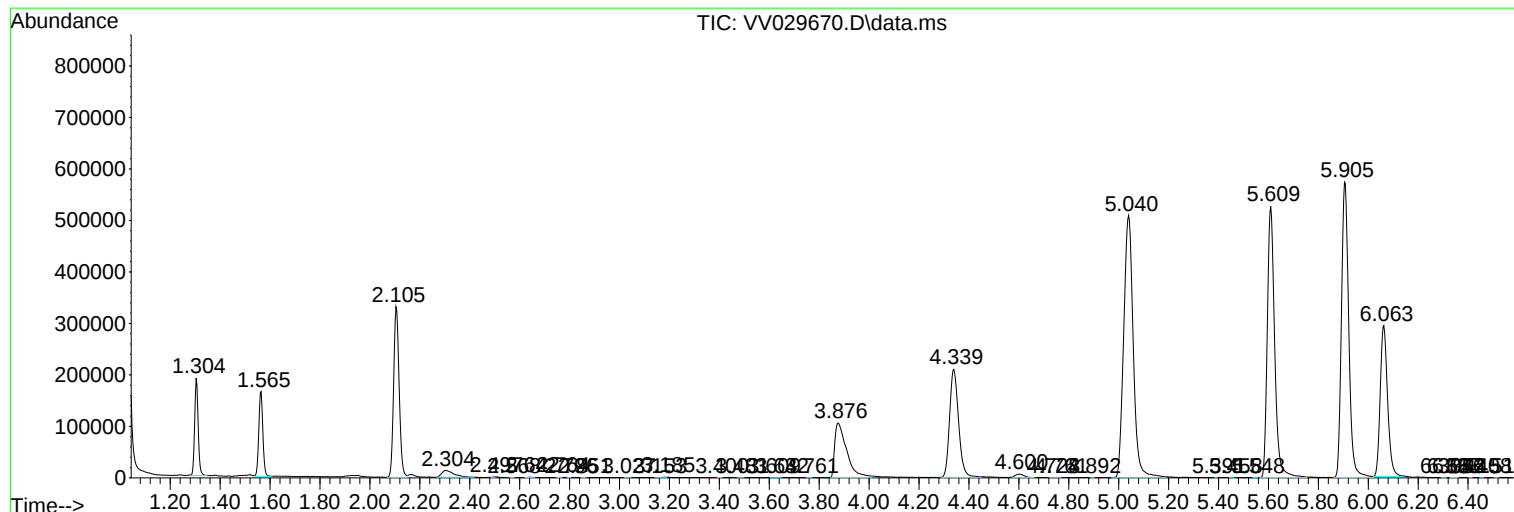

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029670.D
Acq On : 13 Dec 2022 23:04
Operator : SY/MD
Sample : N5980-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029670.D
Acq On : 13 Dec 2022 23:04
Operator : SY/MD
Sample : N5980-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc