

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029671.D
 Acq On : 13 Dec 2022 23:28
 Operator : SY/MD
 Sample : N5980-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	189714	188764	13.76%	1.640%
2	1.564	156	163	176	rVB	173812	192573	14.04%	1.673%
3	2.105	320	331	345	rBV	315725	450962	32.88%	3.917%
4	2.574	473	477	478	rBV2	160	119	0.01%	0.001%
5	2.645	496	499	502	rBV2	339	186	0.01%	0.002%
6	2.764	533	536	537	rBV2	525	242	0.02%	0.002%
7	2.998	605	609	613	rBV2	284	173	0.01%	0.002%
8	3.027	616	618	622	rVB2	285	148	0.01%	0.001%
9	3.137	647	652	654	rBV2	109	117	0.01%	0.001%
10	3.153	654	657	661	rBV2	248	137	0.01%	0.001%
11	3.468	751	755	757	rBV2	138	101	0.01%	0.001%
12	3.490	757	762	764	rBV2	209	199	0.01%	0.002%
13	3.548	777	780	783	rVB	279	182	0.01%	0.002%
14	3.703	825	828	835	rVV2	178	196	0.01%	0.002%
15	3.876	872	882	917	rBV	101850	293742	21.42%	2.551%
16	4.339	1009	1026	1057	rBV	211438	530514	38.68%	4.608%
17	4.661	1123	1126	1131	rVB3	464	400	0.03%	0.003%
18	4.696	1132	1137	1141	rVB3	271	298	0.02%	0.003%
19	4.728	1144	1147	1153	rVB	346	223	0.02%	0.002%
20	4.764	1154	1158	1160	rBV	237	171	0.01%	0.001%
21	4.777	1160	1162	1165	rVB	186	100	0.01%	0.001%
22	4.802	1165	1170	1175	rBV	154	204	0.01%	0.002%
23	4.844	1180	1183	1185	rBV2	143	98	0.01%	0.001%
24	4.896	1194	1199	1200	rBV2	165	135	0.01%	0.001%
25	5.040	1225	1244	1286	rBV2	519354	1371378	100.00%	11.911%
26	5.330	1332	1334	1337	rBV	300	138	0.01%	0.001%
27	5.461	1372	1375	1376	rBV2	294	172	0.01%	0.001%
28	5.609	1408	1421	1458	rBV	540367	1103689	80.48%	9.586%
29	5.905	1501	1513	1529	rVB8	5493	12719	0.93%	0.110%
30	5.998	1537	1542	1547	rBV2	369	437	0.03%	0.004%
31	6.063	1547	1562	1587	rBV	297075	616906	44.98%	5.358%
32	6.313	1635	1640	1644	rVB2	292	221	0.02%	0.002%
33	6.336	1644	1647	1649	rBV2	179	124	0.01%	0.001%
34	6.349	1649	1651	1657	rVB2	390	303	0.02%	0.003%
35	6.471	1686	1689	1692	rBV2	277	229	0.02%	0.002%
36	6.535	1705	1709	1712	rBV	231	141	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029671.D
 Acq On : 13 Dec 2022 23:28
 Operator : SY/MD
 Sample : N5980-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.561	1712	1717	1719	rBV3	230	173	0.01%	0.002%
38	6.625	1728	1737	1742	rBV4	818	1163	0.08%	0.010%
39	6.696	1758	1759	1764	rBV	186	147	0.01%	0.001%
40	6.760	1772	1779	1781	rBV2	184	176	0.01%	0.002%
41	6.924	1822	1830	1833	rBV2	215	241	0.02%	0.002%
42	6.979	1833	1847	1864	rBV	143748	265679	19.37%	2.308%
43	7.153	1897	1901	1902	rBV2	650	368	0.03%	0.003%
44	7.262	1933	1935	1937	rBV	283	152	0.01%	0.001%
45	7.307	1937	1949	1987	rVV	628478	1115429	81.34%	9.688%
46	7.612	2035	2044	2070	rBV	102910	181034	13.20%	1.572%
47	7.802	2097	2103	2106	rVB4	606	450	0.03%	0.004%
48	7.831	2107	2112	2113	rBV3	455	306	0.02%	0.003%
49	7.841	2113	2115	2120	rVB2	301	145	0.01%	0.001%
50	7.863	2120	2122	2129	rVB4	468	455	0.03%	0.004%
51	7.892	2129	2131	2132	rBV2	210	89	0.01%	0.001%
52	7.931	2132	2143	2153	rBV3	2733	5340	0.39%	0.046%
53	8.085	2180	2191	2230	rBV	378995	699401	51.00%	6.075%
54	8.468	2307	2310	2313	rVB3	553	326	0.02%	0.003%
55	8.490	2313	2317	2318	rBV	280	202	0.01%	0.002%
56	8.606	2351	2353	2358	rBV3	384	322	0.02%	0.003%
57	8.638	2361	2363	2365	rVV3	267	106	0.01%	0.001%
58	8.722	2386	2389	2390	rBV	268	127	0.01%	0.001%
59	8.747	2393	2397	2399	rBV	248	168	0.01%	0.001%
60	8.783	2405	2408	2414	rBV2	218	199	0.01%	0.002%
61	8.844	2414	2427	2447	rBV	793042	1297781	94.63%	11.272%
62	9.101	2504	2507	2511	rBV2	428	425	0.03%	0.004%
63	9.326	2574	2577	2584	rVB2	252	246	0.02%	0.002%
64	9.448	2612	2615	2617	rVB	180	103	0.01%	0.001%
65	9.493	2625	2629	2632	rBV3	212	178	0.01%	0.002%
66	9.538	2640	2643	2647	rBV2	287	264	0.02%	0.002%
67	9.564	2647	2651	2653	rVV3	457	346	0.03%	0.003%
68	9.590	2657	2659	2661	rVB	262	112	0.01%	0.001%
69	9.661	2678	2681	2683	rBV3	182	124	0.01%	0.001%
70	9.702	2690	2694	2697	rBV	379	306	0.02%	0.003%
71	9.770	2713	2715	2720	rVB3	354	249	0.02%	0.002%
72	9.815	2727	2729	2732	rVV	249	115	0.01%	0.001%
73	9.924	2758	2763	2769	rBV2	453	492	0.04%	0.004%
74	10.120	2820	2824	2827	rVB2	206	173	0.01%	0.002%
75	10.162	2827	2837	2841	rBV2	18849	27132	1.98%	0.236%
76	10.207	2842	2851	2870	rVB	447670	702254	51.21%	6.100%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029671.D
 Acq On : 13 Dec 2022 23:28
 Operator : SY/MD
 Sample : N5980-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.313	2882	2884	2888	rBV2	284	218	0.02%	0.002%
78	10.374	2896	2903	2912	rVB4	3140	4495	0.33%	0.039%
79	10.532	2945	2952	2954	rBV3	587	621	0.05%	0.005%
80	10.567	2955	2963	2978	rVB2	8551	14179	1.03%	0.123%
81	10.735	3011	3015	3016	rBV	197	122	0.01%	0.001%
82	10.789	3030	3032	3033	rBV	310	135	0.01%	0.001%
83	10.837	3044	3047	3052	rBV	250	192	0.01%	0.002%
84	10.879	3058	3060	3064	rBV	265	171	0.01%	0.001%
85	10.902	3064	3067	3069	rBV2	700	479	0.03%	0.004%
86	10.944	3078	3080	3085	rBV3	279	205	0.01%	0.002%
87	11.034	3104	3108	3111	rVB	225	181	0.01%	0.002%
88	11.053	3111	3114	3116	rBV2	209	111	0.01%	0.001%
89	11.091	3123	3126	3130	rBV3	379	305	0.02%	0.003%
90	11.117	3130	3134	3139	rVB2	191	186	0.01%	0.002%
91	11.236	3159	3171	3199	rBV	874847	1342978	97.93%	11.665%
92	11.551	3267	3269	3271	rBV2	405	145	0.01%	0.001%
93	11.612	3275	3288	3312	rBV	678056	1078001	78.61%	9.363%
94	11.805	3345	3348	3352	rVB	500	291	0.02%	0.003%
95	11.837	3353	3358	3359	rBV	315	261	0.02%	0.002%
96	11.892	3372	3375	3378	rVB3	272	135	0.01%	0.001%
97	11.921	3382	3384	3387	rBV	345	192	0.01%	0.002%
98	12.371	3521	3524	3526	rBV2	235	163	0.01%	0.001%
99	12.503	3561	3565	3568	rBV2	324	303	0.02%	0.003%
100	13.320	3817	3819	3821	rBV2	512	243	0.02%	0.002%




Sum of corrected areas: 11513251

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029671.D
Acq On : 13 Dec 2022 23:28
Operator : SY/MD
Sample : N5980-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

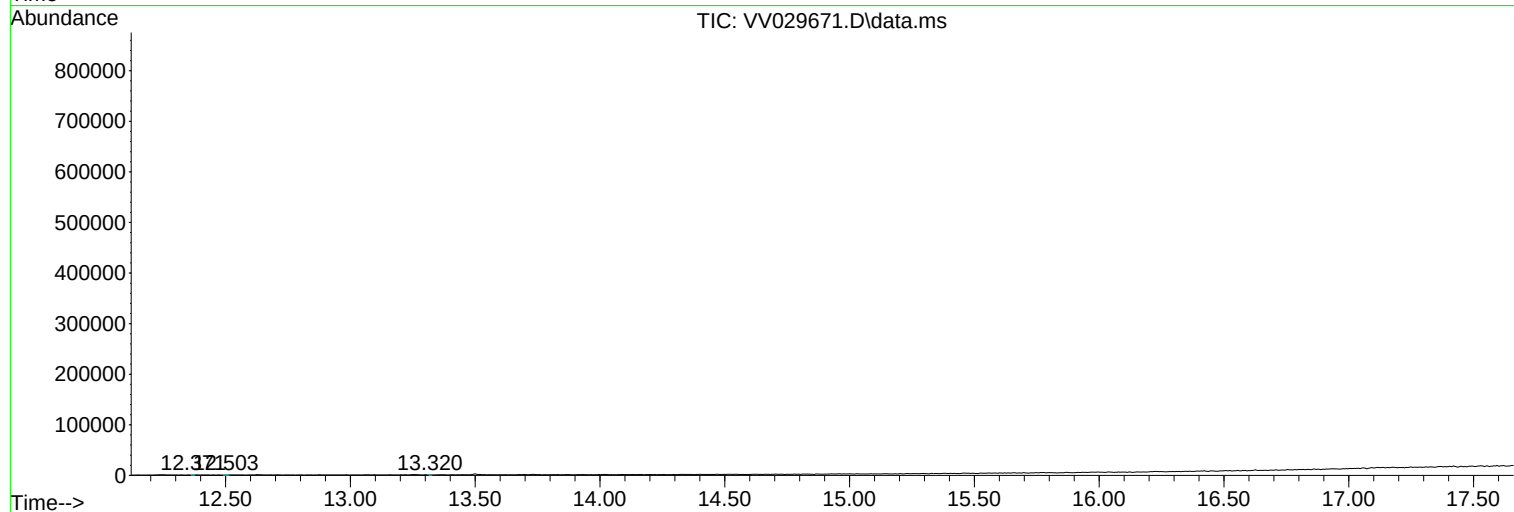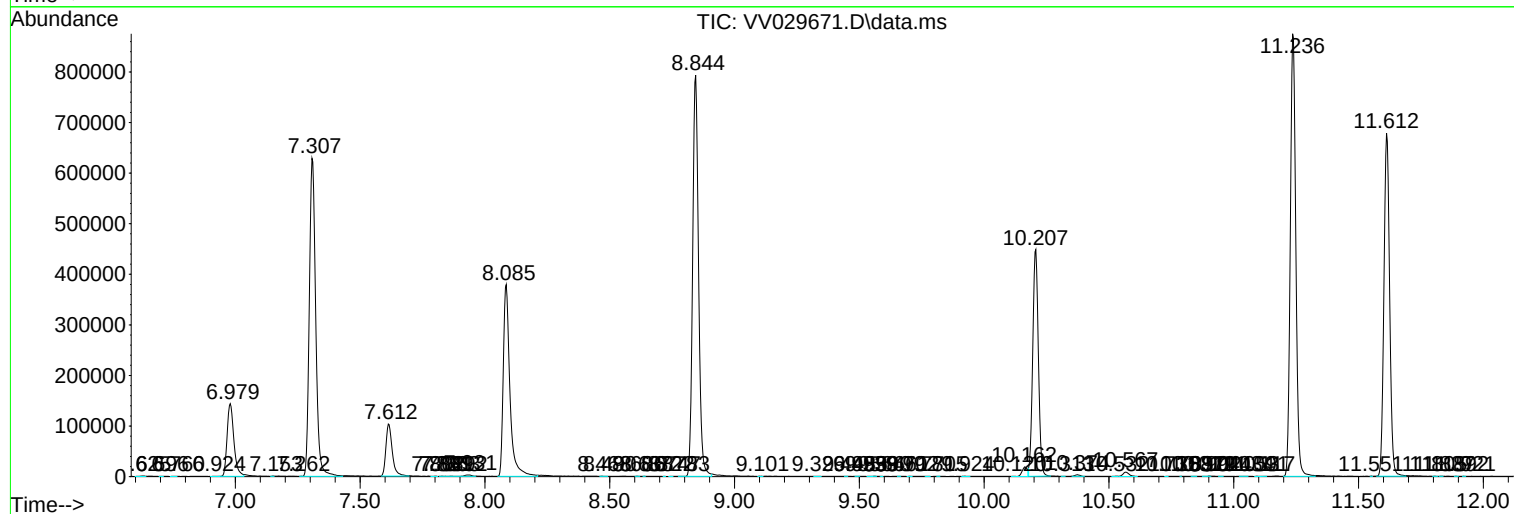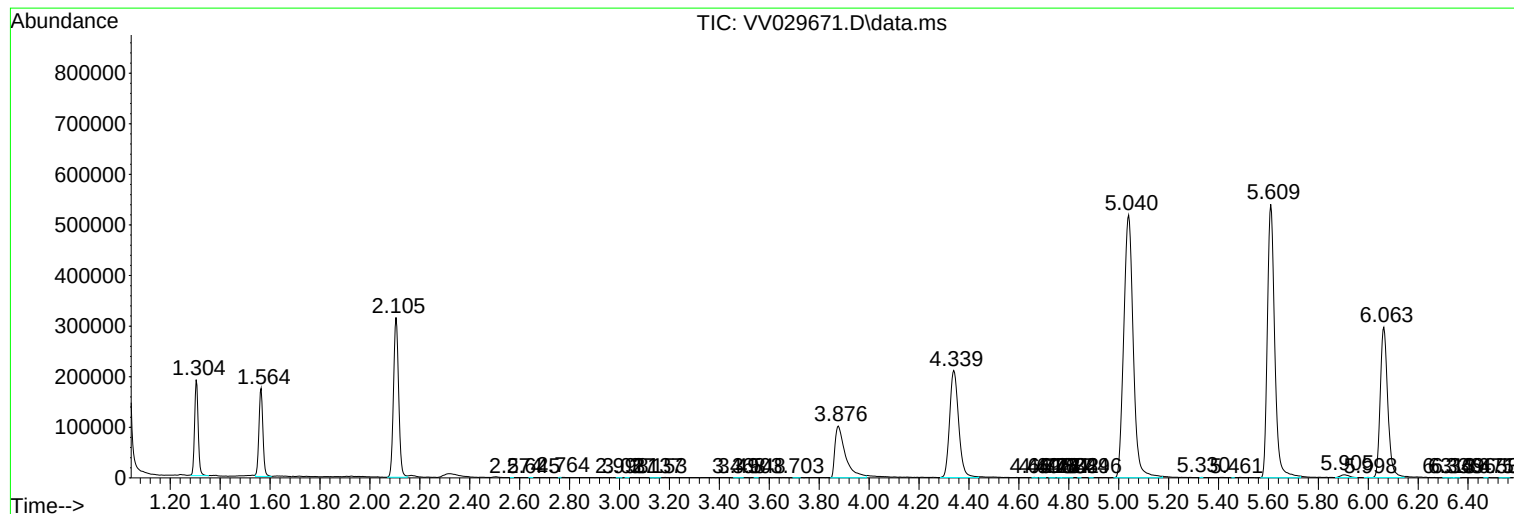

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029671.D
Acq On : 13 Dec 2022 23:28
Operator : SY/MD
Sample : N5980-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029671.D
Acq On : 13 Dec 2022 23:28
Operator : SY/MD
Sample : N5980-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc