

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029672.D
 Acq On : 13 Dec 2022 23:51
 Operator : SY/MD
 Sample : N5980-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	190743	188231	13.60%	1.431%
2	1.565	155	163	178	rVB	164930	187574	13.55%	1.426%
3	2.105	320	331	346	rBV2	345016	527803	38.13%	4.012%
4	2.590	476	482	485	rBV2	433	346	0.02%	0.003%
5	2.635	493	496	497	rBV2	315	172	0.01%	0.001%
6	2.712	516	520	522	rBV2	428	220	0.02%	0.002%
7	2.799	543	547	550	rBV2	202	176	0.01%	0.001%
8	2.838	556	559	562	rBV	315	176	0.01%	0.001%
9	3.095	636	639	644	rBV2	284	223	0.02%	0.002%
10	3.127	645	649	652	rVB3	207	179	0.01%	0.001%
11	3.185	660	667	669	rBV3	958	975	0.07%	0.007%
12	3.230	679	681	686	rVB2	233	133	0.01%	0.001%
13	3.381	725	728	730	rBV	161	114	0.01%	0.001%
14	3.519	766	771	777	rBV	181	203	0.01%	0.002%
15	3.600	792	796	799	rBV3	277	225	0.02%	0.002%
16	3.658	812	814	817	rVB2	261	147	0.01%	0.001%
17	3.677	817	820	825	rBV2	177	134	0.01%	0.001%
18	3.828	865	867	872	rVB2	211	144	0.01%	0.001%
19	3.876	872	882	929	rBV2	106674	371720	26.85%	2.826%
20	4.339	1010	1026	1055	rBV	216163	539208	38.96%	4.099%
21	4.677	1128	1131	1135	rBV3	333	259	0.02%	0.002%
22	4.722	1143	1145	1150	rBV2	230	159	0.01%	0.001%
23	4.744	1150	1152	1155	rVB3	228	121	0.01%	0.001%
24	4.815	1168	1174	1178	rBV3	391	401	0.03%	0.003%
25	4.854	1183	1186	1192	rVB3	263	325	0.02%	0.002%
26	4.896	1196	1199	1203	rBV2	284	176	0.01%	0.001%
27	4.947	1212	1215	1218	rBV2	260	164	0.01%	0.001%
28	5.040	1225	1244	1277	rBV2	525480	1384178	100.00%	10.522%
29	5.400	1353	1356	1359	rBV2	494	323	0.02%	0.002%
30	5.429	1362	1365	1366	rBV	197	139	0.01%	0.001%
31	5.513	1387	1391	1393	rVB	244	105	0.01%	0.001%
32	5.539	1397	1399	1402	rVB	155	94	0.01%	0.001%
33	5.609	1408	1421	1465	rBV	544679	1120835	80.97%	8.520%
34	5.905	1499	1513	1548	rBV	680858	1361390	98.35%	10.349%
35	6.063	1550	1562	1600	rVB	304301	630719	45.57%	4.794%
36	6.288	1630	1632	1637	rVB3	380	292	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029672.D
 Acq On : 13 Dec 2022 23:51
 Operator : SY/MD
 Sample : N5980-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.314	1637	1640	1647	rVB2	179	161	0.01%	0.001%
38	6.352	1647	1652	1653	rBV	110	94	0.01%	0.001%
39	6.378	1655	1660	1661	rBV2	141	113	0.01%	0.001%
40	6.465	1683	1687	1689	rBV	235	135	0.01%	0.001%
41	6.539	1706	1710	1713	rBV2	244	162	0.01%	0.001%
42	6.584	1718	1724	1727	rBV2	231	179	0.01%	0.001%
43	6.622	1732	1736	1738	rBV	810	534	0.04%	0.004%
44	6.696	1757	1759	1761	rBV	180	92	0.01%	0.001%
45	6.767	1778	1781	1782	rBV	249	112	0.01%	0.001%
46	6.834	1798	1802	1805	rVB2	262	199	0.01%	0.002%
47	6.879	1814	1816	1819	rBV2	185	113	0.01%	0.001%
48	6.899	1819	1822	1826	rBB2	237	171	0.01%	0.001%
49	6.924	1826	1830	1832	rBV	240	185	0.01%	0.001%
50	6.979	1836	1847	1872	rBV	145968	270362	19.53%	2.055%
51	7.127	1891	1893	1897	rVB2	300	87	0.01%	0.001%
52	7.214	1917	1920	1923	rVB3	383	268	0.02%	0.002%
53	7.236	1923	1927	1934	rVB3	510	451	0.03%	0.003%
54	7.307	1934	1949	1981	rBV	644232	1134122	81.93%	8.621%
55	7.613	2034	2044	2072	rBV	101435	182460	13.18%	1.387%
56	7.773	2091	2094	2097	rBV4	475	327	0.02%	0.002%
57	7.838	2110	2114	2116	rBV2	621	442	0.03%	0.003%
58	8.085	2180	2191	2229	rBV	370916	694780	50.19%	5.281%
59	8.420	2290	2295	2298	rBV2	508	536	0.04%	0.004%
60	8.510	2321	2323	2325	rBV2	322	199	0.01%	0.002%
61	8.580	2342	2345	2348	rBV2	158	110	0.01%	0.001%
62	8.603	2348	2352	2356	rBV4	454	396	0.03%	0.003%
63	8.651	2366	2367	2370	rBV	211	110	0.01%	0.001%
64	8.703	2381	2383	2390	rVB3	268	205	0.01%	0.002%
65	8.731	2390	2392	2394	rBV	378	108	0.01%	0.001%
66	8.844	2414	2427	2463	rBV	800198	1325893	95.79%	10.079%
67	9.104	2505	2508	2510	rBV2	277	175	0.01%	0.001%
68	9.288	2559	2565	2566	rBV2	116	104	0.01%	0.001%
69	9.307	2569	2571	2574	rBV2	267	157	0.01%	0.001%
70	9.336	2579	2580	2585	rVB	241	124	0.01%	0.001%
71	9.458	2614	2618	2621	rBV2	319	244	0.02%	0.002%
72	9.529	2637	2640	2641	rBV	314	146	0.01%	0.001%
73	9.612	2663	2666	2670	rBV2	164	151	0.01%	0.001%
74	9.651	2675	2678	2680	rBV	203	91	0.01%	0.001%
75	9.802	2722	2725	2728	rBV2	258	185	0.01%	0.001%
76	9.899	2751	2755	2756	rBV2	244	127	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029672.D
 Acq On : 13 Dec 2022 23:51
 Operator : SY/MD
 Sample : N5980-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.918	2757	2761	2765	rBV2	336	396	0.03%	0.003%
78	9.973	2776	2778	2785	rVB2	234	145	0.01%	0.001%
79	10.005	2785	2788	2790	rBV	275	142	0.01%	0.001%
80	10.165	2828	2838	2841	rBV2	18431	26607	1.92%	0.202%
81	10.207	2842	2851	2872	rVB	452220	711717	51.42%	5.410%
82	10.371	2897	2902	2913	rVB4	2478	3586	0.26%	0.027%
83	10.529	2947	2951	2954	rBV3	487	512	0.04%	0.004%
84	10.567	2955	2963	2977	rVB2	8548	14361	1.04%	0.109%
85	10.709	3005	3007	3011	rBV2	241	159	0.01%	0.001%
86	10.963	3083	3086	3089	rVB	248	159	0.01%	0.001%
87	10.989	3091	3094	3097	rBV2	285	215	0.02%	0.002%
88	11.088	3122	3125	3127	rBV2	148	107	0.01%	0.001%
89	11.114	3131	3133	3135	rBV2	237	118	0.01%	0.001%
90	11.236	3160	3171	3200	rBV	892318	1369224	98.92%	10.408%
91	11.516	3255	3258	3261	rBV2	173	183	0.01%	0.001%
92	11.538	3263	3265	3268	rVB	353	190	0.01%	0.001%
93	11.612	3276	3288	3311	rBV	692716	1093683	79.01%	8.314%
94	11.899	3374	3377	3379	rBV	413	241	0.02%	0.002%
95	11.947	3389	3392	3395	rBV2	340	267	0.02%	0.002%
96	12.207	3472	3473	3476	rBV2	259	148	0.01%	0.001%
97	12.307	3501	3504	3506	rBV2	335	195	0.01%	0.001%
98	12.403	3531	3534	3535	rBV2	184	112	0.01%	0.001%
99	12.583	3588	3590	3592	rBV2	314	89	0.01%	0.001%
100	12.735	3635	3637	3641	rBV3	272	136	0.01%	0.001%




Sum of corrected areas: 13155085

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029672.D
Acq On : 13 Dec 2022 23:51
Operator : SY/MD
Sample : N5980-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

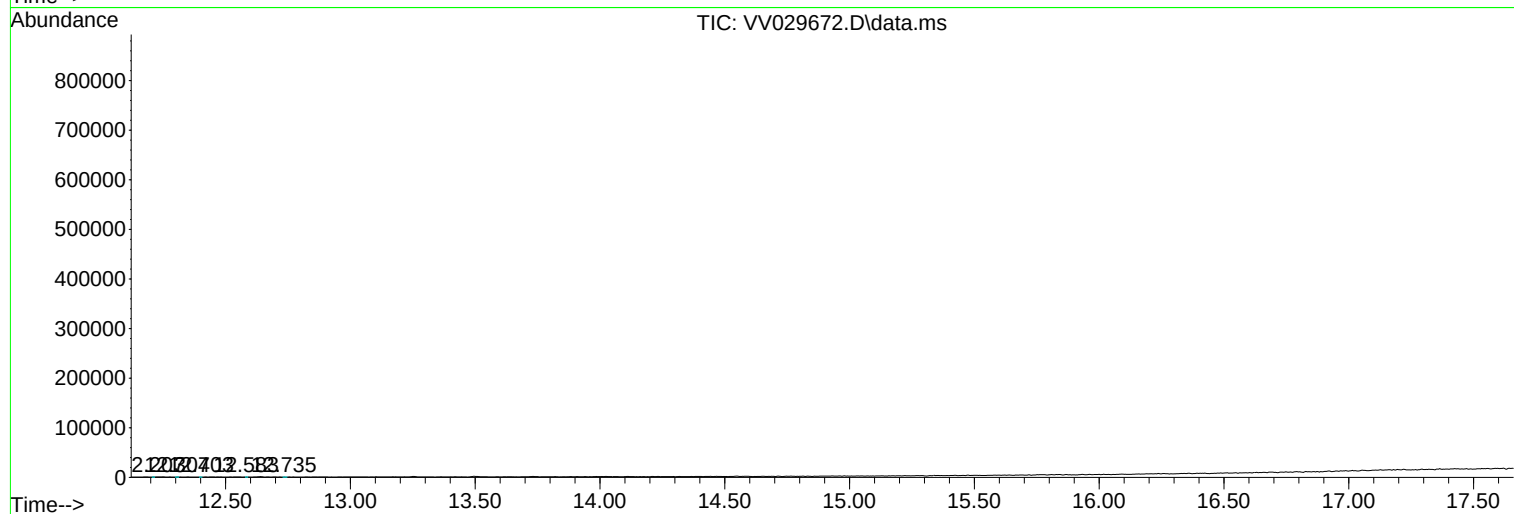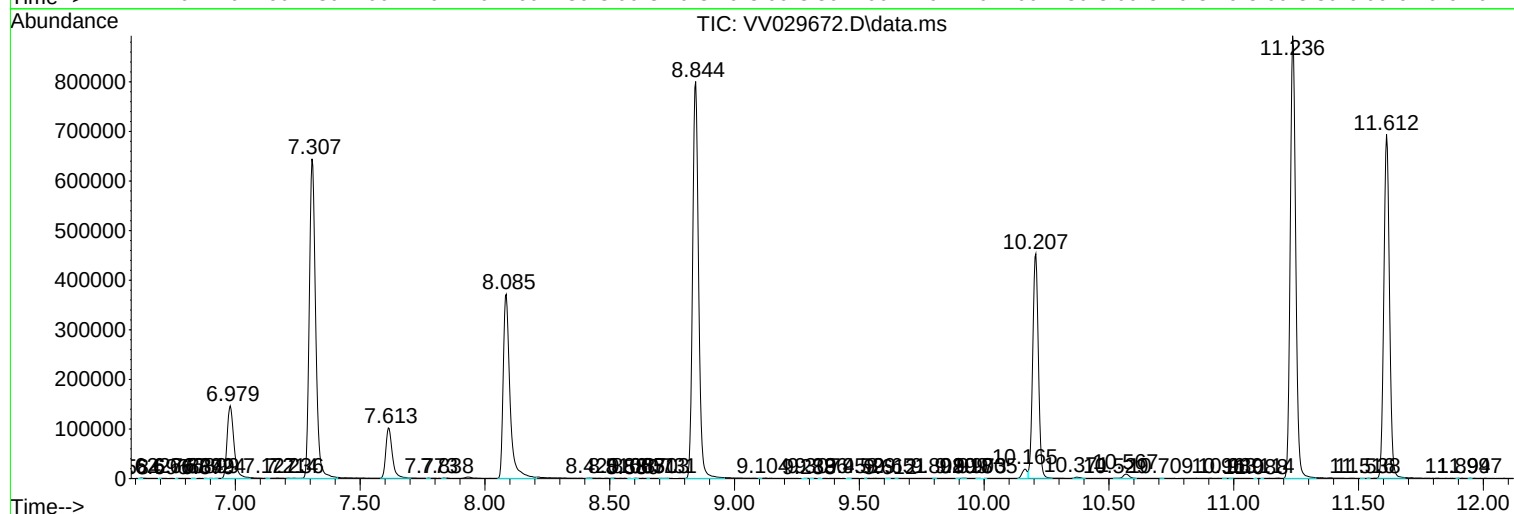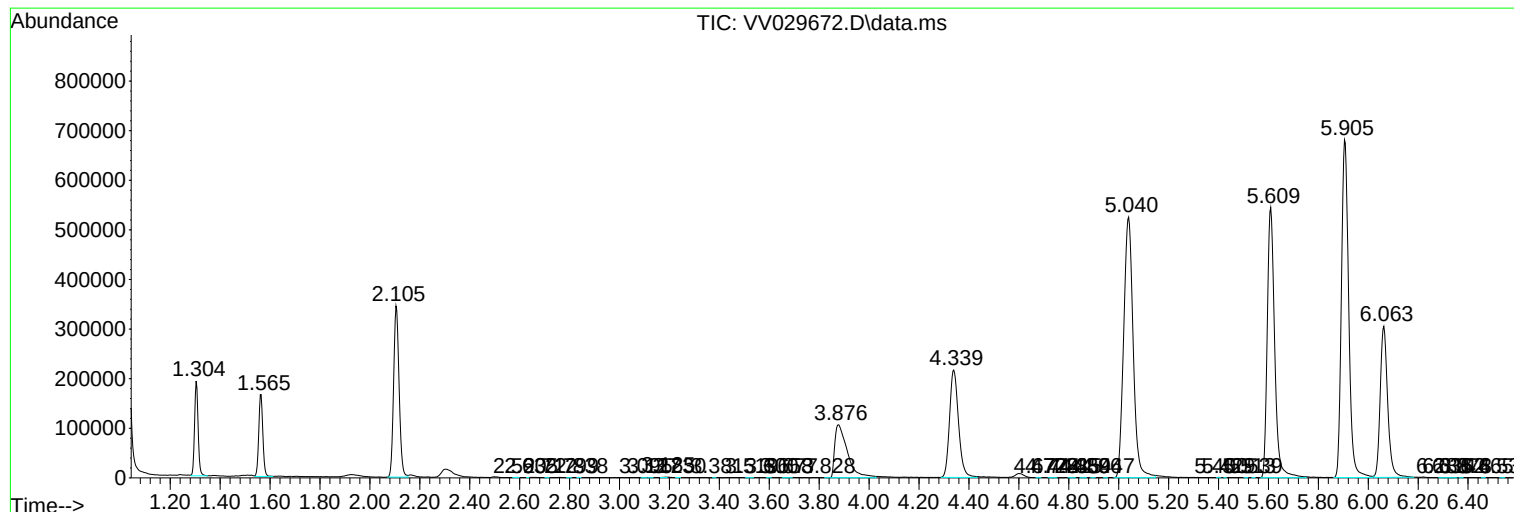

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029672.D
Acq On : 13 Dec 2022 23:51
Operator : SY/MD
Sample : N5980-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029672.D
Acq On : 13 Dec 2022 23:51
Operator : SY/MD
Sample : N5980-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc