

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029673.D
 Acq On : 14 Dec 2022 00:15
 Operator : SY/MD
 Sample : N5980-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029673.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	183670	182813	13.71%	1.611%
2	1.565	155	163	178	rVB	162802	183056	13.73%	1.613%
3	2.105	320	331	345	rBV2	327301	497865	37.34%	4.388%
4	2.304	382	393	422	rVB2	12347	40473	3.04%	0.357%
5	2.507	449	456	463	rVB5	1130	1755	0.13%	0.015%
6	2.597	480	484	487	rBV	312	257	0.02%	0.002%
7	2.735	524	527	531	rBV3	179	152	0.01%	0.001%
8	2.757	532	534	535	rBV3	287	101	0.01%	0.001%
9	2.854	562	564	567	rBV	234	134	0.01%	0.001%
10	2.886	571	574	576	rBV2	194	144	0.01%	0.001%
11	2.970	597	600	604	rVB2	312	177	0.01%	0.002%
12	3.249	682	687	694	rBV2	153	211	0.02%	0.002%
13	3.285	694	698	702	rBV2	169	137	0.01%	0.001%
14	3.307	702	705	710	rVV2	182	128	0.01%	0.001%
15	3.381	723	728	734	rBV2	362	356	0.03%	0.003%
16	3.529	772	774	777	rVV	195	98	0.01%	0.001%
17	3.564	783	785	791	rVB2	202	128	0.01%	0.001%
18	3.876	872	882	921	rBV	101302	343333	25.75%	3.026%
19	4.339	1010	1026	1064	rBV	207870	520411	39.03%	4.587%
20	4.603	1094	1108	1126	rVB3	11326	28010	2.10%	0.247%
21	4.670	1126	1129	1131	rBV	296	130	0.01%	0.001%
22	4.680	1131	1132	1138	rVB3	359	225	0.02%	0.002%
23	4.896	1193	1199	1201	rBV2	158	143	0.01%	0.001%
24	5.040	1225	1244	1292	rBV2	503109	1333224	100.00%	11.751%
25	5.359	1338	1343	1345	rBV	427	360	0.03%	0.003%
26	5.535	1396	1398	1403	rVB3	214	152	0.01%	0.001%
27	5.558	1403	1405	1408	rBV2	236	165	0.01%	0.001%
28	5.609	1408	1421	1467	rBV	520312	1053353	79.01%	9.284%
29	5.908	1503	1514	1533	rVB8	11276	26112	1.96%	0.230%
30	5.986	1537	1538	1541	rVB2	378	169	0.01%	0.001%
31	6.005	1541	1544	1547	rBV	218	166	0.01%	0.001%
32	6.063	1548	1562	1586	rBV	289848	594304	44.58%	5.238%
33	6.288	1629	1632	1635	rBV	148	123	0.01%	0.001%
34	6.352	1649	1652	1655	rBV	185	118	0.01%	0.001%
35	6.436	1673	1678	1681	rBV	133	133	0.01%	0.001%
36	6.500	1692	1698	1702	rVB2	155	175	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029673.D
 Acq On : 14 Dec 2022 00:15
 Operator : SY/MD
 Sample : N5980-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.564	1711	1718	1723	rBV2	204	305	0.02%	0.003%
38	6.622	1732	1736	1737	rBV3	594	382	0.03%	0.003%
39	6.744	1772	1774	1776	rVV	259	136	0.01%	0.001%
40	6.789	1782	1788	1790	rBV2	262	224	0.02%	0.002%
41	6.831	1798	1801	1802	rBV	174	97	0.01%	0.001%
42	6.854	1805	1808	1811	rBV	193	113	0.01%	0.001%
43	6.873	1811	1814	1816	rBV	244	119	0.01%	0.001%
44	6.928	1827	1831	1834	rBV	243	153	0.01%	0.001%
45	6.979	1836	1847	1872	rBV	138368	257746	19.33%	2.272%
46	7.249	1927	1931	1932	rBV2	275	196	0.01%	0.002%
47	7.307	1937	1949	1968	rBV	619555	1083753	81.29%	9.552%
48	7.500	2005	2009	2016	rVB4	743	596	0.04%	0.005%
49	7.612	2033	2044	2068	rBV	98953	175827	13.19%	1.550%
50	7.809	2101	2105	2111	rBV4	425	476	0.04%	0.004%
51	7.899	2129	2133	2135	rBV	389	322	0.02%	0.003%
52	8.030	2173	2174	2177	rBV2	263	119	0.01%	0.001%
53	8.085	2180	2191	2225	rBV	358729	660912	49.57%	5.825%
54	8.358	2274	2276	2277	rBV	359	139	0.01%	0.001%
55	8.397	2286	2288	2290	rBV2	320	178	0.01%	0.002%
56	8.519	2322	2326	2327	rBV2	263	161	0.01%	0.001%
57	8.625	2356	2359	2362	rVV3	282	160	0.01%	0.001%
58	8.641	2362	2364	2368	rVB2	266	140	0.01%	0.001%
59	8.686	2376	2378	2380	rBV	196	117	0.01%	0.001%
60	8.738	2393	2394	2398	rVB	236	139	0.01%	0.001%
61	8.776	2405	2406	2408	rBV	192	100	0.01%	0.001%
62	8.844	2414	2427	2458	rBV	763745	1254823	94.12%	11.060%
63	9.133	2508	2517	2527	rVB2	3004	4772	0.36%	0.042%
64	9.207	2538	2540	2543	rVV2	303	129	0.01%	0.001%
65	9.223	2543	2545	2549	rVB2	362	226	0.02%	0.002%
66	9.394	2595	2598	2601	rBV2	268	179	0.01%	0.002%
67	9.513	2628	2635	2637	rBV2	313	350	0.03%	0.003%
68	9.535	2637	2642	2647	rVV5	1093	1346	0.10%	0.012%
69	9.612	2662	2666	2667	rBV	204	128	0.01%	0.001%
70	9.670	2682	2684	2687	rBV	233	153	0.01%	0.001%
71	9.725	2699	2701	2704	rVB	351	160	0.01%	0.001%
72	9.818	2728	2730	2736	rVB	259	221	0.02%	0.002%
73	9.850	2737	2740	2741	rBV	238	122	0.01%	0.001%
74	9.899	2751	2755	2758	rBV3	196	143	0.01%	0.001%
75	10.162	2826	2837	2840	rBV3	17869	23984	1.80%	0.211%
76	10.207	2842	2851	2870	rVB	430866	686521	51.49%	6.051%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029673.D
 Acq On : 14 Dec 2022 00:15
 Operator : SY/MD
 Sample : N5980-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.339	2890	2892	2895	rVB	356	158	0.01%	0.001%
78	10.374	2895	2903	2912	rBV2	2539	3463	0.26%	0.031%
79	10.442	2921	2924	2928	rBV4	399	322	0.02%	0.003%
80	10.567	2955	2963	2973	rVB2	8089	12614	0.95%	0.111%
81	10.747	3013	3019	3023	rBV2	272	341	0.03%	0.003%
82	10.815	3037	3040	3044	rBV3	163	183	0.01%	0.002%
83	10.905	3062	3068	3077	rBV4	1017	1564	0.12%	0.014%
84	10.950	3077	3082	3085	rBV2	250	224	0.02%	0.002%
85	11.008	3096	3100	3103	rBV3	320	221	0.02%	0.002%
86	11.159	3143	3147	3149	rBV	509	357	0.03%	0.003%
87	11.239	3159	3172	3195	rBV	839330	1305341	97.91%	11.505%
88	11.442	3233	3235	3237	rBV2	320	127	0.01%	0.001%
89	11.519	3256	3259	3261	rBV2	333	206	0.02%	0.002%
90	11.548	3265	3268	3270	rBV2	375	231	0.02%	0.002%
91	11.612	3276	3288	3308	rBV	672771	1052937	78.98%	9.280%
92	11.780	3337	3340	3342	rBV	244	127	0.01%	0.001%
93	11.927	3385	3386	3391	rVB	258	102	0.01%	0.001%
94	12.037	3417	3420	3428	rVB2	253	271	0.02%	0.002%
95	12.333	3508	3512	3514	rBV3	453	292	0.02%	0.003%
96	12.519	3567	3570	3574	rBV3	293	261	0.02%	0.002%
97	12.538	3574	3576	3579	rBV2	436	279	0.02%	0.002%
98	12.583	3588	3590	3592	rBV	334	197	0.01%	0.002%
99	12.641	3600	3608	3612	rBV4	803	1043	0.08%	0.009%
100	12.767	3645	3647	3652	rVB3	479	332	0.02%	0.003%




Sum of corrected areas: 11345851

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029673.D
Acq On : 14 Dec 2022 00:15
Operator : SY/MD
Sample : N5980-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

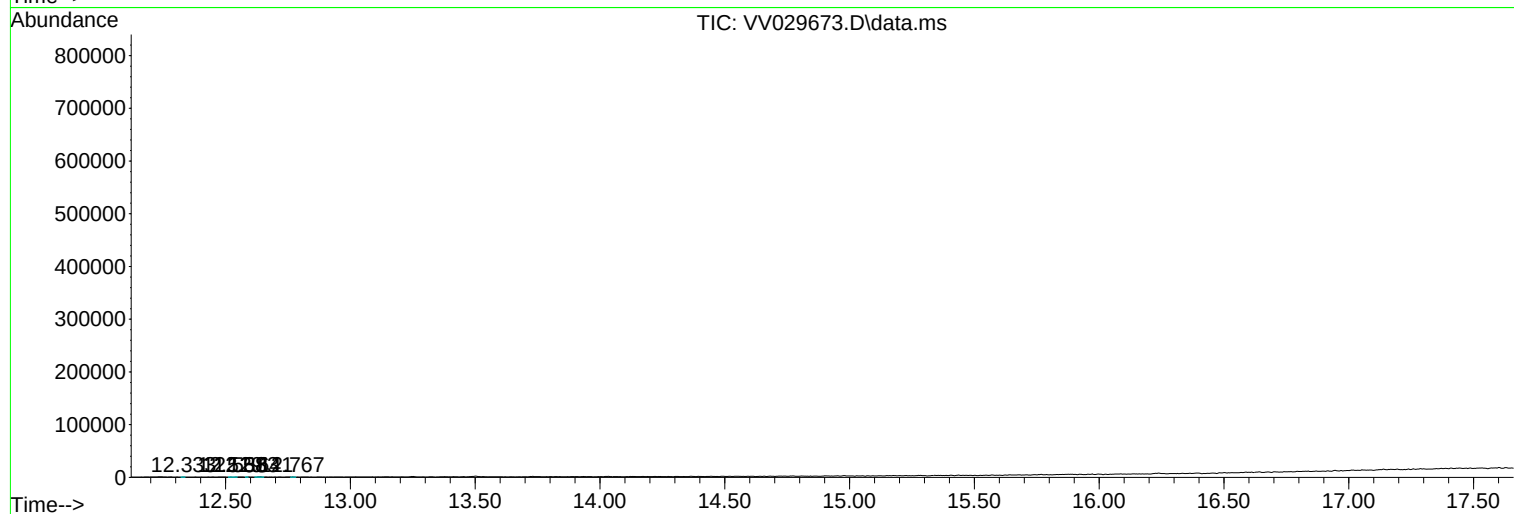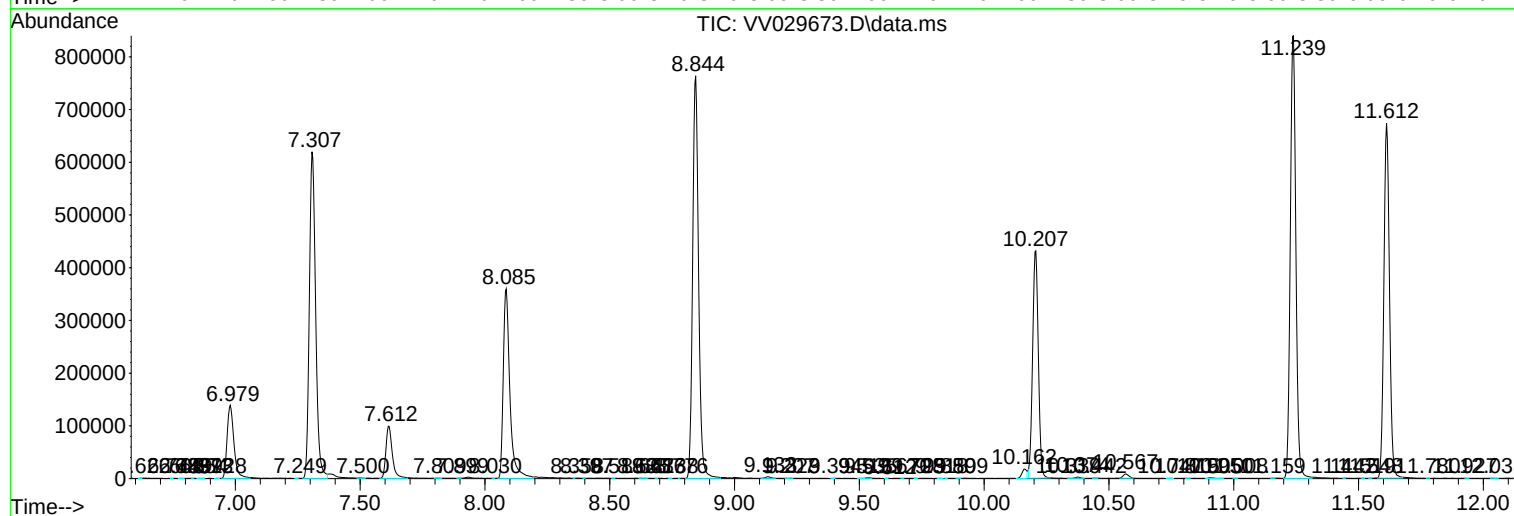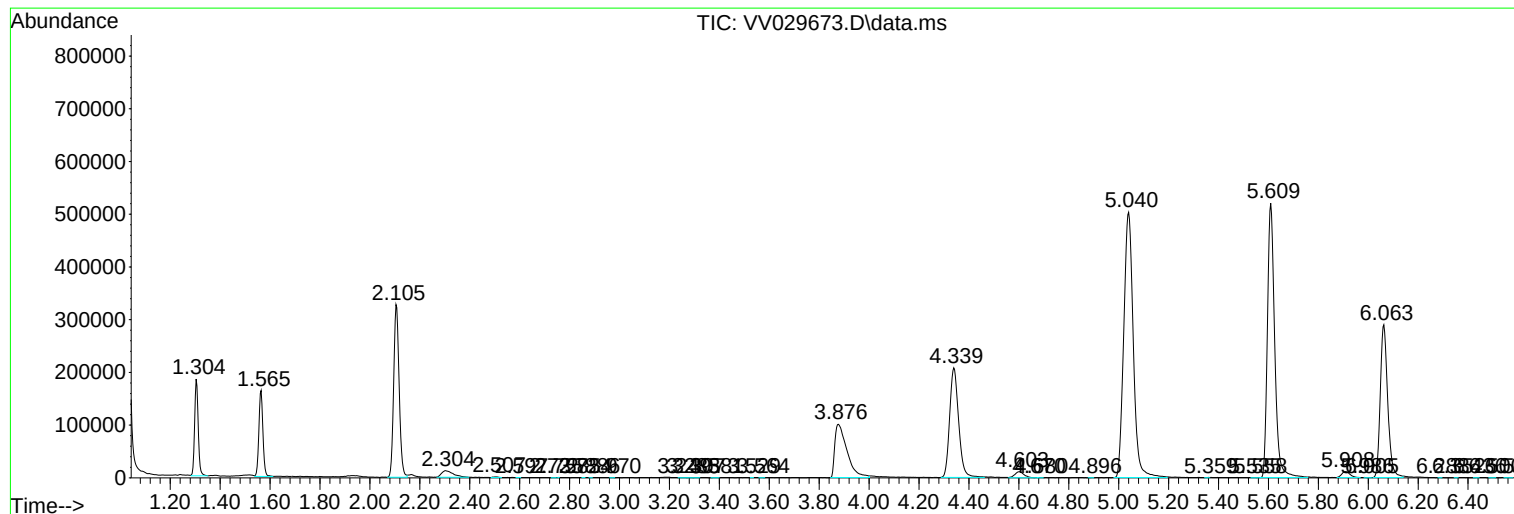

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029673.D
Acq On : 14 Dec 2022 00:15
Operator : SY/MD
Sample : N5980-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029673.D
Acq On : 14 Dec 2022 00:15
Operator : SY/MD
Sample : N5980-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------