

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029674.D
 Acq On : 14 Dec 2022 00:38
 Operator : SY/MD
 Sample : N5980-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029674.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	187172	188822	13.59%	1.501%
2	1.564	156	163	182	rVB	176014	192193	13.84%	1.528%
3	2.105	320	331	347	rBV2	329819	498187	35.87%	3.961%
4	2.272	381	383	384	rBV2	659	299	0.02%	0.002%
5	2.500	448	454	455	rBV4	1512	1050	0.08%	0.008%
6	2.597	482	484	487	rBV	232	111	0.01%	0.001%
7	2.889	572	575	581	rBV2	198	171	0.01%	0.001%
8	2.921	583	585	591	rVB3	197	162	0.01%	0.001%
9	3.143	651	654	659	rBV2	284	272	0.02%	0.002%
10	3.185	659	667	676	rVV4	1087	1983	0.14%	0.016%
11	3.246	681	686	688	rBV	261	202	0.01%	0.002%
12	3.429	739	743	748	rBV2	119	131	0.01%	0.001%
13	3.465	750	754	755	rBV	281	174	0.01%	0.001%
14	3.828	861	867	869	rBV	139	149	0.01%	0.001%
15	3.879	873	883	922	rBV	107680	363324	26.16%	2.889%
16	4.339	1011	1026	1061	rBV	217751	545889	39.30%	4.340%
17	4.542	1087	1089	1090	rBV	300	114	0.01%	0.001%
18	4.600	1096	1107	1126	rVB4	10217	25734	1.85%	0.205%
19	4.751	1150	1154	1161	rVB2	323	329	0.02%	0.003%
20	4.789	1161	1166	1170	rBV2	243	224	0.02%	0.002%
21	4.831	1177	1179	1182	rVB3	207	113	0.01%	0.001%
22	4.860	1186	1188	1191	rVB	152	105	0.01%	0.001%
23	4.886	1191	1196	1199	rBV2	154	153	0.01%	0.001%
24	4.902	1199	1201	1205	rVB2	226	146	0.01%	0.001%
25	4.969	1219	1222	1224	rBV	124	86	0.01%	0.001%
26	5.040	1224	1244	1277	rBV2	525615	1389060	100.00%	11.044%
27	5.542	1395	1400	1402	rBV2	105	101	0.01%	0.001%
28	5.609	1408	1421	1463	rBV	546820	1123536	80.88%	8.933%
29	5.908	1500	1514	1548	rBV	395782	800216	57.61%	6.362%
30	6.063	1549	1562	1593	rVB	312327	628519	45.25%	4.997%
31	6.288	1630	1632	1636	rVB3	295	232	0.02%	0.002%
32	6.317	1636	1641	1645	rBV	198	201	0.01%	0.002%
33	6.387	1660	1663	1666	rBV	251	159	0.01%	0.001%
34	6.487	1691	1694	1698	rVB	239	146	0.01%	0.001%
35	6.539	1706	1710	1711	rBV2	260	150	0.01%	0.001%
36	6.616	1731	1734	1736	rBV3	489	328	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029674.D
 Acq On : 14 Dec 2022 00:38
 Operator : SY/MD
 Sample : N5980-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.696	1757	1759	1766	rVB3	334	285	0.02%	0.002%
38	6.728	1766	1769	1771	rBV	161	107	0.01%	0.001%
39	6.751	1774	1776	1777	rBV	166	75	0.01%	0.001%
40	6.783	1783	1786	1789	rBV2	310	203	0.01%	0.002%
41	6.818	1794	1797	1801	rBV2	374	290	0.02%	0.002%
42	6.876	1812	1815	1824	rBV2	251	261	0.02%	0.002%
43	6.979	1835	1847	1877	rBV	146958	274596	19.77%	2.183%
44	7.249	1928	1931	1932	rBV3	169	81	0.01%	0.001%
45	7.307	1936	1949	1981	rBV	647184	1145702	82.48%	9.109%
46	7.612	2034	2044	2067	rBV	102853	184580	13.29%	1.468%
47	8.018	2165	2170	2173	rBV2	477	460	0.03%	0.004%
48	8.085	2181	2191	2227	rBV	383576	700793	50.45%	5.572%
49	8.474	2309	2312	2314	rBV3	366	224	0.02%	0.002%
50	8.551	2334	2336	2339	rBV3	313	181	0.01%	0.001%
51	8.603	2348	2352	2353	rBV	509	356	0.03%	0.003%
52	8.651	2363	2367	2370	rBV2	181	170	0.01%	0.001%
53	8.667	2370	2372	2374	rVB	284	93	0.01%	0.001%
54	8.680	2374	2376	2379	rBV2	270	162	0.01%	0.001%
55	8.712	2383	2386	2387	rBV2	219	141	0.01%	0.001%
56	8.760	2396	2401	2404	rBV2	309	243	0.02%	0.002%
57	8.792	2408	2411	2413	rBV	99	71	0.01%	0.001%
58	8.844	2414	2427	2458	rBV	806171	1329179	95.69%	10.568%
59	9.133	2513	2517	2524	rVB4	971	1166	0.08%	0.009%
60	9.162	2524	2526	2529	rBV	262	162	0.01%	0.001%
61	9.214	2540	2542	2547	rVB	310	123	0.01%	0.001%
62	9.275	2558	2561	2563	rBV	277	131	0.01%	0.001%
63	9.297	2566	2568	2570	rBV3	128	77	0.01%	0.001%
64	9.333	2577	2579	2582	rVB	183	72	0.01%	0.001%
65	9.468	2616	2621	2623	rBV2	151	149	0.01%	0.001%
66	9.481	2623	2625	2631	rVB2	237	127	0.01%	0.001%
67	9.522	2633	2638	2641	rBV	342	282	0.02%	0.002%
68	9.542	2641	2644	2648	rVB3	553	476	0.03%	0.004%
69	9.612	2664	2666	2674	rVB3	300	262	0.02%	0.002%
70	9.979	2777	2780	2784	rVB	254	148	0.01%	0.001%
71	10.001	2784	2787	2790	rBV2	140	92	0.01%	0.001%
72	10.162	2828	2837	2841	rBV2	17346	25720	1.85%	0.204%
73	10.204	2842	2850	2874	rVB	457847	718387	51.72%	5.712%
74	10.378	2897	2904	2912	rVB3	2042	3039	0.22%	0.024%
75	10.455	2925	2928	2933	rBV2	271	247	0.02%	0.002%
76	10.490	2937	2939	2941	rBV2	194	72	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029674.D
 Acq On : 14 Dec 2022 00:38
 Operator : SY/MD
 Sample : N5980-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.532	2947	2952	2954	rBV2	589	527	0.04%	0.004%
78	10.571	2956	2964	2975	rVB2	8677	13455	0.97%	0.107%
79	10.661	2990	2992	2996	rVB	314	158	0.01%	0.001%
80	10.683	2996	2999	3000	rBV	174	84	0.01%	0.001%
81	10.722	3007	3011	3015	rBV	217	225	0.02%	0.002%
82	10.837	3044	3047	3048	rBV	232	101	0.01%	0.001%
83	10.972	3087	3089	3092	rBV	304	170	0.01%	0.001%
84	11.111	3129	3132	3136	rVB	208	145	0.01%	0.001%
85	11.143	3139	3142	3144	rBV2	203	95	0.01%	0.001%
86	11.236	3160	3171	3200	rBV	876948	1361958	98.05%	10.829%
87	11.471	3242	3244	3246	rBV3	240	141	0.01%	0.001%
88	11.612	3276	3288	3305	rBV	659610	1045215	75.25%	8.310%
89	11.979	3399	3402	3404	rBV2	288	198	0.01%	0.002%
90	12.034	3415	3419	3421	rBV2	219	186	0.01%	0.001%
91	12.201	3469	3471	3475	rVB2	397	199	0.01%	0.002%
92	12.226	3475	3479	3480	rBV	504	352	0.03%	0.003%
93	12.374	3523	3525	3529	rBV	283	266	0.02%	0.002%
94	12.558	3579	3582	3587	rBV2	281	313	0.02%	0.002%
95	12.702	3626	3627	3632	rBV2	357	236	0.02%	0.002%
96	12.841	3668	3670	3672	rBV2	351	161	0.01%	0.001%
97	12.915	3691	3693	3701	rVB3	368	255	0.02%	0.002%
98	13.214	3784	3786	3788	rBV	342	184	0.01%	0.001%
99	13.242	3793	3795	3798	rBV2	499	337	0.02%	0.003%
100	13.599	3902	3906	3909	rBV3	580	461	0.03%	0.004%



Sum of corrected areas: 12577178

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029674.D
Acq On : 14 Dec 2022 00:38
Operator : SY/MD
Sample : N5980-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

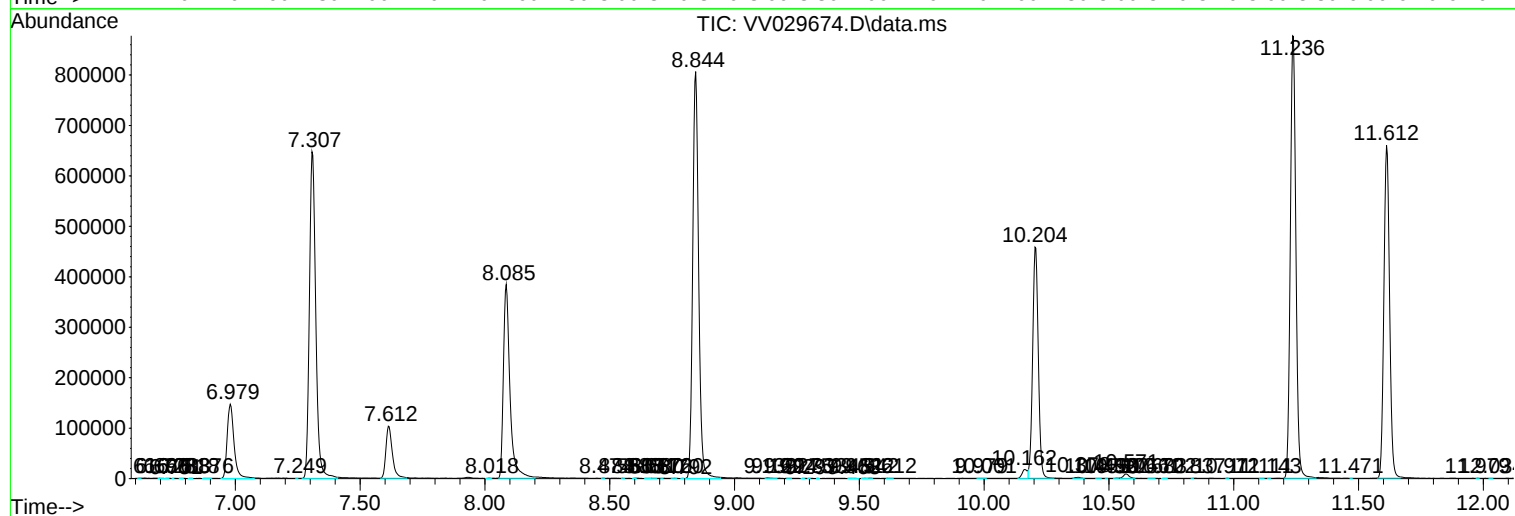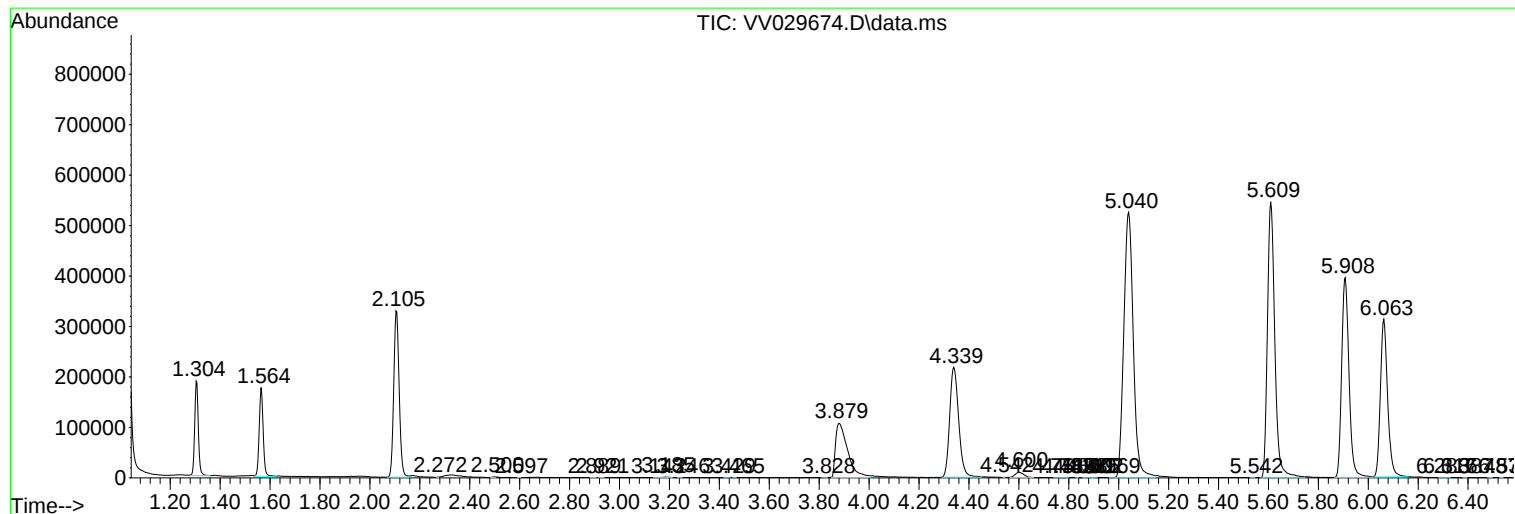

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029674.D
Acq On : 14 Dec 2022 00:38
Operator : SY/MD
Sample : N5980-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029674.D
Acq On : 14 Dec 2022 00:38
Operator : SY/MD
Sample : N5980-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------