

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029675.D
 Acq On : 14 Dec 2022 01:02
 Operator : SY/MD
 Sample : N5980-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	184148	183840	13.26%	1.614%
2	1.564	155	163	178	rVB	164968	184571	13.31%	1.621%
3	2.105	320	331	345	rBV	314333	453958	32.73%	3.986%
4	2.500	450	454	456	rBV3	999	969	0.07%	0.009%
5	2.680	507	510	512	rBV	289	154	0.01%	0.001%
6	2.738	525	528	532	rVB2	242	181	0.01%	0.002%
7	2.764	534	536	537	rBV	233	126	0.01%	0.001%
8	2.992	605	607	612	rVB	168	98	0.01%	0.001%
9	3.018	612	615	617	rBV	132	107	0.01%	0.001%
10	3.076	630	633	641	rVB2	151	207	0.01%	0.002%
11	3.214	673	676	679	rBV2	152	114	0.01%	0.001%
12	3.278	693	696	700	rBV2	256	201	0.01%	0.002%
13	3.346	716	717	721	rVB2	221	102	0.01%	0.001%
14	3.378	721	727	731	rBV2	203	261	0.02%	0.002%
15	3.420	737	740	743	rBV	245	185	0.01%	0.002%
16	3.526	768	773	774	rBV	167	145	0.01%	0.001%
17	3.609	795	799	802	rBV2	204	202	0.01%	0.002%
18	3.658	810	814	817	rBV	266	200	0.01%	0.002%
19	3.754	841	844	849	rVV2	123	144	0.01%	0.001%
20	3.796	854	857	859	rBV2	212	110	0.01%	0.001%
21	3.834	864	869	872	rBV2	140	131	0.01%	0.001%
22	3.873	872	881	920	rBV	104981	296230	21.36%	2.601%
23	4.339	1010	1026	1053	rBV	219013	538244	38.81%	4.726%
24	4.571	1096	1098	1100	rBV2	326	156	0.01%	0.001%
25	4.654	1119	1124	1127	rBV2	247	292	0.02%	0.003%
26	4.709	1138	1141	1143	rBV	173	135	0.01%	0.001%
27	4.754	1153	1155	1158	rVB	197	92	0.01%	0.001%
28	4.789	1163	1166	1168	rVV	208	96	0.01%	0.001%
29	4.857	1181	1187	1188	rBV	230	170	0.01%	0.001%
30	5.040	1226	1244	1284	rBV2	522635	1386840	100.00%	12.177%
31	5.394	1350	1354	1357	rVV3	338	338	0.02%	0.003%
32	5.429	1363	1365	1369	rVB2	279	201	0.01%	0.002%
33	5.474	1375	1379	1381	rBV4	336	270	0.02%	0.002%
34	5.558	1401	1405	1408	rBV	133	137	0.01%	0.001%
35	5.609	1408	1421	1463	rBV	512589	1052328	75.88%	9.240%
36	5.905	1503	1513	1531	rVB10	5497	12622	0.91%	0.111%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029675.D
 Acq On : 14 Dec 2022 01:02
 Operator : SY/MD
 Sample : N5980-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.063	1548	1562	1598	rBV	299859	625456	45.10%	5.492%
38	6.278	1628	1629	1631	rBV2	233	98	0.01%	0.001%
39	6.413	1668	1671	1673	rBV2	194	113	0.01%	0.001%
40	6.448	1678	1682	1685	rBV2	153	140	0.01%	0.001%
41	6.464	1685	1687	1690	rBV	233	117	0.01%	0.001%
42	6.497	1695	1697	1704	rVB2	338	248	0.02%	0.002%
43	6.628	1730	1738	1739	rBV3	756	821	0.06%	0.007%
44	6.725	1765	1768	1770	rVB2	196	112	0.01%	0.001%
45	6.776	1781	1784	1785	rBV	160	94	0.01%	0.001%
46	6.796	1788	1790	1794	rVB2	172	117	0.01%	0.001%
47	6.828	1797	1800	1802	rBV2	159	94	0.01%	0.001%
48	6.895	1817	1821	1824	rBV2	102	108	0.01%	0.001%
49	6.979	1836	1847	1869	rBV	143396	268585	19.37%	2.358%
50	7.136	1893	1896	1897	rBV	272	151	0.01%	0.001%
51	7.307	1933	1949	1986	rBV	635046	1132215	81.64%	9.942%
52	7.612	2035	2044	2066	rBV	103141	182069	13.13%	1.599%
53	7.802	2100	2103	2105	rBV	256	171	0.01%	0.002%
54	7.815	2105	2107	2110	rVB2	508	233	0.02%	0.002%
55	7.841	2110	2115	2116	rBV2	401	319	0.02%	0.003%
56	7.934	2139	2144	2155	rVB4	2581	4062	0.29%	0.036%
57	8.085	2180	2191	2224	rBV	376242	692264	49.92%	6.079%
58	8.468	2307	2310	2311	rBV	277	141	0.01%	0.001%
59	8.577	2341	2344	2347	rBV3	306	240	0.02%	0.002%
60	8.648	2362	2366	2367	rBV2	187	135	0.01%	0.001%
61	8.689	2376	2379	2382	rVB3	265	198	0.01%	0.002%
62	8.786	2404	2409	2410	rBV	298	211	0.02%	0.002%
63	8.844	2415	2427	2458	rBV	747557	1233270	88.93%	10.829%
64	9.133	2513	2517	2520	rBV4	366	287	0.02%	0.003%
65	9.191	2532	2535	2538	rVV2	341	257	0.02%	0.002%
66	9.210	2538	2541	2547	rVV2	270	244	0.02%	0.002%
67	9.236	2547	2549	2552	rVB2	259	119	0.01%	0.001%
68	9.297	2565	2568	2570	rBV2	214	123	0.01%	0.001%
69	9.442	2609	2613	2618	rBV2	245	286	0.02%	0.003%
70	9.468	2618	2621	2623	rBV3	165	99	0.01%	0.001%
71	9.519	2635	2637	2641	rBV3	279	256	0.02%	0.002%
72	9.538	2641	2643	2647	rVB3	327	245	0.02%	0.002%
73	9.580	2654	2656	2659	rBV	213	109	0.01%	0.001%
74	9.644	2672	2676	2679	rBV2	285	213	0.02%	0.002%
75	9.693	2685	2691	2694	rBV4	185	250	0.02%	0.002%
76	9.712	2695	2697	2703	rVB	400	255	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029675.D
 Acq On : 14 Dec 2022 01:02
 Operator : SY/MD
 Sample : N5980-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.898	2750	2755	2757	rVV3	219	243	0.02%	0.002%
78	9.924	2761	2763	2767	rVV2	350	204	0.01%	0.002%
79	10.059	2803	2805	2808	rVB	237	93	0.01%	0.001%
80	10.078	2808	2811	2814	rBV2	117	96	0.01%	0.001%
81	10.098	2815	2817	2822	rVV3	183	140	0.01%	0.001%
82	10.162	2828	2837	2841	rBV2	19174	27124	1.96%	0.238%
83	10.207	2842	2851	2868	rVB	455335	713419	51.44%	6.264%
84	10.374	2893	2903	2912	rVB2	2679	3882	0.28%	0.034%
85	10.567	2955	2963	2978	rVB2	8911	14710	1.06%	0.129%
86	10.667	2991	2994	2996	rBV2	220	161	0.01%	0.001%
87	11.130	3135	3138	3140	rBV2	271	145	0.01%	0.001%
88	11.178	3150	3153	3154	rBV	272	136	0.01%	0.001%
89	11.239	3160	3172	3202	rBV	811549	1275954	92.00%	11.204%
90	11.554	3267	3270	3275	rBV5	931	924	0.07%	0.008%
91	11.612	3276	3288	3310	rVV	693999	1090147	78.61%	9.572%
92	11.795	3340	3345	3348	rBV2	443	416	0.03%	0.004%
93	11.834	3354	3357	3360	rVB2	285	180	0.01%	0.002%
94	11.934	3384	3388	3394	rBV2	300	375	0.03%	0.003%
95	12.139	3449	3452	3453	rBV	183	97	0.01%	0.001%
96	12.230	3476	3480	3481	rBV3	668	481	0.03%	0.004%
97	12.387	3524	3529	3533	rBV3	248	353	0.03%	0.003%
98	12.532	3571	3574	3575	rVB2	329	141	0.01%	0.001%
99	12.606	3595	3597	3600	rBV2	247	178	0.01%	0.002%
100	12.873	3677	3680	3685	rBV3	289	272	0.02%	0.002%




Sum of corrected areas: 11388553

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029675.D
Acq On : 14 Dec 2022 01:02
Operator : SY/MD
Sample : N5980-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

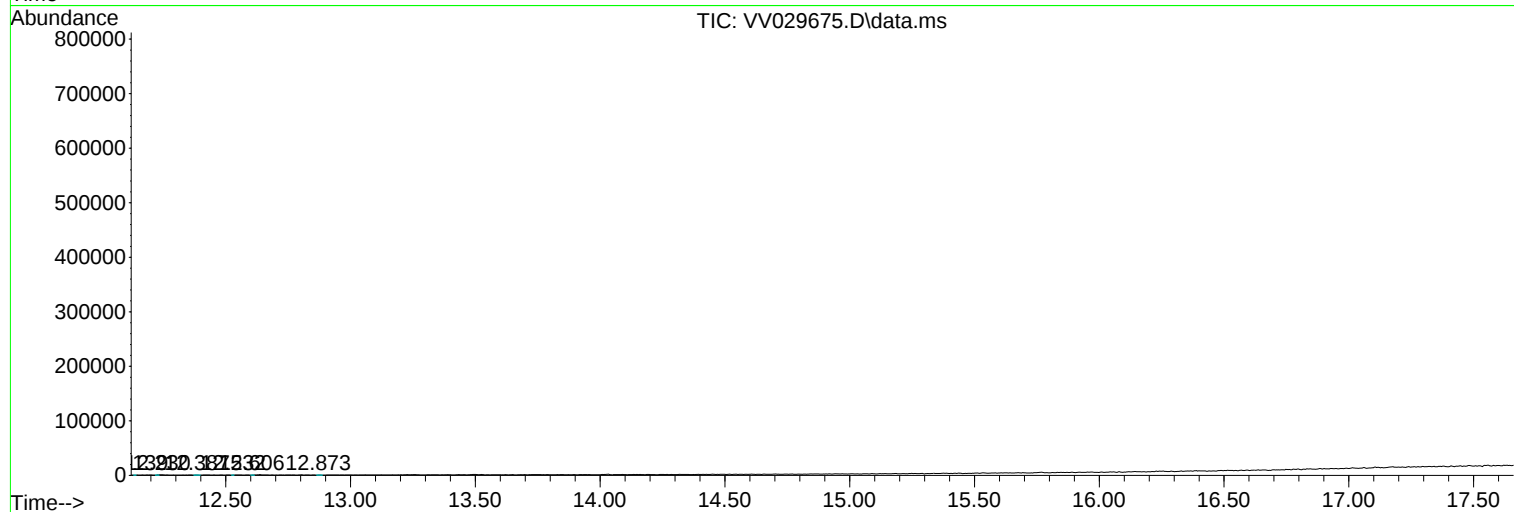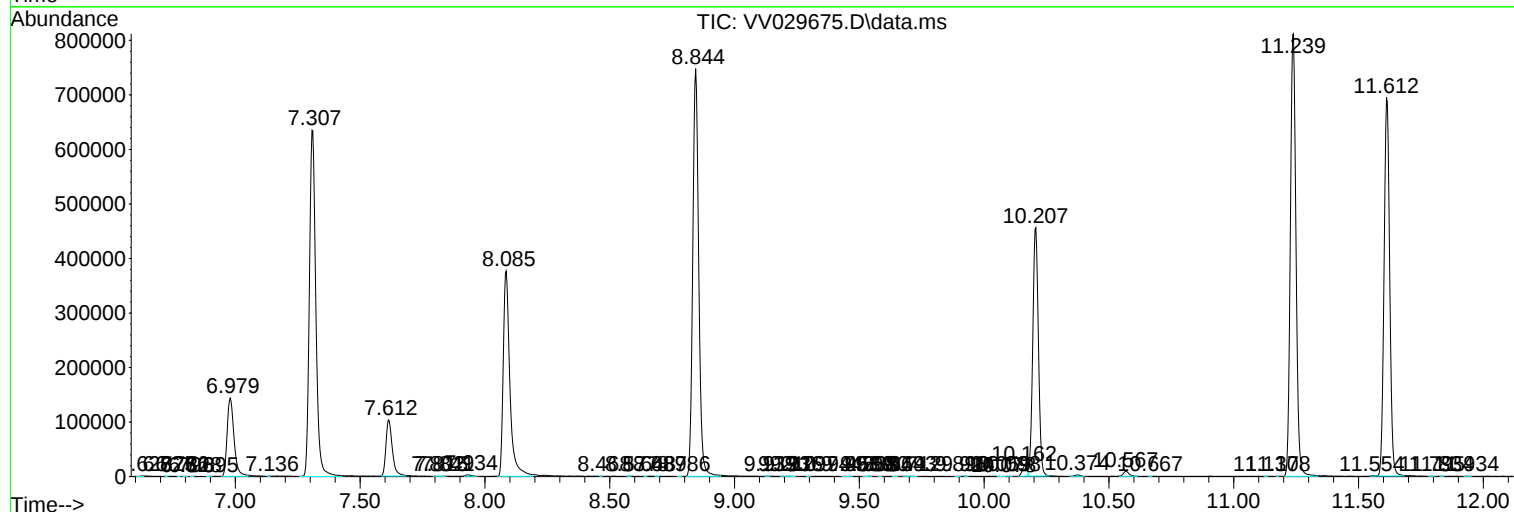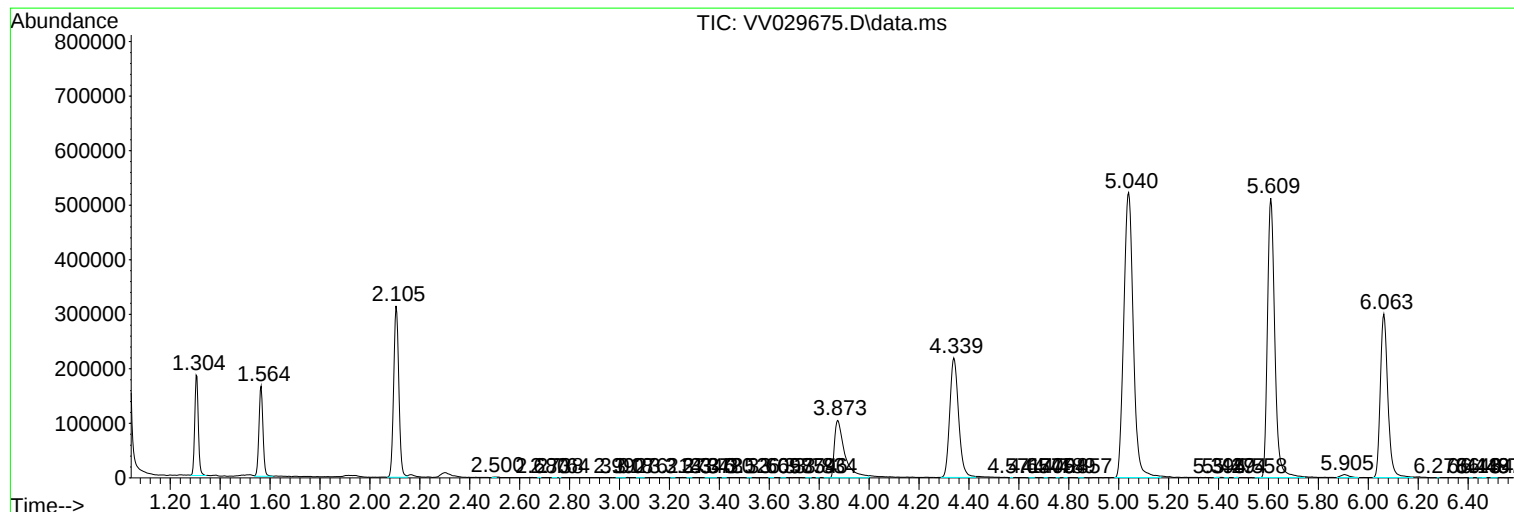

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029675.D
Acq On : 14 Dec 2022 01:02
Operator : SY/MD
Sample : N5980-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029675.D
Acq On : 14 Dec 2022 01:02
Operator : SY/MD
Sample : N5980-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc