

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029676.D
 Acq On : 14 Dec 2022 01:25
 Operator : SY/MD
 Sample : N5980-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	189075	189510	13.31%	1.596%
2	1.565	156	163	178	rVB	166521	187618	13.18%	1.580%
3	2.105	320	331	345	rBV	318372	457981	32.18%	3.856%
4	2.507	449	456	462	rVB4	1422	1914	0.13%	0.016%
5	2.581	477	479	482	rVB	294	142	0.01%	0.001%
6	2.925	583	586	588	rBV2	196	139	0.01%	0.001%
7	3.076	631	633	635	rBV	209	114	0.01%	0.001%
8	3.182	663	666	667	rBV	289	161	0.01%	0.001%
9	3.272	688	694	700	rBV2	241	367	0.03%	0.003%
10	3.574	785	788	790	rBV2	115	78	0.01%	0.001%
11	3.626	801	804	806	rBV	94	50	0.00%	0.000%
12	3.658	811	814	818	rVB	307	260	0.02%	0.002%
13	3.690	820	824	831	rVB2	224	260	0.02%	0.002%
14	3.744	831	841	845	rBV2	259	414	0.03%	0.003%
15	3.876	872	882	932	rBV	102036	301976	21.22%	2.543%
16	4.339	1011	1026	1054	rBV	220627	547501	38.47%	4.610%
17	4.725	1143	1146	1147	rBV2	226	135	0.01%	0.001%
18	4.754	1152	1155	1158	rVB	160	96	0.01%	0.001%
19	4.777	1158	1162	1164	rBV	202	168	0.01%	0.001%
20	4.812	1170	1173	1175	rBV2	150	97	0.01%	0.001%
21	4.825	1175	1177	1178	rBV	223	88	0.01%	0.001%
22	4.854	1185	1186	1187	rBV	243	51	0.00%	0.000%
23	4.928	1207	1209	1211	rBV	243	115	0.01%	0.001%
24	4.941	1211	1213	1215	rVB2	168	69	0.00%	0.001%
25	4.970	1220	1222	1223	rBV	136	66	0.00%	0.001%
26	5.040	1226	1244	1295	rBV2	540203	1423364	100.00%	11.985%
27	5.497	1383	1386	1390	rBV3	190	134	0.01%	0.001%
28	5.539	1395	1399	1401	rBV2	373	240	0.02%	0.002%
29	5.609	1408	1421	1451	rBV	554578	1125213	79.05%	9.475%
30	5.912	1504	1515	1534	rVB8	8903	22052	1.55%	0.186%
31	5.982	1535	1537	1539	rBV	213	107	0.01%	0.001%
32	6.063	1547	1562	1597	rBV	310920	646406	45.41%	5.443%
33	6.330	1642	1645	1649	rVB2	286	233	0.02%	0.002%
34	6.378	1657	1660	1663	rVB2	145	97	0.01%	0.001%
35	6.410	1668	1670	1673	rVB	251	63	0.00%	0.001%
36	6.465	1685	1687	1694	rVB2	221	157	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029676.D
 Acq On : 14 Dec 2022 01:25
 Operator : SY/MD
 Sample : N5980-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.494	1694	1696	1699	rVB	123	58	0.00%	0.000%
38	6.523	1699	1705	1707	rBV2	323	335	0.02%	0.003%
39	6.548	1711	1713	1718	rVB2	245	121	0.01%	0.001%
40	6.568	1718	1719	1722	rVB	156	42	0.00%	0.000%
41	6.596	1726	1728	1731	rVB	146	79	0.01%	0.001%
42	6.622	1731	1736	1738	rBV2	840	695	0.05%	0.006%
43	6.863	1809	1811	1813	rBV	160	71	0.00%	0.001%
44	6.905	1822	1824	1827	rVB2	242	146	0.01%	0.001%
45	6.928	1827	1831	1832	rBV	214	151	0.01%	0.001%
46	6.979	1835	1847	1882	rVV	149718	279990	19.67%	2.358%
47	7.243	1926	1929	1935	rVB3	367	321	0.02%	0.003%
48	7.307	1935	1949	1984	rBV	648862	1164099	81.79%	9.802%
49	7.613	2034	2044	2067	rBV	106033	188810	13.27%	1.590%
50	7.854	2118	2119	2120	rBV	200	63	0.00%	0.001%
51	8.005	2165	2166	2169	rVB	296	68	0.00%	0.001%
52	8.085	2180	2191	2226	rBV	388319	709873	49.87%	5.977%
53	8.580	2343	2345	2349	rBV	235	135	0.01%	0.001%
54	8.693	2377	2380	2381	rBV	120	66	0.00%	0.001%
55	8.764	2397	2402	2405	rBV	234	224	0.02%	0.002%
56	8.780	2405	2407	2408	rBV	147	69	0.00%	0.001%
57	8.844	2414	2427	2459	rBV	817313	1334702	93.77%	11.239%
58	9.059	2490	2494	2497	rVB2	536	378	0.03%	0.003%
59	9.075	2497	2499	2504	rBV	231	112	0.01%	0.001%
60	9.114	2509	2511	2512	rBV	238	69	0.00%	0.001%
61	9.127	2512	2515	2516	rBV	293	160	0.01%	0.001%
62	9.262	2554	2557	2559	rBV	108	84	0.01%	0.001%
63	9.278	2559	2562	2565	rVV2	264	192	0.01%	0.002%
64	9.301	2567	2569	2575	rVB3	372	269	0.02%	0.002%
65	9.333	2575	2579	2584	rVB2	354	396	0.03%	0.003%
66	9.365	2584	2589	2590	rBV2	272	191	0.01%	0.002%
67	9.420	2605	2606	2607	rVB	237	46	0.00%	0.000%
68	9.561	2648	2650	2652	rBV	319	169	0.01%	0.001%
69	9.638	2671	2674	2675	rBV	149	89	0.01%	0.001%
70	9.915	2757	2760	2761	rBV	274	156	0.01%	0.001%
71	9.928	2761	2764	2768	rVB3	538	398	0.03%	0.003%
72	10.043	2796	2800	2801	rBV3	280	207	0.01%	0.002%
73	10.120	2822	2824	2826	rBV	185	103	0.01%	0.001%
74	10.162	2828	2837	2841	rVV2	19162	27736	1.95%	0.234%
75	10.207	2842	2851	2868	rVB	466518	732695	51.48%	6.170%
76	10.374	2896	2903	2916	rVB3	3250	5396	0.38%	0.045%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029676.D
 Acq On : 14 Dec 2022 01:25
 Operator : SY/MD
 Sample : N5980-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.445	2922	2925	2927	rBV2	164	109	0.01%	0.001%
78	10.461	2927	2930	2934	rVV2	260	245	0.02%	0.002%
79	10.535	2946	2953	2954	rBV2	535	534	0.04%	0.004%
80	10.567	2955	2963	2978	rVB2	9058	15111	1.06%	0.127%
81	10.635	2982	2984	2986	rBV2	177	80	0.01%	0.001%
82	10.648	2986	2988	2989	rBV2	139	36	0.00%	0.000%
83	10.767	3023	3025	3027	rVB2	199	59	0.00%	0.000%
84	11.091	3124	3126	3128	rBV2	182	70	0.00%	0.001%
85	11.236	3159	3171	3199	rBV	885234	1383576	97.20%	11.650%
86	11.493	3249	3251	3252	rBV	243	81	0.01%	0.001%
87	11.548	3266	3268	3270	rBV2	481	300	0.02%	0.003%
88	11.612	3276	3288	3313	rBV	712753	1119330	78.64%	9.425%
89	12.381	3524	3527	3529	rVB	228	122	0.01%	0.001%




Sum of corrected areas: 11876053

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029676.D
Acq On : 14 Dec 2022 01:25
Operator : SY/MD
Sample : N5980-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

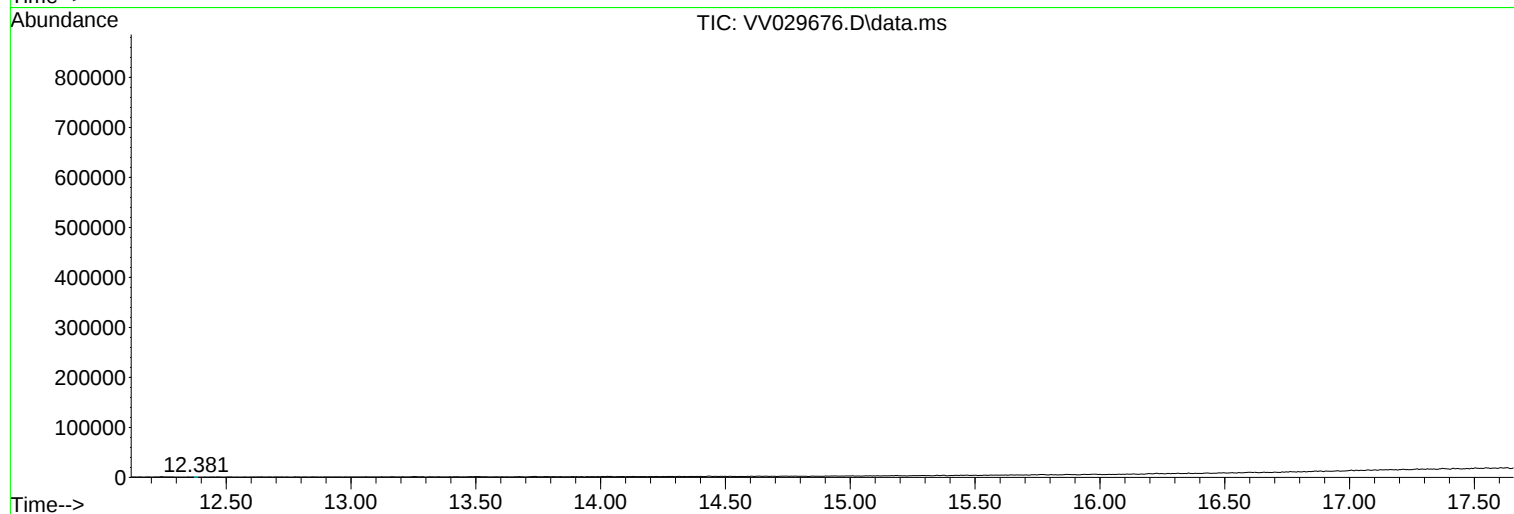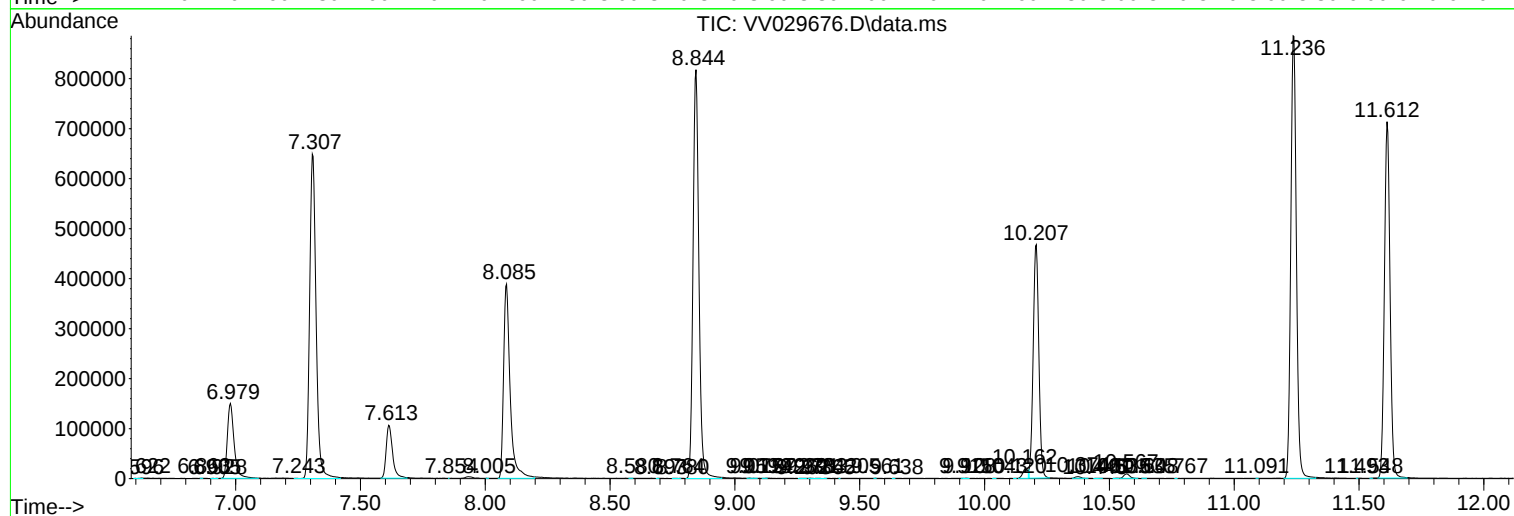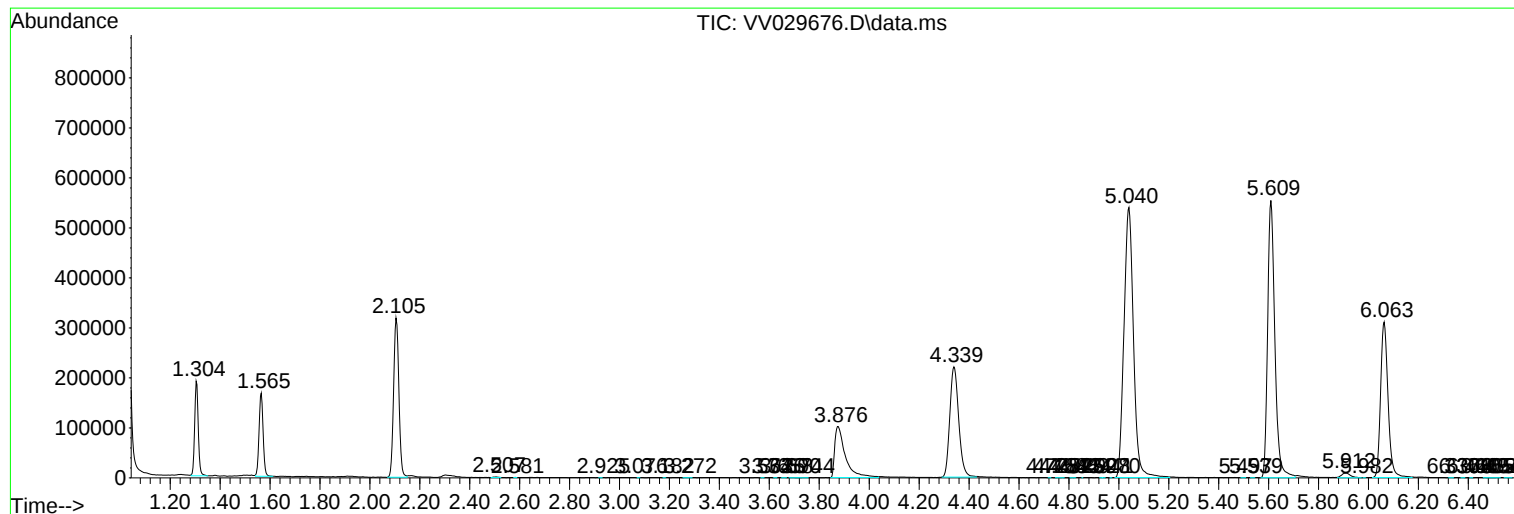

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029676.D
Acq On : 14 Dec 2022 01:25
Operator : SY/MD
Sample : N5980-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029676.D
Acq On : 14 Dec 2022 01:25
Operator : SY/MD
Sample : N5980-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc