

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029677.D
 Acq On : 14 Dec 2022 01:49
 Operator : SY/MD
 Sample : N5980-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ER1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VW029677.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	183110	183340	13.31%	1.603%
2	1.565	156	163	176	rVB	171452	185268	13.45%	1.620%
3	2.105	321	331	345	rBV	312330	447907	32.51%	3.916%
4	2.571	474	476	479	rVB2	200	108	0.01%	0.001%
5	2.658	492	503	509	rBV4	893	1667	0.12%	0.015%
6	2.761	531	535	536	rBV2	307	195	0.01%	0.002%
7	2.950	591	594	600	rVB4	323	294	0.02%	0.003%
8	3.169	658	662	663	rBV	192	126	0.01%	0.001%
9	3.391	729	731	733	rBV	237	95	0.01%	0.001%
10	3.507	762	767	769	rBV2	228	202	0.01%	0.002%
11	3.654	809	813	818	rVB	202	225	0.02%	0.002%
12	3.732	832	837	843	rBV2	161	225	0.02%	0.002%
13	3.844	866	872	873	rBV	198	157	0.01%	0.001%
14	3.880	873	883	926	rBV	102408	302224	21.94%	2.642%
15	4.339	1010	1026	1054	rBV	213642	532262	38.63%	4.653%
16	4.600	1105	1107	1109	rBV2	370	222	0.02%	0.002%
17	4.654	1122	1124	1126	rBV2	188	107	0.01%	0.001%
18	4.719	1140	1144	1147	rBV2	146	122	0.01%	0.001%
19	4.764	1154	1158	1163	rVB	258	248	0.02%	0.002%
20	4.841	1179	1182	1185	rVB2	202	121	0.01%	0.001%
21	4.889	1195	1197	1207	rVB2	292	298	0.02%	0.003%
22	4.934	1208	1211	1212	rBV	167	80	0.01%	0.001%
23	5.040	1225	1244	1301	rBV2	520040	1377749	100.00%	12.044%
24	5.394	1351	1354	1356	rBV2	335	222	0.02%	0.002%
25	5.426	1361	1364	1366	rBV	213	137	0.01%	0.001%
26	5.439	1366	1368	1372	rBV	185	160	0.01%	0.001%
27	5.510	1387	1390	1392	rBV2	372	234	0.02%	0.002%
28	5.564	1405	1407	1408	rBV	171	84	0.01%	0.001%
29	5.609	1408	1421	1455	rBV	523707	1069352	77.62%	9.348%
30	5.905	1501	1513	1523	rBV4	4453	9785	0.71%	0.086%
31	6.008	1544	1545	1547	rBV2	198	75	0.01%	0.001%
32	6.063	1547	1562	1585	rBV	303385	619206	44.94%	5.413%
33	6.342	1645	1649	1653	rBV2	213	188	0.01%	0.002%
34	6.365	1654	1656	1658	rBV	178	78	0.01%	0.001%
35	6.420	1670	1673	1676	rBV	188	185	0.01%	0.002%
36	6.545	1709	1712	1713	rBV	215	130	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029677.D
 Acq On : 14 Dec 2022 01:49
 Operator : SY/MD
 Sample : N5980-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ER1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.625	1731	1737	1740	rBV5	645	661	0.05%	0.006%
38	6.738	1770	1772	1774	rVB	242	74	0.01%	0.001%
39	6.783	1784	1786	1787	rBV	165	70	0.01%	0.001%
40	6.828	1798	1800	1806	rVB2	200	170	0.01%	0.001%
41	6.892	1818	1820	1824	rVB2	188	87	0.01%	0.001%
42	6.931	1830	1832	1836	rVB	281	114	0.01%	0.001%
43	6.979	1836	1847	1875	rBV	144660	269509	19.56%	2.356%
44	7.230	1923	1925	1928	rVB3	776	381	0.03%	0.003%
45	7.246	1928	1930	1931	rBV3	249	68	0.00%	0.001%
46	7.259	1931	1934	1936	rBV2	412	247	0.02%	0.002%
47	7.307	1936	1949	1981	rBV	631200	1115177	80.94%	9.749%
48	7.613	2035	2044	2068	rBV	101529	179348	13.02%	1.568%
49	7.934	2136	2144	2153	rVB5	2094	3532	0.26%	0.031%
50	8.085	2180	2191	2223	rBV	377817	700891	50.87%	6.127%
51	8.474	2309	2312	2314	rBV2	295	193	0.01%	0.002%
52	8.526	2325	2328	2329	rBV2	348	167	0.01%	0.001%
53	8.539	2329	2332	2334	rBV	213	116	0.01%	0.001%
54	8.551	2334	2336	2337	rVB	236	95	0.01%	0.001%
55	8.600	2348	2351	2354	rBV	360	305	0.02%	0.003%
56	8.728	2389	2391	2393	rBV	158	62	0.00%	0.001%
57	8.767	2401	2403	2404	rVB	248	67	0.00%	0.001%
58	8.844	2414	2427	2457	rBV	777831	1271888	92.32%	11.119%
59	9.130	2514	2516	2520	rVB4	790	412	0.03%	0.004%
60	9.182	2529	2532	2535	rBV	180	111	0.01%	0.001%
61	9.262	2554	2557	2562	rBV2	322	276	0.02%	0.002%
62	9.284	2562	2564	2569	rVV2	293	197	0.01%	0.002%
63	9.429	2607	2609	2611	rBV	146	66	0.00%	0.001%
64	9.539	2640	2643	2646	rBV2	232	143	0.01%	0.001%
65	9.783	2715	2719	2723	rBV2	289	303	0.02%	0.003%
66	9.809	2723	2727	2729	rBV2	179	127	0.01%	0.001%
67	9.854	2737	2741	2745	rBV2	250	219	0.02%	0.002%
68	9.924	2758	2763	2768	rBV4	435	550	0.04%	0.005%
69	9.973	2776	2778	2781	rVV2	219	85	0.01%	0.001%
70	9.989	2781	2783	2784	rVB	202	63	0.00%	0.001%
71	10.002	2784	2787	2790	rBV	195	118	0.01%	0.001%
72	10.075	2808	2810	2813	rBV	167	75	0.01%	0.001%
73	10.162	2827	2837	2841	rBV	18057	26463	1.92%	0.231%
74	10.207	2841	2851	2872	rVB	447160	714530	51.86%	6.247%
75	10.342	2889	2893	2894	rBV2	246	185	0.01%	0.002%
76	10.374	2895	2903	2915	rVB3	2607	3759	0.27%	0.033%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029677.D
 Acq On : 14 Dec 2022 01:49
 Operator : SY/MD
 Sample : N5980-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ER1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.445	2920	2925	2927	rBV2	155	158	0.01%	0.001%
78	10.458	2927	2929	2931	rBV	170	73	0.01%	0.001%
79	10.490	2937	2939	2940	rBV	258	123	0.01%	0.001%
80	10.522	2947	2949	2952	rBV2	291	175	0.01%	0.002%
81	10.567	2955	2963	2976	rVB2	8167	13889	1.01%	0.121%
82	10.641	2983	2986	2988	rBV2	262	156	0.01%	0.001%
83	10.709	3004	3007	3010	rBV2	212	151	0.01%	0.001%
84	10.757	3019	3022	3023	rBV	221	129	0.01%	0.001%
85	10.812	3036	3039	3042	rBV	202	150	0.01%	0.001%
86	10.841	3046	3048	3050	rBV2	374	218	0.02%	0.002%
87	11.001	3093	3098	3101	rBV2	224	223	0.02%	0.002%
88	11.053	3110	3114	3115	rBV	226	161	0.01%	0.001%
89	11.082	3120	3123	3124	rBV	235	136	0.01%	0.001%
90	11.175	3147	3152	3157	rBV3	551	562	0.04%	0.005%
91	11.236	3159	3171	3195	rBV	843880	1313154	95.31%	11.480%
92	11.484	3246	3248	3252	rBV2	269	164	0.01%	0.001%
93	11.612	3276	3288	3311	rBV	679896	1083165	78.62%	9.469%
94	11.844	3358	3360	3363	rVB2	301	120	0.01%	0.001%
95	11.950	3390	3393	3395	rBV3	244	147	0.01%	0.001%
96	12.217	3473	3476	3477	rBV	161	85	0.01%	0.001%
97	12.236	3477	3482	3488	rVV3	793	973	0.07%	0.009%
98	12.722	3630	3633	3635	rBV3	318	202	0.01%	0.002%
99	12.918	3691	3694	3696	rBV2	284	165	0.01%	0.001%
100	13.059	3735	3738	3743	rBV2	450	420	0.03%	0.004%




Sum of corrected areas: 11438881

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029677.D
Acq On : 14 Dec 2022 01:49
Operator : SY/MD
Sample : N5980-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ER1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

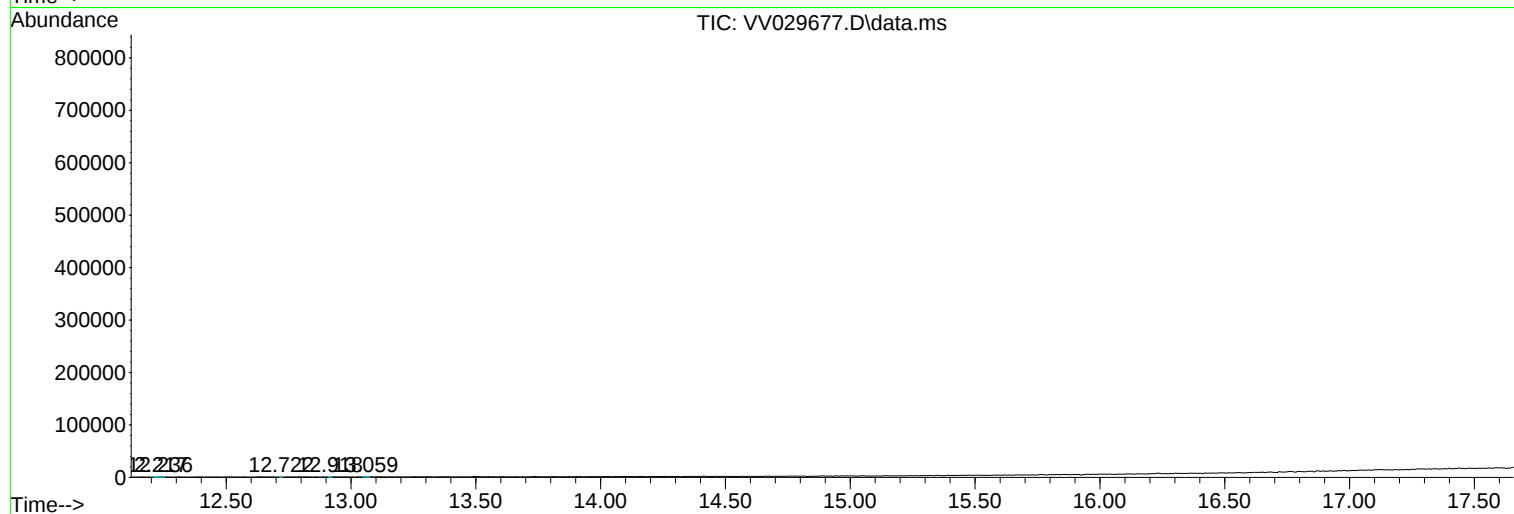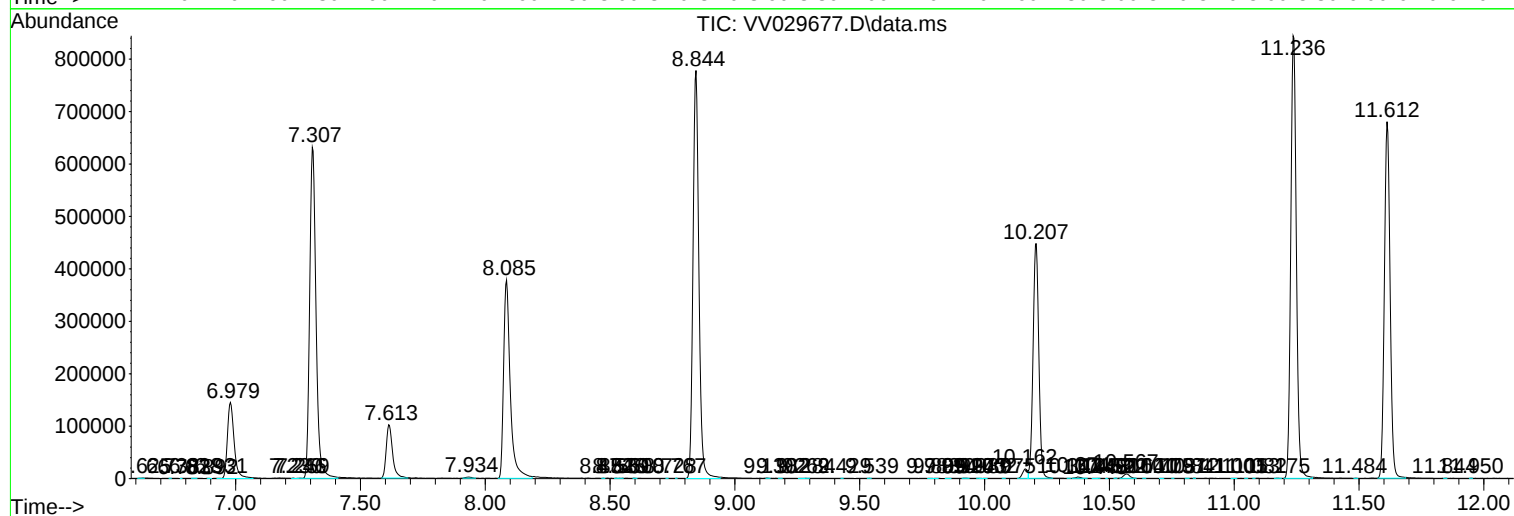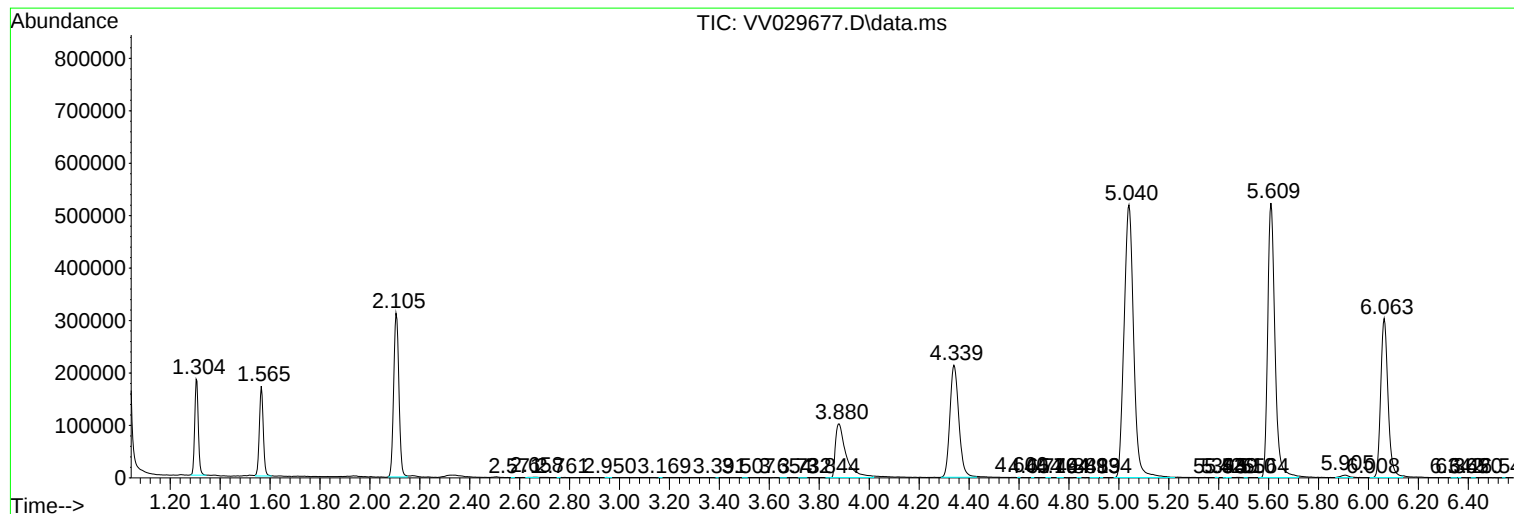

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029677.D
Acq On : 14 Dec 2022 01:49
Operator : SY/MD
Sample : N5980-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ER1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029677.D
Acq On : 14 Dec 2022 01:49
Operator : SY/MD
Sample : N5980-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ER1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------