

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029680.D
 Acq On : 14 Dec 2022 02:59
 Operator : SY/MD
 Sample : N5980-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ES2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	191386	188729	13.87%	1.649%
2	1.564	156	163	175	rVB	170474	188163	13.83%	1.645%
3	2.105	320	331	345	rBV	312619	447612	32.90%	3.912%
4	2.503	450	455	463	rVB2	1248	1587	0.12%	0.014%
5	2.558	470	472	475	rBV2	199	92	0.01%	0.001%
6	2.642	494	498	503	rBV3	419	487	0.04%	0.004%
7	2.757	530	534	538	rBV2	444	375	0.03%	0.003%
8	2.831	555	557	561	rBV	114	93	0.01%	0.001%
9	2.986	603	605	606	rBV	168	50	0.00%	0.000%
10	3.371	723	725	726	rBV	123	62	0.00%	0.001%
11	3.564	782	785	787	rBV	122	66	0.00%	0.001%
12	3.596	792	795	798	rBV2	131	83	0.01%	0.001%
13	3.754	841	844	845	rBV2	85	56	0.00%	0.000%
14	3.818	859	864	865	rBV	119	105	0.01%	0.001%
15	3.876	872	882	925	rBV	100621	291365	21.42%	2.547%
16	4.339	1010	1026	1055	rBV2	208436	524359	38.54%	4.583%
17	4.635	1113	1118	1120	rBV2	227	211	0.02%	0.002%
18	4.728	1145	1147	1149	rBV	210	105	0.01%	0.001%
19	4.825	1174	1177	1179	rBV2	322	211	0.02%	0.002%
20	4.857	1184	1187	1191	rVB2	193	130	0.01%	0.001%
21	4.889	1194	1197	1199	rBV	225	168	0.01%	0.001%
22	4.976	1221	1224	1225	rBV	130	82	0.01%	0.001%
23	5.040	1226	1244	1275	rBV2	512174	1347263	99.03%	11.775%
24	5.439	1366	1368	1371	rBV3	271	189	0.01%	0.002%
25	5.474	1375	1379	1384	rVV2	409	412	0.03%	0.004%
26	5.497	1384	1386	1387	rVV	243	93	0.01%	0.001%
27	5.510	1388	1390	1393	rVB2	310	142	0.01%	0.001%
28	5.609	1407	1421	1452	rBV	542037	1102068	81.01%	9.632%
29	5.902	1503	1512	1526	rVB6	4929	10186	0.75%	0.089%
30	6.063	1548	1562	1599	rBV	290782	612353	45.01%	5.352%
31	6.333	1644	1646	1647	rVB2	241	54	0.00%	0.000%
32	6.346	1647	1650	1654	rBV2	87	83	0.01%	0.001%
33	6.590	1724	1726	1728	rBV	136	85	0.01%	0.001%
34	6.603	1728	1730	1733	rBV2	177	104	0.01%	0.001%
35	6.764	1775	1780	1785	rBV2	163	192	0.01%	0.002%
36	6.783	1785	1786	1789	rVB	179	63	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029680.D
 Acq On : 14 Dec 2022 02:59
 Operator : SY/MD
 Sample : N5980-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ES2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.809	1793	1794	1797	rBV2	205	82	0.01%	0.001%
38	6.825	1797	1799	1801	rVV	275	104	0.01%	0.001%
39	6.860	1805	1810	1813	rBV2	230	210	0.02%	0.002%
40	6.908	1821	1825	1827	rBV	229	134	0.01%	0.001%
41	6.979	1835	1847	1871	rBV	142458	263345	19.36%	2.302%
42	7.162	1899	1904	1907	rBV3	600	539	0.04%	0.005%
43	7.236	1924	1927	1929	rBV	284	206	0.02%	0.002%
44	7.307	1937	1949	1984	rBV	624270	1110717	81.64%	9.708%
45	7.612	2034	2044	2069	rBV	101273	178289	13.10%	1.558%
46	7.828	2108	2111	2113	rBV3	311	180	0.01%	0.002%
47	7.931	2139	2143	2152	rVB5	1723	2565	0.19%	0.022%
48	8.085	2180	2191	2222	rBV	364492	677588	49.80%	5.922%
49	8.490	2315	2317	2320	rBV	328	189	0.01%	0.002%
50	8.593	2345	2349	2354	rBV2	272	253	0.02%	0.002%
51	8.619	2354	2357	2359	rVB	221	141	0.01%	0.001%
52	8.645	2359	2365	2367	rBV3	231	200	0.01%	0.002%
53	8.657	2367	2369	2376	rVB3	225	188	0.01%	0.002%
54	8.706	2382	2384	2387	rVB	205	93	0.01%	0.001%
55	8.722	2387	2389	2390	rBV	147	62	0.00%	0.001%
56	8.735	2390	2393	2396	rBV	261	132	0.01%	0.001%
57	8.767	2402	2403	2406	rBV	235	83	0.01%	0.001%
58	8.783	2406	2408	2410	rVB	178	85	0.01%	0.001%
59	8.844	2414	2427	2463	rBV	803277	1312101	96.44%	11.468%
60	9.136	2513	2518	2523	rBV4	499	535	0.04%	0.005%
61	9.178	2528	2531	2533	rBV3	210	132	0.01%	0.001%
62	9.236	2547	2549	2551	rBV	232	109	0.01%	0.001%
63	9.268	2556	2559	2560	rVV	129	57	0.00%	0.000%
64	9.281	2560	2563	2567	rVV2	169	127	0.01%	0.001%
65	9.381	2592	2594	2601	rVB2	370	288	0.02%	0.003%
66	9.410	2601	2603	2604	rBV2	235	77	0.01%	0.001%
67	9.503	2629	2632	2640	rBV	192	199	0.01%	0.002%
68	9.538	2640	2643	2644	rBV	248	145	0.01%	0.001%
69	9.558	2647	2649	2654	rBV2	332	289	0.02%	0.003%
70	9.680	2684	2687	2690	rBV	149	103	0.01%	0.001%
71	9.760	2709	2712	2718	rBV2	241	193	0.01%	0.002%
72	9.863	2741	2744	2746	rBV	131	78	0.01%	0.001%
73	9.921	2758	2762	2769	rVB3	413	494	0.04%	0.004%
74	10.014	2788	2791	2793	rBV2	339	173	0.01%	0.002%
75	10.046	2799	2801	2803	rVB2	215	69	0.01%	0.001%
76	10.059	2803	2805	2807	rBV	122	68	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029680.D
 Acq On : 14 Dec 2022 02:59
 Operator : SY/MD
 Sample : N5980-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ES2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.098	2814	2817	2819	rBV2	203	124	0.01%	0.001%
78	10.162	2827	2837	2841	rBV2	18386	26298	1.93%	0.230%
79	10.204	2842	2850	2872	rVB	440776	696504	51.20%	6.087%
80	10.371	2896	2902	2909	rBV3	1856	2301	0.17%	0.020%
81	10.452	2924	2927	2928	rBV3	170	81	0.01%	0.001%
82	10.503	2940	2943	2948	rVB3	224	172	0.01%	0.002%
83	10.567	2953	2963	2975	rVB3	8092	13044	0.96%	0.114%
84	10.641	2984	2986	2990	rBV2	176	115	0.01%	0.001%
85	10.693	2999	3002	3005	rBV	267	190	0.01%	0.002%
86	11.024	3102	3105	3109	rBV2	275	207	0.02%	0.002%
87	11.082	3122	3123	3126	rBV	202	105	0.01%	0.001%
88	11.175	3147	3152	3156	rVB3	661	595	0.04%	0.005%
89	11.236	3159	3171	3202	rBV	867248	1360488	100.00%	11.891%
90	11.558	3265	3271	3276	rBV3	1348	1628	0.12%	0.014%
91	11.612	3276	3288	3309	rVV	687976	1069830	78.64%	9.350%
92	11.940	3386	3390	3395	rBV2	506	455	0.03%	0.004%
93	11.992	3403	3406	3409	rBV2	274	219	0.02%	0.002%
94	12.037	3418	3420	3423	rBV2	201	96	0.01%	0.001%
95	12.377	3523	3526	3527	rBV2	167	95	0.01%	0.001%
96	12.631	3602	3605	3606	rBV2	320	174	0.01%	0.002%
97	12.699	3623	3626	3628	rBV2	303	249	0.02%	0.002%
98	12.747	3639	3641	3643	rVB2	490	153	0.01%	0.001%
99	12.802	3655	3658	3659	rBV	297	171	0.01%	0.001%
100	12.992	3713	3717	3720	rBV2	386	350	0.03%	0.003%


Sum of corrected areas: 11441744

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029680.D
Acq On : 14 Dec 2022 02:59
Operator : SY/MD
Sample : N5980-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ES2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

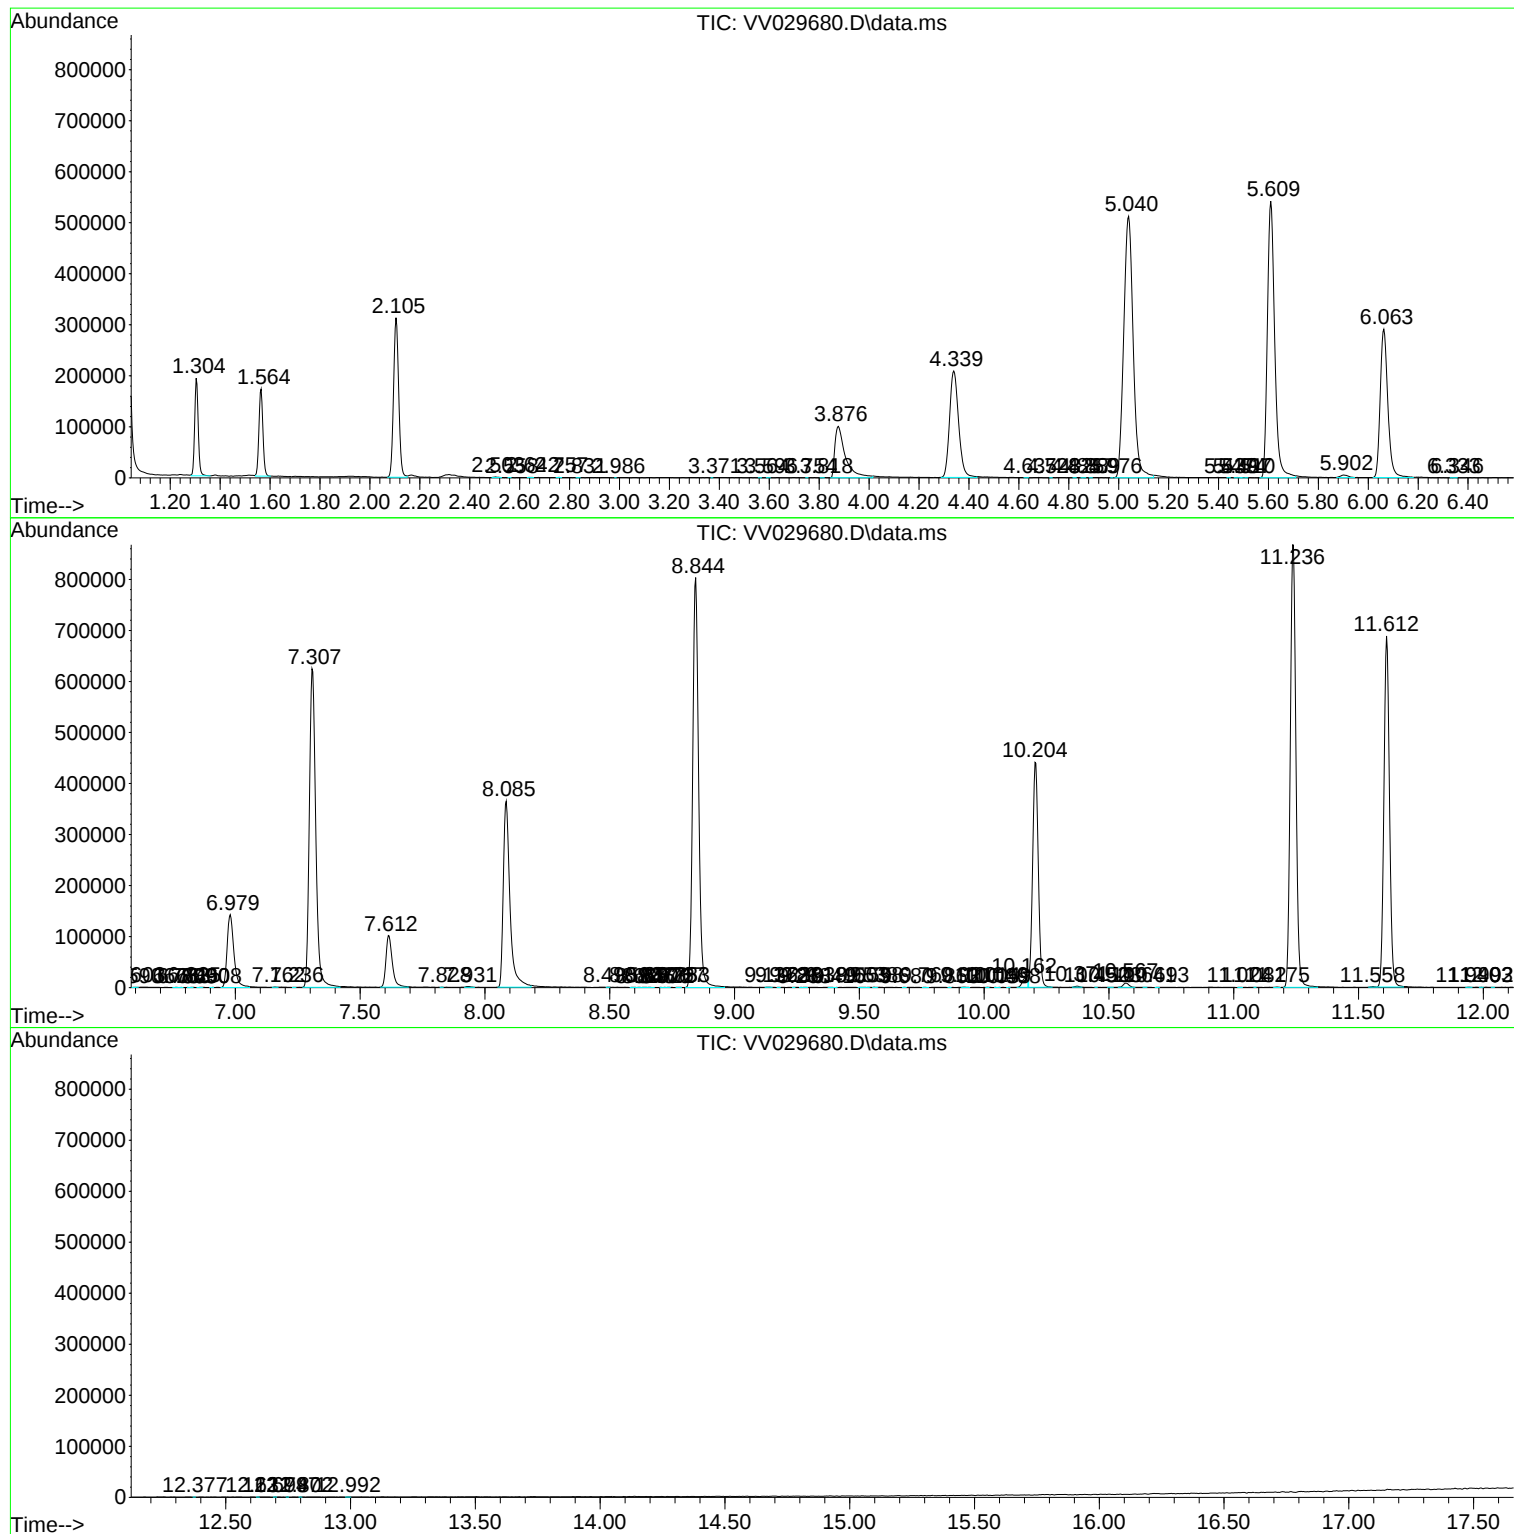

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029680.D
Acq On : 14 Dec 2022 02:59
Operator : SY/MD
Sample : N5980-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ES2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029680.D
Acq On : 14 Dec 2022 02:59
Operator : SY/MD
Sample : N5980-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ES2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------