

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029681.D
 Acq On : 14 Dec 2022 03:23
 Operator : SY/MD
 Sample : N5980-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ES3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029681.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	184274	185373	13.50%	1.429%
2	1.564	156	163	178	rVB	163473	185009	13.47%	1.426%
3	2.105	321	331	347	rBV2	336626	518730	37.78%	3.998%
4	2.500	451	454	465	rVB4	1393	2042	0.15%	0.016%
5	2.545	466	468	473	rBV2	224	175	0.01%	0.001%
6	2.712	516	520	524	rVB3	395	348	0.03%	0.003%
7	2.764	533	536	538	rBV2	224	130	0.01%	0.001%
8	2.899	573	578	582	rBV3	317	283	0.02%	0.002%
9	3.166	657	661	662	rBV2	351	257	0.02%	0.002%
10	3.236	679	683	688	rBV2	183	189	0.01%	0.001%
11	3.343	713	716	721	rBV2	154	156	0.01%	0.001%
12	3.388	726	730	732	rVB2	204	112	0.01%	0.001%
13	3.404	732	735	740	rBB2	132	115	0.01%	0.001%
14	3.806	858	860	864	rVB2	206	110	0.01%	0.001%
15	3.834	865	869	872	rBV2	122	112	0.01%	0.001%
16	3.876	872	882	926	rBV2	105393	365638	26.63%	2.818%
17	4.339	1010	1026	1049	rBV	213564	533379	38.85%	4.111%
18	4.603	1094	1108	1126	rVB5	8684	22282	1.62%	0.172%
19	4.674	1126	1130	1134	rBV2	161	114	0.01%	0.001%
20	4.706	1138	1140	1143	rBV	220	138	0.01%	0.001%
21	4.770	1158	1160	1165	rVB2	209	110	0.01%	0.001%
22	4.799	1165	1169	1173	rBV2	97	98	0.01%	0.001%
23	4.825	1173	1177	1182	rBV	286	300	0.02%	0.002%
24	5.040	1226	1244	1272	rBV2	520966	1360217	99.06%	10.484%
25	5.394	1349	1354	1357	rBV2	380	386	0.03%	0.003%
26	5.458	1372	1374	1376	rBV	195	134	0.01%	0.001%
27	5.609	1408	1421	1459	rBV	538667	1100556	80.15%	8.483%
28	5.905	1500	1513	1548	rBV	690597	1373058	100.00%	10.583%
29	6.063	1550	1562	1586	rVB	302303	609842	44.41%	4.700%
30	6.246	1617	1619	1623	rVB3	504	280	0.02%	0.002%
31	6.285	1628	1631	1633	rBV2	240	176	0.01%	0.001%
32	6.362	1651	1655	1658	rBV2	197	125	0.01%	0.001%
33	6.461	1683	1686	1691	rBV2	380	295	0.02%	0.002%
34	6.522	1696	1705	1709	rBV2	173	290	0.02%	0.002%
35	6.616	1730	1734	1736	rBV2	477	352	0.03%	0.003%
36	6.703	1759	1761	1765	rVB3	380	193	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029681.D
 Acq On : 14 Dec 2022 03:23
 Operator : SY/MD
 Sample : N5980-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ES3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.744	1771	1774	1777	rVB2	239	133	0.01%	0.001%
38	6.802	1790	1792	1799	rVB2	260	214	0.02%	0.002%
39	6.895	1818	1821	1823	rBV2	235	134	0.01%	0.001%
40	6.979	1833	1847	1877	rBV	141989	265261	19.32%	2.045%
41	7.256	1932	1933	1937	rBV2	238	123	0.01%	0.001%
42	7.307	1937	1949	1981	rBV	624960	1113653	81.11%	8.584%
43	7.577	2031	2033	2034	rBV2	366	157	0.01%	0.001%
44	7.612	2034	2044	2074	rVV	100273	181043	13.19%	1.395%
45	7.741	2081	2084	2086	rBV2	461	292	0.02%	0.002%
46	7.838	2111	2114	2122	rVB7	1019	1131	0.08%	0.009%
47	7.876	2122	2126	2128	rBV2	505	404	0.03%	0.003%
48	7.908	2134	2136	2137	rBV	490	194	0.01%	0.001%
49	8.001	2163	2165	2171	rBV2	272	267	0.02%	0.002%
50	8.085	2180	2191	2219	rBV	367294	677305	49.33%	5.220%
51	8.419	2293	2295	2299	rBV3	409	278	0.02%	0.002%
52	8.474	2310	2312	2316	rBV2	412	365	0.03%	0.003%
53	8.567	2339	2341	2344	rVB2	329	165	0.01%	0.001%
54	8.590	2344	2348	2355	rBV3	483	550	0.04%	0.004%
55	8.641	2362	2364	2366	rBV2	313	158	0.01%	0.001%
56	8.754	2397	2399	2404	rBV2	248	144	0.01%	0.001%
57	8.792	2409	2411	2413	rBV	202	107	0.01%	0.001%
58	8.844	2414	2427	2464	rBV	783965	1301349	94.78%	10.030%
59	9.133	2514	2517	2523	rVB4	462	487	0.04%	0.004%
60	9.181	2529	2532	2536	rVB2	186	165	0.01%	0.001%
61	9.249	2550	2553	2557	rBV2	140	163	0.01%	0.001%
62	9.304	2568	2570	2573	rVV	259	127	0.01%	0.001%
63	9.345	2581	2583	2585	rBV	263	109	0.01%	0.001%
64	9.497	2627	2630	2633	rBV3	252	193	0.01%	0.001%
65	9.535	2639	2642	2645	rBV3	436	240	0.02%	0.002%
66	9.654	2676	2679	2681	rBV2	349	190	0.01%	0.001%
67	9.696	2689	2692	2695	rBV2	253	187	0.01%	0.001%
68	9.808	2724	2727	2732	rVB	308	290	0.02%	0.002%
69	9.834	2732	2735	2736	rBV	258	131	0.01%	0.001%
70	10.043	2797	2800	2805	rVB2	302	181	0.01%	0.001%
71	10.079	2809	2811	2816	rVV	172	138	0.01%	0.001%
72	10.162	2823	2837	2841	rBV2	17884	26754	1.95%	0.206%
73	10.204	2841	2850	2874	rVB	448461	704729	51.33%	5.432%
74	10.371	2897	2902	2916	rVB7	1809	3214	0.23%	0.025%
75	10.532	2949	2952	2954	rBV2	377	216	0.02%	0.002%
76	10.571	2954	2964	2973	rBV	8228	13512	0.98%	0.104%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029681.D
 Acq On : 14 Dec 2022 03:23
 Operator : SY/MD
 Sample : N5980-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ES3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	10.902	3064	3067	3069	rBV2	406	286	0.02%	0.002%
78	11.011	3098	3101	3107	rVV	195	187	0.01%	0.001%
79	11.082	3120	3123	3125	rBV3	278	170	0.01%	0.001%
80	11.178	3151	3153	3155	rVB2	481	194	0.01%	0.001%
81	11.191	3155	3157	3159	rBV2	278	137	0.01%	0.001%
82	11.236	3159	3171	3193	rBV	867756	1340448	97.63%	10.332%
83	11.484	3246	3248	3252	rBV3	239	162	0.01%	0.001%
84	11.500	3252	3253	3256	rVB	351	138	0.01%	0.001%
85	11.519	3256	3259	3262	rBV	159	117	0.01%	0.001%
86	11.535	3262	3264	3265	rBV	372	194	0.01%	0.001%
87	11.551	3266	3269	3273	rBV4	831	709	0.05%	0.005%
88	11.612	3276	3288	3312	rBV	688167	1072531	78.11%	8.267%
89	11.808	3348	3349	3354	rVB2	415	271	0.02%	0.002%
90	11.831	3354	3356	3357	rBV	368	176	0.01%	0.001%
91	11.866	3365	3367	3371	rBV2	238	244	0.02%	0.002%
92	11.905	3376	3379	3380	rBV	213	120	0.01%	0.001%
93	11.953	3392	3394	3395	rBV	331	124	0.01%	0.001%
94	12.233	3478	3481	3485	rBV3	747	590	0.04%	0.005%
95	12.271	3491	3493	3497	rVB2	423	275	0.02%	0.002%
96	12.378	3522	3526	3528	rBV	310	254	0.02%	0.002%
97	12.426	3539	3541	3544	rVB2	352	150	0.01%	0.001%
98	12.451	3544	3549	3551	rBV3	407	385	0.03%	0.003%
99	12.580	3585	3589	3592	rBV2	576	458	0.03%	0.004%
100	12.628	3602	3604	3606	rBV2	318	187	0.01%	0.001%




Sum of corrected areas: 12974064

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029681.D
Acq On : 14 Dec 2022 03:23
Operator : SY/MD
Sample : N5980-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ES3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

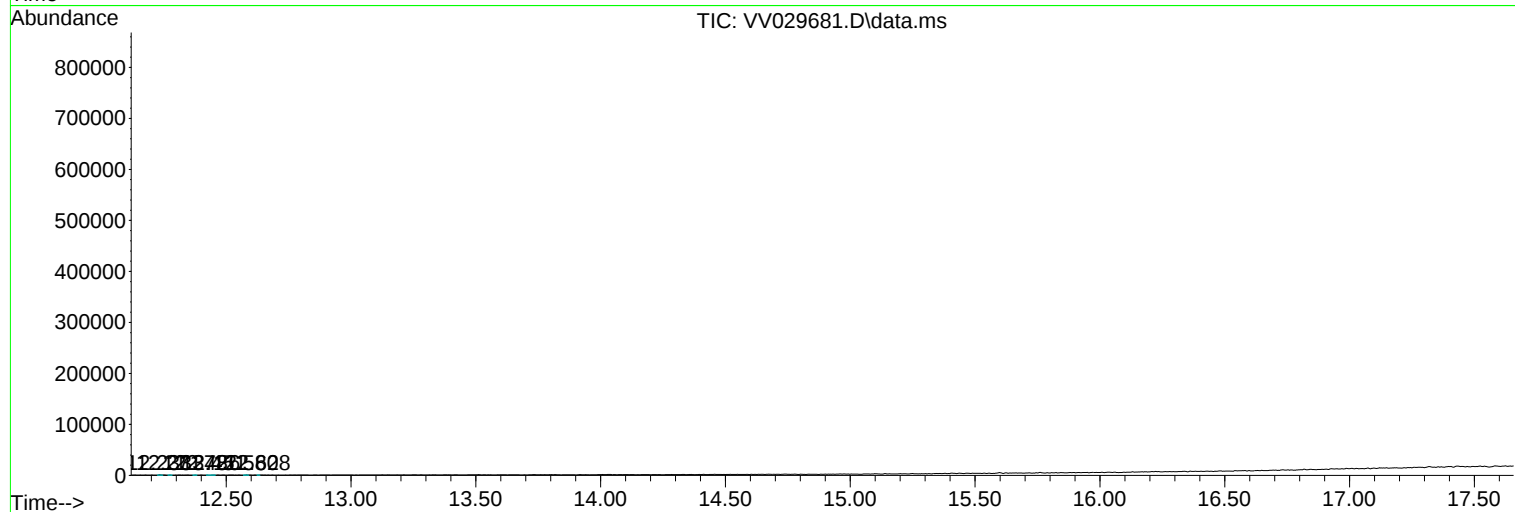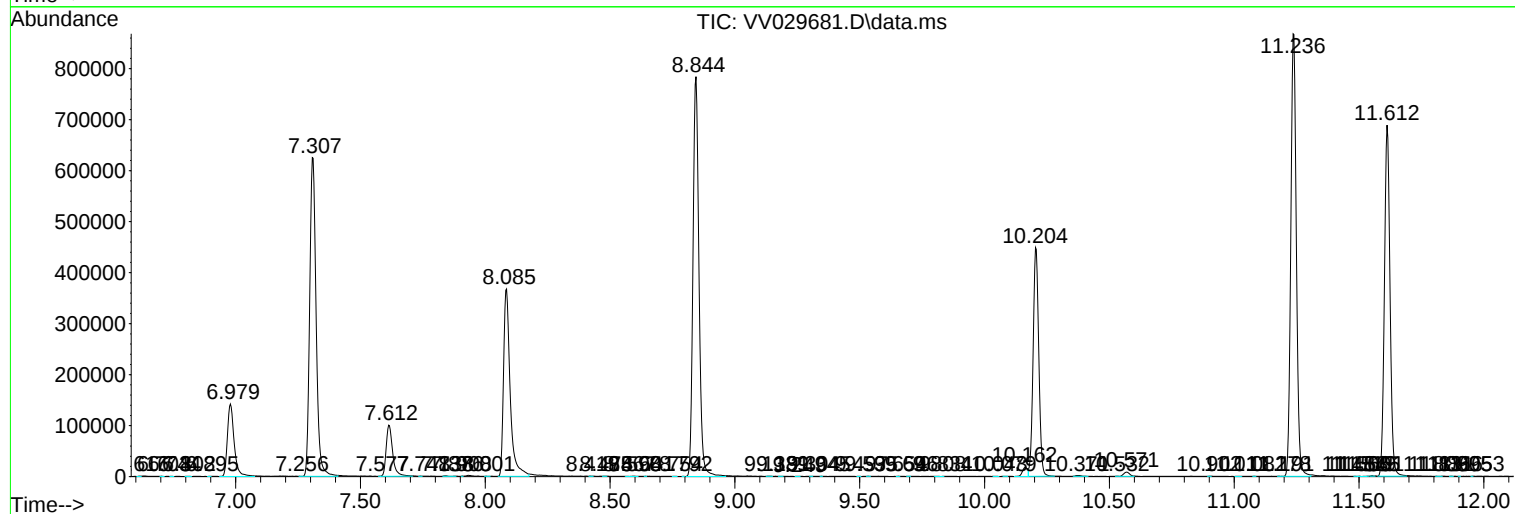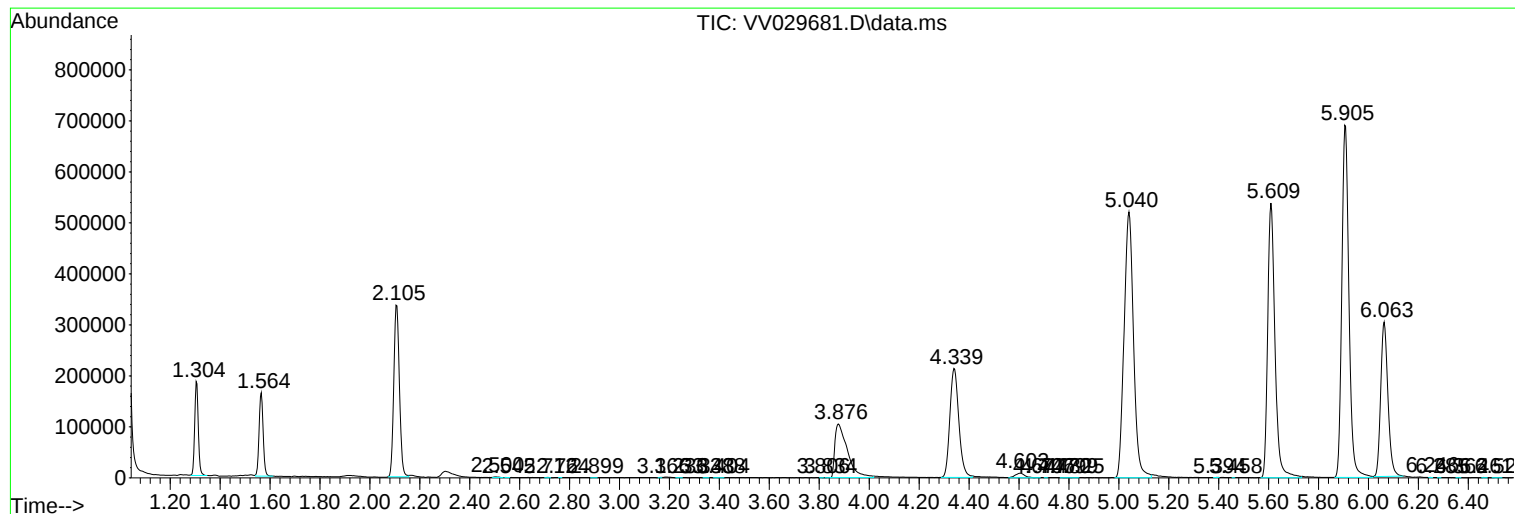

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029681.D
Acq On : 14 Dec 2022 03:23
Operator : SY/MD
Sample : N5980-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ES3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029681.D
Acq On : 14 Dec 2022 03:23
Operator : SY/MD
Sample : N5980-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ES3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc