

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029682.D
 Acq On : 14 Dec 2022 03:46
 Operator : SY/MD
 Sample : N5980-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ES5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

Signal : TIC: VV029682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	193950	195998	14.39%	1.740%
2	1.564	156	163	177	rVB	165970	181731	13.35%	1.613%
3	2.104	320	331	344	rBV	313816	452294	33.22%	4.015%
4	2.291	378	389	418	rVB2	15618	39883	2.93%	0.354%
5	2.468	441	444	446	rBV	323	200	0.01%	0.002%
6	2.635	488	496	497	rBV2	510	595	0.04%	0.005%
7	2.783	537	542	550	rBV2	206	324	0.02%	0.003%
8	2.912	580	582	584	rVB2	188	91	0.01%	0.001%
9	3.095	637	639	642	rBV2	153	107	0.01%	0.001%
10	3.143	649	654	656	rBV2	129	104	0.01%	0.001%
11	3.194	666	670	673	rBV	219	154	0.01%	0.001%
12	3.239	678	684	686	rBV2	194	190	0.01%	0.002%
13	3.272	691	694	699	rBV	101	94	0.01%	0.001%
14	3.352	716	719	721	rBV2	119	90	0.01%	0.001%
15	3.394	728	732	734	rBV	175	158	0.01%	0.001%
16	3.667	810	817	819	rBV2	230	309	0.02%	0.003%
17	3.873	871	881	912	rBV	98753	273584	20.09%	2.428%
18	4.339	1009	1026	1056	rBV	214769	538792	39.57%	4.783%
19	4.645	1115	1121	1122	rBV	174	132	0.01%	0.001%
20	4.657	1122	1125	1130	rVB3	307	270	0.02%	0.002%
21	4.702	1137	1139	1142	rBV	194	95	0.01%	0.001%
22	4.760	1154	1157	1160	rBV2	234	209	0.02%	0.002%
23	4.776	1160	1162	1168	rVB2	214	143	0.01%	0.001%
24	4.834	1175	1180	1185	rVB2	189	223	0.02%	0.002%
25	4.940	1208	1213	1221	rBV2	176	243	0.02%	0.002%
26	4.979	1221	1225	1227	rBV2	208	168	0.01%	0.001%
27	5.040	1227	1244	1276	rBV2	523038	1361585	100.00%	12.086%
28	5.445	1368	1370	1373	rBV2	148	96	0.01%	0.001%
29	5.522	1391	1394	1395	rBV	205	91	0.01%	0.001%
30	5.558	1399	1405	1408	rBV2	189	158	0.01%	0.001%
31	5.609	1408	1421	1460	rBV	509222	1038093	76.24%	9.215%
32	5.905	1503	1513	1529	rVB6	6436	14665	1.08%	0.130%
33	5.995	1539	1541	1544	rVB3	263	153	0.01%	0.001%
34	6.063	1547	1562	1600	rBV	299035	620736	45.59%	5.510%
35	6.362	1652	1655	1659	rBV3	233	173	0.01%	0.002%
36	6.397	1664	1666	1667	rBV3	169	81	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121322\
 Data File : VW029682.D
 Acq On : 14 Dec 2022 03:46
 Operator : SY/MD
 Sample : N5980-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ES5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

37	6.532	1705	1708	1711	rBV	163	113	0.01%	0.001%
38	6.606	1728	1731	1732	rBV	236	115	0.01%	0.001%
39	6.622	1733	1736	1737	rBV	300	154	0.01%	0.001%
40	6.709	1761	1763	1766	rBV	205	120	0.01%	0.001%
41	6.792	1783	1789	1792	rBV	75	81	0.01%	0.001%
42	6.812	1792	1795	1797	rBV	218	131	0.01%	0.001%
43	6.837	1801	1803	1809	rVB2	291	204	0.01%	0.002%
44	6.911	1823	1826	1829	rVB2	200	130	0.01%	0.001%
45	6.979	1836	1847	1878	rBV	142583	264996	19.46%	2.352%
46	7.136	1894	1896	1899	rVB2	274	116	0.01%	0.001%
47	7.159	1899	1903	1910	rBV4	855	1053	0.08%	0.009%
48	7.307	1934	1949	1981	rBV	631110	1120487	82.29%	9.946%
49	7.612	2033	2044	2071	rBV	102789	180329	13.24%	1.601%
50	7.934	2136	2144	2155	rVB5	2005	3379	0.25%	0.030%
51	7.998	2159	2164	2167	rBV2	231	300	0.02%	0.003%
52	8.085	2180	2191	2227	rBV	357709	654280	48.05%	5.808%
53	8.390	2284	2286	2288	rBV2	280	142	0.01%	0.001%
54	8.435	2296	2300	2303	rBV3	321	226	0.02%	0.002%
55	8.464	2306	2309	2310	rBV2	211	121	0.01%	0.001%
56	8.497	2313	2319	2323	rBV2	636	632	0.05%	0.006%
57	8.522	2324	2327	2328	rBV	302	174	0.01%	0.002%
58	8.561	2337	2339	2340	rBV	259	132	0.01%	0.001%
59	8.590	2346	2348	2351	rBV	252	130	0.01%	0.001%
60	8.612	2353	2355	2356	rBV	217	77	0.01%	0.001%
61	8.654	2365	2368	2370	rBV2	343	249	0.02%	0.002%
62	8.731	2388	2392	2394	rVB	204	142	0.01%	0.001%
63	8.844	2414	2427	2457	rBV	750535	1229231	90.28%	10.911%
64	9.178	2529	2531	2533	rBV	177	76	0.01%	0.001%
65	9.278	2559	2562	2565	rBV2	174	125	0.01%	0.001%
66	9.355	2583	2586	2589	rVB	215	132	0.01%	0.001%
67	9.384	2592	2595	2598	rVB2	189	122	0.01%	0.001%
68	9.480	2623	2625	2628	rBV2	143	83	0.01%	0.001%
69	9.503	2629	2632	2634	rVB	267	152	0.01%	0.001%
70	9.532	2638	2641	2642	rBV	207	113	0.01%	0.001%
71	9.570	2651	2653	2654	rBV	360	122	0.01%	0.001%
72	9.641	2672	2675	2679	rBV	234	169	0.01%	0.002%
73	9.689	2687	2690	2693	rBV2	146	88	0.01%	0.001%
74	9.712	2693	2697	2698	rBV2	279	189	0.01%	0.002%
75	9.863	2742	2744	2746	rBV	158	82	0.01%	0.001%
76	9.898	2754	2755	2758	rBV2	248	119	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
 Data File : VV029682.D
 Acq On : 14 Dec 2022 03:46
 Operator : SY/MD
 Sample : N5980-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ES5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
 Title : VOC Analysis

77	9.959	2771	2774	2776	rBV	182	136	0.01%	0.001%
78	9.998	2783	2786	2788	rBV	223	129	0.01%	0.001%
79	10.162	2828	2837	2841	rBV2	17243	25631	1.88%	0.228%
80	10.204	2842	2850	2873	rVB	443541	697089	51.20%	6.188%
81	10.442	2921	2924	2927	rBV	210	114	0.01%	0.001%
82	10.532	2947	2952	2954	rVV3	409	385	0.03%	0.003%
83	10.567	2955	2963	2974	rVB	8429	13595	1.00%	0.121%
84	10.696	3001	3003	3006	rBV2	183	109	0.01%	0.001%
85	10.750	3017	3020	3023	rBV2	204	130	0.01%	0.001%
86	10.840	3046	3048	3050	rVB	395	166	0.01%	0.001%
87	10.927	3073	3075	3077	rBV	263	115	0.01%	0.001%
88	10.998	3094	3097	3099	rBV2	237	150	0.01%	0.001%
89	11.175	3148	3152	3156	rVB2	457	296	0.02%	0.003%
90	11.236	3159	3171	3199	rBV	821361	1267547	93.09%	11.251%
91	11.516	3256	3258	3261	rBV2	274	141	0.01%	0.001%
92	11.551	3262	3269	3270	rBV4	941	874	0.06%	0.008%
93	11.612	3276	3288	3311	rBV	681872	1076368	79.05%	9.554%
94	11.892	3373	3375	3380	rBV2	237	186	0.01%	0.002%
95	11.950	3391	3393	3397	rVB	247	142	0.01%	0.001%
96	12.004	3406	3410	3413	rBV2	326	288	0.02%	0.003%
97	12.098	3436	3439	3442	rBV2	273	191	0.01%	0.002%
98	12.229	3476	3480	3481	rBV	494	339	0.02%	0.003%
99	12.535	3572	3575	3577	rBV2	331	243	0.02%	0.002%
100	12.840	3667	3670	3676	rBV3	427	404	0.03%	0.004%




Sum of corrected areas: 11265596

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029682.D
Acq On : 14 Dec 2022 03:46
Operator : SY/MD
Sample : N5980-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ES5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

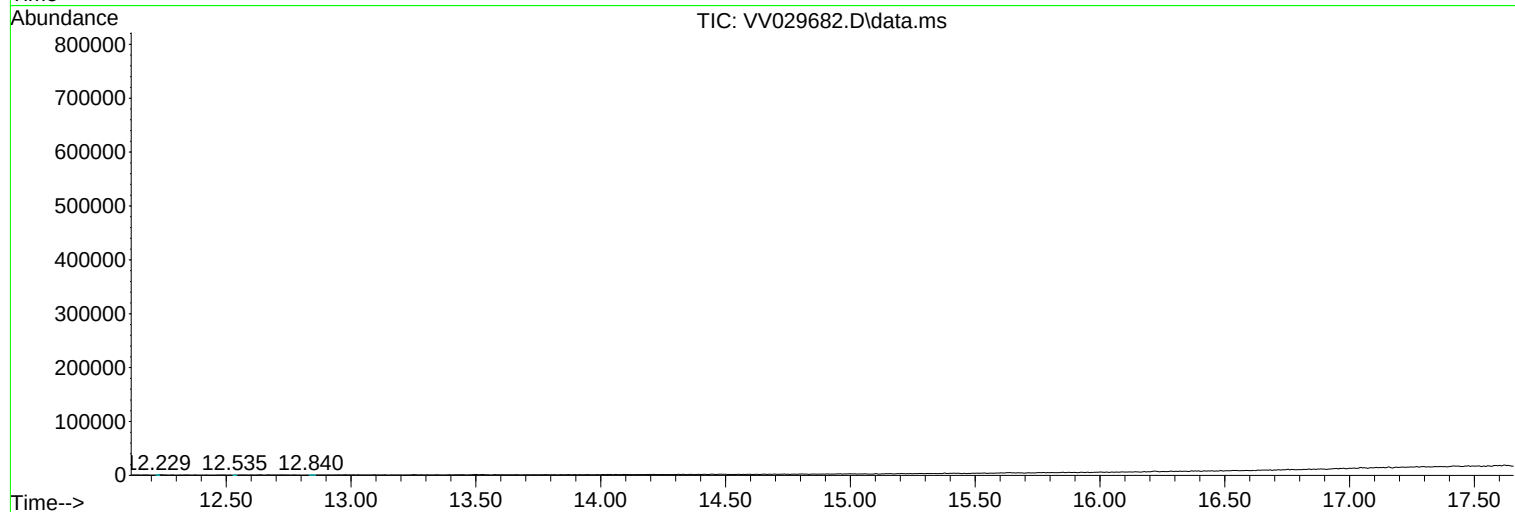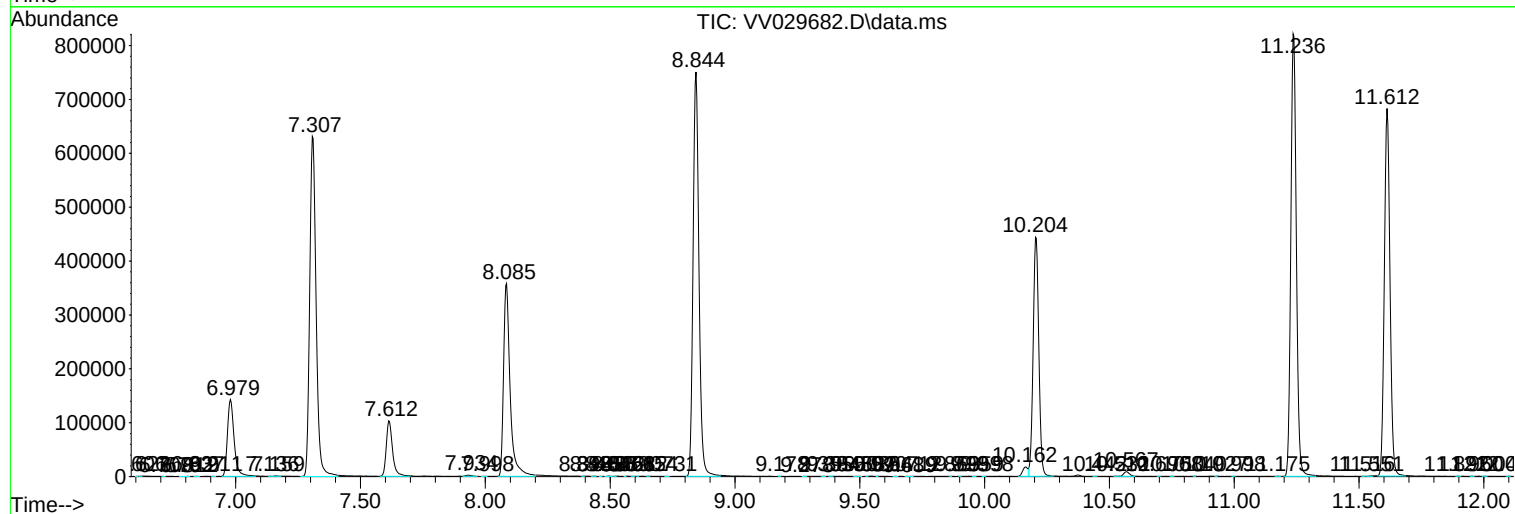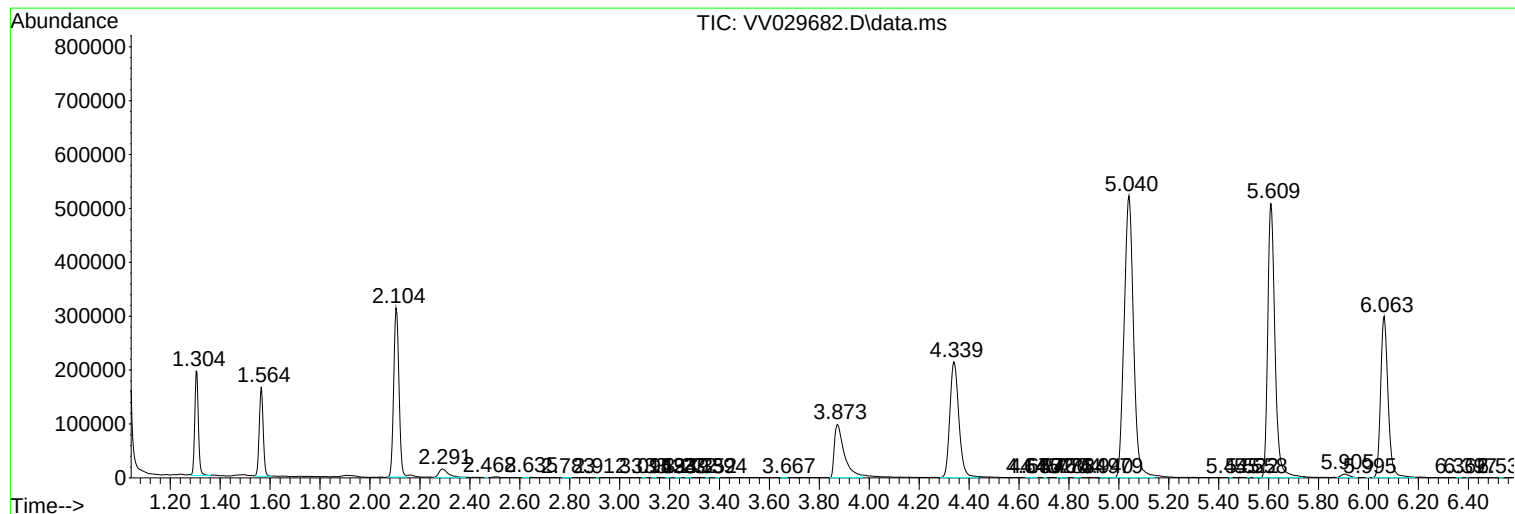

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029682.D
Acq On : 14 Dec 2022 03:46
Operator : SY/MD
Sample : N5980-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ES5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029682.D
Acq On : 14 Dec 2022 03:46
Operator : SY/MD
Sample : N5980-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ES5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc