
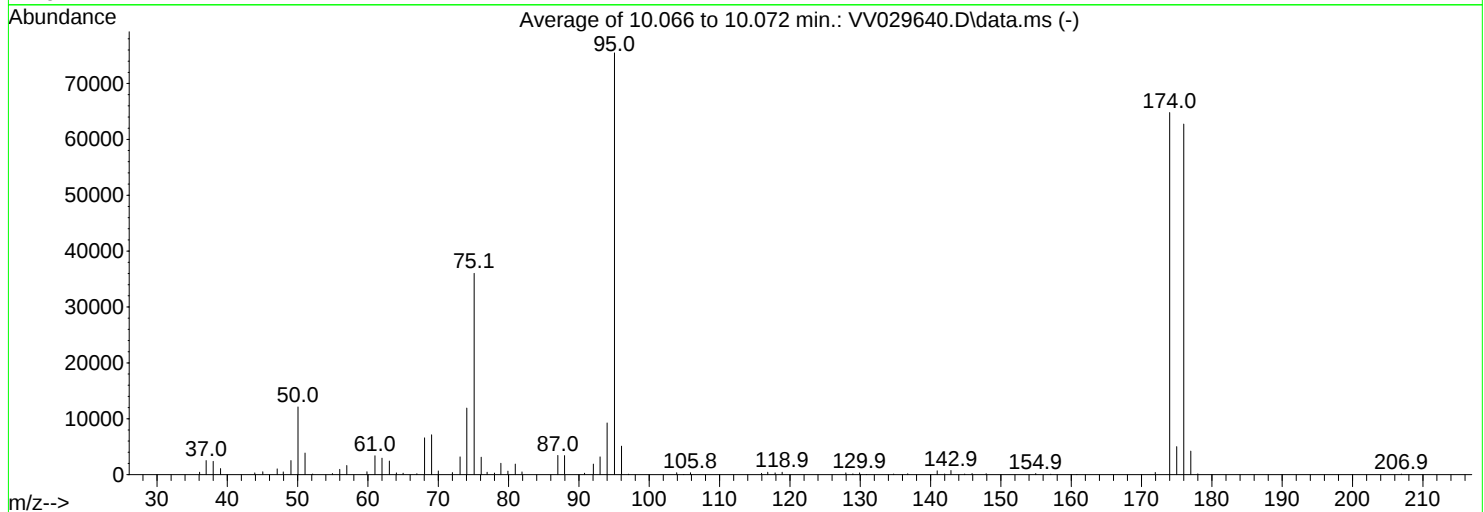


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121322\
Data File : VV029640.D
Acq On : 13 Dec 2022 09:25
Operator : SY/MD
Sample : BFB355
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 54 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB355

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120722WMA.M
Title : VOC Analysis
Last Update : Tue Dec 13 23:56:43 2022

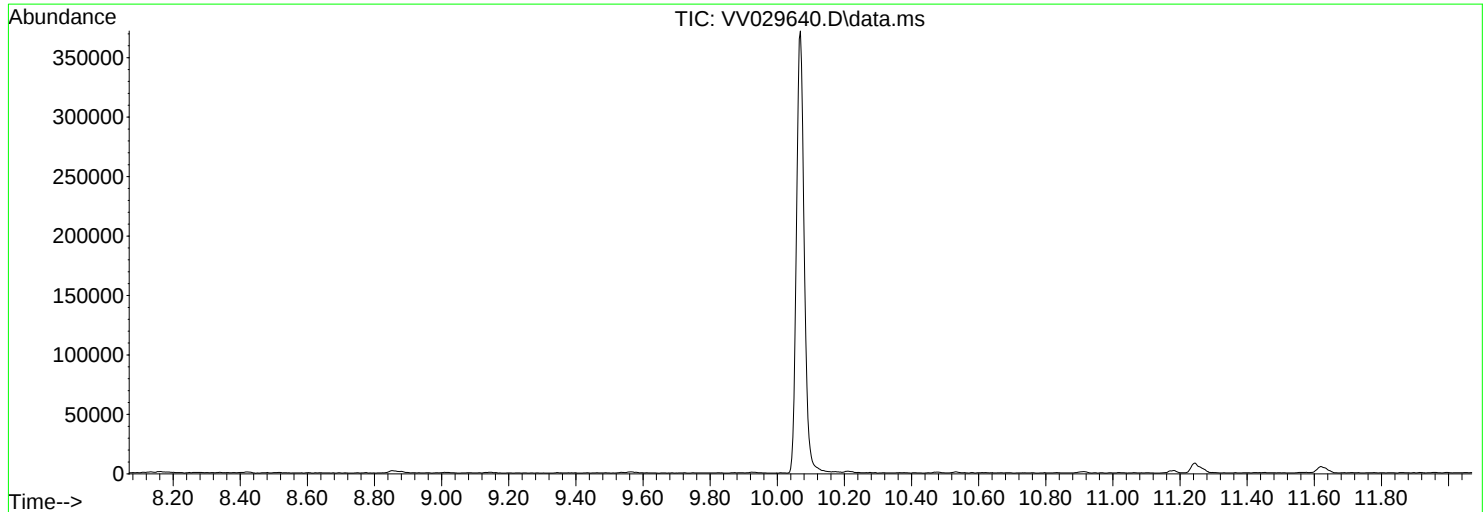

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	12100	PASS
75	95	30	80	47.7	36035	PASS
95	95	100	100	100.0	75488	PASS
96	95	5	9	6.8	5112	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.8	64800	PASS
175	174	5	9	7.8	5023	PASS
176	174	95	105	96.8	62739	PASS
177	176	5	10	6.7	4214	PASS

m/z	Abundance
39.90	474.0
43.90	250.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355

m/z	Abundance
36.00	496.0
37.00	2589.0
38.00	2410.0
39.10	1200.0
39.90	462.0
44.00	591.0
45.10	514.0
47.10	1062.0
48.00	488.0
49.00	2619.0
50.00	12236.0
51.10	4051.0
52.20	118.0
54.90	198.0
56.00	919.0
57.00	1665.0
59.90	493.0
61.00	3626.0
62.00	3048.0
63.00	2412.0
64.10	341.0
65.00	280.0
67.00	193.0
68.00	6787.0
69.00	7044.0
70.00	669.0
71.90	370.0
73.10	3216.0
74.10	12355.0
75.10	36592.0
76.10	3321.0
76.90	450.0
78.00	296.0
78.90	2169.0
79.90	596.0
81.00	1954.0
81.90	505.0
87.00	3789.0
88.00	3555.0
90.80	254.0
92.10	1869.0
93.00	3408.0
94.00	9530.0
95.00	76768.0
96.00	5307.0
97.00	135.0
103.90	338.0
104.90	108.0
105.80	370.0
115.90	258.0
116.80	399.0
117.90	291.0
118.90	418.0
127.90	303.0
128.90	139.0
129.90	321.0
130.90	103.0
134.70	150.0
136.70	153.0
140.90	722.0
142.00	112.0
142.90	769.0
144.90	148.0
145.90	225.0
147.90	186.0
154.90	213.0
157.10	137.0
160.80	102.0
172.00	461.0
174.00	64936.0
175.00	4997.0
176.00	61944.0
177.00	4247.0
178.00	112.0
206.90	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355

m/z	Abundance
36.00	428.0
37.00	2566.0
38.00	2431.0
39.10	1139.0
40.00	443.0
43.90	576.0
45.00	520.0
47.10	1098.0
48.00	491.0
49.00	2585.0
50.00	12447.0
51.10	4014.0
52.20	140.0
54.90	189.0
56.00	987.0
57.00	1649.0
59.80	538.0
61.00	3520.0
62.00	2990.0
63.00	2528.0
64.00	338.0
65.00	256.0
66.90	197.0
68.00	6771.0
69.10	7444.0
70.00	685.0
72.00	383.0
73.10	3309.0
74.00	12177.0
75.10	37280.0
76.10	3243.0
77.00	428.0
78.00	285.0
78.90	2106.0
79.90	663.0
81.00	1921.0
81.90	485.0
87.00	3489.0
87.90	3518.0
90.80	268.0
92.00	1914.0
93.00	3275.0
94.00	9696.0
95.10	77928.0
96.00	5306.0
97.10	116.0
103.90	369.0
105.90	367.0
116.00	236.0
116.90	415.0
117.90	330.0
118.90	458.0
127.90	335.0
128.90	131.0
129.90	343.0
134.70	132.0
136.70	192.0
141.00	706.0
142.00	121.0
142.90	780.0
144.90	130.0
145.90	214.0
147.90	178.0
154.90	214.0
157.10	110.0
171.90	411.0
174.00	66984.0
175.00	5195.0
176.00	64656.0
177.00	4384.0
178.00	144.0
206.90	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355

m/z	Abundance
36.10	377.0
37.00	2427.0
38.00	2290.0
39.00	956.0
39.90	440.0
44.00	571.0
45.00	487.0
47.10	904.0
47.90	453.0
49.10	2391.0
50.10	11617.0
51.00	3508.0
52.10	131.0
55.00	196.0
56.00	926.0
57.00	1545.0
59.90	480.0
61.00	2965.0
62.00	2814.0
63.10	2391.0
64.00	283.0
65.00	218.0
67.00	161.0
68.10	6184.0
69.10	6925.0
70.00	629.0
72.10	379.0
73.10	3055.0
74.00	11189.0
75.10	34232.0
76.10	2811.0
77.00	437.0
78.00	265.0
78.90	1866.0
79.90	656.0
80.90	1770.0
81.90	444.0
87.00	3010.0
87.90	3154.0
90.80	264.0
92.00	1878.0
93.00	2881.0
94.00	8567.0
95.10	71768.0
96.10	4724.0
103.90	331.0
105.90	322.0
116.00	210.0
116.90	448.0
117.90	314.0
118.90	440.0
128.00	327.0
129.00	128.0
129.90	321.0
134.80	108.0
136.80	168.0
141.00	608.0
142.00	109.0
142.90	693.0
144.80	100.0
145.90	151.0
147.90	139.0
155.00	192.0
171.90	384.0
174.00	62480.0
175.00	4876.0
176.00	61616.0
177.00	4012.0
178.00	149.0
207.00	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355