

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121323\
 Data File : VW033295.D
 Acq On : 13 Dec 2023 22:44
 Operator : SY/MD
 Sample : 05731-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y67

Quant Time: Dec 13 23:38:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 23:30:39 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	120169	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	121612	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	60407	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	37773	4.903	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.000%
7) Chloroethane-d5	1.532	69	29069	5.074	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.400%
11) 1,1-Dichloroethene-d2	2.060	65	14646	4.777	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	95.600%
20) 2-Butanone-d5	3.799	46	44879	49.229	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.460%
24) Chloroform-d	4.249	84	82588	5.140	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.800%
26) 1,2-Dichloroethane-d4	4.947	65	38654	5.536	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.800%
32) Benzene-d6	4.960	84	159804	5.080	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.600%
36) 1,2-Dichloropropane-d6	5.989	67	38455	5.370	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.400%
41) Toluene-d8	7.243	98	151217	4.933	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.600%
43) trans-1,3-Dichloroprop...	7.558	79	16153	4.945	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.800%
46) 2-Hexanone-d5	8.027	63	50587	55.471	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	110.940%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	25548	5.275	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.600%
66) 1,2-Dichlorobenzene-d4	11.561	152	59342	5.577	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	111.600%
Target Compounds						
					Qvalue	
3) Chloromethane	1.214	50	1725	0.201	ug/L	98
13) Acetone	2.127	43	1878	2.911	ug/L	90
33) Benzene	5.018	78	8795	0.270	ug/L	100
34) Trichloroethene	5.834	95	21435	2.256	ug/L	95
35) Methylcyclohexane	6.047	83	3486	0.248	ug/L	96
37) 1,2-Dichloropropane	5.989	63	5235	0.799	ug/L #	81
39) cis-1,3-Dichloropropene	6.918	75	1075	0.101	ug/L #	69
42) Toluene	7.320	91	29403	0.788	ug/L	96
47) Tetrachloroethene	7.908	164	2318	0.258	ug/L	86
49) Dibromochloromethane	7.908	129	2299	0.325	ug/L #	11
52) Ethylbenzene	8.953	91	6684	0.160	ug/L	98
53) m,p-Xylene	9.079	106	3251	0.189	ug/L	92
54) o-Xylene	9.484	106	1413	0.087	ug/L	68
61) 1,2,3-Trichloropropane	11.185	75	5069	1.583	ug/L #	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033295.D
Acq On : 13 Dec 2023 22:44
Operator : SY/MD
Sample : 05731-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOY67

Quant Time: Dec 13 23:38:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 13 23:30:39 2023
Response via : Initial Calibration




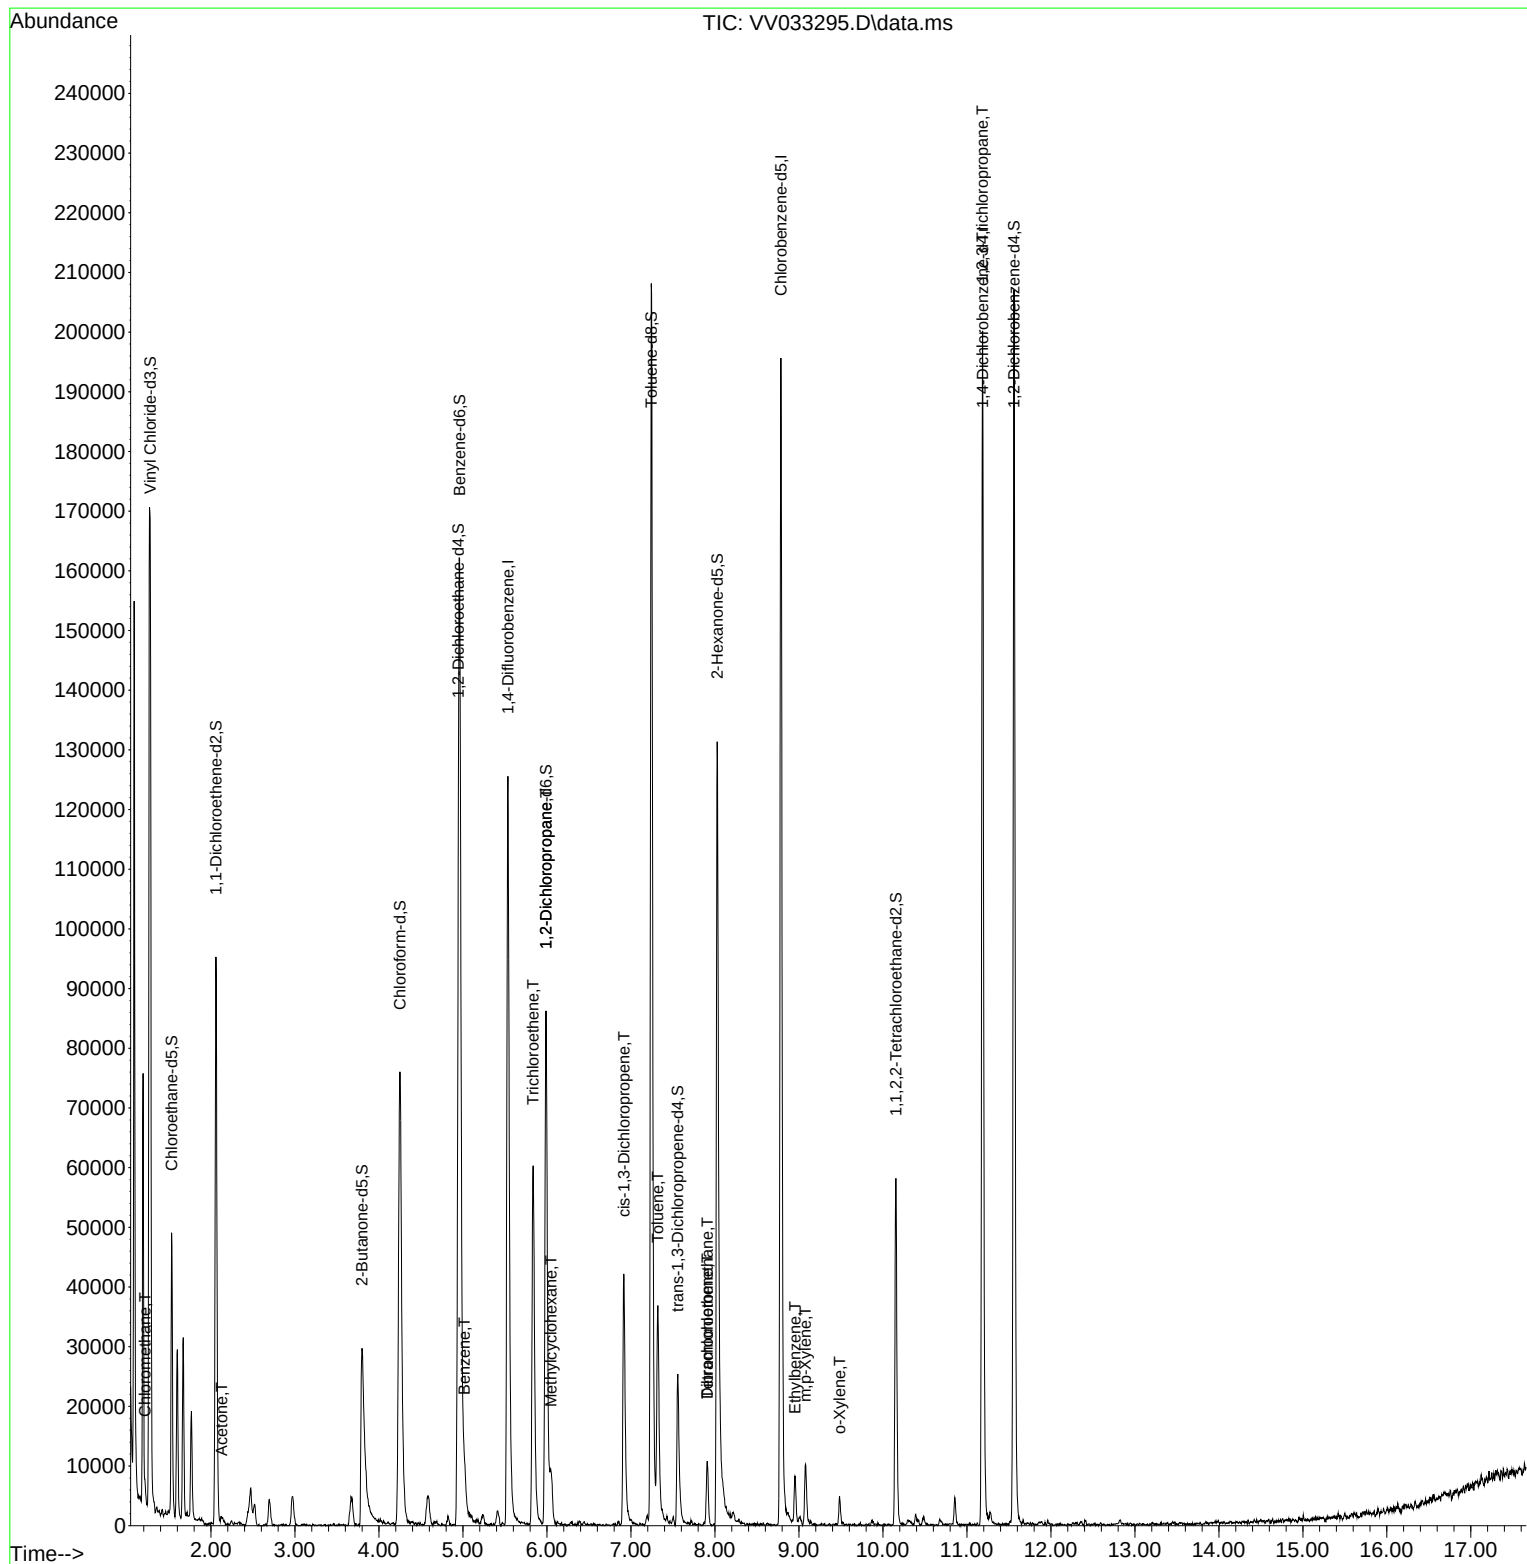


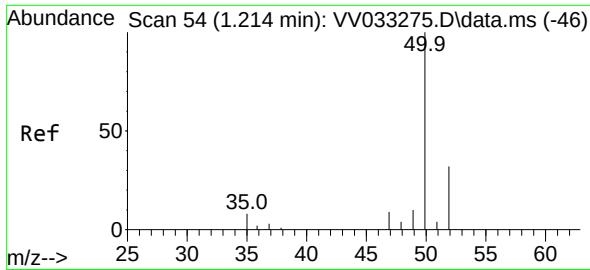

#3
Chloromethane
Concen: 0.201 ug/L
RT: 1.214 min Scan# 54
Delta R.T. 0.000 min
Lab File: VV033295.D
Acq: 13 Dec 2023 22:44




Instrument :
MSVOA_V
ClientSampleId :
E0Y67


Tgt Ion: 50 Resp: 1725
Ion Ratio Lower Upper
50 100
52 35.4 23.8 44.2

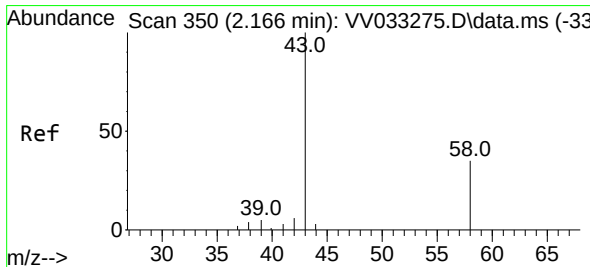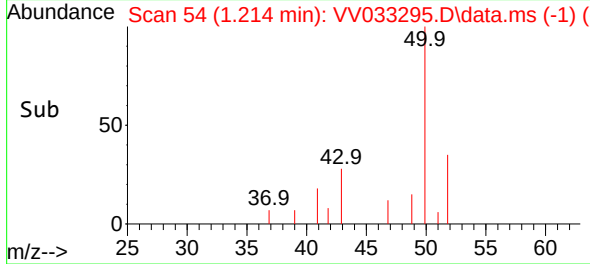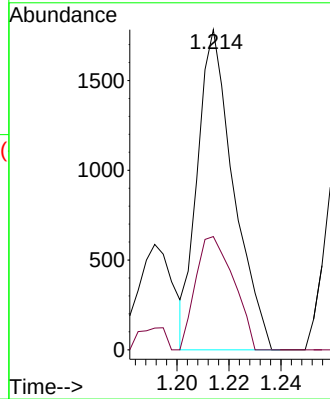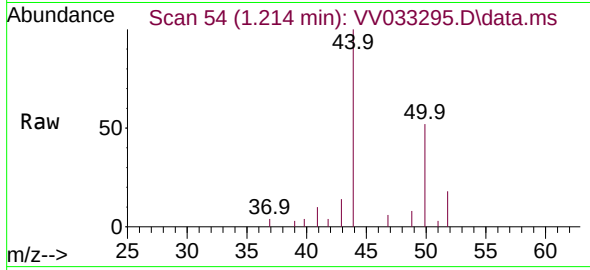

#13
Acetone
Concen: 2.911 ug/L
RT: 2.127 min Scan# 338
Delta R.T. -0.039 min
Lab File: VV033295.D
Acq: 13 Dec 2023 22:44

Tgt Ion: 43 Resp: 1878
Ion Ratio Lower Upper
43 100
58 19.1 0.0 30.2

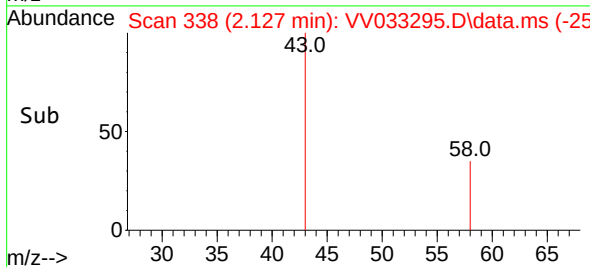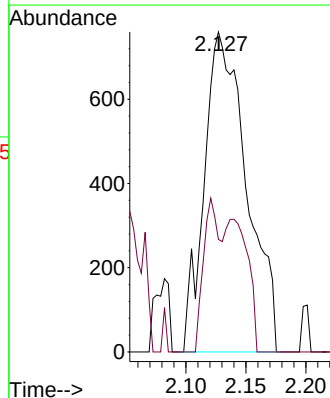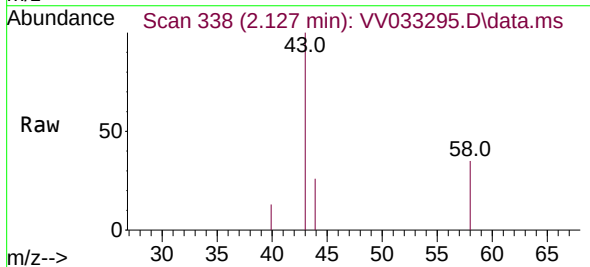

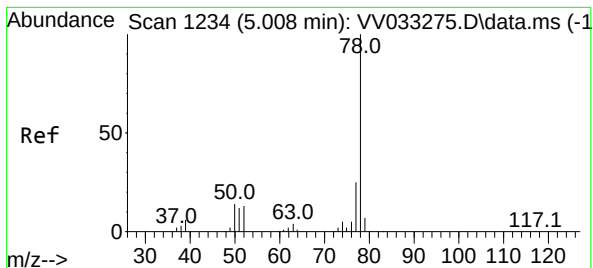

#33

Benzene

Concen: 0.270 ug/L

RT: 5.018 min Scan# 1

Delta R.T. 0.010 min

Lab File: VV033295.D

Acq: 13 Dec 2023 22:44





Instrument :

MSVOA_V

ClientSampleId :

E0Y67

Tgt Ion: 78 Resp: 8795

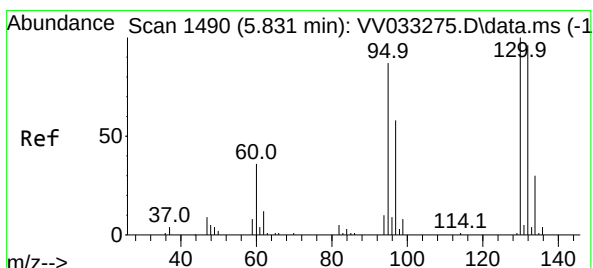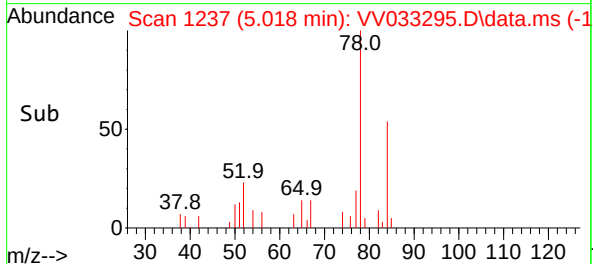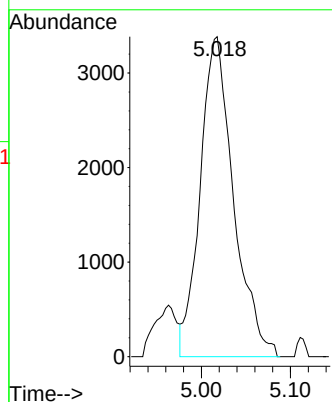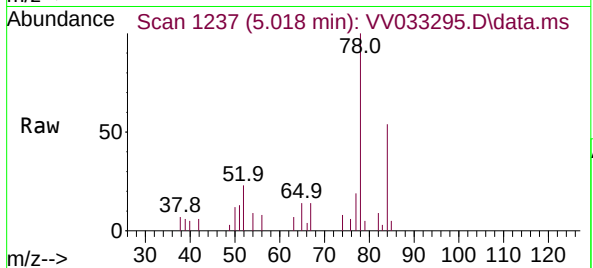

#34

Trichloroethene

Concen: 2.256 ug/L

RT: 5.834 min Scan# 1491

Delta R.T. 0.003 min

Lab File: VV033295.D

Acq: 13 Dec 2023 22:44

Tgt Ion: 95 Resp: 21435




Ion Ratio Lower Upper


95 100

97 57.9 46.5 86.5

132 104.5 75.1 139.5

130 108.9 79.3 147.3


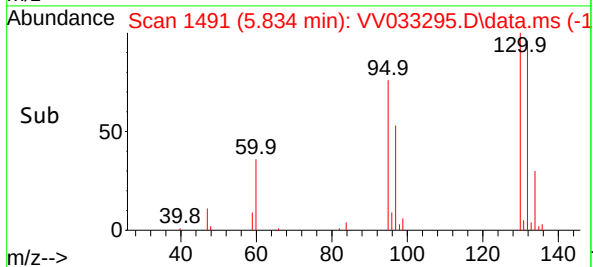
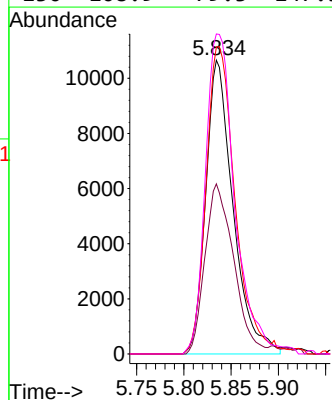
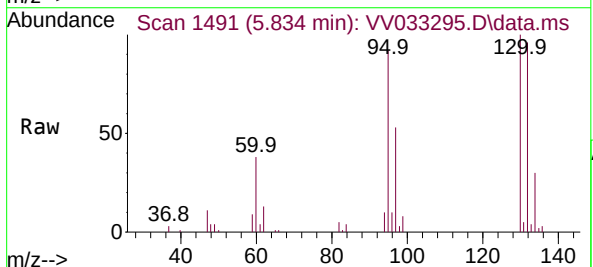


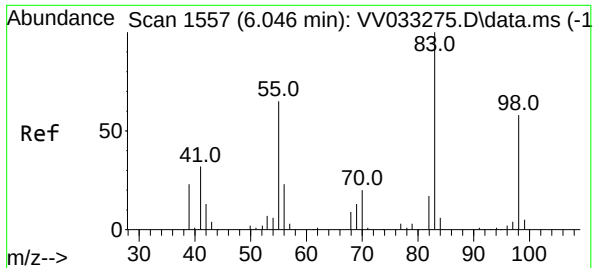

#35
Methylcyclohexane
Concen: 0.248 ug/L
RT: 6.047 min Scan# 11
Delta R.T. 0.000 min
Lab File: VV033295.D
Acq: 13 Dec 2023 22:44




Instrument :
MSVOA_V
ClientSampleId :
E0Y67


Tgt Ion: 83 Resp: 3486
Ion Ratio Lower Upper
83 100
55 67.6 50.7 76.1
98 55.2 42.4 63.6

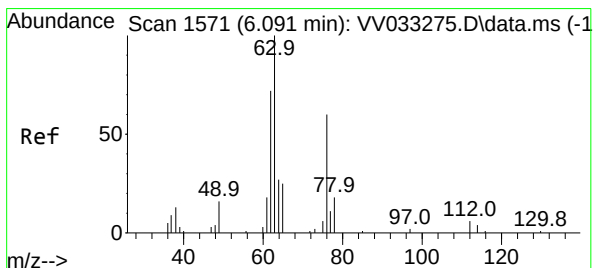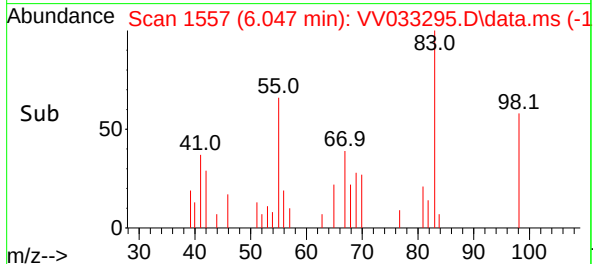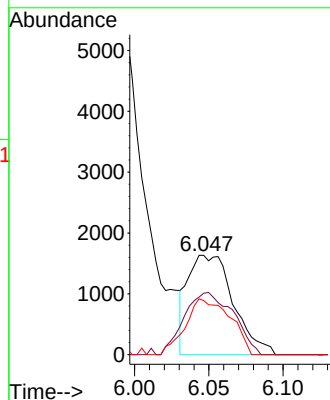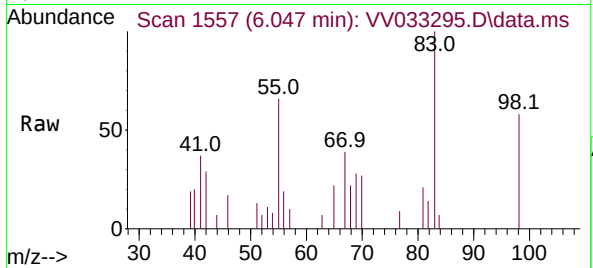

#37
1,2-Dichloropropane
Concen: 0.799 ug/L
RT: 5.989 min Scan# 1539
Delta R.T. -0.103 min
Lab File: VV033295.D
Acq: 13 Dec 2023 22:44

Tgt Ion: 63 Resp: 5235
Ion Ratio Lower Upper
63 100
112 0.0 5.0 7.6#

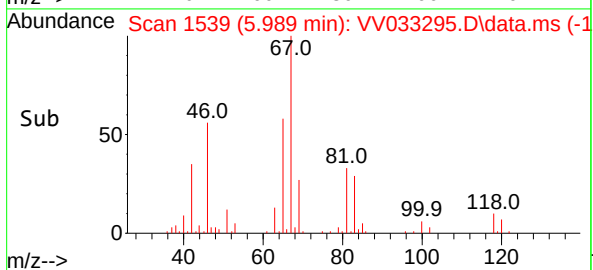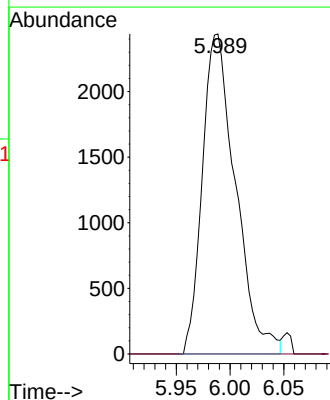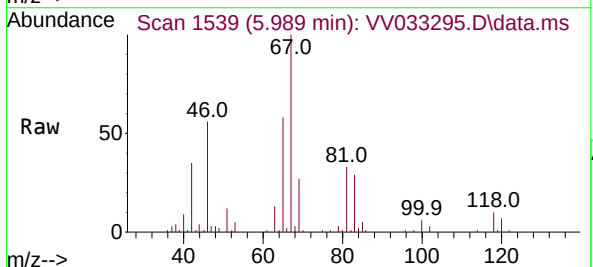

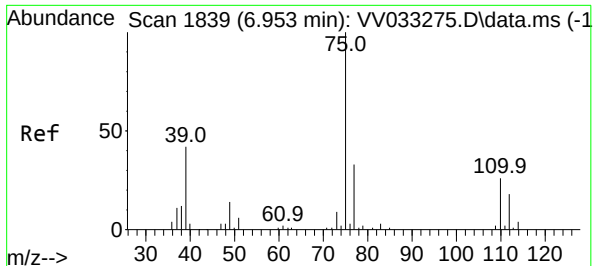

#39

cis-1,3-Dichloropropene

Concen: 0.101 ug/L

RT: 6.918 min Scan# 1828

Delta R.T. -0.035 min

Lab File: VV033295.D

Acq: 13 Dec 2023 22:44

Instrument :

MSVOA_V

ClientSampleId :





E0Y67

Tgt Ion: 75 Resp: 1075

Ion Ratio Lower Upper

75 100

77 48.8 22.1 41.1#

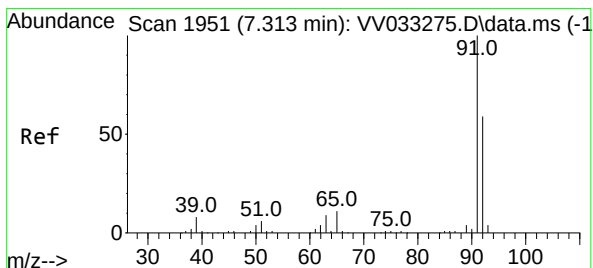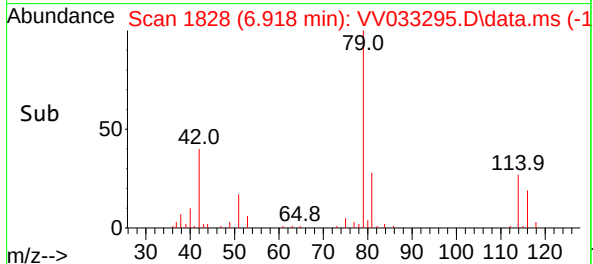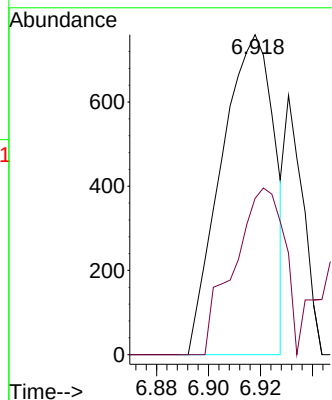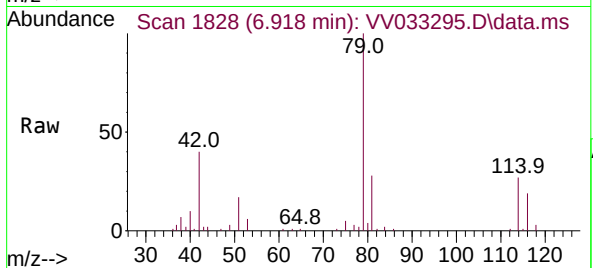

#42

Toluene

Concen: 0.788 ug/L

RT: 7.320 min Scan# 1953

Delta R.T. 0.007 min

Lab File: VV033295.D




Acq: 13 Dec 2023 22:44


Tgt Ion: 91 Resp: 29403

Ion Ratio Lower Upper

91 100

92 60.4 40.2 74.6

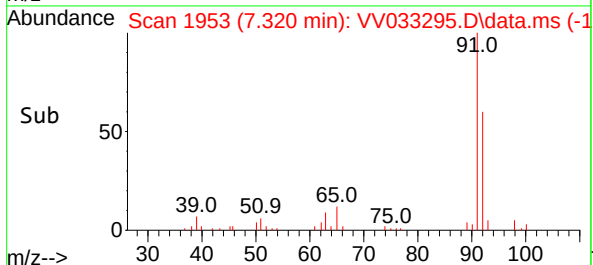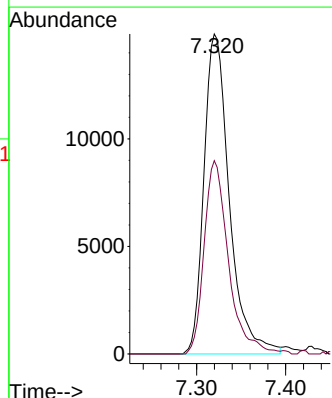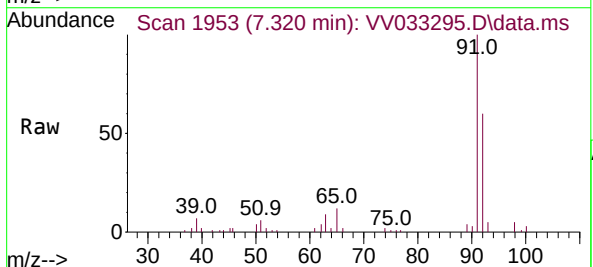

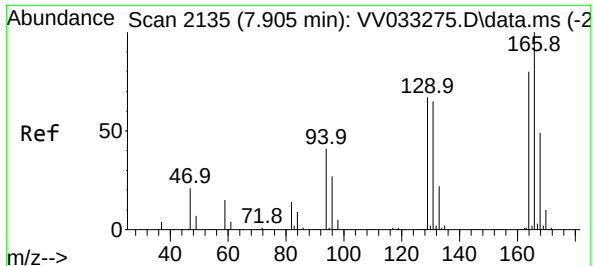

#47

Tetrachloroethene

Concen: 0.258 ug/L

RT: 7.908 min Scan# 2136

Delta R.T. 0.003 min

Lab File: VV033295.D

Acq: 13 Dec 2023 22:44

Instrument :

MSVOA_V

ClientSampleId :

E0Y67

Tgt Ion:164 Resp: 2318





Ion Ratio Lower Upper

164 100

129 103.4 62.6 116.3

131 100.4 62.6 116.3

166 146.7 90.2 167.6

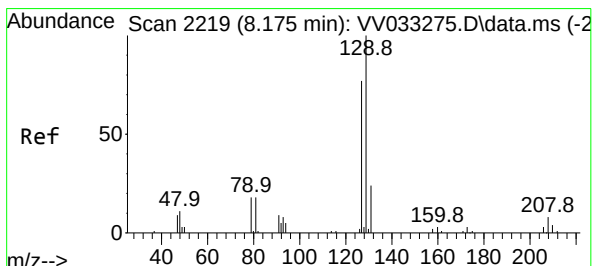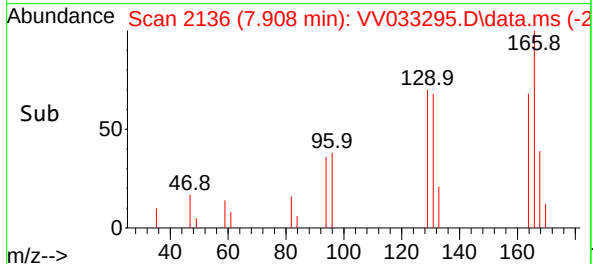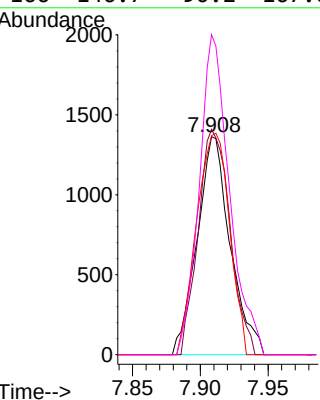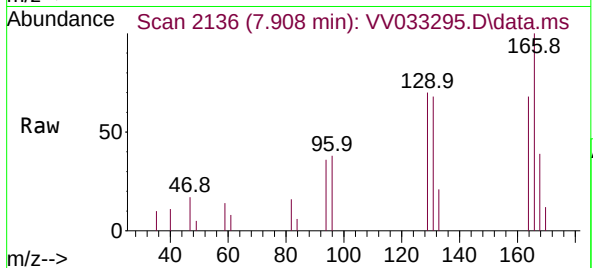

#49

Dibromochloromethane

Concen: 0.325 ug/L

RT: 7.908 min Scan# 2136

Delta R.T. -0.267 min

Lab File: VV033295.D




Acq: 13 Dec 2023 22:44


Tgt Ion:129 Resp: 2299

Ion Ratio Lower Upper

129 100

127 0.0 53.2 98.8#


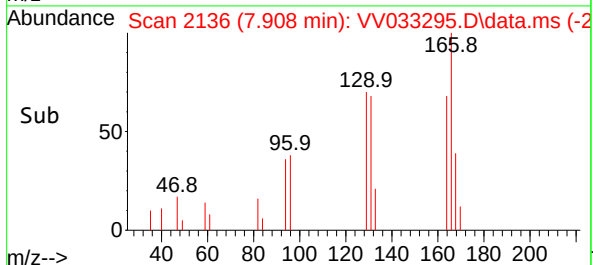
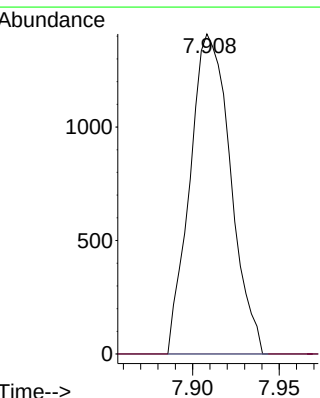
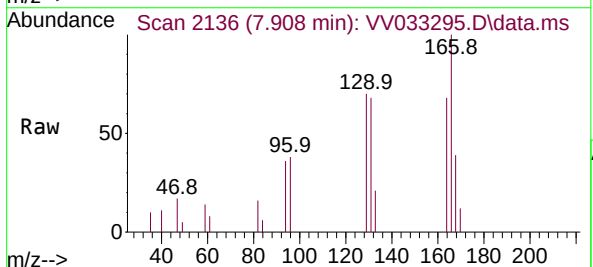


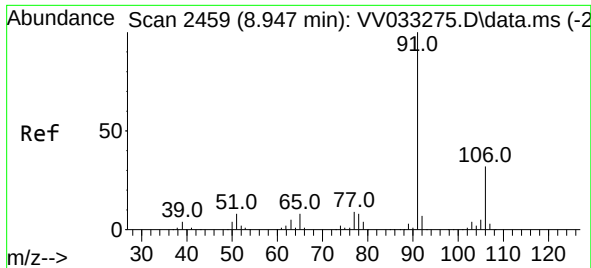

#52
Ethylbenzene
Concen: 0.160 ug/L
RT: 8.953 min Scan# 2459
Delta R.T. 0.007 min
Lab File: VV033295.D
Acq: 13 Dec 2023 22:44




Instrument :
MSVOA_V
ClientSampleId :
E0Y67


Tgt Ion: 91 Resp: 6684
Ion Ratio Lower Upper
91 100
106 33.9 22.7 42.3

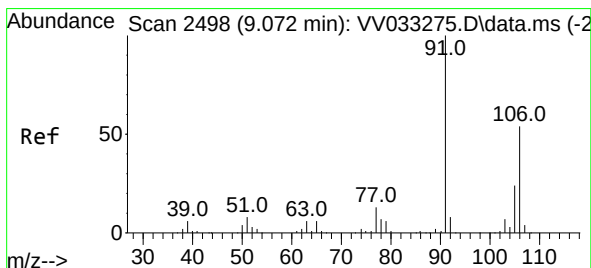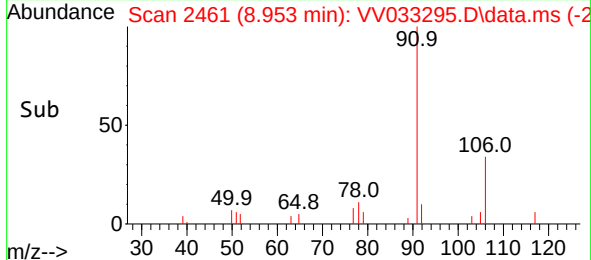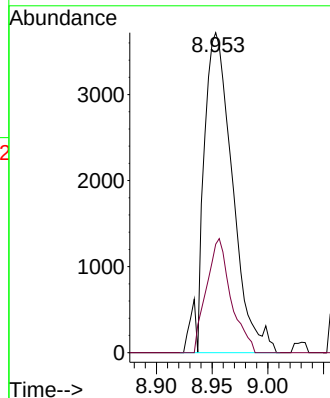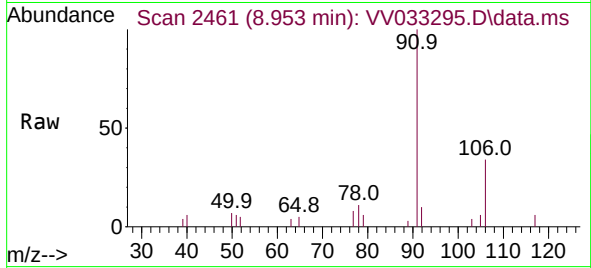

#53
m,p-Xylene
Concen: 0.189 ug/L
RT: 9.079 min Scan# 2500
Delta R.T. 0.006 min
Lab File: VV033295.D
Acq: 13 Dec 2023 22:44

Tgt Ion: 106 Resp: 3251
Ion Ratio Lower Upper
106 100
91 184.1 136.8 254.0

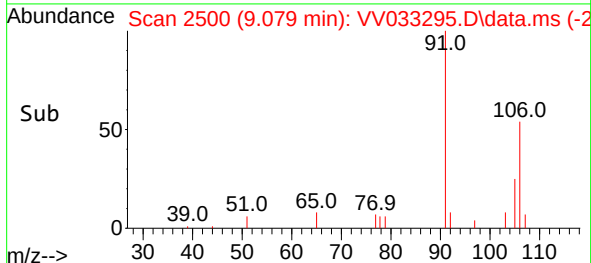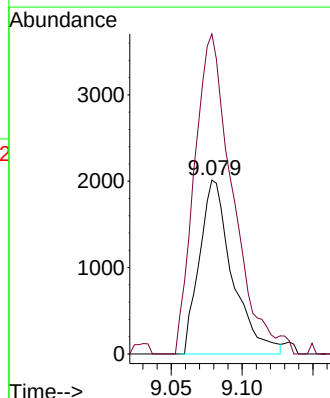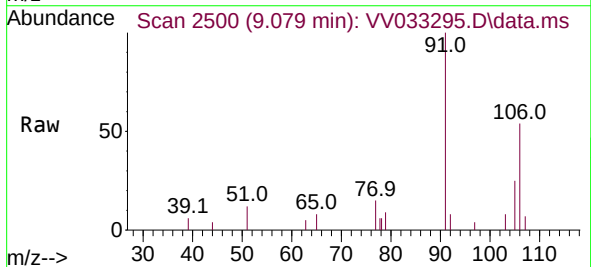

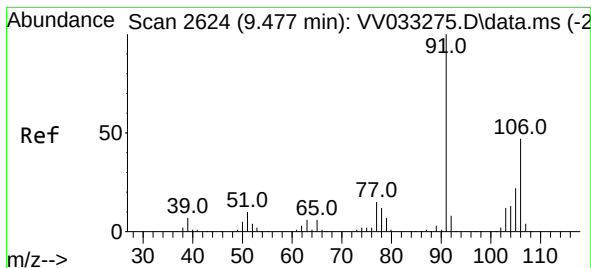

#54

o-Xylene

Concen: 0.087 ug/L

RT: 9.484 min Scan# 2

Delta R.T. 0.007 min

Lab File: VV033295.D

Acq: 13 Dec 2023 22:44

Instrument :

MSVOA_V

ClientSampleId :





E0Y67

Tgt Ion:106 Resp: 1413

Ion Ratio Lower Upper

106 100

91 164.3 149.9 278.5

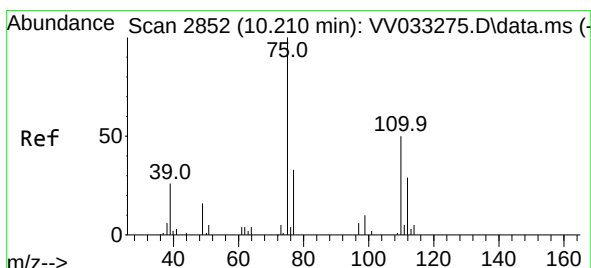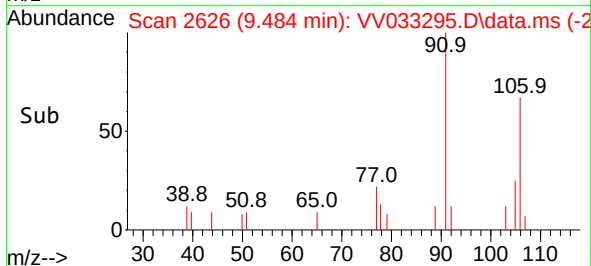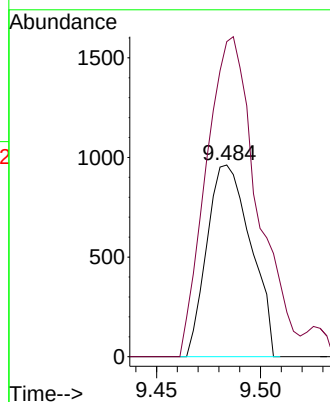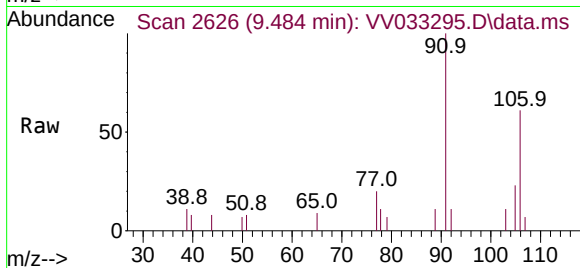

#61

1,2,3-Trichloropropane

Concen: 1.583 ug/L

RT: 11.185 min Scan# 3155

Delta R.T. 0.974 min

Lab File: VV033295.D

Acq: 13 Dec 2023 22:44

Tgt Ion: 75 Resp: 5069

Ion Ratio Lower Upper

75 100

77 38.1 27.4 41.2

110 3.3 39.4 59.2#

