




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033269.D
 Acq On : 13 Dec 2023 09:50
 Operator : SY/MD
 Sample : VSTD0.516
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5216

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 13 23:00:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 22:59:35 2023
 Response via : Initial Calibration

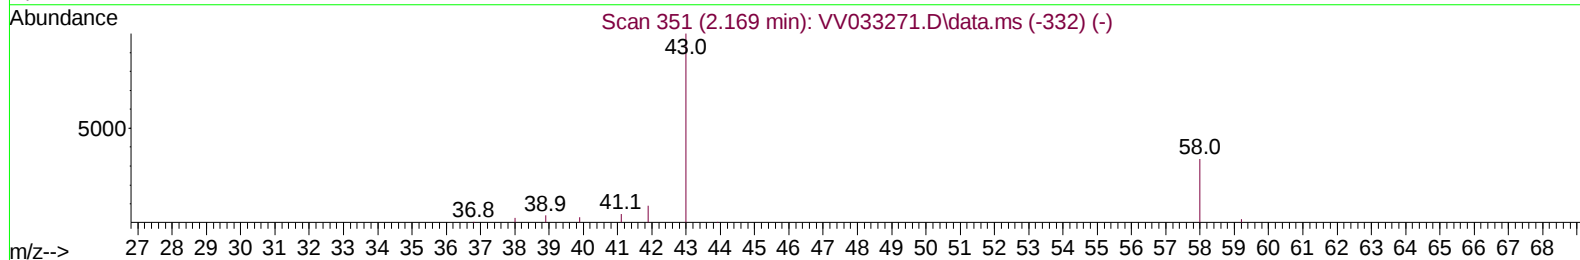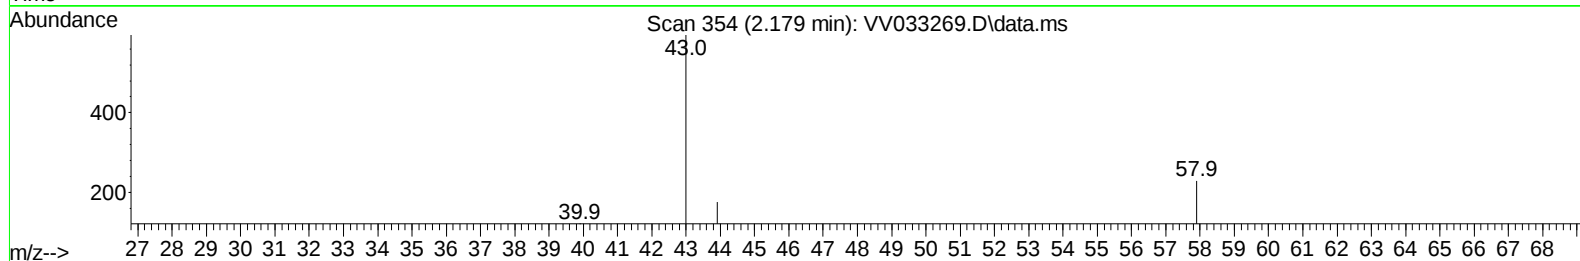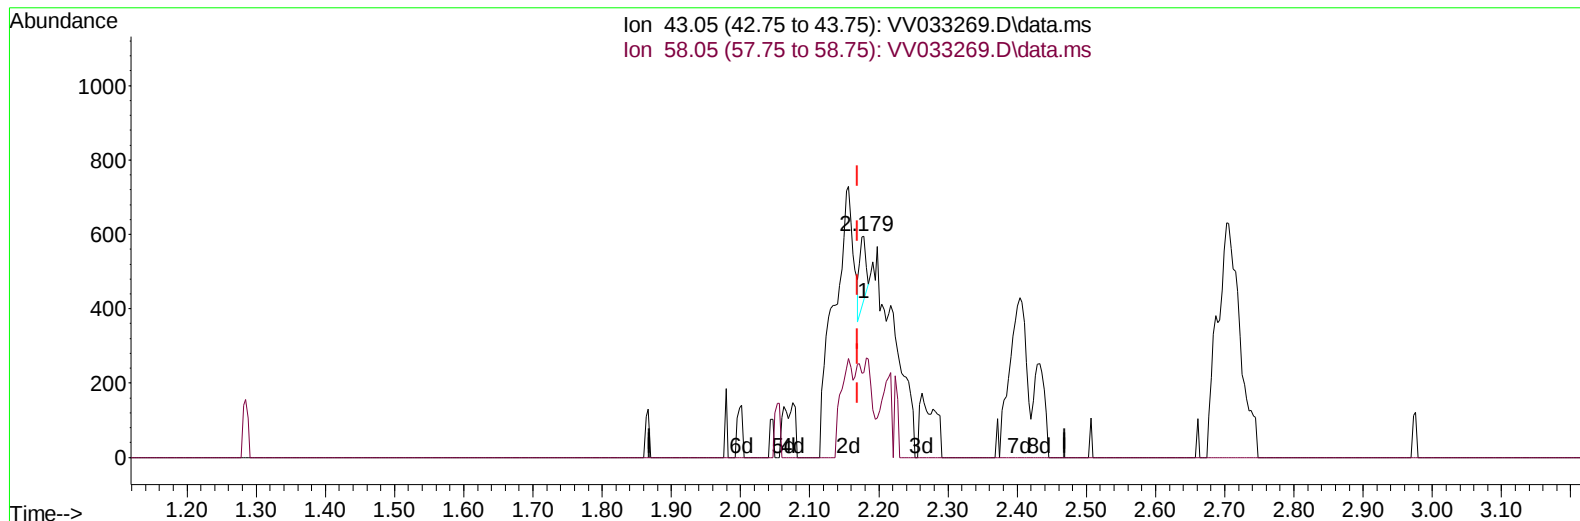

TIC: VV033269.D\data.ms

(13) Acetone (T)

2.179min (+ 0.010) 0.09 ug/L

response 117

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	15.10	23.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033269.D
Acq On : 13 Dec 2023 09:50
Operator : SY/MD
Sample : VSTD0.516
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5216

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 13 23:00:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 13 22:59:35 2023
Response via : Initial Calibration

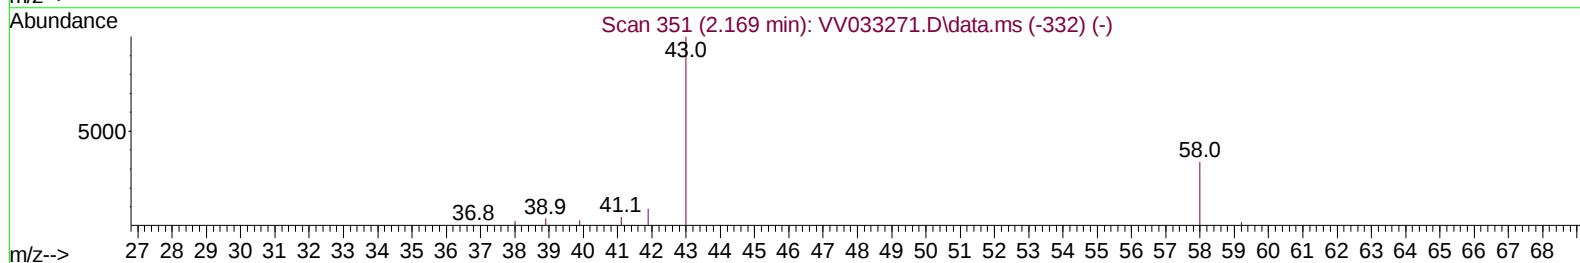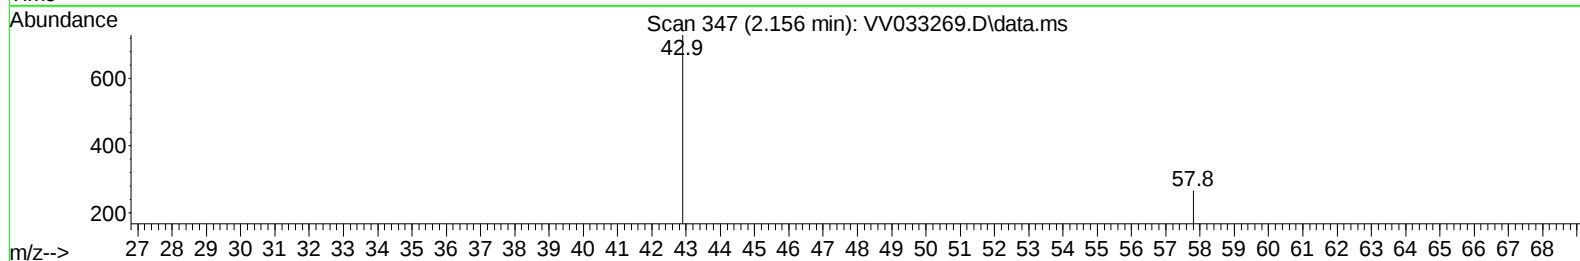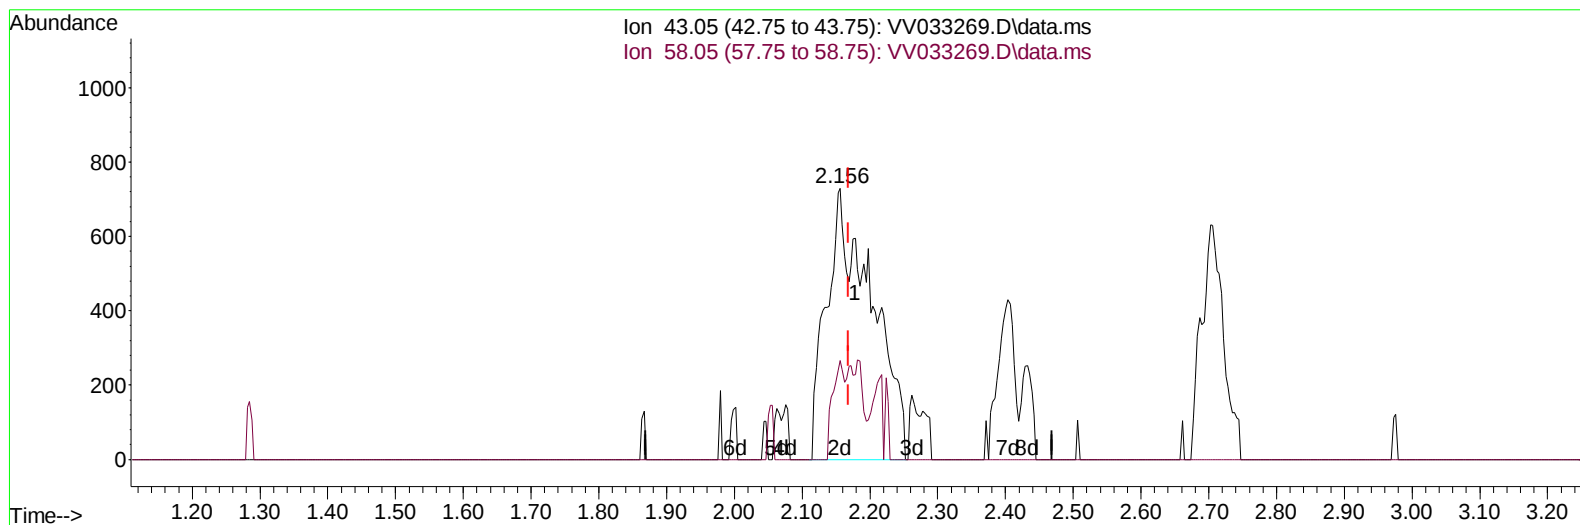

TIC: VV033269.D\data.ms

(13) Acetone (T)

2.156min (-0.013) 2.47 ug/L m

response 3369

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	15.10	0.80
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033269.D
 Acq On : 13 Dec 2023 09:50
 Operator : SY/MD
 Sample : VSTD0.516
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5216

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 13 23:00:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 22:59:35 2023
 Response via : Initial Calibration

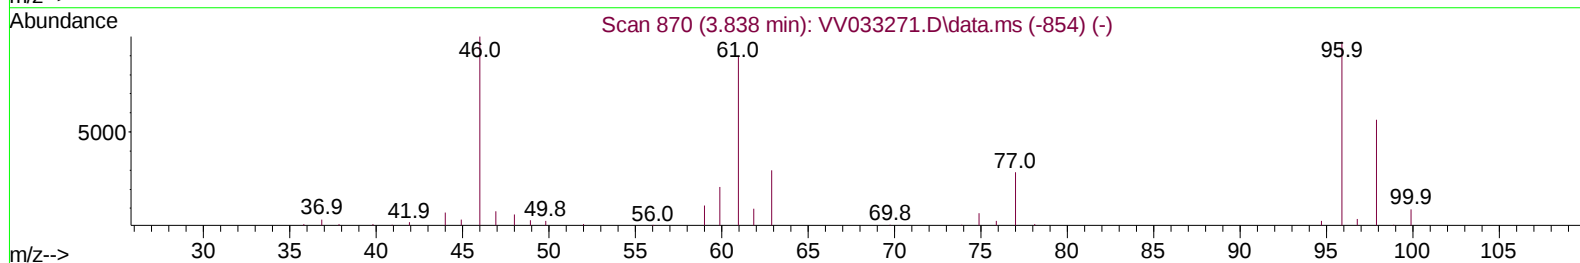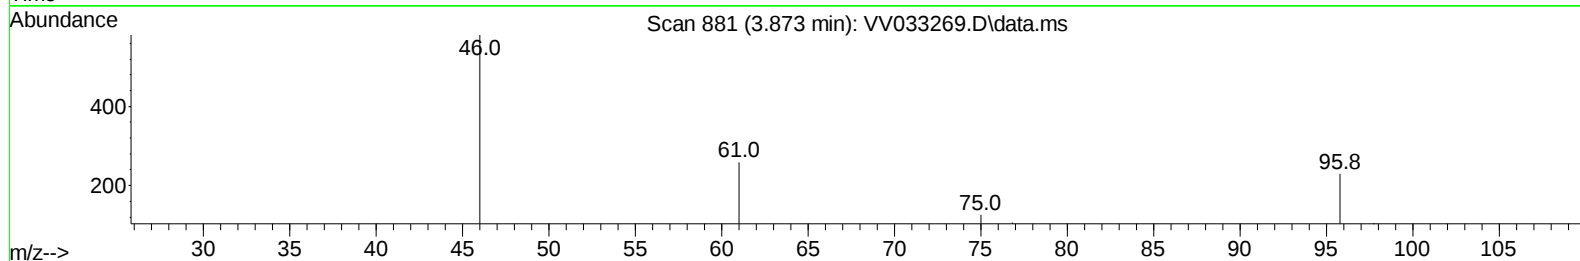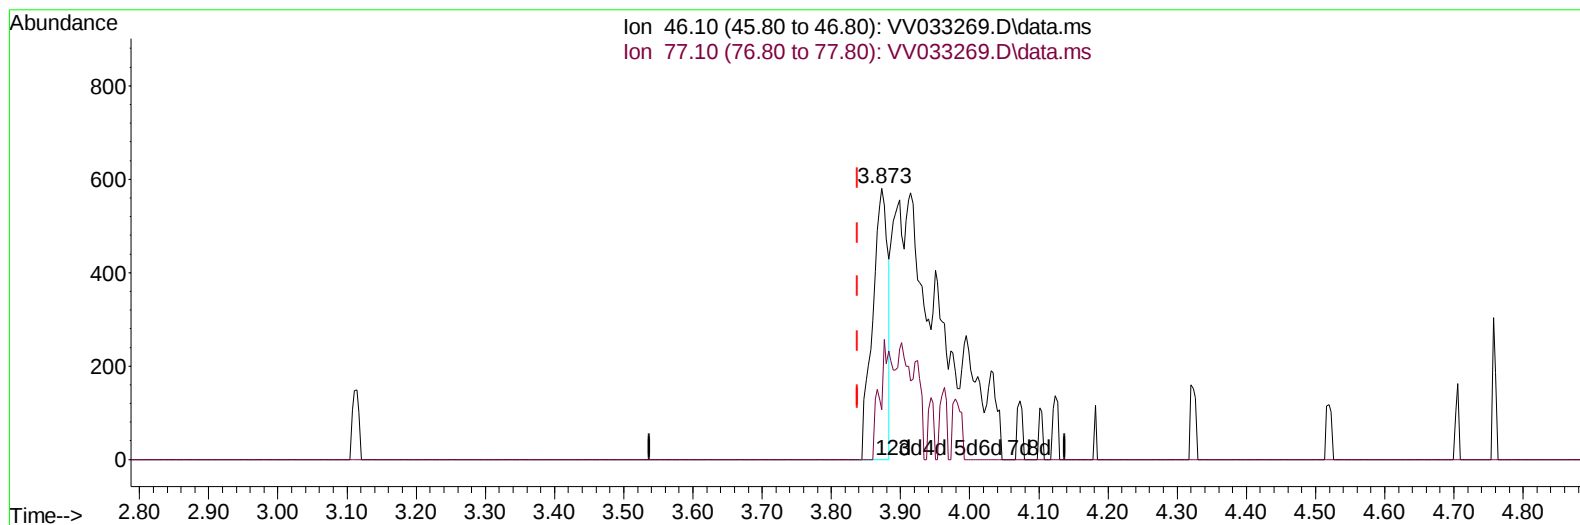

TIC: VV033269.D\data.ms

(20) 2-Butanone-d5 (S)

3.873min (+ 0.035) 0.58 ug/L

response 868

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.80	40.09#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033269.D
Acq On : 13 Dec 2023 09:50
Operator : SY/MD
Sample : VSTD0.516
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5216

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 13 23:00:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 13 22:59:35 2023
Response via : Initial Calibration

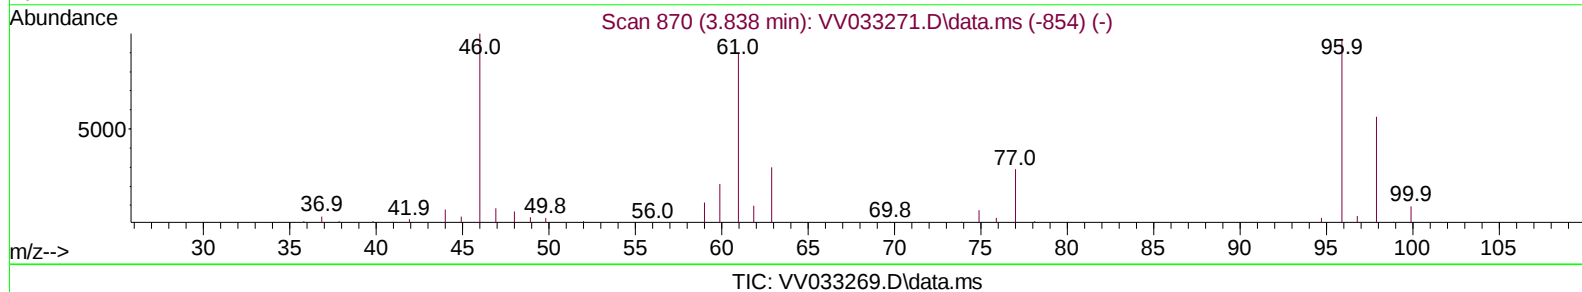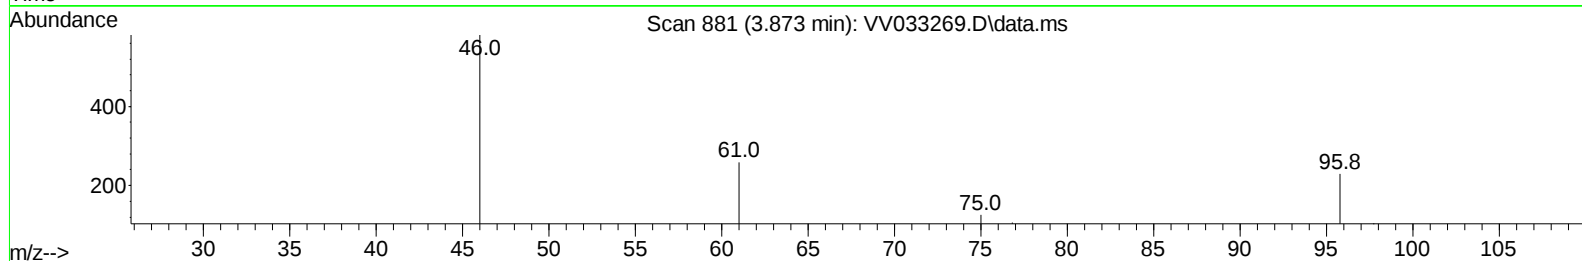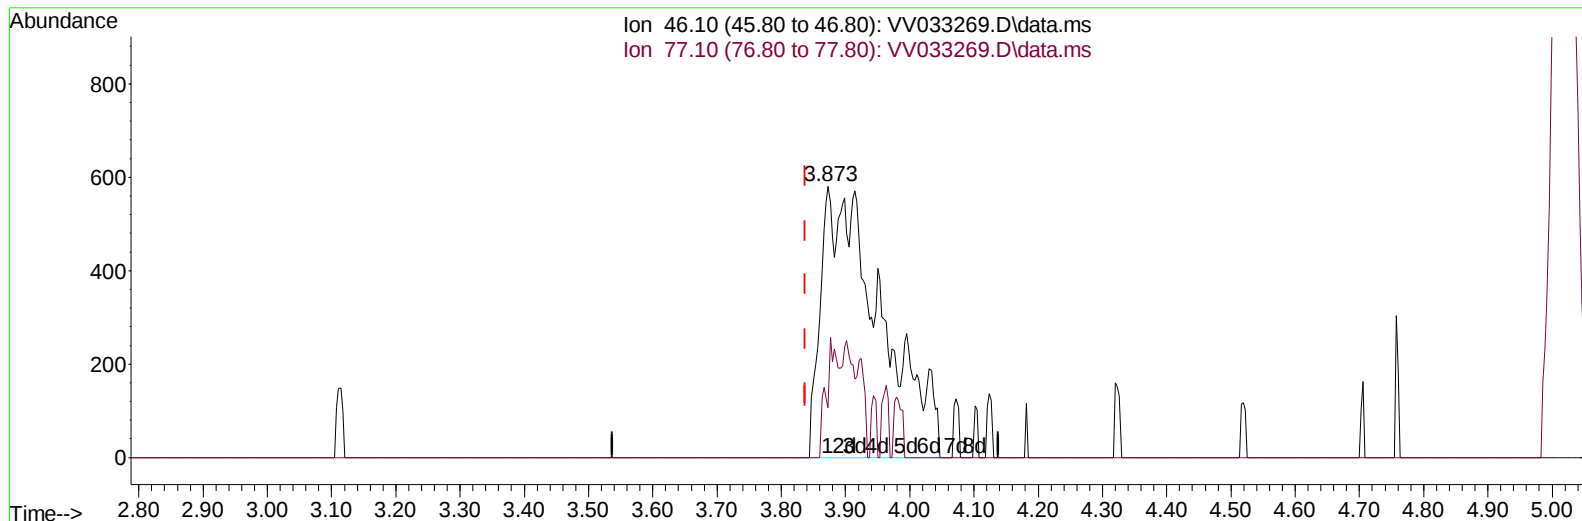**(20) 2-Butanone-d5 (S)**

3.873min (+ 0.035) 2.50 ug/L m

response 3739

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.80	9.31
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033269.D
 Acq On : 13 Dec 2023 09:50
 Operator : SY/MD
 Sample : VSTD0.516
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5216

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 13 23:00:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 22:59:35 2023
 Response via : Initial Calibration

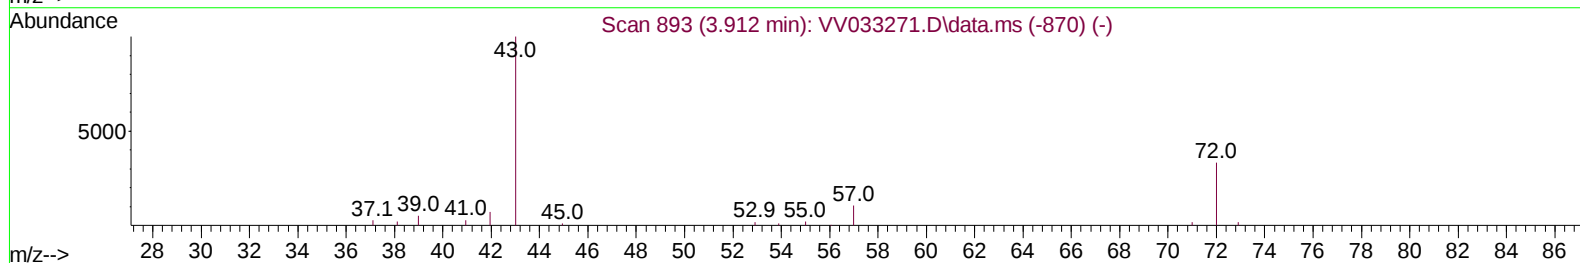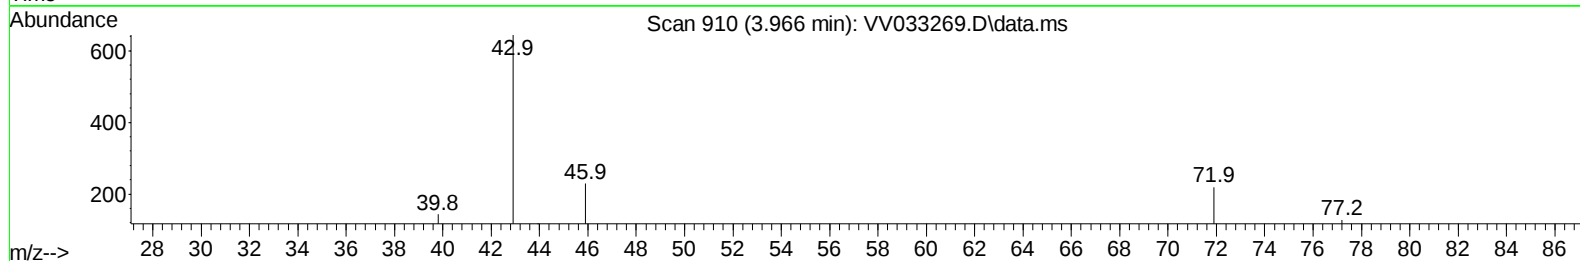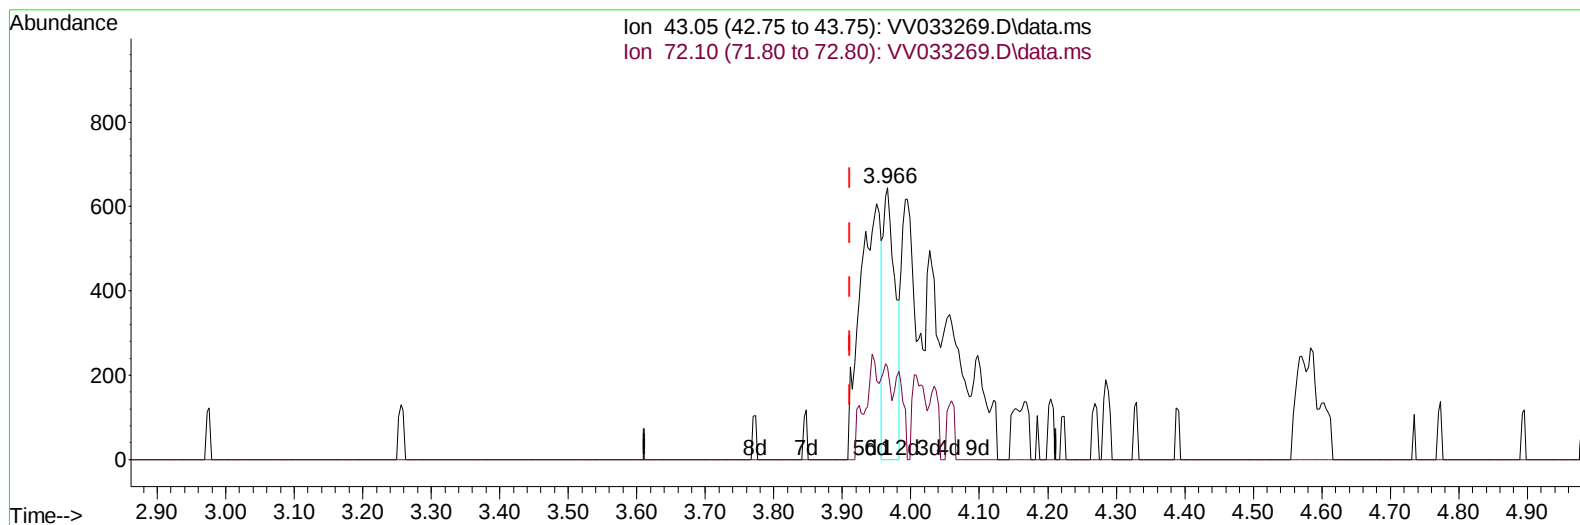

TIC: VV033269.D\data.ms

(21) 2-Butanone (T)

3.966min (+ 0.055) 0.46 ug/L

response 776

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	29.50	28.74
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033269.D
 Acq On : 13 Dec 2023 09:50
 Operator : SY/MD
 Sample : VSTD0.516
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5216

Manual IntegrationsAPPROVED

Quant Time: Dec 13 23:00:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 22:59:35 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

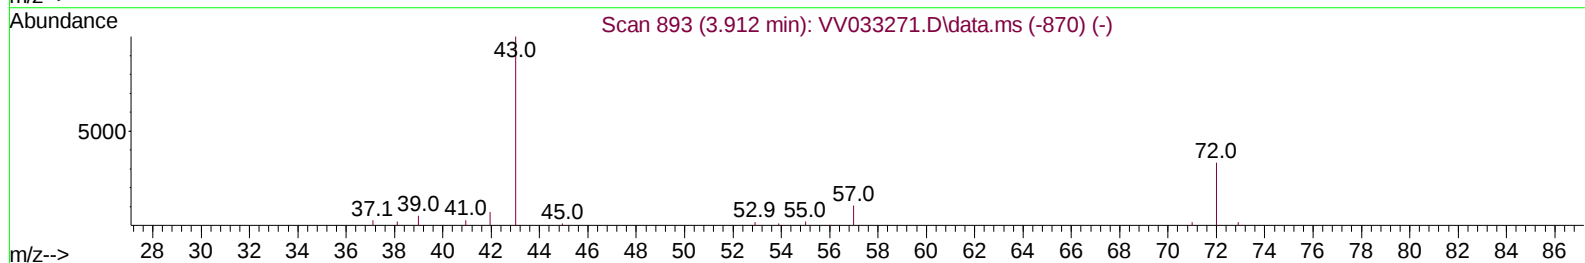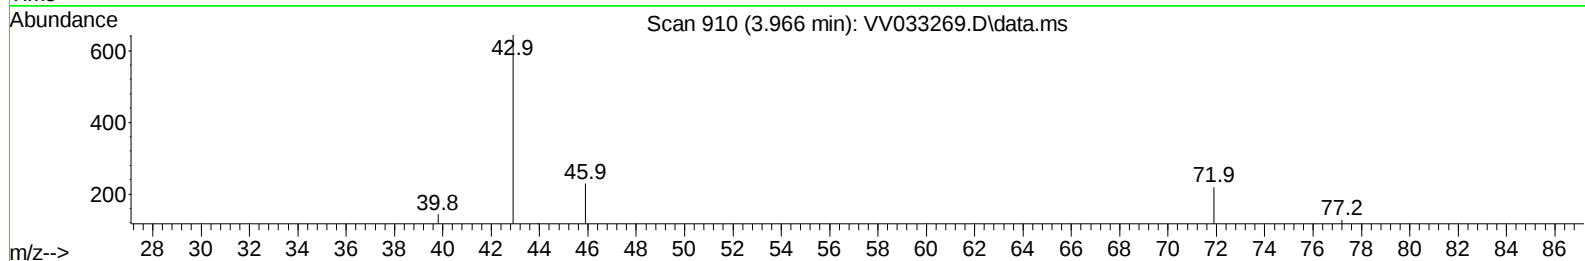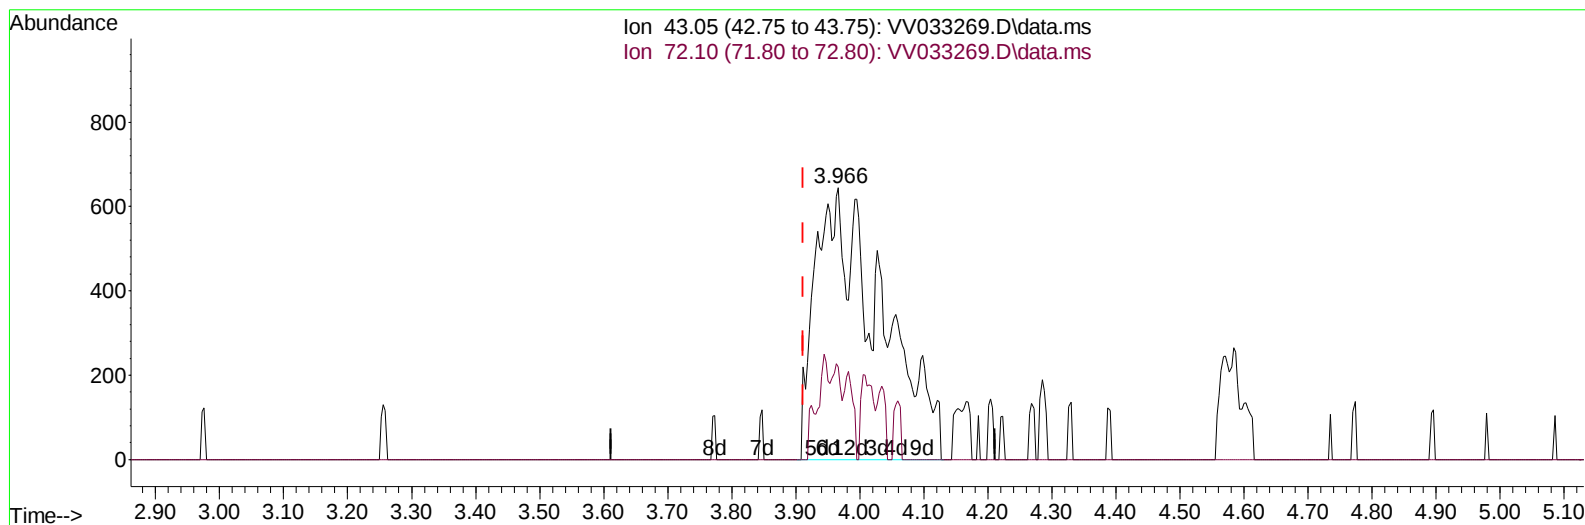

TIC: VV033269.D\data.ms

(21) 2-Butanone (T)

3.966min (+ 0.055) 2.70 ug/L m

response 4573

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	29.50	4.88#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033269.D
 Acq On : 13 Dec 2023 09:50
 Operator : SY/MD
 Sample : VSTD0.516
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5216

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 13 23:00:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 22:59:35 2023
 Response via : Initial Calibration

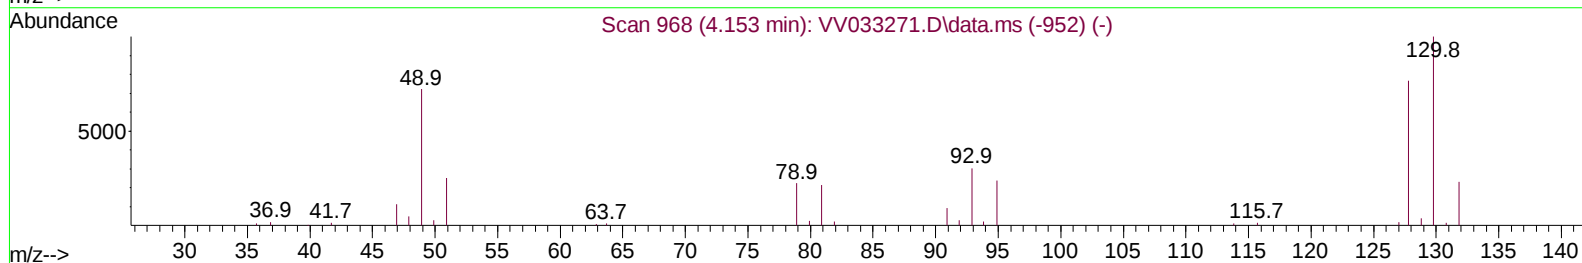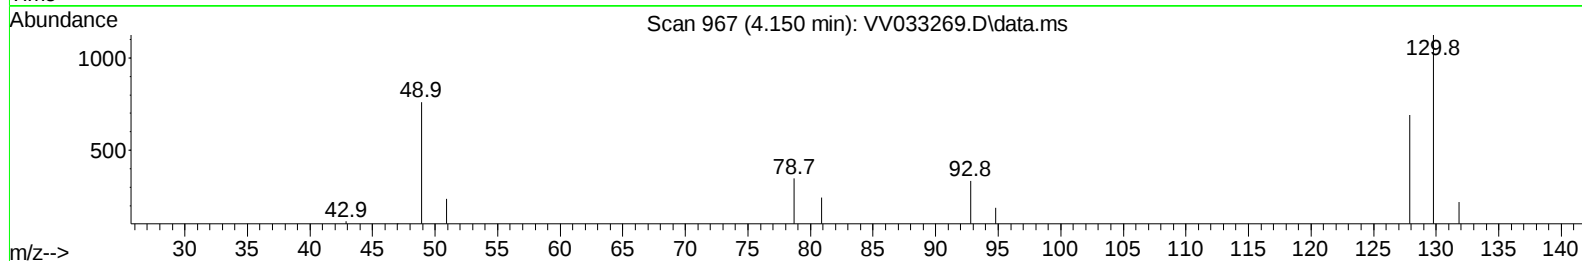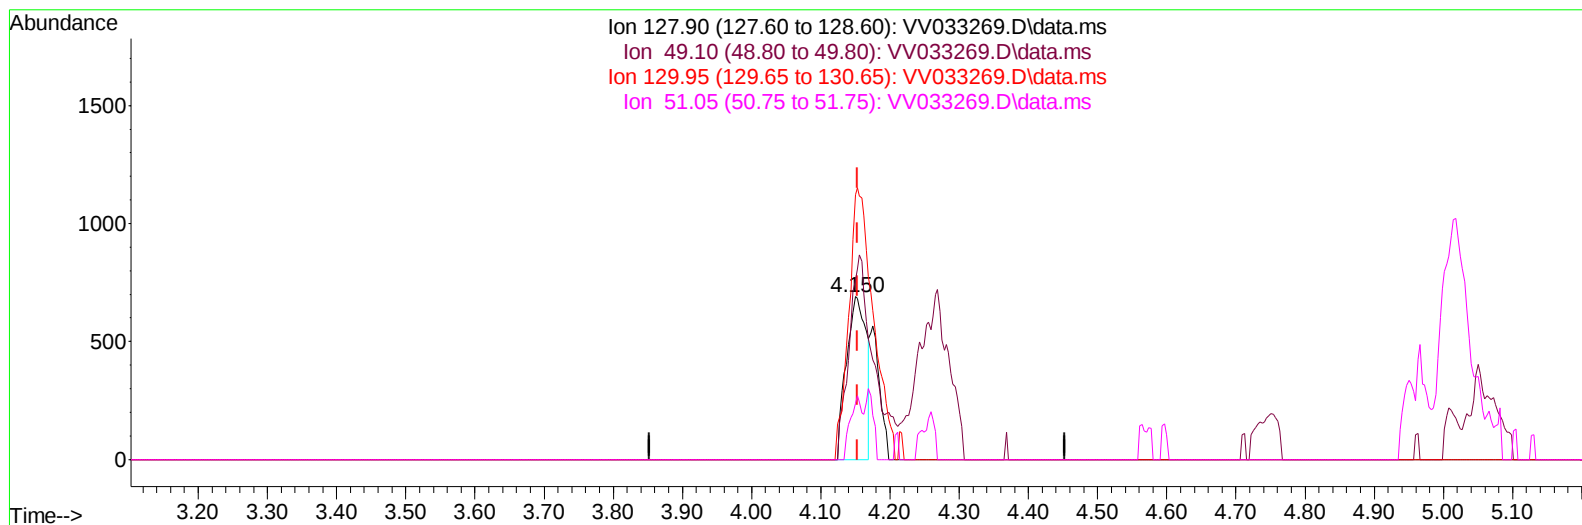

TIC: VV033269.D\data.ms

(23) Bromochloromethane (T)

4.150min (-0.003) 0.27 ug/L

response 1378

Ion	Exp%	Act%
127.90	100.00	100.00
49.10	94.00	110.29
129.95	130.20	162.75
51.05	32.80	34.49




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033269.D
 Acq On : 13 Dec 2023 09:50
 Operator : SY/MD
 Sample : VSTD0.516
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5216

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 13 23:00:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 22:59:35 2023
 Response via : Initial Calibration

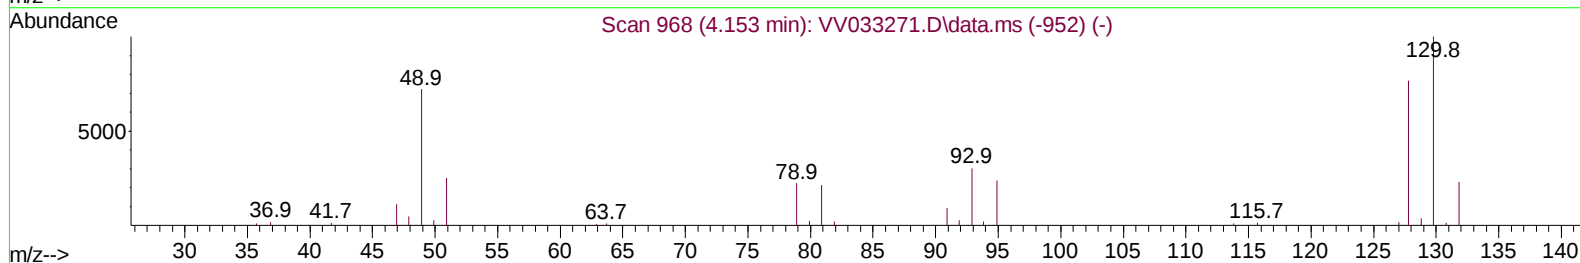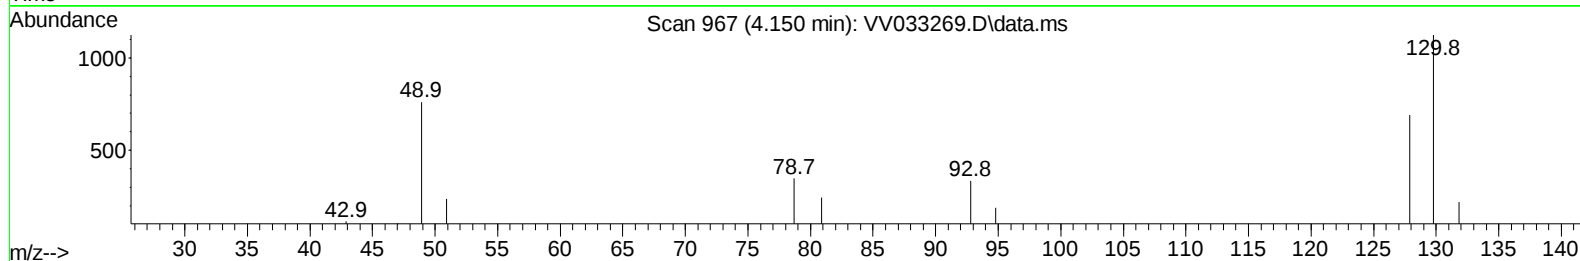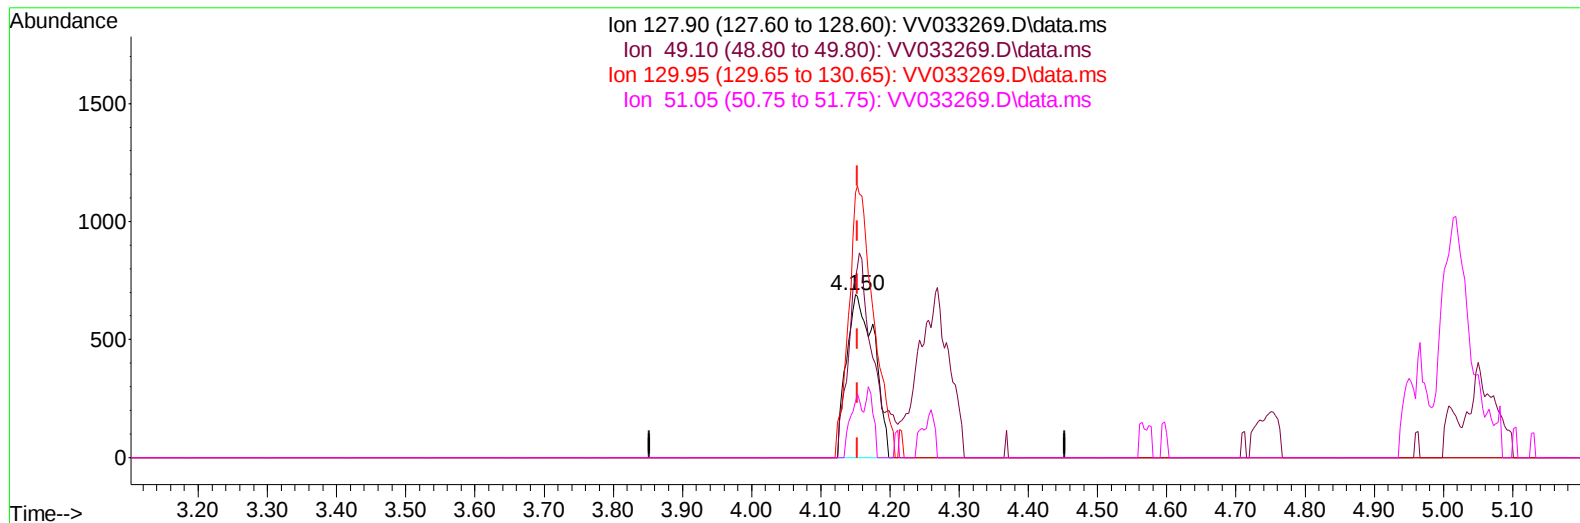

TIC: VV033269.D\data.ms

(23) Bromochloromethane (T)

4.150min (-0.003) 0.37 ug/L m

response 1925

Ion	Exp%	Act%
127.90	100.00	100.00
49.10	94.00	110.29
129.95	130.20	162.75
51.05	32.80	34.49

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033269.D
 Acq On : 13 Dec 2023 09:50
 Operator : SY/MD
 Sample : VSTD0.516
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5216

Manual IntegrationsAPPROVED

Quant Time: Dec 13 23:00:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 22:59:35 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	139047	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117	133335	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	69490	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	4264	0.379	ug/L	0.00
7) Chloroethane-d5	1.532	69	3309	0.314	ug/L	0.00
11) 1,1-Dichloroethene-d2	2.056	65	1685	0.338	ug/L	0.00
20) 2-Butanone-d5	3.873	46	3739m	2.502	ug/L	0.04
24) Chloroform-d	4.256	84	7944	0.394	ug/L	0.00
26) 1,2-Dichloroethane-d4	4.960	65	3237	0.362	ug/L	0.02
32) Benzene-d6	4.966	84	14292	0.409	ug/L	0.00
36) 1,2-Dichloropropane-d6	5.998	67	3248	0.341	ug/L	0.00
41) Toluene-d8	7.249	98	13403	0.403	ug/L	0.00
43) trans-1,3-Dichloroprop...	7.571	79	1324	0.344	ug/L	0.02
46) 2-Hexanone-d5	8.047	63	3285	2.577	ug/L	0.02
56) 1,1,2,2-Tetrachloroeth...	10.159	84	2081	0.299	ug/L	0.00
66) 1,2-Dichlorobenzene-d4	11.564	152	5495	0.449	ug/L	0.00
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.105	85	8454	0.530	ug/L	99
3) Chloromethane	1.214	50	5466	0.388	ug/L	95
5) Vinyl chloride	1.282	62	5036	0.370	ug/L	99
6) Bromomethane	1.487	94	3466	0.359	ug/L	85
8) Chloroethane	1.548	64	3479	0.352	ug/L	97
9) Trichlorofluoromethane	1.716	101	9350	0.427	ug/L	98
10) 1,1,2-Trichloro-1,2,2-...	2.069	101	4417	0.369	ug/L	94
12) 1,1-Dichloroethene	2.069	96	3895	0.350	ug/L	89
13) Acetone	2.156	43	3369m	2.468	ug/L	
14) Carbon disulfide	2.240	76	13108	0.400	ug/L	96
15) Methyl Acetate	2.404	43	743	0.246	ug/L	98
16) Methylene chloride	2.449	84	5497	0.410	ug/L	93
17) Methyl tert-butyl Ether	2.706	73	7624	0.394	ug/L	98
18) trans-1,2-Dichloroethene	2.693	96	4818	0.439	ug/L	90
19) 1,1-Dichloroethane	3.117	63	7720	0.405	ug/L	94
21) 2-Butanone	3.966	43	4573m	2.702	ug/L	
22) cis-1,2-Dichloroethene	3.825	96	4504	0.396	ug/L	89
23) Bromochloromethane	4.150	128	1925m	0.374	ug/L	
25) Chloroform	4.278	83	8558	0.401	ug/L	96
27) 1,2-Dichloroethane	5.056	62	4418	0.386	ug/L #	72
29) 1,1,1-Trichloroethane	4.506	97	8947	0.480	ug/L	98
30) Cyclohexane	4.580	56	5399	0.421	ug/L	93
31) Carbon tetrachloride	4.735	117	8506	0.519	ug/L	97
33) Benzene	5.014	78	16870	0.435	ug/L	100
34) Trichloroethene	5.841	95	4927	0.452	ug/L	95
35) Methylcyclohexane	6.053	83	7265	0.491	ug/L	94
37) 1,2-Dichloropropane	6.095	63	3574	0.386	ug/L #	91
38) Bromodichloromethane	6.439	83	5310	0.399	ug/L #	99
39) cis-1,3-Dichloropropene	6.963	75	4697	0.352	ug/L	97
40) 4-Methyl-2-pentanone	7.169	43	9911	2.747	ug/L	98
42) Toluene	7.320	91	18462	0.429	ug/L	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033269.D
 Acq On : 13 Dec 2023 09:50
 Operator : SY/MD
 Sample : VSTD0.516
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5216

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 13 23:00:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 22:59:35 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) trans-1,3-Dichloropropene	7.590	75	3920	0.363	ug/L	93
45) 1,1,2-Trichloroethane	7.776	97	2584	0.380	ug/L	93
47) Tetrachloroethene	7.908	164	4854	0.515	ug/L	93
48) 2-Hexanone	8.095	43	6778	2.514	ug/L	96
49) Dibromochloromethane	8.182	129	3454	0.409	ug/L	76
50) 1,2-Dibromoethane	8.294	107	2026	0.312	ug/L #	99
51) Chlorobenzene	8.815	112	13204	0.455	ug/L	97
52) Ethylbenzene	8.950	91	20048	0.441	ug/L	100
53) m,p-Xylene	9.079	106	8606	0.480	ug/L	87
54) o-Xylene	9.481	106	7941	0.470	ug/L	93
55) Styrene	9.503	104	11705	0.405	ug/L	94
57) 1,1,2,2-Tetrachloroethane	10.185	83	2515	0.339	ug/L #	94
59) Bromoform	9.670	173	1904	0.429	ug/L	96
60) Isopropylbenzene	9.866	105	21216	0.481	ug/L	99
61) 1,2,3-Trichloropropane	10.217	75	1871	0.387	ug/L	91
62) 1,3,5-Trimethylbenzene	10.477	105	16982	0.484	ug/L	100
63) 1,2,4-Trimethylbenzene	10.853	105	15321	0.436	ug/L	91
64) 1,3-Dichlorobenzene	11.124	146	11123	0.476	ug/L	98
65) 1,4-Dichlorobenzene	11.210	146	11691	0.492	ug/L	98
67) 1,2-Dichlorobenzene	11.583	146	9470	0.460	ug/L	96
68) 1,2-Dibromo-3-chloropr...	12.368	75	325	0.273	ug/L #	66
69) 1,3,5-Trichlorobenzene	12.587	180	8890	0.502	ug/L	99
70) 1,2,4-trichlorobenzene	13.201	180	6728	0.471	ug/L	96
71) Naphthalene	13.445	128	7400	0.390	ug/L	97
72) 1,2,3-Trichlorobenzene	13.686	180	5004	0.413	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual IntegrationsAPPROVED

Quant Time: Dec 13 23:00:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : wed Dec 13 22:59:35 2023
Response via : Initial Calibration

