




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033282.D
 Acq On : 13 Dec 2023 17:34
 Operator : SY/MD
 Sample : 05731-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y54

Manual IntegrationsAPPROVED

Quant Time: Dec 13 23:34:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 23:30:39 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

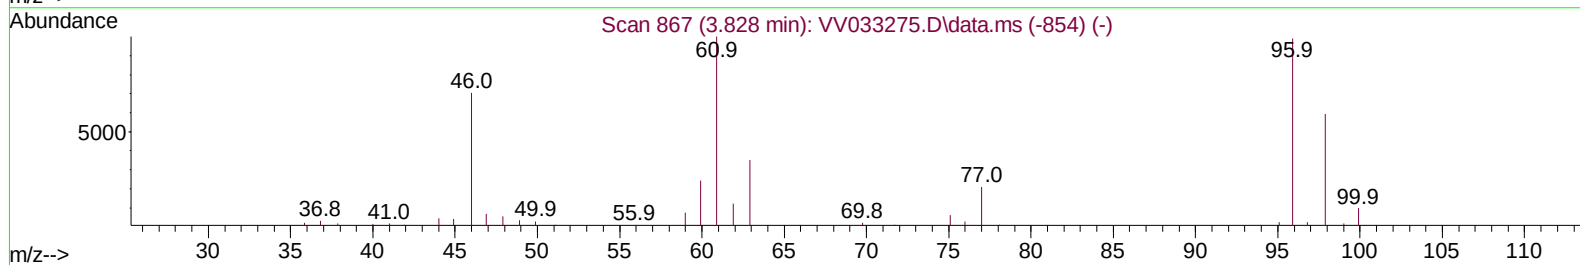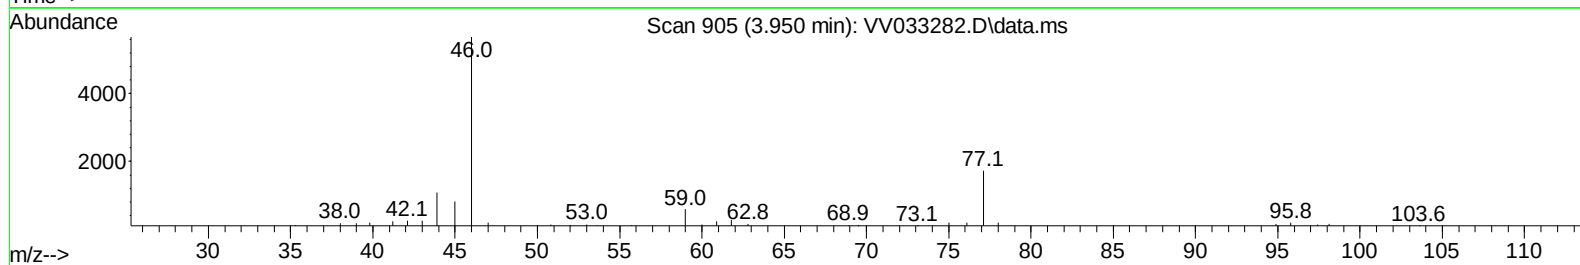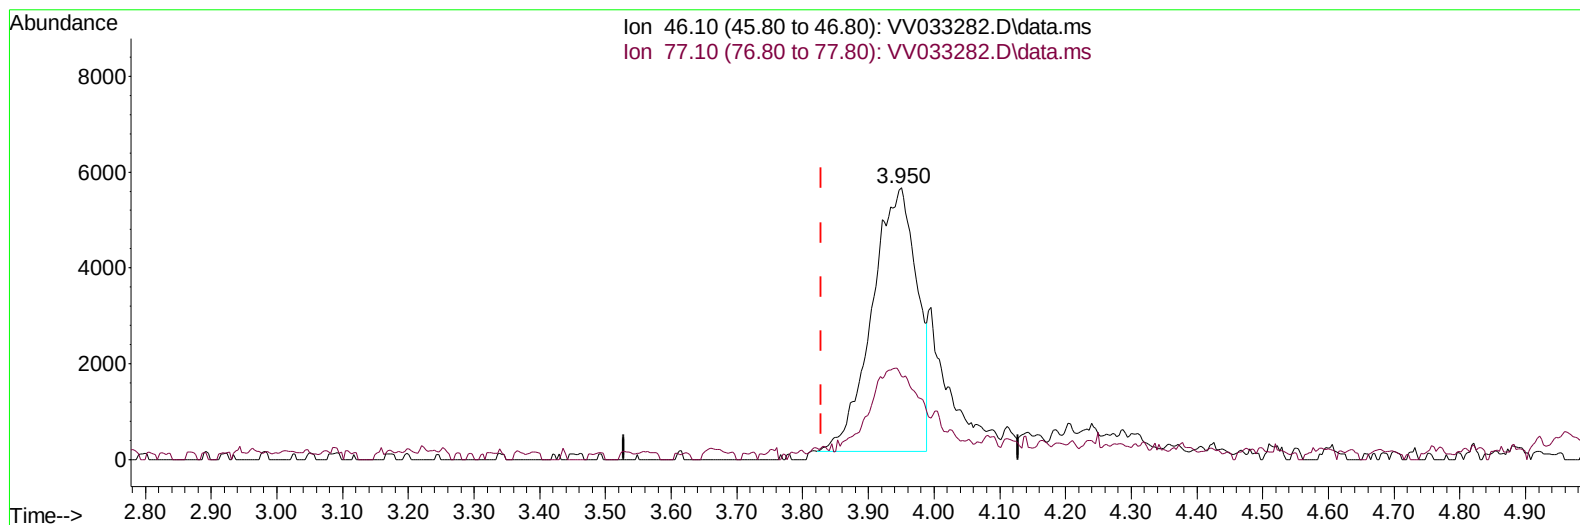

TIC: VV033282.D\data.ms

(20) 2-Butanone-d5 (S)

3.950min (+ 0.122) 21.80 ug/L

response 26068

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.80	34.27#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033282.D
 Acq On : 13 Dec 2023 17:34
 Operator : SY/MD
 Sample : 05731-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y54

Manual IntegrationsAPPROVED

Quant Time: Dec 13 23:34:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 23:30:39 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

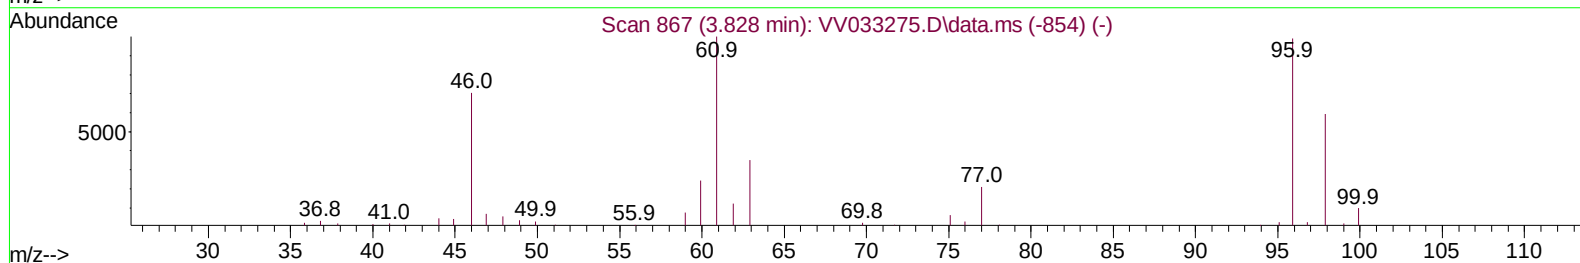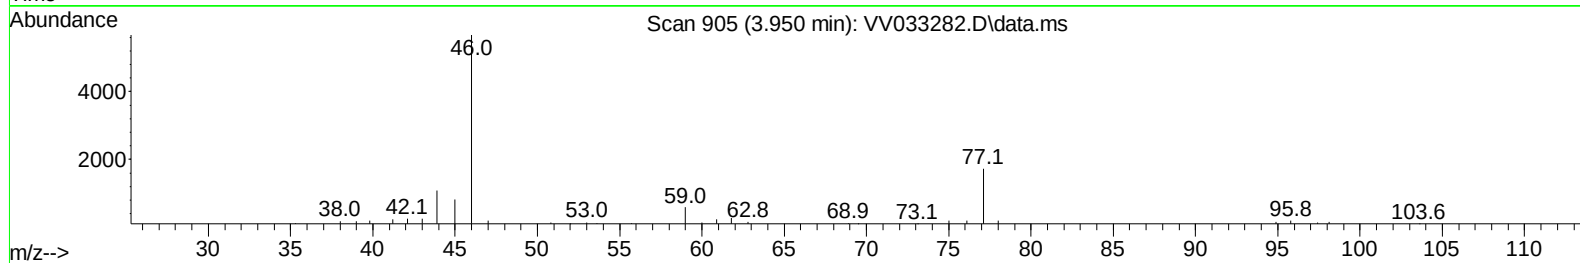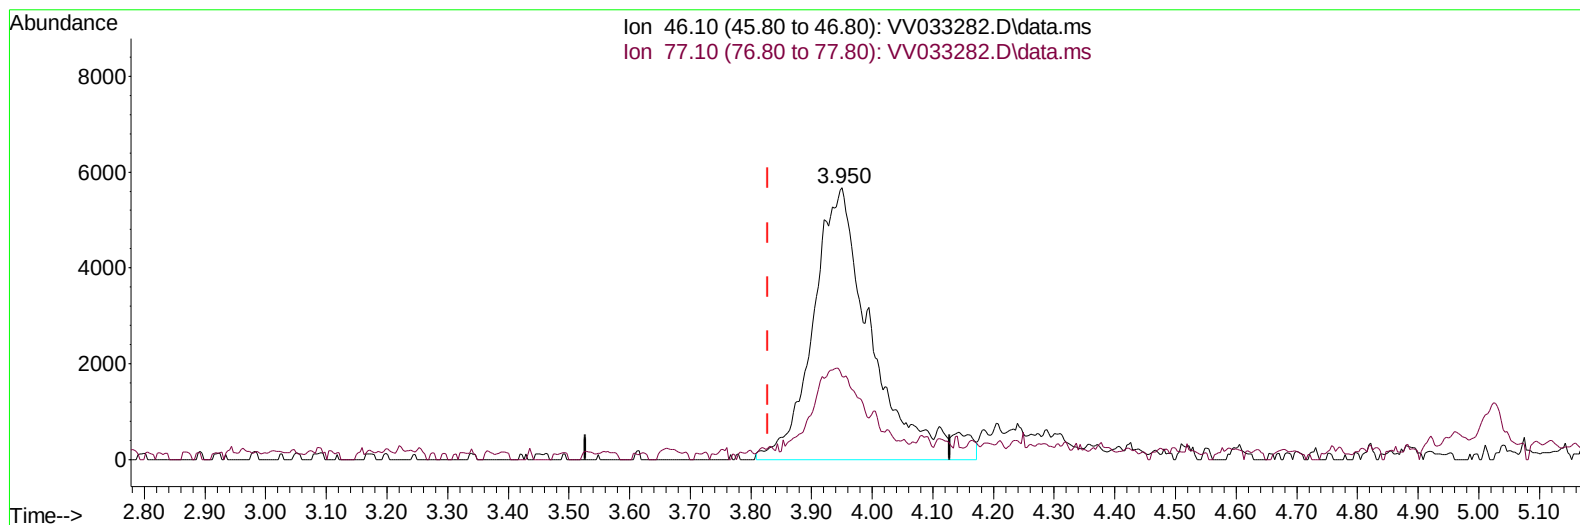

TIC: VV033282.D\data.ms

(20) 2-Butanone-d5 (S)

3.950min (+ 0.122) 31.86 ug/L m

response 38097

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.80	23.45#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033282.D
 Acq On : 13 Dec 2023 17:34
 Operator : SY/MD
 Sample : 05731-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y54

Manual IntegrationsAPPROVED

Quant Time: Dec 13 23:34:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 23:30:39 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.551	114	157616	5.000	ug/L	0.02
28) Chlorobenzene-d5	8.808	117	151004	5.000	ug/L	0.02
58) 1,4-Dichlorobenzene-d4	11.191	152	72713	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.288	65	40216	3.980	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	79.600%	
7) Chloroethane-d5	1.551	69	29352	3.906	ug/L	0.02
Spiked Amount 5.000	Range 65	- 130	Recovery	=	78.200%	
11) 1,1-Dichloroethene-d2	2.076	65	16453	4.091	ug/L	0.02
Spiked Amount 5.000	Range 60	- 125	Recovery	=	81.800%	
20) 2-Butanone-d5	3.950	46	38097m	31.861	ug/L	0.12
Spiked Amount 50.000	Range 40	- 130	Recovery	=	63.720%	
24) Chloroform-d	4.288	84	78631	3.731	ug/L	0.04
Spiked Amount 5.000	Range 70	- 125	Recovery	=	74.600%	
26) 1,2-Dichloroethane-d4	4.969	65	43580	4.759	ug/L	0.03
Spiked Amount 5.000	Range 70	- 130	Recovery	=	95.200%	
32) Benzene-d6	4.973	84	162220	4.153	ug/L	0.01
Spiked Amount 5.000	Range 70	- 125	Recovery	=	83.000%	
36) 1,2-Dichloropropane-d6	6.034	67	36303	4.083	ug/L	0.05
Spiked Amount 5.000	Range 60	- 140	Recovery	=	81.600%	
41) Toluene-d8	7.291	98	138312	3.634	ug/L	0.05
Spiked Amount 5.000	Range 70	- 130	Recovery	=	72.600%	
43) trans-1,3-Dichloroprop...	7.593	79	15271	3.765	ug/L	0.04
Spiked Amount 5.000	Range 55	- 130	Recovery	=	75.200%	
46) 2-Hexanone-d5	8.066	63	38606	34.093	ug/L	0.04
Spiked Amount 50.000	Range 45	- 130	Recovery	=	68.180%	
56) 1,1,2,2-Tetrachloroeth...	10.165	84	21569	3.587	ug/L	0.01
Spiked Amount 5.000	Range 65	- 120	Recovery	=	71.800%	
66) 1,2-Dichlorobenzene-d4	11.567	152	56436	4.407	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	88.200%	
Target Compounds						
					Qvalue	
18) trans-1,2-Dichloroethene	2.728	96	1907	0.175	ug/L	96
22) cis-1,2-Dichloroethene	3.850	96	61211	5.423	ug/L	95
33) Benzene	5.021	78	8774	0.217	ug/L	100
34) Trichloroethene	5.860	95	7571	0.642	ug/L	92
42) Toluene	7.365	91	19386	0.418	ug/L	100
47) Tetrachloroethene	7.944	164	2376	0.213	ug/L	93
51) Chlorobenzene	8.837	112	31401	0.989	ug/L	99
52) Ethylbenzene	8.969	91	4760	0.092	ug/L	95
53) m,p-Xylene	9.098	106	3067	0.144	ug/L	71
65) 1,4-Dichlorobenzene	11.217	146	5803	0.238	ug/L	93
67) 1,2-Dichlorobenzene	11.586	146	2411	0.114	ug/L #	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033282.D
Acq On : 13 Dec 2023 17:34
Operator : SY/MD
Sample : 05731-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
E0Y54

Manual IntegrationsAPPROVED

Quant Time: Dec 13 23:34:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 13 23:30:39 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
Supervised By :Mahesh Dadoda 12/18/2023

