




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033288.D
 Acq On : 13 Dec 2023 19:58
 Operator : SY/MD
 Sample : 05731-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y60

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 13 23:35:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 23:30:39 2023
 Response via : Initial Calibration

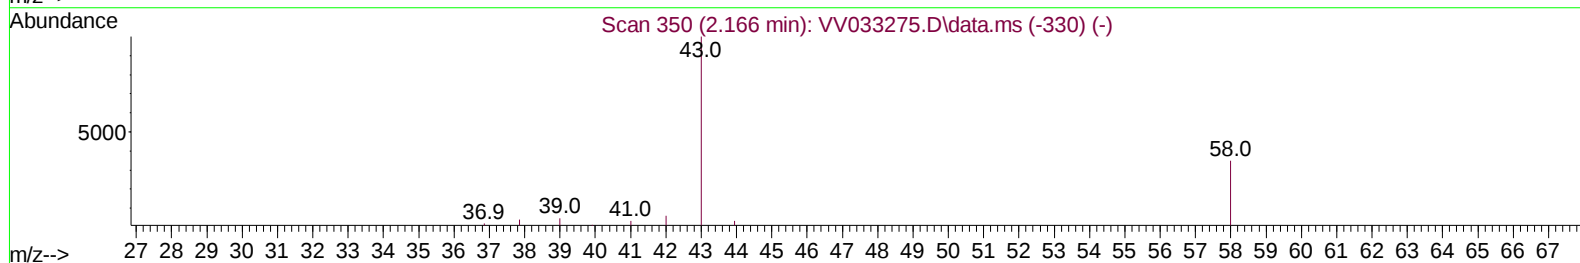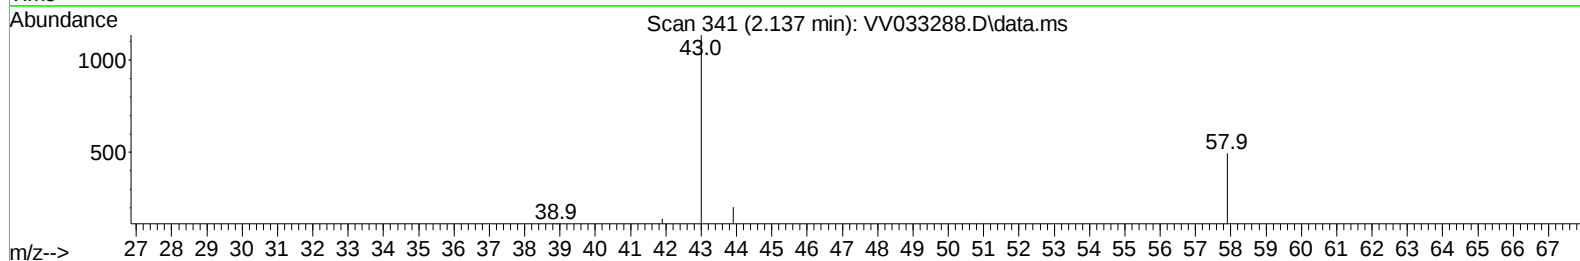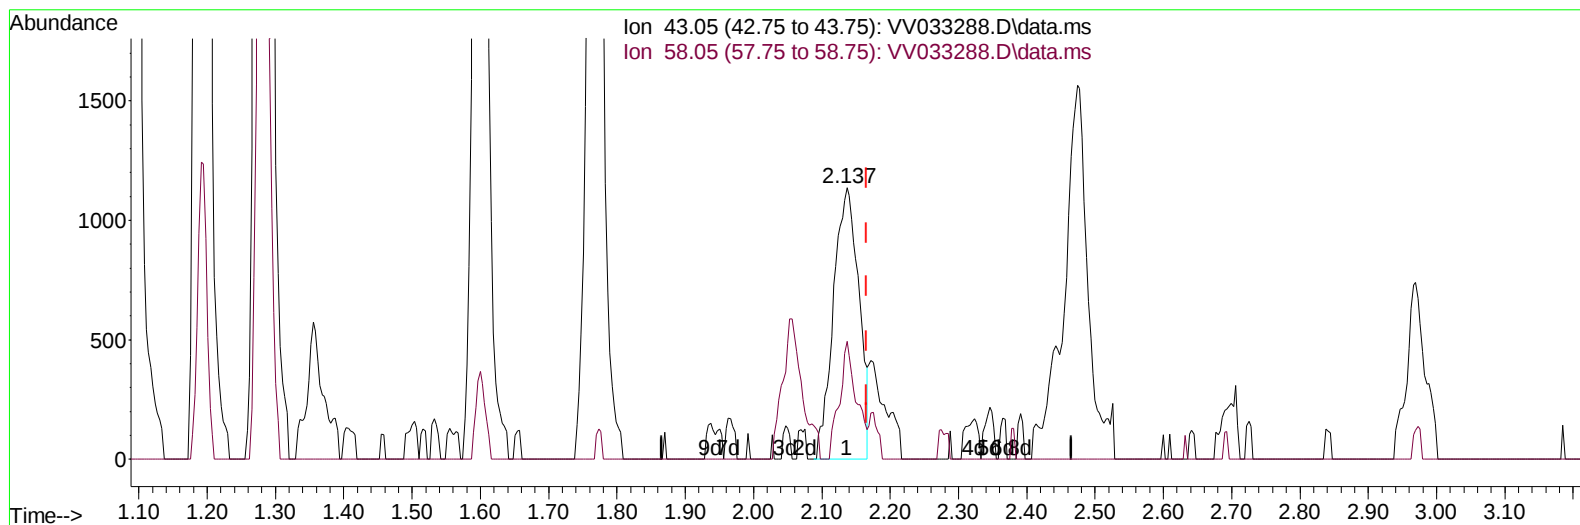

TIC: VV033288.D\data.ms

(13) Acetone (T)

2.137min (-0.029) 4.36 ug/L

response 2919

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	15.10	29.39
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033288.D
Acq On : 13 Dec 2023 19:58
Operator : SY/MD
Sample : 05731-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y60

Manual IntegrationsAPPROVED

Quant Time: Dec 13 23:35:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 13 23:30:39 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
Supervised By :Mahesh Dadoda 12/18/2023

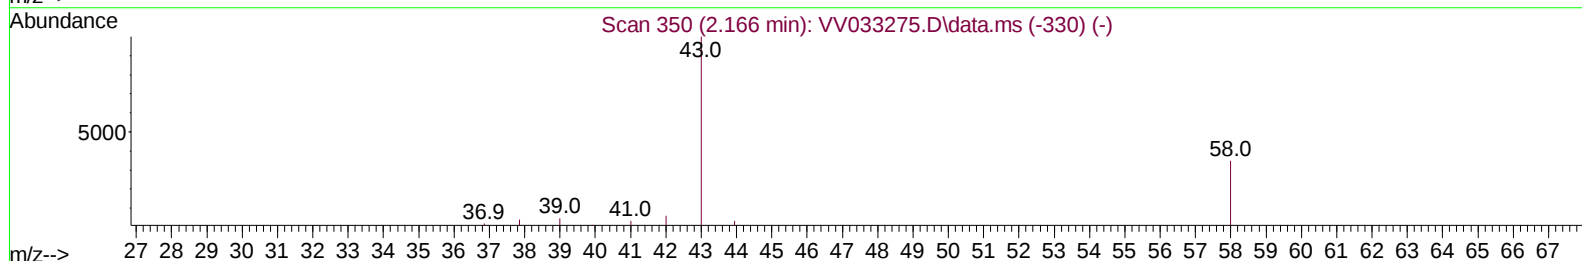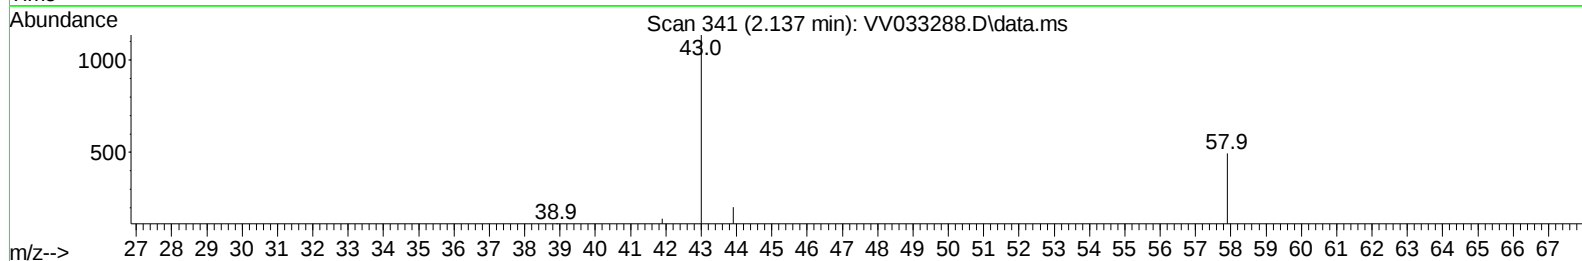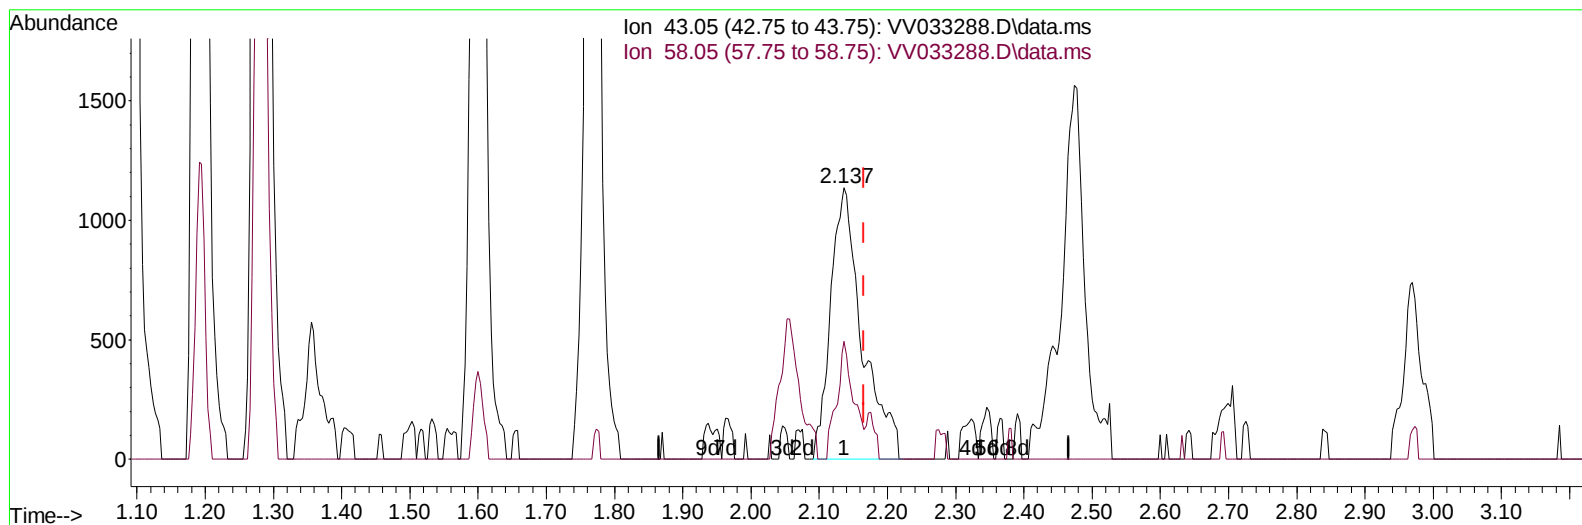

TIC: VV033288.D\data.ms

(13) Acetone (T)

2.137min (-0.029) 5.45 ug/L m

response 3646

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	15.10	23.53
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033288.D
 Acq On : 13 Dec 2023 19:58
 Operator : SY/MD
 Sample : 05731-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y60

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Quant Time: Dec 13 23:35:57 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 13 23:30:39 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		124669	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		125173	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		63893	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		41448	5.186	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	103.800%	
7) Chloroethane-d5	1.535	69		31396	5.282	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	105.600%	
11) 1,1-Dichloroethene-d2	2.060	65		16069	5.052	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	101.000%	
20) 2-Butanone-d5	3.805	46		52708	55.730	ug/L	-0.02
Spiked Amount 50.000	Range 40	- 130		Recovery	=	111.460%	
24) Chloroform-d	4.249	84		90239	5.413	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	108.200%	
26) 1,2-Dichloroethane-d4	4.944	65		42006	5.799	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	116.000%	
32) Benzene-d6	4.960	84		172220	5.319	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	106.400%	
36) 1,2-Dichloropropane-d6	5.992	67		42197	5.725	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	114.600%	
41) Toluene-d8	7.246	98		159372	5.051	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	101.000%	
43) trans-1,3-Dichloroprop...	7.554	79		17810	5.297	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	106.000%	
46) 2-Hexanone-d5	8.030	63		57425	61.178	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	122.360%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84		28447	5.707	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	114.200%	
66) 1,2-Dichlorobenzene-d4	11.561	152		66820	5.938	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	118.800%	
Target Compounds						Qvalue	
13) Acetone	2.137	43		3646m	5.447	ug/L	
14) Carbon disulfide	2.243	76		2570	0.111	ug/L	100
22) cis-1,2-Dichloroethene	3.821	96		2448	0.274	ug/L	96
30) Cyclohexane	4.580	56		2455	0.222	ug/L #	16
33) Benzene	5.021	78		11740	0.350	ug/L	100
34) Trichloroethene	5.834	95		63570	6.501	ug/L	98
35) Methylcyclohexane	6.047	83		3761	0.260	ug/L	91
42) Toluene	7.320	91		29355	0.764	ug/L	97
47) Tetrachloroethene	7.911	164		3167	0.342	ug/L	96
52) Ethylbenzene	8.953	91		9048	0.210	ug/L	97
53) m,p-Xylene	9.079	106		4427	0.250	ug/L	88
54) o-Xylene	9.480	106		1867	0.111	ug/L	95
63) 1,2,4-Trimethylbenzene	10.860	105		3714	0.108	ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033288.D
Acq On : 13 Dec 2023 19:58
Operator : SY/MD
Sample : 05731-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y60

Manual IntegrationsAPPROVED

Quant Time: Dec 13 23:35:57 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 13 23:30:39 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
Supervised By :Mahesh Dadoda 12/18/2023

