




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033310.D
 Acq On : 14 Dec 2023 05:07
 Operator : SY/MD
 Sample : 05770-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y82

Manual IntegrationsAPPROVED

Quant Time: Dec 14 05:46:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 14 01:07:25 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

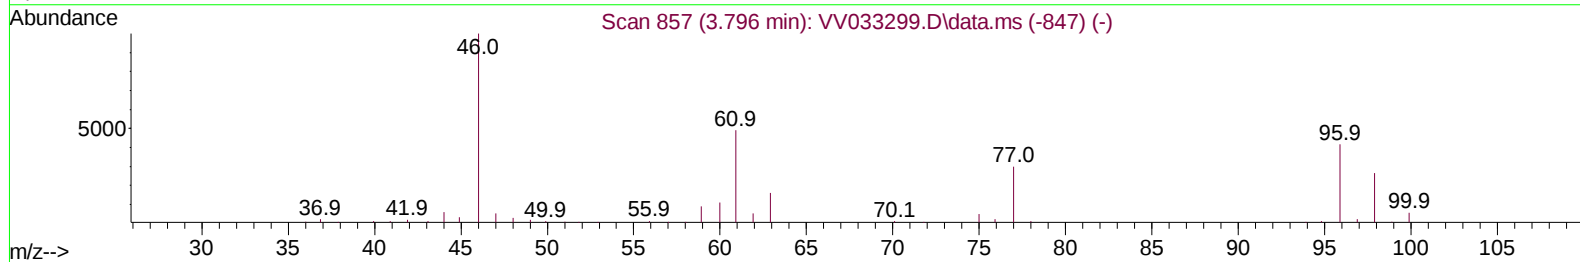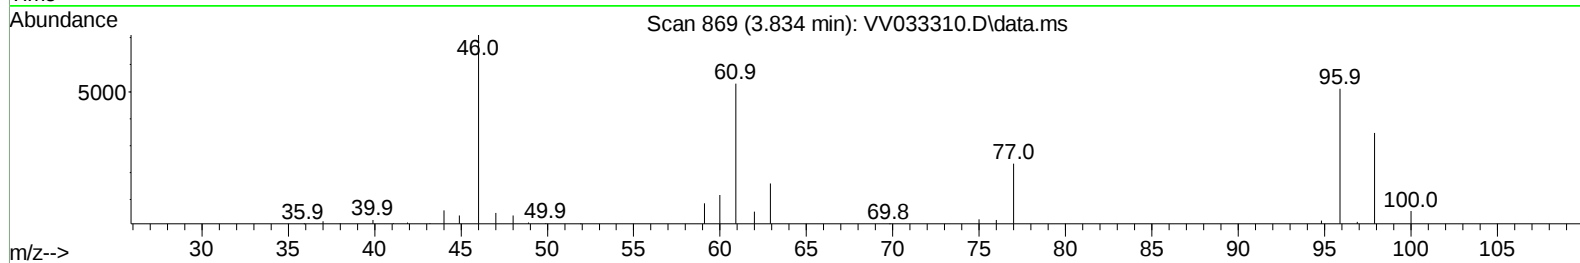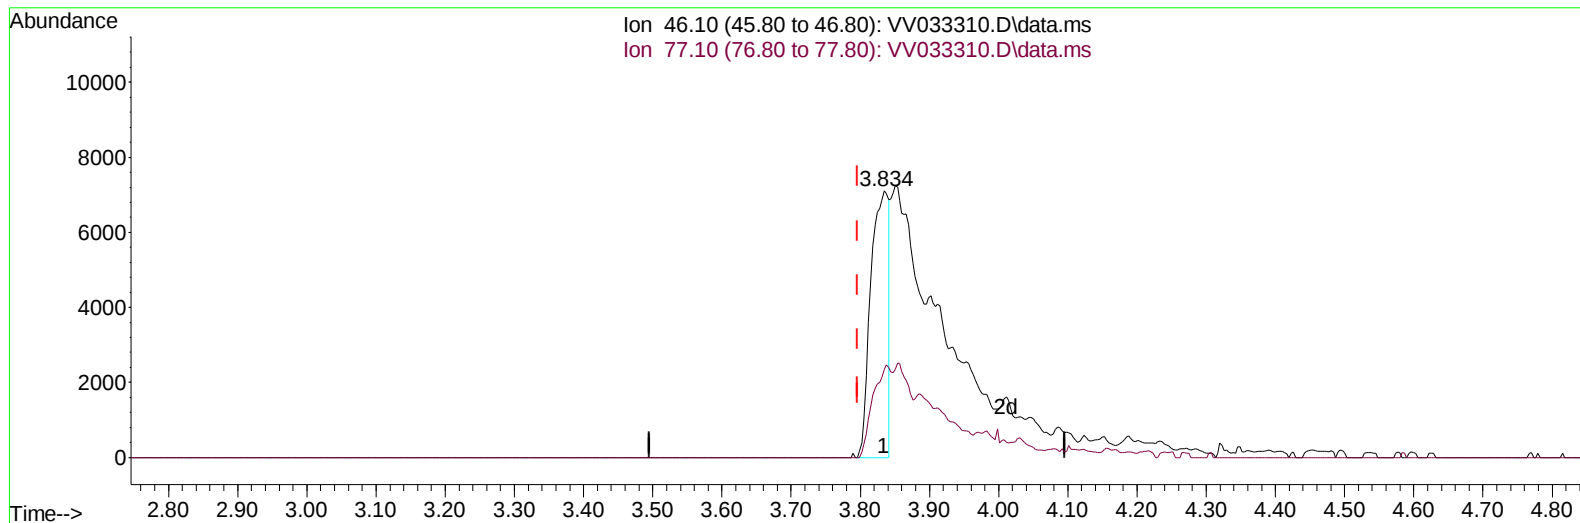

TIC: VV033310.D\data.ms

(20) 2-Butanone-d5 (S)

3.834min (+ 0.039) 12.90 ug/L

response 12542

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.80	38.30#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033310.D
 Acq On : 14 Dec 2023 05:07
 Operator : SY/MD
 Sample : 05770-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y82

Manual IntegrationsAPPROVED

Quant Time: Dec 14 05:46:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 14 01:07:25 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

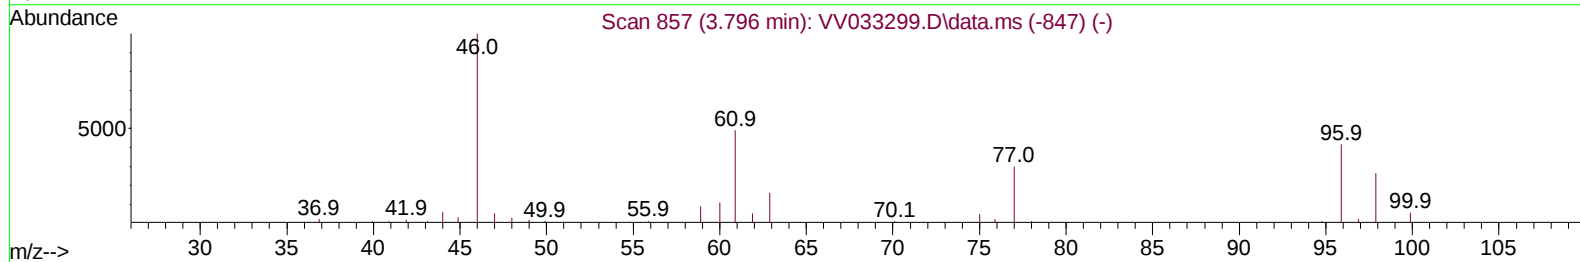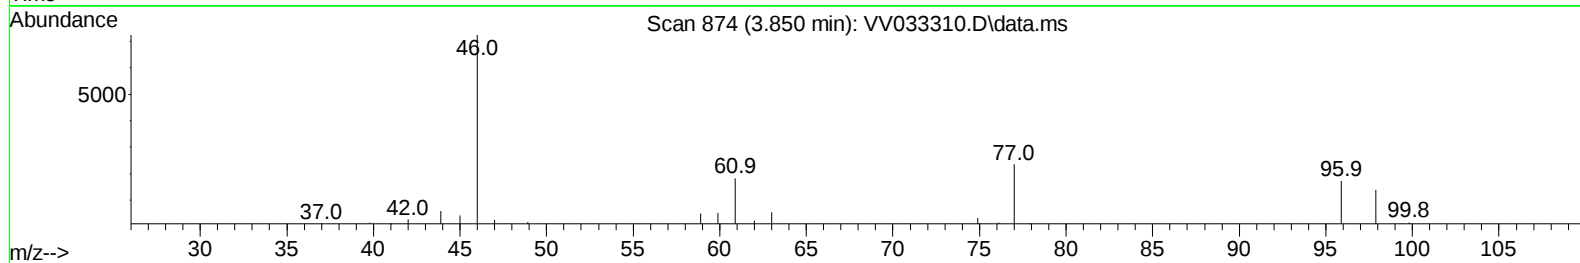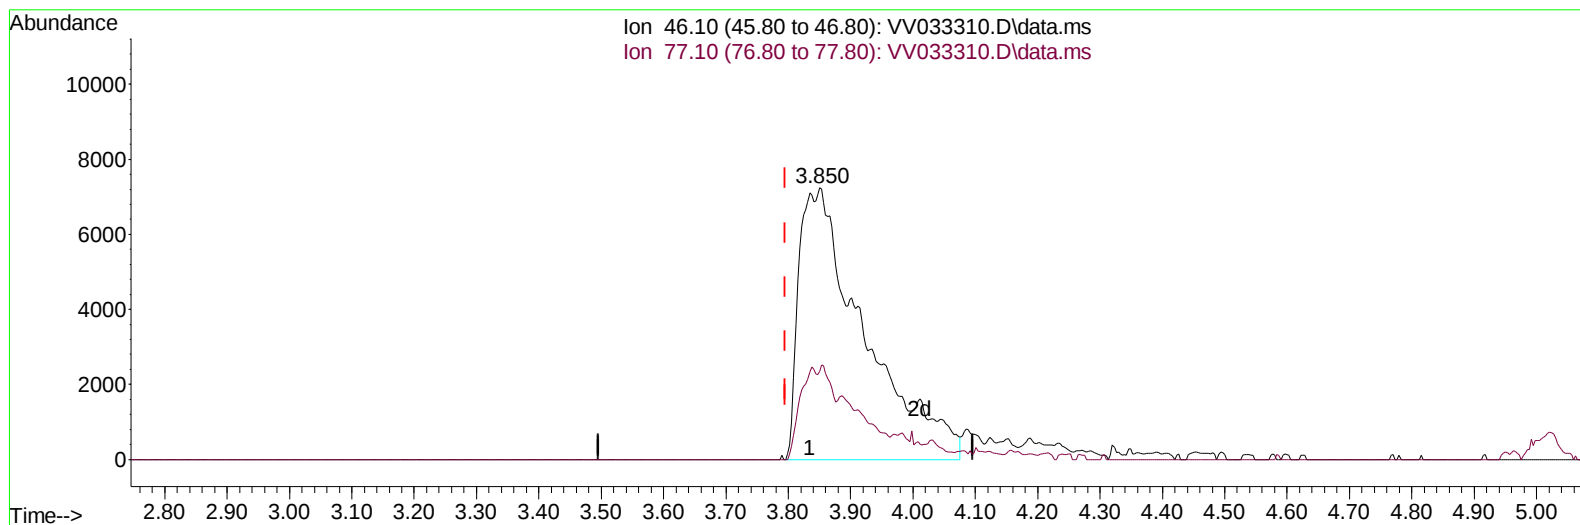

TIC: VV033310.D\data.ms

(20) 2-Butanone-d5 (S)

3.850min (+ 0.055) 53.99 ug/L m

response 52482

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	9.80	9.15
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033310.D
 Acq On : 14 Dec 2023 05:07
 Operator : SY/MD
 Sample : 05770-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y82

Manual IntegrationsAPPROVED

Quant Time: Dec 14 05:46:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Dec 14 01:07:25 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
 Supervised By :Mahesh Dadoda 12/18/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.535	114		128138	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		128755	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		65917	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		39291	4.783	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	95.600%	
7) Chloroethane-d5	1.532	69		30057	4.920	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	98.400%	
11) 1,1-Dichloroethene-d2	2.059	65		15340	4.692	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	93.800%	
20) 2-Butanone-d5	3.850	46		52482m	53.989	ug/L	0.05
Spiked Amount 50.000	Range 40	- 130		Recovery	=	107.980%	
24) Chloroform-d	4.249	84		88729	5.179	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	103.600%	
26) 1,2-Dichloroethane-d4	4.944	65		41024	5.510	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	110.200%	
32) Benzene-d6	4.960	84		168094	5.047	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	101.000%	
36) 1,2-Dichloropropane-d6	5.989	67		40960	5.403	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	108.000%	
41) Toluene-d8	7.243	98		156440	4.820	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	96.400%	
43) trans-1,3-Dichloroprop...	7.558	79		16370	4.733	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	94.600%	
46) 2-Hexanone-d5	8.034	63		51275	53.106	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	106.220%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84		28369	5.533	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	110.600%	
66) 1,2-Dichlorobenzene-d4	11.561	152		64564	5.561	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	111.200%	
Target Compounds							
						Qvalue	
5) Vinyl chloride	1.281	62		4614	0.499	ug/L	89
14) Carbon disulfide	2.240	76		13249	0.555	ug/L	97
22) cis-1,2-Dichloroethene	3.815	96		19024	2.073	ug/L	86
33) Benzene	5.021	78		6946	0.201	ug/L	100
34) Trichloroethene	5.841	95		4967	0.494	ug/L #	76
42) Toluene	7.320	91		56835	1.438	ug/L	99
51) Chlorobenzene	8.818	112		2920	0.108	ug/L	87
52) Ethylbenzene	8.953	91		5262	0.119	ug/L	91
53) m,p-Xylene	9.082	106		2929	0.161	ug/L	98
54) o-Xylene	9.487	106		1116	0.065	ug/L	81
63) 1,2,4-Trimethylbenzene	10.857	105		3454	0.098	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033310.D
Acq On : 14 Dec 2023 05:07
Operator : SY/MD
Sample : 05770-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y82

Manual IntegrationsAPPROVED

Quant Time: Dec 14 05:46:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Dec 14 01:07:25 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/16/2023
Supervised By :Mahesh Dadoda 12/18/2023

