

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033276.D
 Acq On : 13 Dec 2023 15:04
 Operator : SY/MD
 Sample : VV1213WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK388

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	72948	78909	16.35%	2.097%
2	1.532	145	153	165	rVB	54389	64003	13.26%	1.701%
3	2.056	306	316	333	rVB	120439	173406	35.92%	4.609%
4	2.445	428	437	452	rVB4	5326	9525	1.97%	0.253%
5	3.828	857	867	898	rBV2	14885	74942	15.52%	1.992%
6	4.246	978	997	1021	rBV	83491	220054	45.58%	5.848%
7	4.957	1203	1218	1247	rBV3	190520	482768	100.00%	12.831%
8	5.532	1386	1397	1421	rBV	158044	331233	68.61%	8.803%
9	5.834	1483	1491	1501	rVB6	2883	4955	1.03%	0.132%
10	5.989	1525	1539	1562	rBV2	94106	203390	42.13%	5.406%
11	6.915	1816	1827	1844	rBV	49505	95694	19.82%	2.543%
12	7.243	1916	1929	1952	rBV	248710	447226	92.64%	11.886%
13	7.558	2017	2027	2050	rBV2	29173	55253	11.45%	1.468%
14	8.030	2163	2174	2210	rBV	121739	275215	57.01%	7.314%
15	8.786	2396	2409	2433	rBV	240395	400782	83.02%	10.652%
16	10.156	2825	2835	2848	rBV	58090	93568	19.38%	2.487%
17	11.185	3145	3155	3175	rBV	233106	371557	76.96%	9.875%
18	11.561	3261	3272	3289	rBV	218508	347953	72.07%	9.248%
19	13.210	3774	3785	3800	rVB3	5152	9074	1.88%	0.241%
20	13.448	3849	3859	3871	rBV2	8677	13918	2.88%	0.370%
21	13.686	3924	3933	3946	rBV4	6069	9177	1.90%	0.244%




Sum of corrected areas: 3762602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033276.D
Acq On : 13 Dec 2023 15:04
Operator : SY/MD
Sample : VV1213WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK388

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

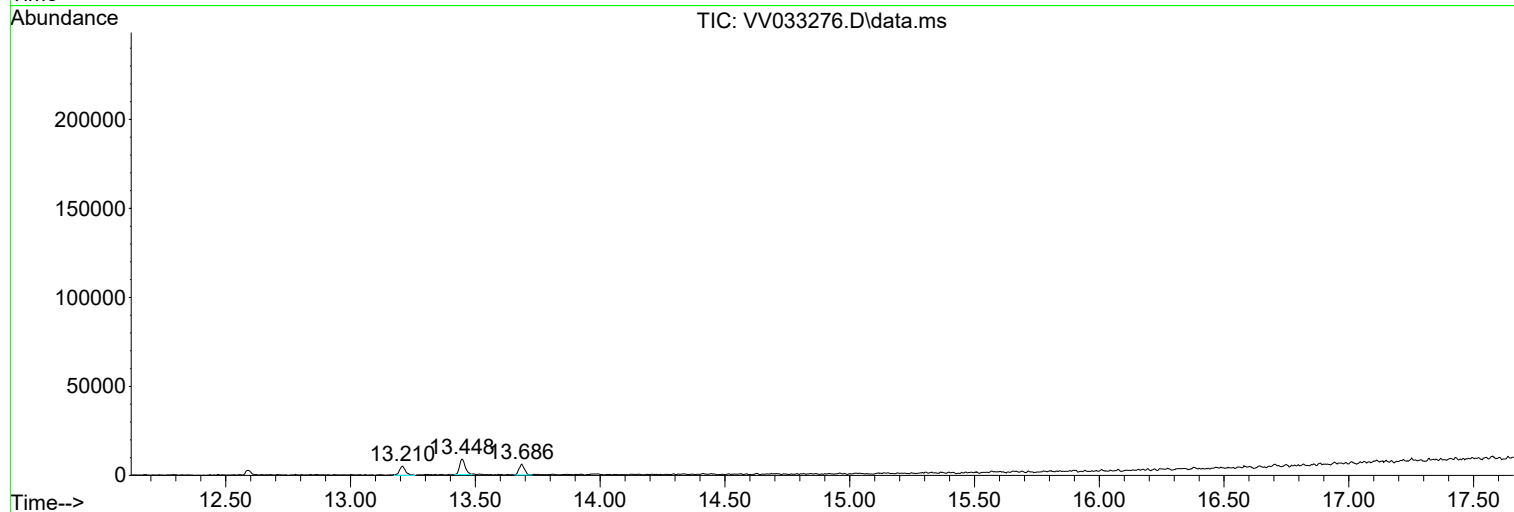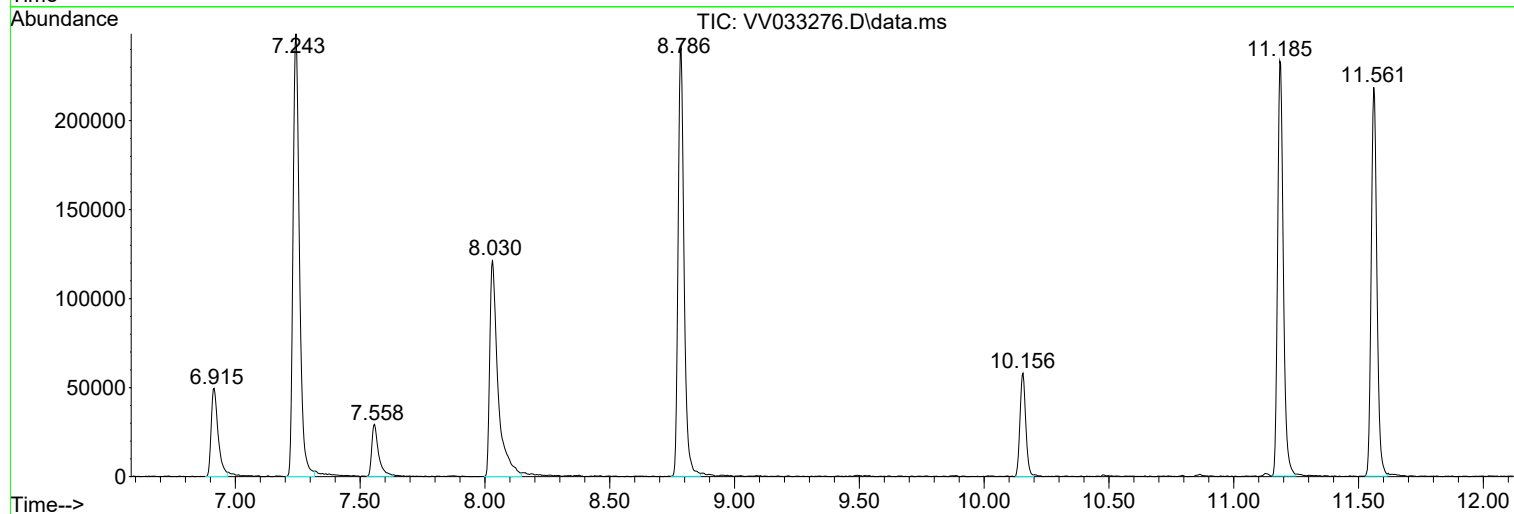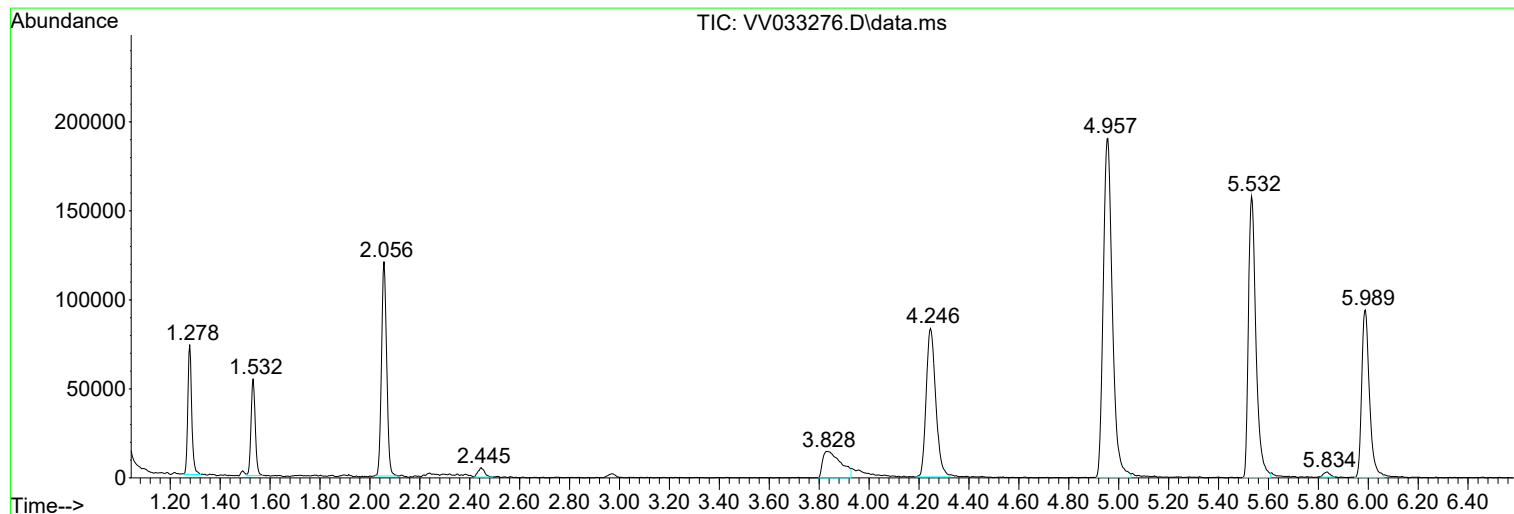

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033276.D
Acq On : 13 Dec 2023 15:04
Operator : SY/MD
Sample : VV1213WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK388

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033276.D
Acq On : 13 Dec 2023 15:04
Operator : SY/MD
Sample : VV1213WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK388

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------