

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033280.D
 Acq On : 13 Dec 2023 16:47
 Operator : SY/MD
 Sample : 05731-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y52

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033280.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	68	73	80	rVB3	3922	4722	1.07%	0.116%
2	1.349	84	96	109	rBV2	72560	127128	28.71%	3.121%
3	1.619	167	180	181	rBV10	20548	37566	8.48%	0.922%
4	1.645	181	188	196	rVV	55733	80218	18.12%	1.969%
5	1.786	227	232	240	rVB	17174	18630	4.21%	0.457%
6	2.179	340	354	368	rBV	106692	165860	37.46%	4.072%
7	2.825	549	555	561	rBV9	3817	4533	1.02%	0.111%
8	3.957	890	907	925	rBV	175134	441226	99.66%	10.831%
9	4.378	1023	1038	1055	rBV2	77326	190729	43.08%	4.682%
10	5.043	1232	1245	1269	rBV3	192291	442750	100.00%	10.869%
11	5.629	1412	1427	1453	rBV2	138749	309080	69.81%	7.587%
12	5.937	1512	1523	1534	rBV6	4376	9607	2.17%	0.236%
13	6.111	1560	1577	1596	rBV	79795	177985	40.20%	4.369%
14	7.001	1843	1854	1872	rBV	42027	78992	17.84%	1.939%
15	7.249	1917	1931	1942	rBV3	29443	59356	13.41%	1.457%
16	7.317	1942	1952	1966	rVV	219875	388159	87.67%	9.529%
17	7.391	1968	1975	1987	rVB2	20304	38102	8.61%	0.935%
18	7.619	2036	2046	2068	rBV2	23143	44536	10.06%	1.093%
19	8.085	2181	2191	2202	rBV2	88554	176149	39.79%	4.324%
20	8.821	2408	2420	2426	rBV	235129	412350	93.13%	10.122%
21	9.111	2499	2510	2523	rBV4	4187	7567	1.71%	0.186%
22	10.169	2827	2839	2860	rVB	46022	76799	17.35%	1.885%
23	11.194	3147	3158	3180	rBV	236318	412381	93.14%	10.123%
24	11.474	3236	3245	3255	rBV2	6556	10331	2.33%	0.254%
25	11.570	3263	3275	3303	rVB	200822	334466	75.54%	8.210%
26	13.445	3850	3858	3869	rBV3	5188	8622	1.95%	0.212%
27	14.577	4203	4210	4218	rBV2	4452	6255	1.41%	0.154%
28	16.249	4724	4730	4741	rBV3	7323	9559	2.16%	0.235%




Sum of corrected areas: 4073658

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033280.D
Acq On : 13 Dec 2023 16:47
Operator : SY/MD
Sample : 05731-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

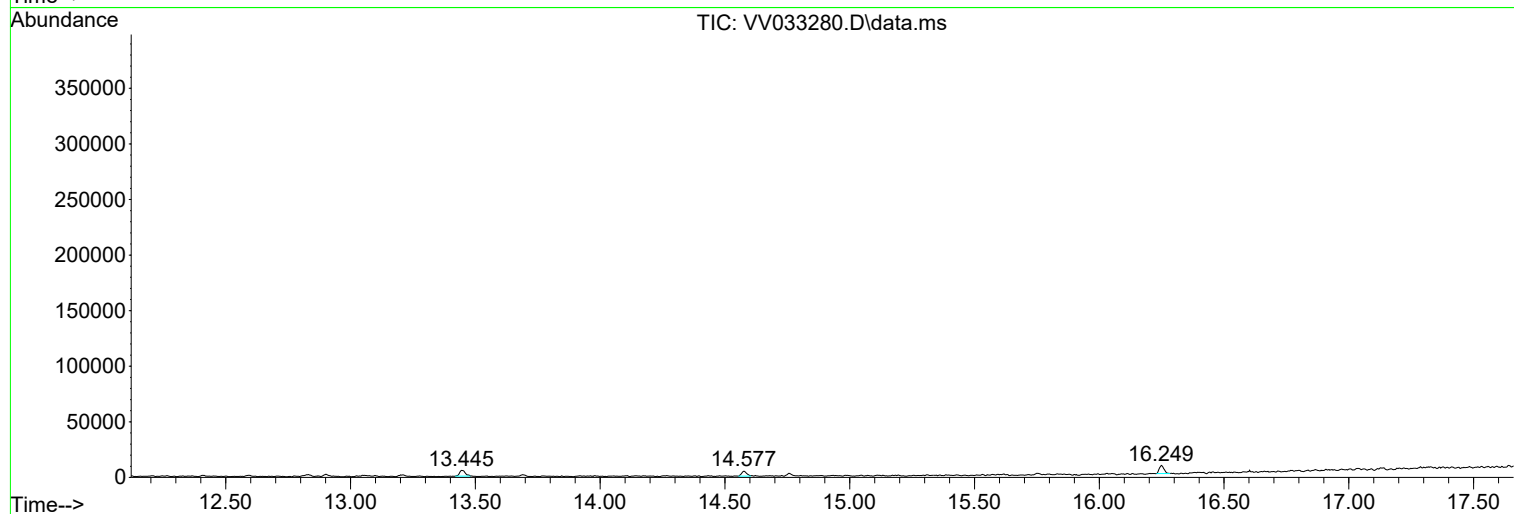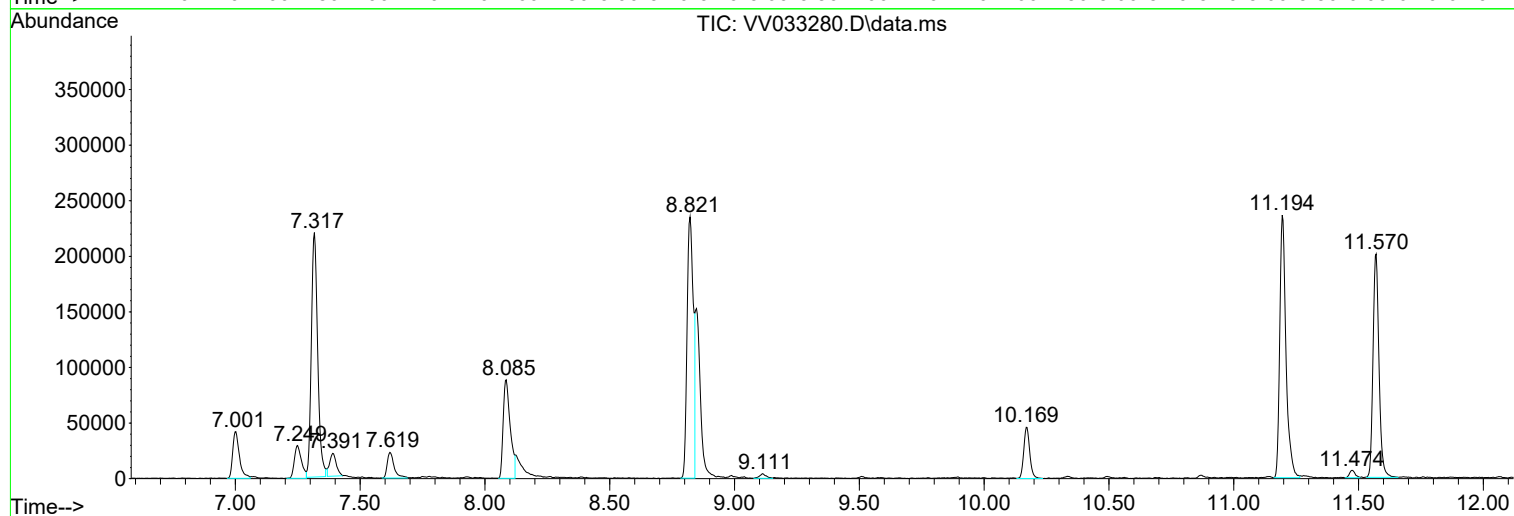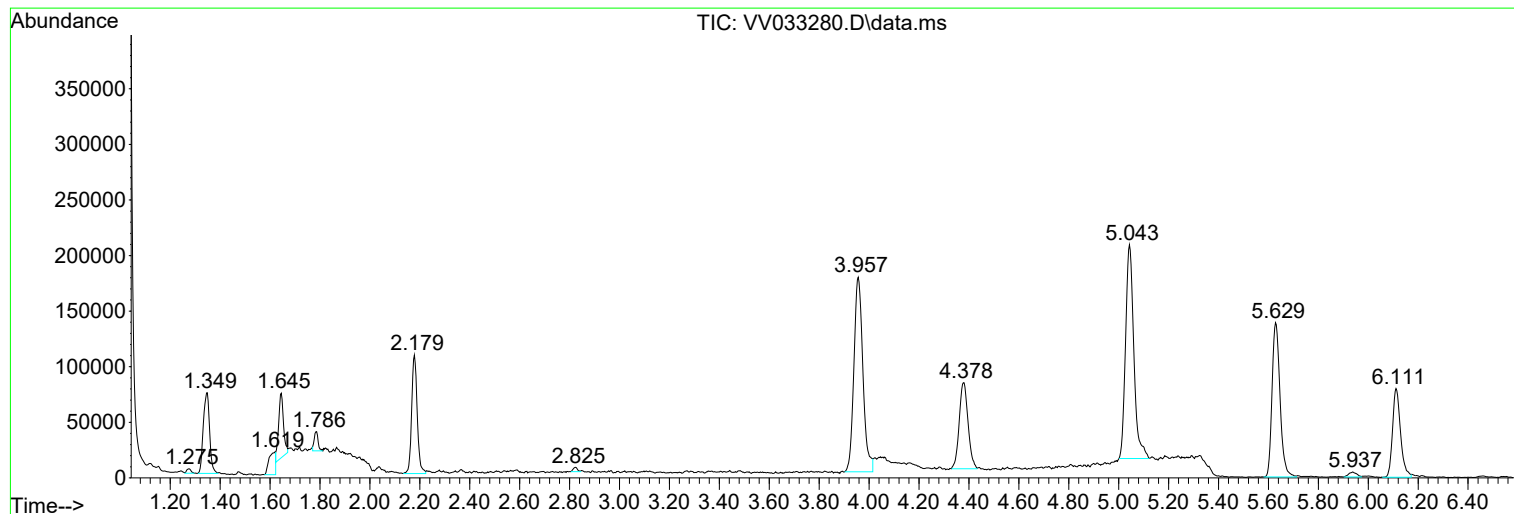

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033280.D
Acq On : 13 Dec 2023 16:47
Operator : SY/MD
Sample : 05731-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033280.D
Acq On : 13 Dec 2023 16:47
Operator : SY/MD
Sample : 05731-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc