

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033281.D
 Acq On : 13 Dec 2023 17:10
 Operator : SY/MD
 Sample : 05731-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y53

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV033281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	25	rVV2	7327	7284	1.67%	0.203%
2	1.134	25	29	40	rVB	9781	11224	2.57%	0.313%
3	1.307	74	83	97	rBV3	116464	195198	44.77%	5.450%
4	1.455	116	129	137	rVB2	10019	15969	3.66%	0.446%
5	1.590	163	171	182	rBV	41390	51728	11.86%	1.444%
6	1.651	187	190	199	rVB7	4611	6126	1.41%	0.171%
7	1.732	207	215	230	rVB	42020	59641	13.68%	1.665%
8	2.134	327	340	358	rBV	94588	151102	34.66%	4.219%
9	2.465	439	443	450	rVB10	3995	5060	1.16%	0.141%
10	2.561	466	473	485	rVB3	9700	18315	4.20%	0.511%
11	2.780	534	541	552	rBV3	3614	6371	1.46%	0.178%
12	3.928	881	898	915	rBV2	59390	155819	35.74%	4.351%
13	4.355	1018	1031	1051	rVB2	71341	185729	42.60%	5.186%
14	5.018	1223	1237	1249	rBV3	197327	436000	100.00%	12.174%
15	5.567	1397	1408	1422	rBV	158684	315540	72.37%	8.811%
16	6.056	1542	1560	1585	rBV2	67518	161632	37.07%	4.513%
17	6.246	1609	1619	1625	rBV5	2390	4444	1.02%	0.124%
18	6.998	1841	1853	1870	rBV2	36182	66664	15.29%	1.861%
19	7.111	1882	1888	1900	rVB6	2405	4664	1.07%	0.130%
20	7.262	1923	1935	1941	rBV6	4090	8473	1.94%	0.237%
21	7.313	1941	1951	1966	rVV	177766	319485	73.28%	8.921%
22	7.391	1967	1975	1997	rVB4	27241	81450	18.68%	2.274%
23	7.619	2034	2046	2060	rBV2	19795	35547	8.15%	0.993%
24	8.088	2182	2192	2205	rBV	64805	148585	34.08%	4.149%
25	8.818	2409	2419	2426	rBV	197167	356905	81.86%	9.966%
26	9.108	2500	2509	2520	rBV6	4023	7408	1.70%	0.207%
27	10.172	2829	2840	2859	rBV2	38866	75566	17.33%	2.110%
28	11.197	3148	3159	3178	rBV	218189	372460	85.43%	10.400%
29	11.570	3259	3275	3296	rBV	189756	316965	72.70%	8.850%




Sum of corrected areas: 3581354

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033281.D
Acq On : 13 Dec 2023 17:10
Operator : SY/MD
Sample : 05731-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

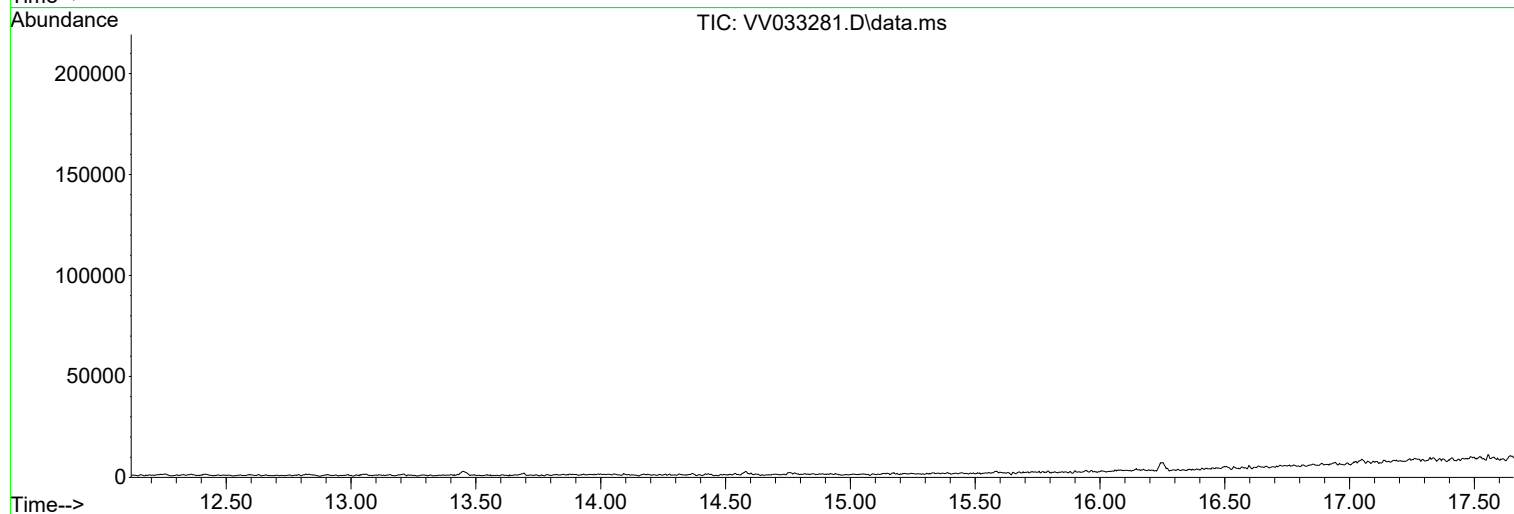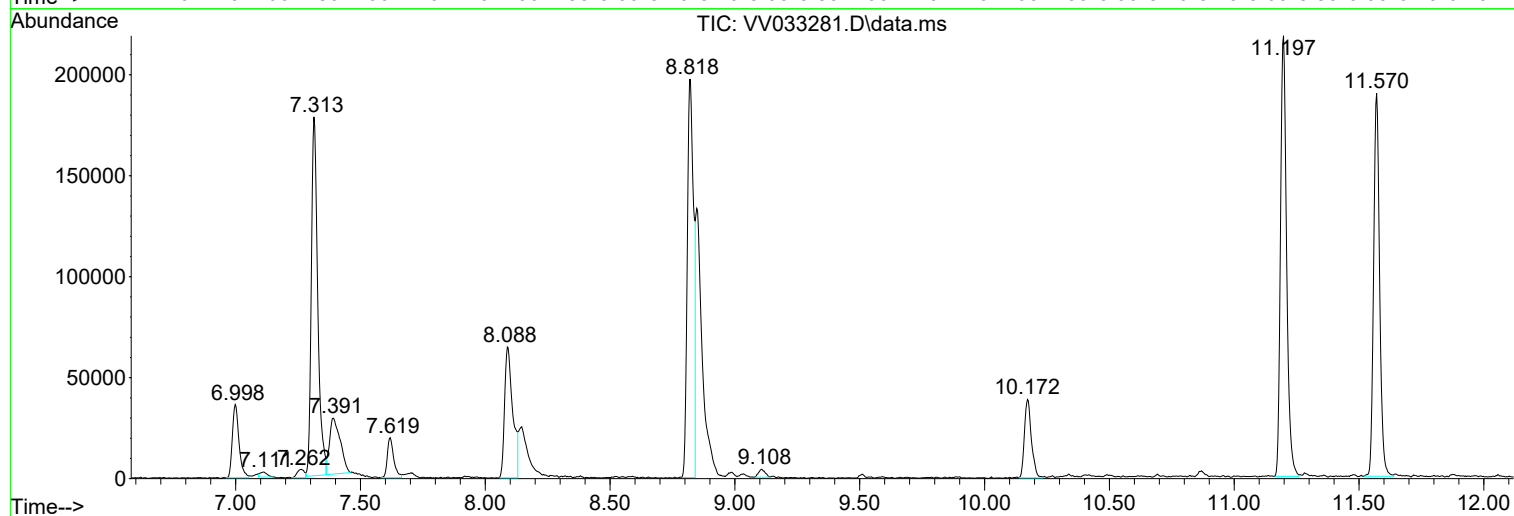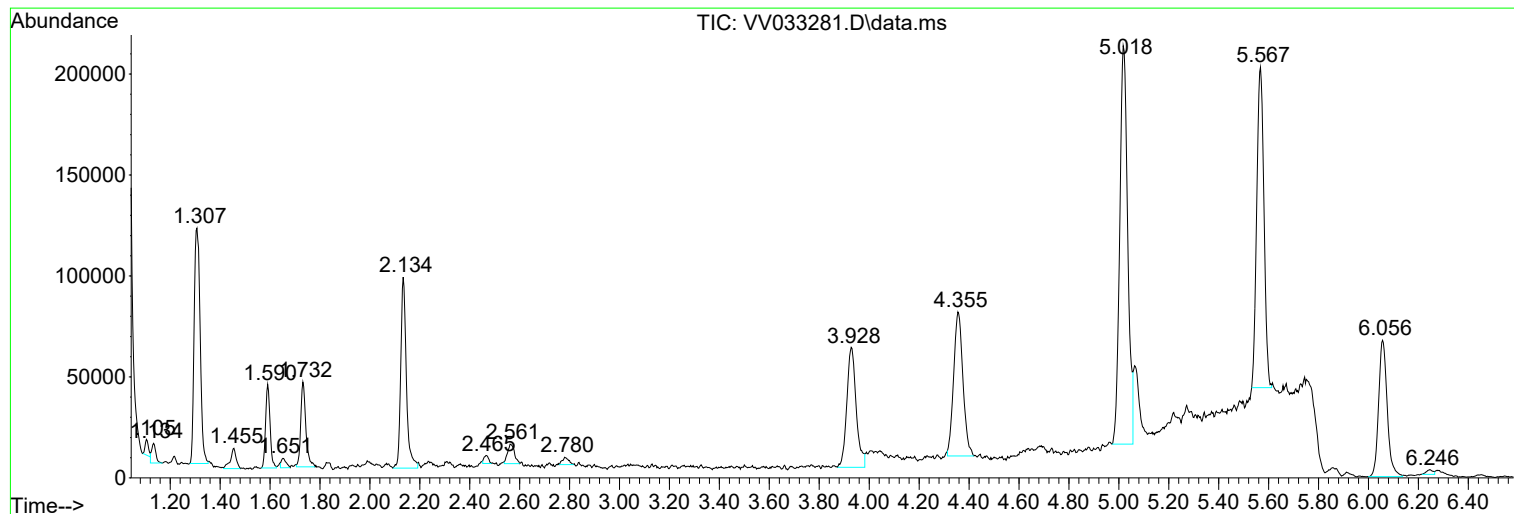

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033281.D
Acq On : 13 Dec 2023 17:10
Operator : SY/MD
Sample : 05731-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y53










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Fluorodichloromethane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.732	0.95 ug/L	59641	1,4-Difluorobenzene	5.567

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Fluorodichloromethane	102	CHCl2F	000075-43-4	94
2			Fluorodichloromethane	102	CHCl2F	000075-43-4	91
3			Fluorodichloromethane	102	CHCl2F	000075-43-4	90
4			Ethane, 1,2-dichloro-1,1,2-trifl...	152	C2HCl2F3	000354-23-4	9
5			Cyclopentene, 1-chloro-	102	C5H7Cl	000930-29-0	5

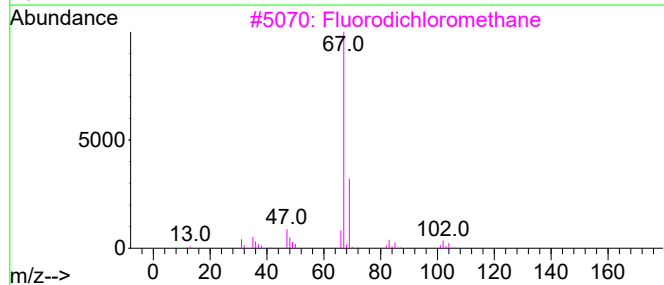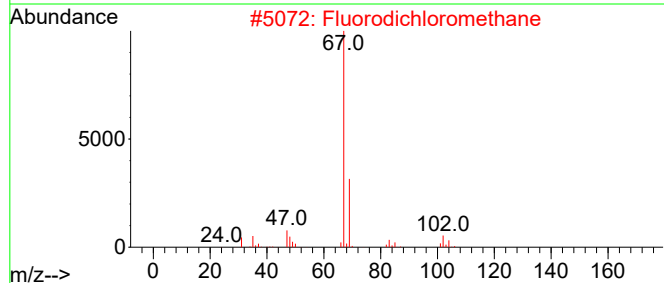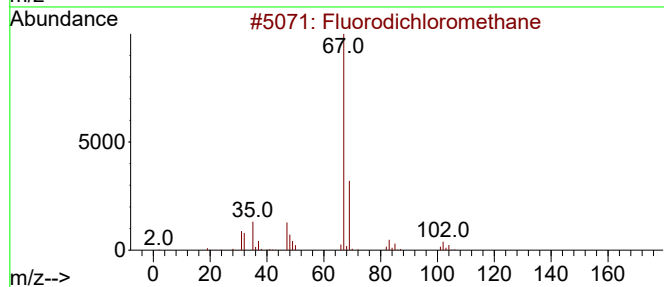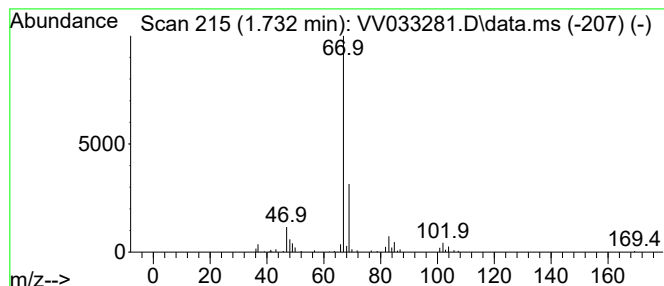

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033281.D
Acq On : 13 Dec 2023 17:10
Operator : SY/MD
Sample : 05731-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Fluorodichlorom...	1.732	0.9	ug/L	59641	1	5.567	315540	5.0