

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033283.D
 Acq On : 13 Dec 2023 17:58
 Operator : SY/MD
 Sample : 05731-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y55

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV033283.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.117	19	24	38	rVB	66500	71750	15.75%	2.031%
2	1.227	52	58	64	rBV	23755	21740	4.77%	0.615%
3	1.320	79	87	102	rVB	86088	100214	22.00%	2.837%
4	1.433	117	122	131	rBV3	4144	5097	1.12%	0.144%
5	1.580	159	168	177	rBV	48707	59087	12.97%	1.673%
6	1.642	182	187	196	rVB4	10619	13147	2.89%	0.372%
7	1.806	232	238	247	rVB2	8687	11530	2.53%	0.326%
8	2.105	320	331	349	rBV	105331	162503	35.68%	4.600%
9	3.873	865	881	893	rBV4	15501	39067	8.58%	1.106%
10	4.307	1001	1016	1036	rVB2	74303	196280	43.10%	5.556%
11	4.982	1209	1226	1250	rBV	199498	455442	100.00%	12.892%
12	5.545	1389	1401	1425	rVB	143097	302886	66.50%	8.574%
13	5.844	1479	1494	1515	rVB3	44849	97273	21.36%	2.753%
14	6.024	1532	1550	1574	rBV	73717	175444	38.52%	4.966%
15	6.973	1835	1845	1862	rBV2	39363	74064	16.26%	2.096%
16	7.291	1931	1944	1960	rBV	199969	349214	76.68%	9.885%
17	7.368	1960	1968	1981	rVB2	18318	34109	7.49%	0.966%
18	7.596	2031	2039	2059	rBV	23776	42607	9.36%	1.206%
19	7.940	2136	2146	2162	rVB2	16224	27141	5.96%	0.768%
20	8.072	2173	2187	2221	rBV2	78051	203414	44.66%	5.758%
21	8.808	2404	2416	2440	rBV	208123	353852	77.69%	10.016%
22	8.969	2455	2466	2476	rVB3	3437	5023	1.10%	0.142%
23	9.095	2497	2505	2518	rVB4	4511	7820	1.72%	0.221%
24	10.165	2825	2838	2853	rBV	49505	79308	17.41%	2.245%
25	11.191	3147	3157	3176	rBV	213100	336688	73.93%	9.530%
26	11.567	3262	3274	3289	rBV	182277	293959	64.54%	8.321%
27	15.786	4570	4586	4587	rBV7	8417	14111	3.10%	0.399%




Sum of corrected areas: 3532770

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033283.D
Acq On : 13 Dec 2023 17:58
Operator : SY/MD
Sample : 05731-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

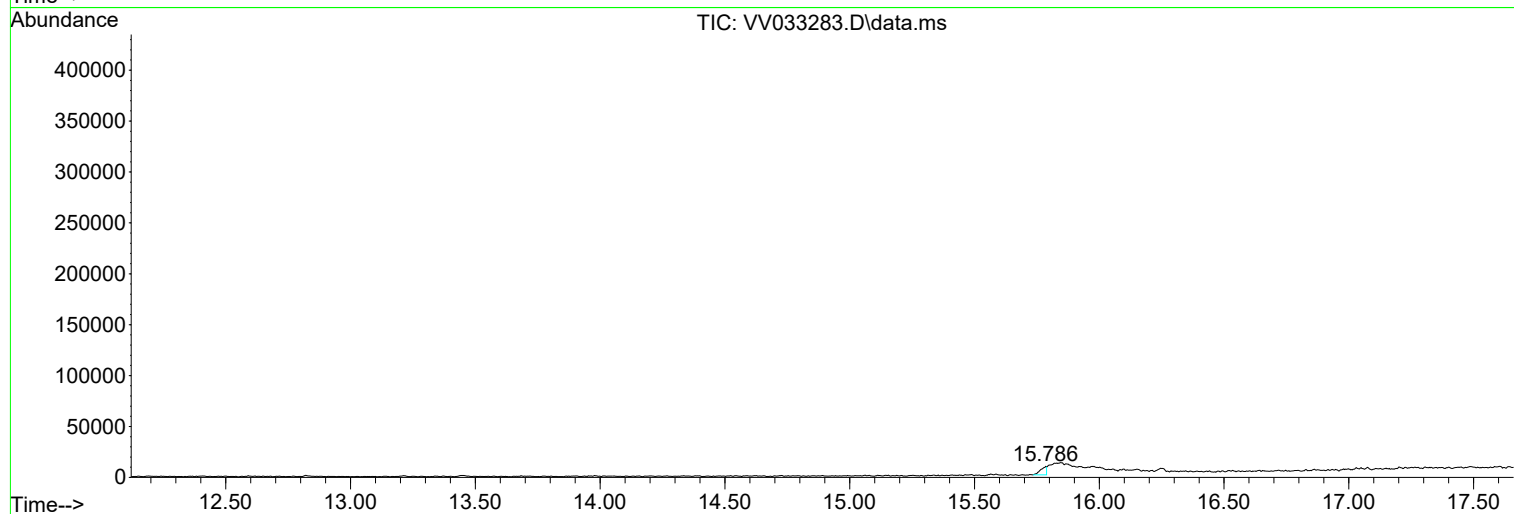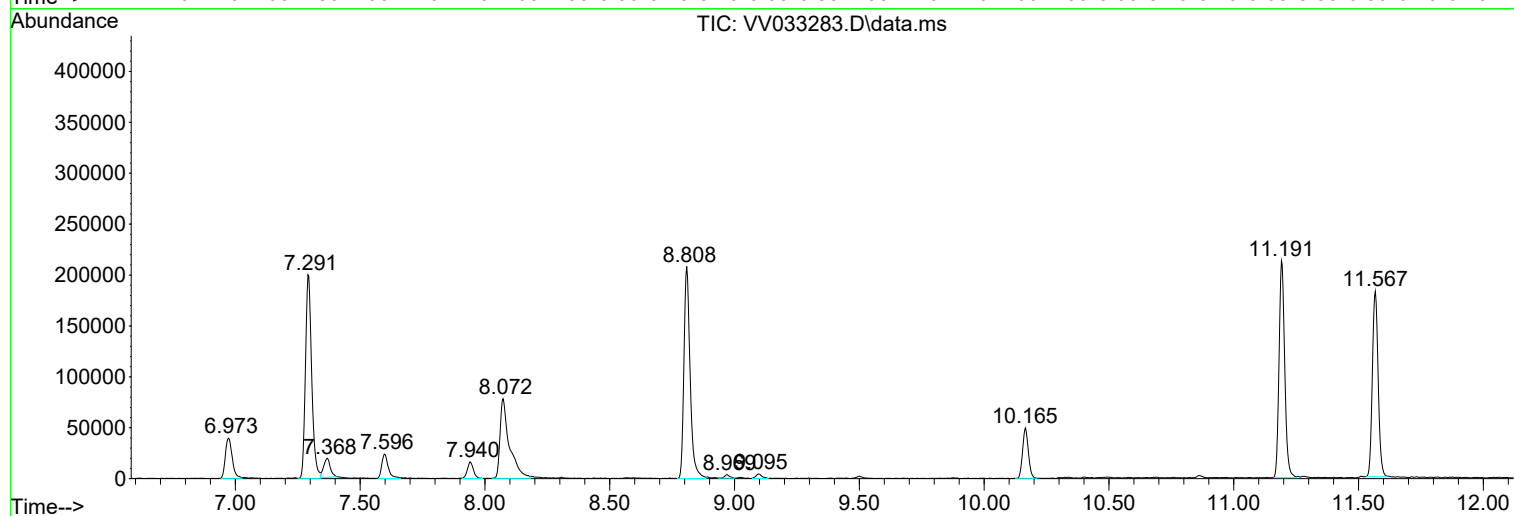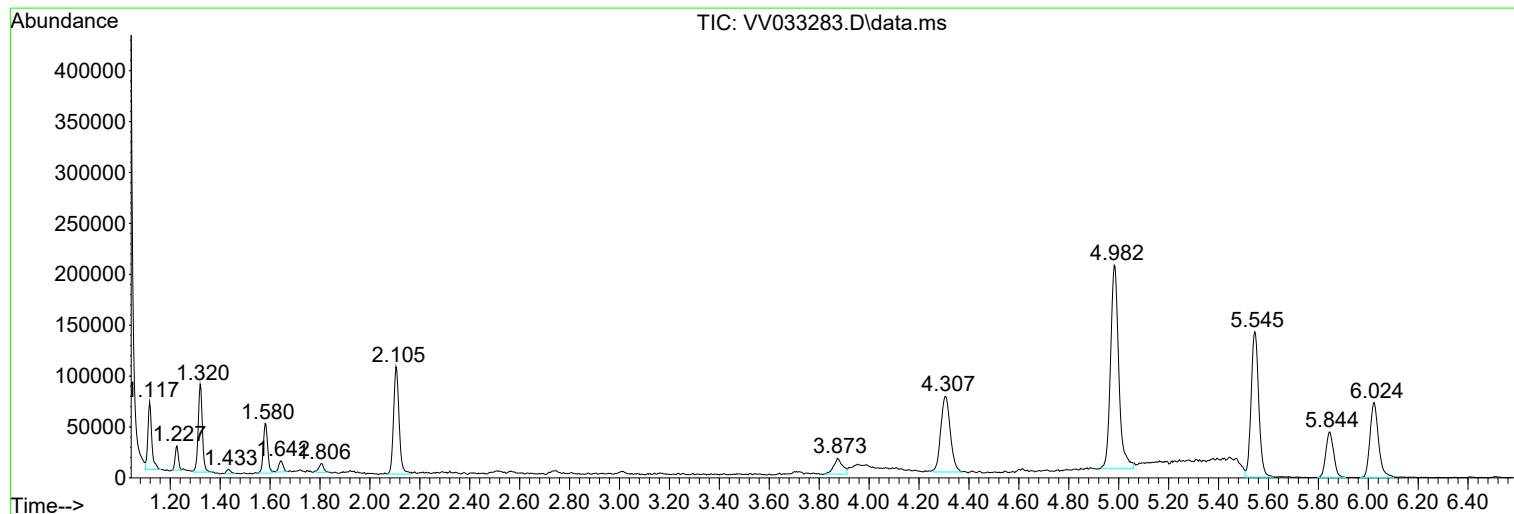

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033283.D
Acq On : 13 Dec 2023 17:58
Operator : SY/MD
Sample : 05731-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y55










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.117	1.18 ug/L	71750	1,4-Difluorobenzene	5.545

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane	44	C3H8	000074-98-6	83
2			Propane	44	C3H8	000074-98-6	56
3			Propane	44	C3H8	000074-98-6	9
4			Propene	42	C3H6	000115-07-1	9
5			Ethylene oxide	44	C2H4O	000075-21-8	5

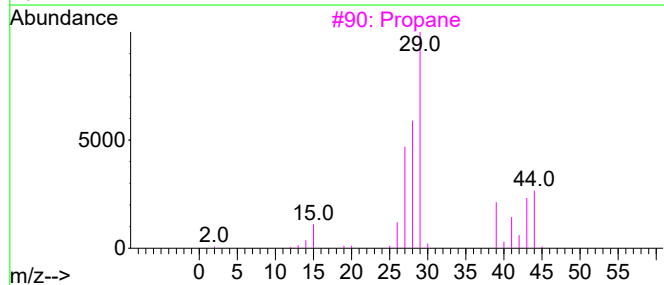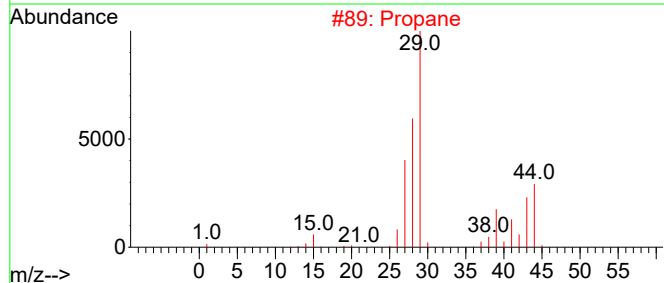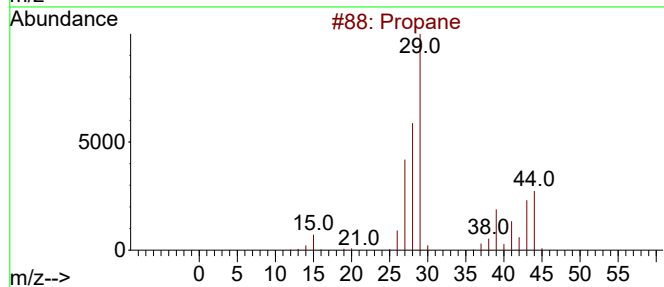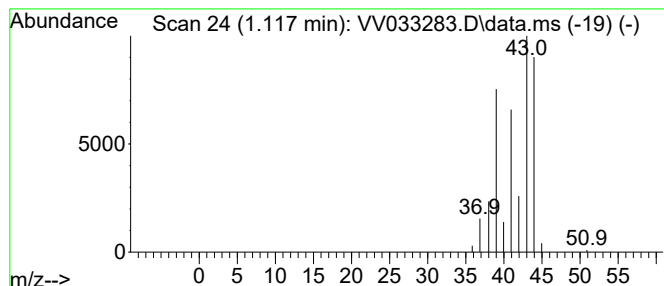

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033283.D
Acq On : 13 Dec 2023 17:58
Operator : SY/MD
Sample : 05731-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.117	1.2	ug/L	71750	1	5.545	302886	5.0