

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
 Data File : VV033306.D
 Acq On : 14 Dec 2023 03:31
 Operator : SY/MD
 Sample : 05770-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0Y78

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV033306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.082	7	13	23	rVB	129197	122709	1.01%	0.626%
2	1.272	62	72	85	rBV2	207589	251583	2.07%	1.284%
3	2.053	302	315	327	rBV	108486	169655	1.40%	0.866%
4	3.802	841	859	889	rBV	5219235	12130395	100.00%	61.910%
5	4.246	980	997	1030	rVB4	87822	284822	2.35%	1.454%
6	4.950	1199	1216	1227	rBV2	184057	434485	3.58%	2.217%
7	5.002	1228	1232	1252	rVB	73330	141345	1.17%	0.721%
8	5.529	1383	1396	1417	rBV	134991	276076	2.28%	1.409%
9	5.825	1470	1488	1520	rBV	971440	1900620	15.67%	9.700%
10	5.989	1526	1539	1552	rBV3	89826	185780	1.53%	0.948%
11	7.240	1919	1928	1940	rVV	230188	405857	3.35%	2.071%
12	7.310	1940	1950	1985	rVB	732453	1276610	10.52%	6.515%
13	8.040	2167	2177	2204	rBV	118005	256535	2.11%	1.309%
14	8.783	2397	2408	2435	rBV	207219	360951	2.98%	1.842%
15	8.947	2447	2459	2474	rBV	155625	253493	2.09%	1.294%
16	9.497	2614	2630	2653	rBV3	94199	193114	1.59%	0.986%
17	10.854	3041	3052	3066	rBV	89422	136828	1.13%	0.698%
18	11.185	3145	3155	3174	rBV2	238686	388248	3.20%	1.981%
19	11.561	3262	3272	3293	rVB	244747	424628	3.50%	2.167%




Sum of corrected areas: 19593734

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033306.D
Acq On : 14 Dec 2023 03:31
Operator : SY/MD
Sample : 05770-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

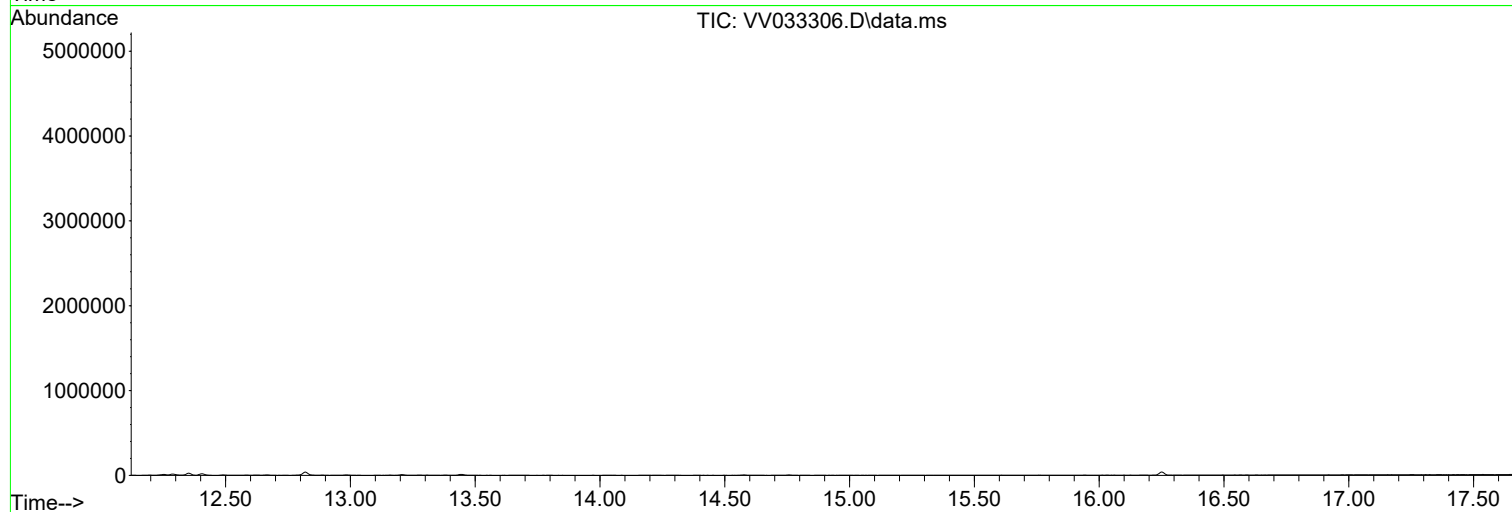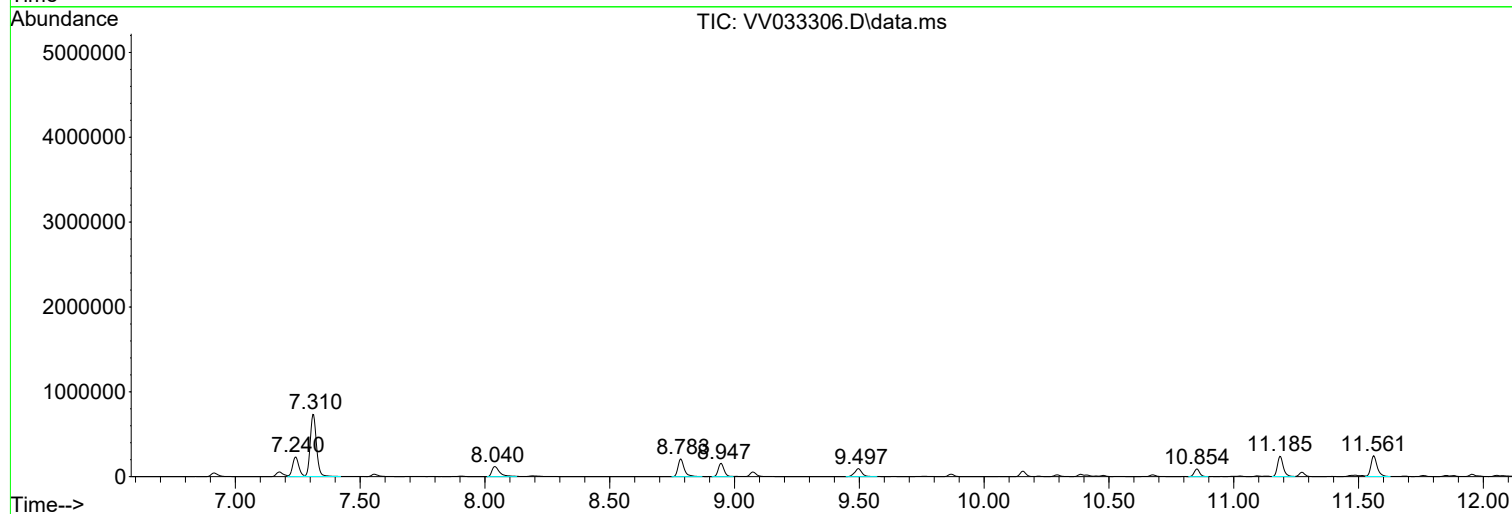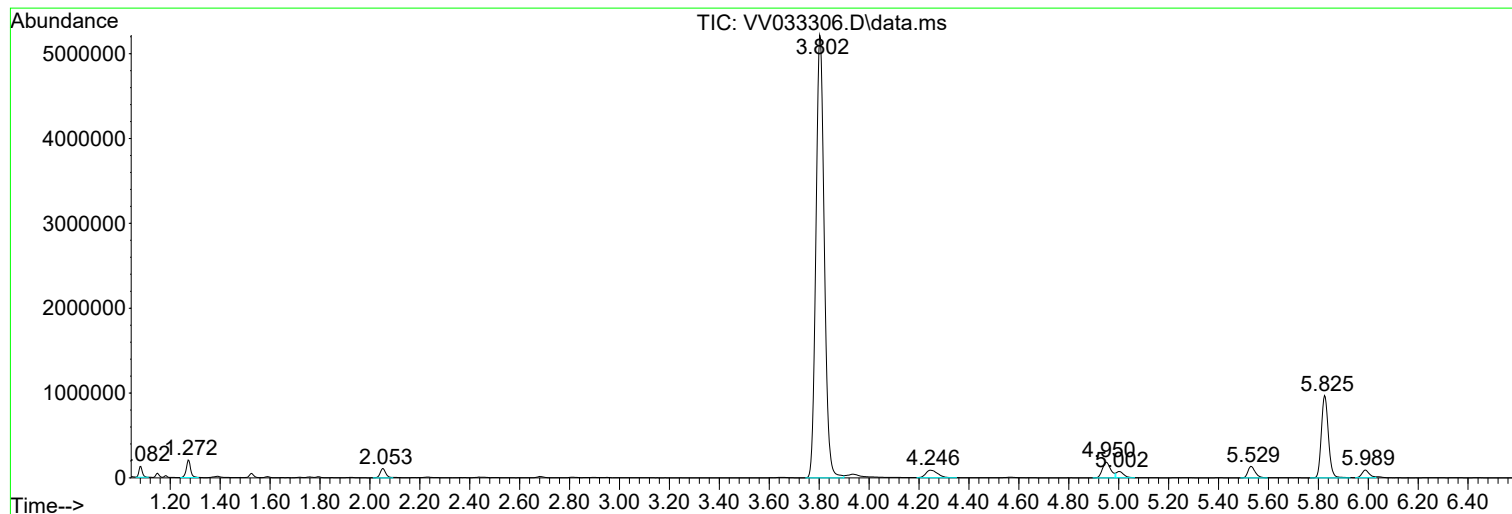

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033306.D
Acq On : 14 Dec 2023 03:31
Operator : SY/MD
Sample : 05770-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y78










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.082	2.22 ug/L	122709	1,4-Difluorobenzene	5.532

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propene	42	C3H6	000115-07-1	64
2			Propene	42	C3H6	000115-07-1	42
3			Cyclopropane	42	C3H6	000075-19-4	7
4			Cyclopropene	40	C3H4	002781-85-3	4
5			2-Oxetanone, 4-methyl-	86	C4H6O2	003068-88-0	4

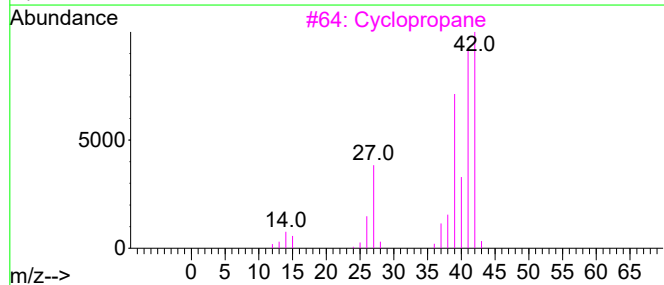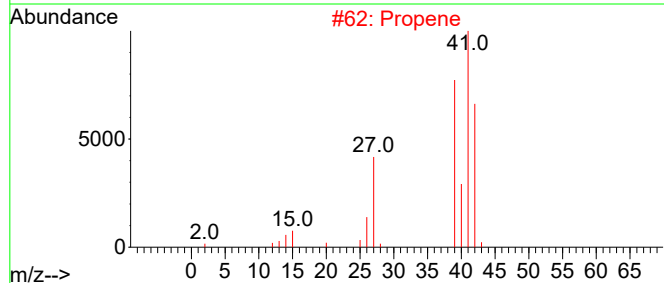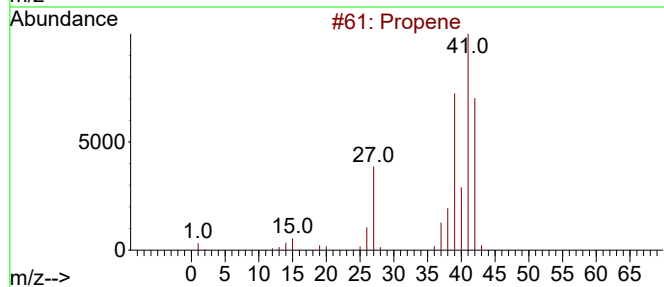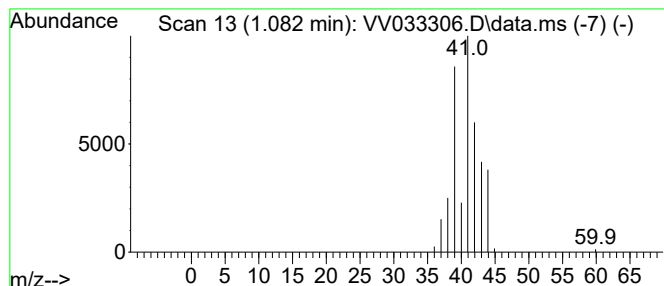

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW121323\
Data File : VV033306.D
Acq On : 14 Dec 2023 03:31
Operator : SY/MD
Sample : 05770-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0Y78

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	1.082	2.2	ug/L	122709	1	5.532	276076	5.0