
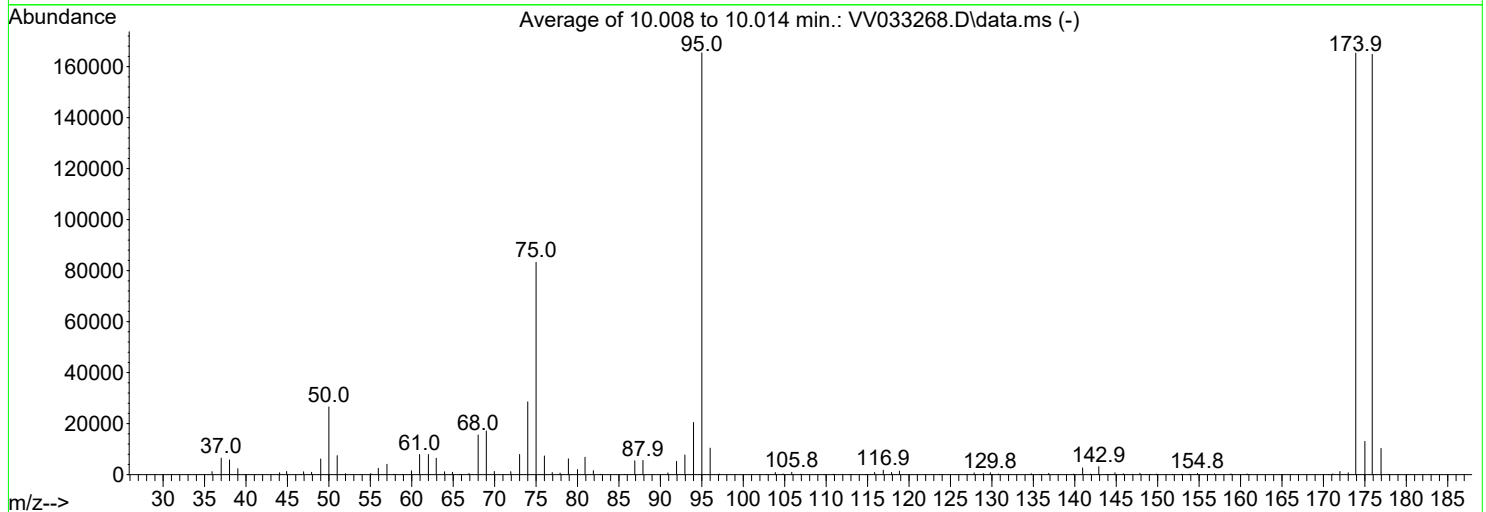


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV121323\
Data File : VV033268.D
Acq On : 13 Dec 2023 09:13
Operator : SY/MD
Sample : BFB234
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB234

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR121323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Dec 14 01:07:25 2023

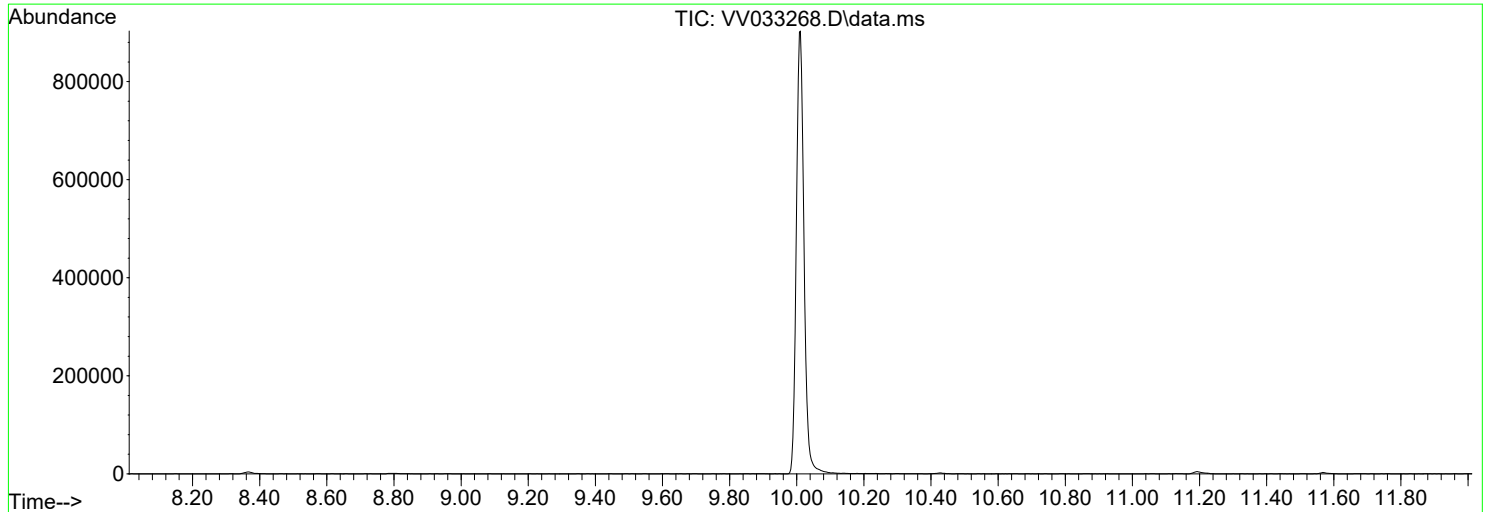

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	26565	PASS
75	95	30	80	50.4	83285	PASS
95	95	100	100	100.0	165397	PASS
96	95	5	9	6.3	10422	PASS
173	174	0.00	2	0.5	768	PASS
174	95	50	120	100.0	165333	PASS
175	174	5	9	7.9	13064	PASS
176	174	95	105	99.7	164800	PASS
177	176	5	10	6.3	10320	PASS

m/z	Abundance
39.80	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
35.90	1097.0
37.00	6562.0
38.00	6063.0
39.00	2449.0
39.90	215.0
41.00	111.0
44.00	767.0
44.90	1284.0
46.00	259.0
46.90	1156.0
47.90	967.0
49.00	6393.0
50.00	27088.0
51.00	7757.0
52.00	331.0
53.70	124.0
55.10	461.0
56.00	2566.0
57.00	4141.0
57.90	251.0
60.00	1533.0
60.90	8175.0
62.00	8150.0
63.00	6935.0
64.00	1187.0
64.90	1032.0
65.70	116.0
66.90	417.0
68.00	16078.0
69.00	17808.0
70.00	1210.0
71.90	1202.0
73.00	8200.0
74.00	29328.0
75.00	85568.0
76.00	7926.0
76.90	918.0
77.80	642.0
78.90	6535.0
80.00	2081.0
80.90	7145.0
81.90	1619.0
82.80	227.0
85.70	165.0
86.90	5831.0
87.90	6162.0
90.90	691.0
92.00	5266.0
92.90	8121.0
94.00	20536.0
95.00	170240.0
96.00	10757.0
97.10	300.0
102.80	133.0
103.90	979.0
104.80	352.0
105.90	941.0
107.00	180.0
109.80	162.0
110.80	207.0
112.00	142.0
112.80	166.0
114.70	162.0
115.80	856.0
116.90	1817.0
117.90	864.0
118.90	1330.0
123.70	125.0
124.00	129.0
125.60	124.0
126.90	111.0
127.90	765.0
129.00	494.0
129.80	806.0
130.90	288.0
134.80	352.0
136.90	549.0
139.80	208.0
141.00	2481.0
141.90	283.0
142.90	3035.0
143.80	165.0
144.20	171.0
144.80	802.0
145.90	414.0
147.00	170.0
147.90	491.0
149.10	202.0
149.90	240.0
151.80	130.0
152.80	221.0
153.80	201.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

154.80	448.0
156.80	414.0
158.80	299.0
160.80	373.0
171.10	465.0
172.00	1193.0
173.00	2303.0
173.90	168768.0
175.00	13639.0
175.90	168384.0
176.90	10826.0
177.90	285.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
35.90	1213.0
37.00	6720.0
38.00	5938.0
39.00	2452.0
39.90	209.0
44.10	803.0
44.90	1336.0
46.00	179.0
46.90	1169.0
47.90	990.0
49.00	6303.0
50.00	27456.0
51.00	7650.0
52.00	363.0
53.70	127.0
55.00	505.0
56.00	2600.0
57.00	4184.0
57.80	239.0
59.90	1569.0
60.90	8154.0
62.00	8030.0
62.90	6628.0
63.90	1135.0
64.90	971.0
65.80	137.0
66.90	484.0
68.00	16095.0
69.00	17632.0
69.90	1293.0
71.90	1294.0
73.00	8144.0
74.00	29456.0
75.00	86184.0
76.00	7530.0
76.90	814.0
77.90	627.0
78.90	6458.0
80.00	2106.0
80.90	7091.0
81.90	1668.0
82.80	194.0
85.70	157.0
86.00	171.0
86.90	5654.0
87.90	5729.0
90.90	732.0
92.00	5411.0
93.00	7934.0
94.00	21168.0
95.00	170752.0
96.00	10813.0
97.10	275.0
102.80	147.0
103.80	917.0
104.80	312.0
105.80	953.0
107.00	219.0
109.70	157.0
110.90	220.0
111.90	179.0
113.00	205.0
114.90	173.0
115.90	915.0
116.90	1833.0
117.90	880.0
118.80	1388.0
125.70	106.0
126.90	110.0
127.80	749.0
128.90	479.0
129.80	831.0
130.80	278.0
134.70	370.0
135.80	106.0
136.80	530.0
139.90	271.0
140.90	2715.0
141.90	274.0
142.90	3278.0
143.80	129.0
144.90	779.0
145.80	388.0
146.90	223.0
147.80	577.0
148.70	171.0
149.10	167.0
149.90	229.0
151.80	149.0
152.80	201.0
153.80	180.0
154.80	534.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

156.20	138.0
156.80	427.0
158.80	292.0
160.80	347.0
171.20	412.0
172.00	1289.0
173.90	170432.0
175.00	13419.0
175.90	170304.0
176.90	10539.0
177.90	218.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

m/z	Abundance
35.90	1201.0
37.00	6136.0
38.00	5345.0
39.00	2012.0
39.90	214.0
44.10	754.0
44.90	1256.0
47.00	1061.0
47.90	860.0
49.00	5755.0
50.00	25152.0
51.00	6988.0
52.00	362.0
52.90	119.0
53.80	120.0
55.00	436.0
55.90	2356.0
57.00	3855.0
57.80	166.0
58.90	113.0
59.90	1390.0
61.00	7444.0
62.00	7486.0
62.90	5896.0
63.90	1016.0
64.90	870.0
65.80	115.0
66.90	483.0
68.00	14563.0
69.00	15884.0
69.90	1199.0
72.00	1180.0
73.00	7430.0
74.00	26912.0
75.00	78104.0
76.00	6573.0
77.00	647.0
78.00	600.0
78.90	5719.0
80.00	1796.0
80.90	6375.0
81.90	1533.0
82.80	139.0
86.00	172.0
86.90	4858.0
87.90	4844.0
90.90	693.0
91.90	4963.0
93.00	7080.0
94.00	19632.0
95.00	155200.0
96.00	9695.0
97.00	191.0
102.80	129.0
103.90	741.0
104.80	221.0
105.80	920.0
106.90	195.0
109.80	114.0
110.90	227.0
111.90	186.0
113.00	246.0
114.90	216.0
115.90	864.0
116.90	1535.0
117.90	862.0
118.80	1346.0
127.80	661.0
128.90	402.0
129.80	695.0
130.70	252.0
134.80	337.0
135.80	115.0
136.80	461.0
139.90	284.0
140.90	2656.0
141.90	262.0
142.90	3178.0
144.90	697.0
145.80	329.0
146.90	206.0
147.80	576.0
148.70	126.0
149.80	210.0
151.80	198.0
152.90	172.0
153.80	163.0
154.80	609.0
156.20	145.0
156.90	368.0
158.90	278.0
160.90	235.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234

170.00	127.0
170.60	245.0
172.00	1279.0
173.90	156800.0
175.00	12135.0
175.90	155712.0
177.00	9595.0
178.00	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB234