


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121418\
 Data File : VV008922.D
 Acq On : 14 Dec 2018 12:07
 Operator : SY/MD
 Sample : BFB60
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB60

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121318WMA.M
 Title : VOC Analysis
 Last Update : Wed Dec 19 00:22:31 2018

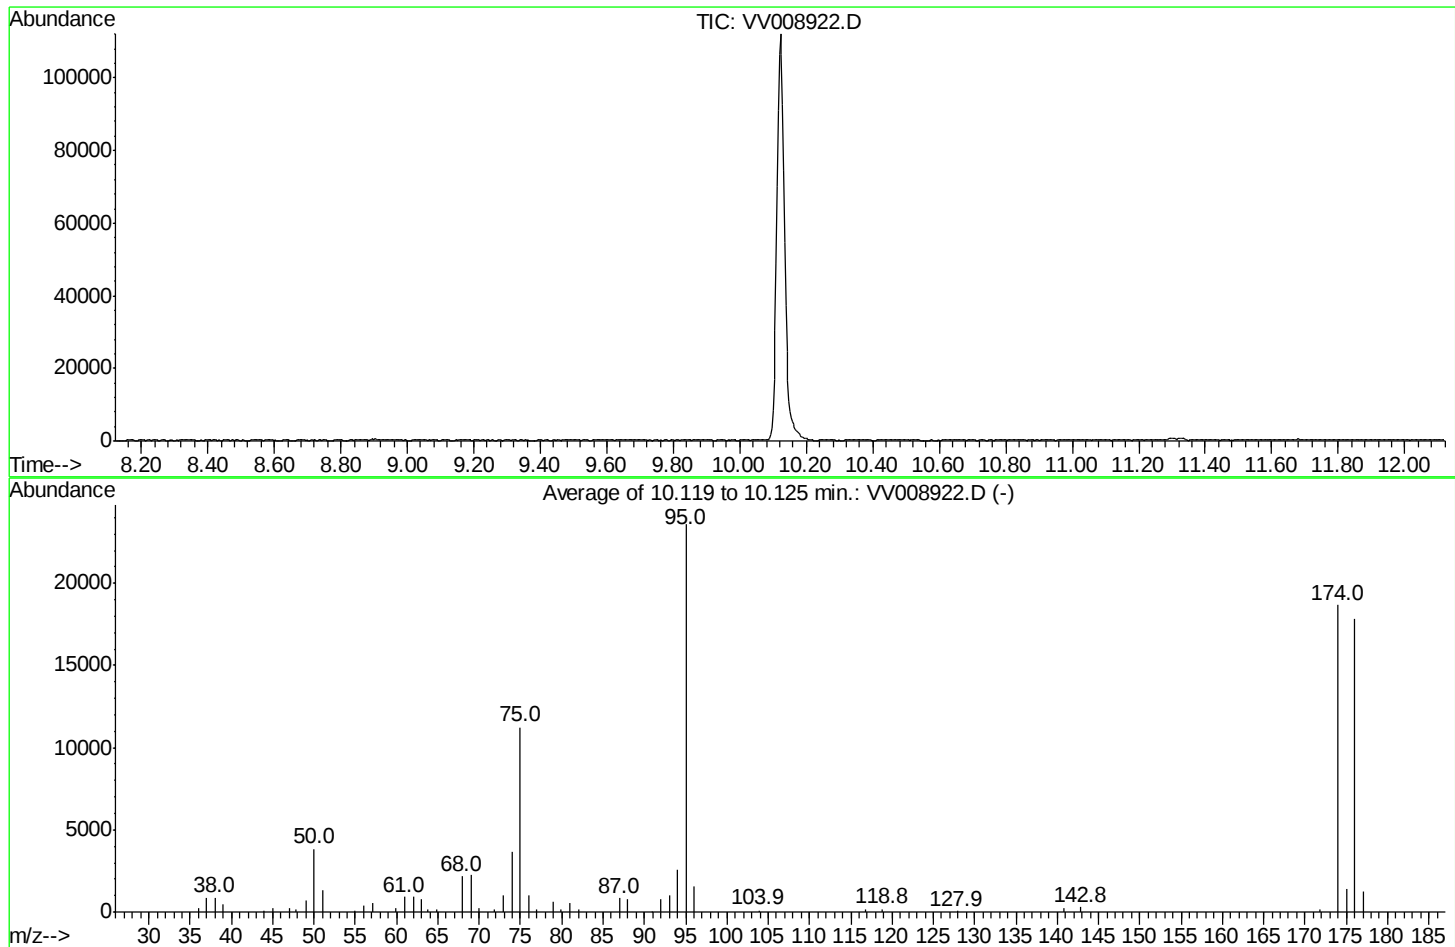

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	3847	PASS
75	95	30	80	47.6	11235	PASS
95	95	100	100	100.0	23589	PASS
96	95	5	9	6.7	1589	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.2	18677	PASS
175	174	5	9	7.5	1395	PASS
176	174	95	101	95.7	17869	PASS
177	176	5	9	7.0	1242	PASS

Scan 2796 (10.080 min): VV008922.D
BFB60

m/z	Abundance
39.90	112.0
43.80	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
35.90	218.0
37.00	798.0
38.00	870.0
39.00	425.0
40.00	113.0
43.90	266.0
45.00	193.0
47.00	211.0
47.70	115.0
49.00	721.0
50.00	3891.0
51.00	1293.0
55.00	103.0
56.00	346.0
57.00	558.0
59.90	262.0
60.90	911.0
62.10	909.0
62.90	749.0
63.80	133.0
64.90	138.0
67.90	2157.0
69.00	2121.0
69.90	245.0
71.90	162.0
72.90	1036.0
74.00	3783.0
75.00	11268.0
76.00	1089.0
77.00	154.0
78.90	582.0
79.90	134.0
80.90	502.0
82.10	134.0
87.00	968.0
87.90	880.0
92.00	771.0
93.00	1019.0
94.00	2578.0
95.00	23640.0
96.00	1554.0
116.90	169.0
118.90	177.0
140.90	185.0
142.90	268.0
171.90	146.0
174.00	17864.0
175.10	1301.0
176.00	17200.0
177.00	1293.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
35.90	211.0
37.00	920.0
38.00	913.0
38.90	481.0
40.00	105.0
43.90	246.0
45.00	213.0
47.10	244.0
47.80	160.0
49.00	680.0
50.00	3977.0
51.00	1345.0
55.00	118.0
55.90	406.0
57.10	542.0
59.90	248.0
61.00	971.0
62.00	1004.0
63.00	787.0
63.80	143.0
64.90	170.0
68.00	2209.0
69.00	2337.0
69.90	289.0
71.90	182.0
72.90	1054.0
74.00	3769.0
75.00	11557.0
76.00	1035.0
76.90	148.0
78.90	651.0
79.90	159.0
80.90	538.0
82.00	129.0
86.90	841.0
87.90	795.0
91.90	808.0
93.00	1048.0
94.00	2721.0
95.00	24400.0
96.00	1647.0
103.90	128.0
116.80	191.0
118.80	211.0
127.90	104.0
140.80	195.0
142.80	323.0
171.80	178.0
174.00	19440.0
175.10	1462.0
176.00	18392.0
177.00	1294.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
36.00	178.0
37.00	918.0
38.00	860.0
38.90	447.0
43.90	242.0
45.00	191.0
47.10	336.0
47.80	188.0
49.00	648.0
50.00	3673.0
51.00	1259.0
55.00	107.0
55.90	396.0
57.10	486.0
59.90	198.0
61.00	914.0
61.90	1008.0
63.00	770.0
63.80	137.0
64.90	185.0
68.00	2127.0
69.00	2371.0
69.90	254.0
71.90	181.0
72.90	970.0
74.00	3441.0
75.00	10881.0
76.00	913.0
77.00	131.0
78.90	699.0
79.80	155.0
80.90	545.0
82.00	114.0
86.90	727.0
88.00	631.0
90.90	107.0
91.90	666.0
93.00	952.0
94.00	2531.0
95.00	22728.0
96.00	1568.0
103.90	127.0
116.80	163.0
118.80	182.0
127.90	102.0
140.80	215.0
142.80	322.0
171.80	188.0
174.00	18728.0
175.10	1422.0
176.00	18016.0
177.00	1140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60